

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX110524\  
 Data File : VX043721.D  
 Acq On : 05 Nov 2024 17:09  
 Operator : JC/MD  
 Sample : P4670-05  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 C0SY7

Quant Time: Nov 06 02:05:11 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXLM110424WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Wed Nov 06 01:38:34 2024  
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----						
Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	164393	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	154970	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	66087	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	41605	47.506	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery =	95.020%		
7) Chloroethane-d5	1.648	69	21865	58.083	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery =	116.160%		
11) 1,1-Dichloroethene-d2	2.294	65	17112	42.326	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery =	84.660%		
21) 2-Butanone-d5	4.465	46	66659	116.248	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery =	116.250%		
24) Chloroform-d	5.056	84	90614	47.995	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	96.000%		
26) 1,2-Dichloroethane-d4	5.952	65	58692	48.936	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	97.880%		
32) Benzene-d6	5.971	84	185986	46.420	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	92.840%		
36) 1,2-Dichloropropane-d6	7.306	67	58906	48.325	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery =	96.640%		
41) Toluene-d8	8.647	98	159016	43.690	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery =	87.380%		
43) trans-1,3-Dichloroprop...	8.952	79	23269	39.916	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery =	79.840%		
47) 2-Hexanone-d5	9.385	63	48509	100.557	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery =	100.560%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	80079	51.202	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery =	102.400%		
66) 1,2-Dichlorobenzene-d4	12.317	152	60854	53.146	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery =	106.300%		
Target Compounds						
13) Acetone	2.392	43	1446	2.711	ug/L	99
-----						


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX110524\  
 Data File : VX043721.D  
 Acq On : 05 Nov 2024 17:09  
 Operator : JC/MD  
 Sample : P4670-05  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 C0SY7

Quant Time: Nov 06 02:05:11 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXLM110424WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Wed Nov 06 01:38:34 2024  
 Response via : Initial Calibration

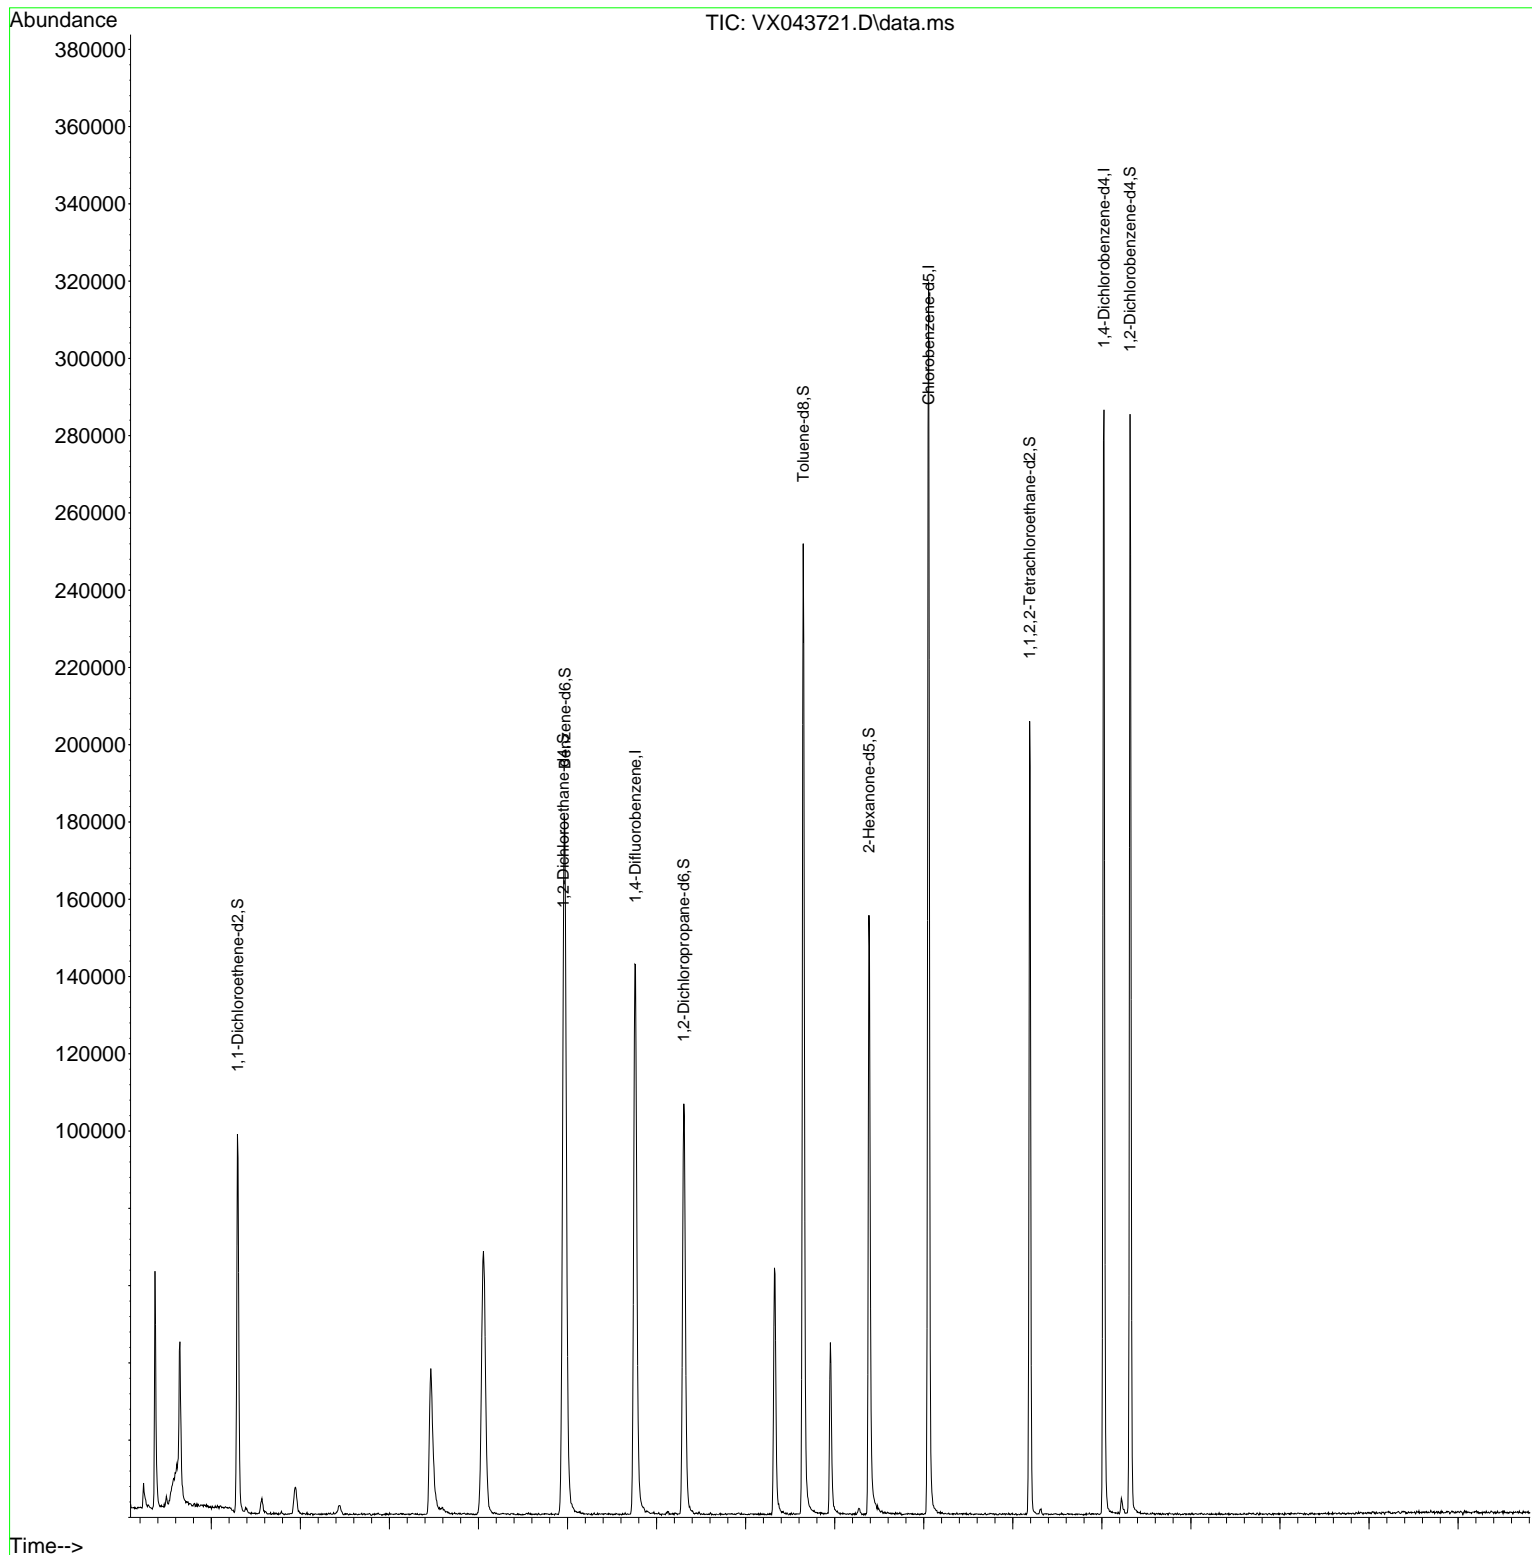

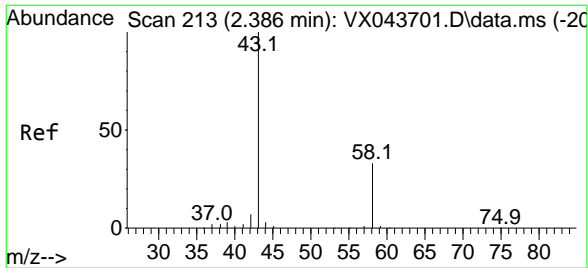

#13  
 Acetone  
 Concen: 2.711 ug/L  
 RT: 2.392 min Scan# 21  
 Delta R.T. 0.006 min  
 Lab File: VX043721.D  
 Acq: 05 Nov 2024 17:09

Instrument : MSVOA\_X  
 ClientSampleId : C0SY7

Tgt Ion	Resp	Lower	Upper
43	1446		
58	32.3	0.0	63.6

