

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043706.D
 Acq On : 05 Nov 2024 11:13
 Operator : JC/MD
 Sample : VIBLK673
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK673

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043706.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	31	rVB2	7363	9884	1.24%	0.165%
2	1.368	43	46	57	rBV	90037	113793	14.31%	1.895%
3	1.642	88	91	103	rVB	50418	79422	9.98%	1.323%
4	2.294	192	198	211	rVB	169619	267933	33.68%	4.462%
5	2.678	258	261	263	rBV3	315	395	0.05%	0.007%
6	2.776	275	277	282	rVB3	1030	1364	0.17%	0.023%
7	2.831	282	286	288	rBV2	499	632	0.08%	0.011%
8	2.940	297	304	312	rBV	4738	11403	1.43%	0.190%
9	3.026	316	318	321	rVV	439	400	0.05%	0.007%
10	3.050	321	322	324	rVV	395	309	0.04%	0.005%
11	3.087	326	328	333	rVB3	634	813	0.10%	0.014%
12	3.434	377	385	391	rBV6	4901	10602	1.33%	0.177%
13	3.507	394	397	399	rBV3	366	509	0.06%	0.008%
14	3.550	402	404	405	rBV	534	295	0.04%	0.005%
15	3.623	415	416	420	rVV2	366	276	0.03%	0.005%
16	3.794	442	444	448	rVB2	264	360	0.05%	0.006%
17	3.831	448	450	452	rBV2	319	389	0.05%	0.006%
18	3.952	467	470	471	rVB3	393	332	0.04%	0.006%
19	3.989	471	476	477	rBV3	354	656	0.08%	0.011%
20	4.135	497	500	503	rVB3	389	457	0.06%	0.008%
21	4.288	522	525	528	rBV	432	458	0.06%	0.008%
22	4.385	539	541	544	rBV2	338	365	0.05%	0.006%
23	4.458	545	553	568	rBV	55597	170332	21.41%	2.836%
24	4.788	606	607	608	rBV	490	273	0.03%	0.005%
25	4.958	634	635	638	rVB2	463	267	0.03%	0.004%
26	5.044	638	649	664	rBV2	96483	307158	38.61%	5.115%
27	5.196	673	674	678	rVB3	526	400	0.05%	0.007%
28	5.288	687	689	692	rVB3	516	438	0.06%	0.007%
29	5.385	699	705	712	rBV4	922	2605	0.33%	0.043%
30	5.525	725	728	729	rBV2	566	636	0.08%	0.011%
31	5.550	729	732	739	rVB4	1152	2551	0.32%	0.042%
32	5.653	747	749	752	rBV2	383	440	0.06%	0.007%
33	5.818	774	776	780	rBV2	272	394	0.05%	0.007%
34	5.958	788	799	820	rBV3	269593	795453	100.00%	13.246%
35	6.202	838	839	841	rBV3	388	293	0.04%	0.005%
36	6.287	851	853	855	rVB2	474	360	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043706.D
 Acq On : 05 Nov 2024 11:13
 Operator : JC/MD
 Sample : VIBLK673
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK673

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	6.318	855	858	860	rBV	532	517	0.06%	0.009%
38	6.586	901	902	904	rBV	462	334	0.04%	0.006%
39	6.757	921	930	944	rVV	195154	487028	61.23%	8.110%
40	7.110	985	988	989	rBV2	1095	1056	0.13%	0.018%
41	7.202	1002	1003	1005	rBV2	330	333	0.04%	0.006%
42	7.305	1011	1020	1039	rBV	150159	353153	44.40%	5.881%
43	7.537	1055	1058	1061	rVB	335	437	0.05%	0.007%
44	7.580	1061	1065	1067	rBV2	224	252	0.03%	0.004%
45	7.683	1080	1082	1085	rVB2	463	388	0.05%	0.006%
46	7.781	1095	1098	1099	rVV2	379	317	0.04%	0.005%
47	8.061	1143	1144	1147	rVB	376	295	0.04%	0.005%
48	8.110	1150	1152	1153	rBV	286	283	0.04%	0.005%
49	8.324	1181	1187	1199	rBV	99122	170988	21.50%	2.847%
50	8.476	1211	1212	1216	rVB2	493	441	0.06%	0.007%
51	8.519	1216	1219	1220	rBV	326	309	0.04%	0.005%
52	8.647	1232	1240	1254	rBV	400776	648277	81.50%	10.795%
53	8.952	1284	1290	1301	rBV	66866	108367	13.62%	1.805%
54	9.104	1313	1315	1316	rBV	464	304	0.04%	0.005%
55	9.275	1340	1343	1345	rBV	664	506	0.06%	0.008%
56	9.384	1356	1361	1379	rBV	249844	395971	49.78%	6.594%
57	9.701	1409	1413	1417	rVB3	1260	1919	0.24%	0.032%
58	9.903	1444	1446	1451	rBV3	313	555	0.07%	0.009%
59	10.049	1465	1470	1483	rBV	388702	574755	72.26%	9.571%
60	10.226	1497	1499	1502	rVB2	458	499	0.06%	0.008%
61	10.457	1535	1537	1539	rVV2	393	310	0.04%	0.005%
62	10.537	1548	1550	1551	rVB	520	255	0.03%	0.004%
63	10.555	1551	1553	1555	rBV2	412	417	0.05%	0.007%
64	10.579	1555	1557	1560	rVB3	317	357	0.04%	0.006%
65	10.628	1564	1565	1568	rBV	372	322	0.04%	0.005%
66	10.811	1592	1595	1597	rBV2	285	333	0.04%	0.006%
67	11.067	1634	1637	1638	rBV2	361	348	0.04%	0.006%
68	11.189	1652	1657	1668	rBV	322402	402336	50.58%	6.700%
69	11.311	1673	1677	1681	rVB3	811	1260	0.16%	0.021%
70	11.488	1704	1706	1708	rBV2	401	398	0.05%	0.007%
71	11.610	1723	1726	1728	rBV2	374	417	0.05%	0.007%
72	11.640	1728	1731	1732	rBV2	339	278	0.03%	0.005%
73	11.975	1782	1786	1788	rBV3	570	778	0.10%	0.013%
74	12.018	1788	1793	1803	rBV	391556	508900	63.98%	8.474%
75	12.317	1837	1842	1860	rBV	426113	543444	68.32%	9.049%
76	12.487	1868	1870	1872	rBV2	459	495	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043706.D
 Acq On : 05 Nov 2024 11:13
 Operator : JC/MD
 Sample : VIBLK673
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK673

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	12.695	1902	1904	1906	rBV2	256	271	0.03%	0.005%
78	12.756	1912	1914	1919	rVB2	989	1127	0.14%	0.019%
79	12.859	1928	1931	1934	rBV	455	635	0.08%	0.011%
80	13.201	1986	1987	1990	rBV2	230	262	0.03%	0.004%
81	13.359	2012	2013	2014	rBV	457	253	0.03%	0.004%
82	13.560	2045	2046	2049	rBV2	301	303	0.04%	0.005%
83	13.591	2049	2051	2052	rBV2	424	336	0.04%	0.006%
84	13.658	2060	2062	2064	rVB	396	315	0.04%	0.005%
85	13.841	2090	2092	2097	rVB2	467	472	0.06%	0.008%
86	14.085	2130	2132	2135	rVB2	570	609	0.08%	0.010%
87	14.127	2135	2139	2144	rBV4	2161	3416	0.43%	0.057%
88	14.201	2148	2151	2154	rVV3	454	559	0.07%	0.009%
89	14.310	2166	2169	2171	rVB3	313	284	0.04%	0.005%
90	14.414	2183	2186	2189	rBV3	427	683	0.09%	0.011%
91	14.585	2212	2214	2215	rBV2	424	321	0.04%	0.005%
92	14.652	2224	2225	2228	rVB2	535	454	0.06%	0.008%
93	14.755	2241	2242	2244	rBV	306	252	0.03%	0.004%
94	14.969	2271	2277	2279	rBV3	702	1134	0.14%	0.019%
95	15.085	2294	2296	2300	rBV5	670	678	0.09%	0.011%
96	15.158	2306	2308	2310	rBV	580	395	0.05%	0.007%
97	15.341	2336	2338	2339	rBV2	433	263	0.03%	0.004%
98	15.396	2343	2347	2348	rBV3	894	1109	0.14%	0.018%
99	15.572	2374	2376	2377	rBV2	539	339	0.04%	0.006%
100	15.902	2428	2430	2431	rBV2	543	310	0.04%	0.005%

Sum of corrected areas: 6005359




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043706.D
Acq On : 05 Nov 2024 11:13
Operator : JC/MD
Sample : VIBLK673
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK673

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

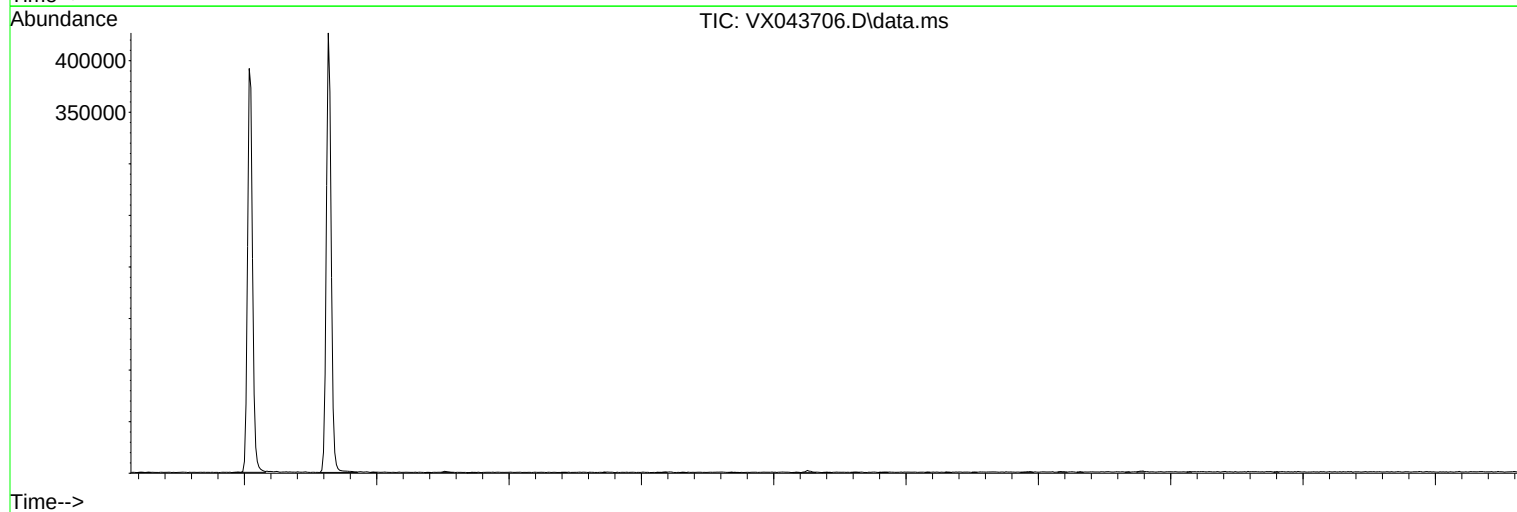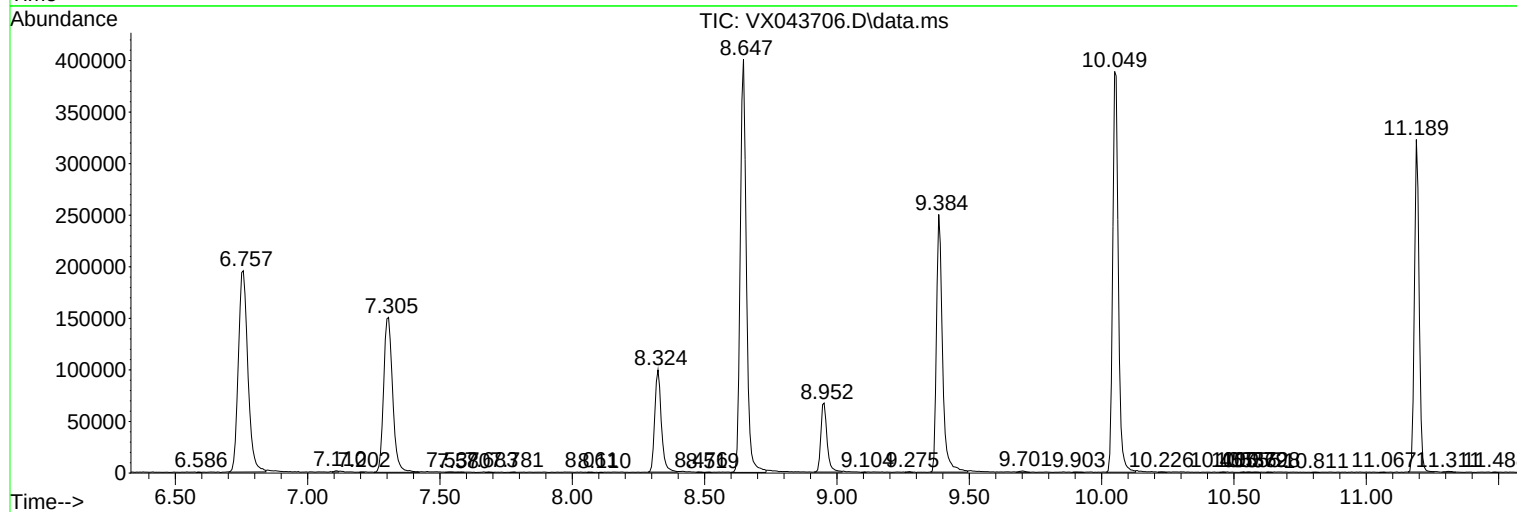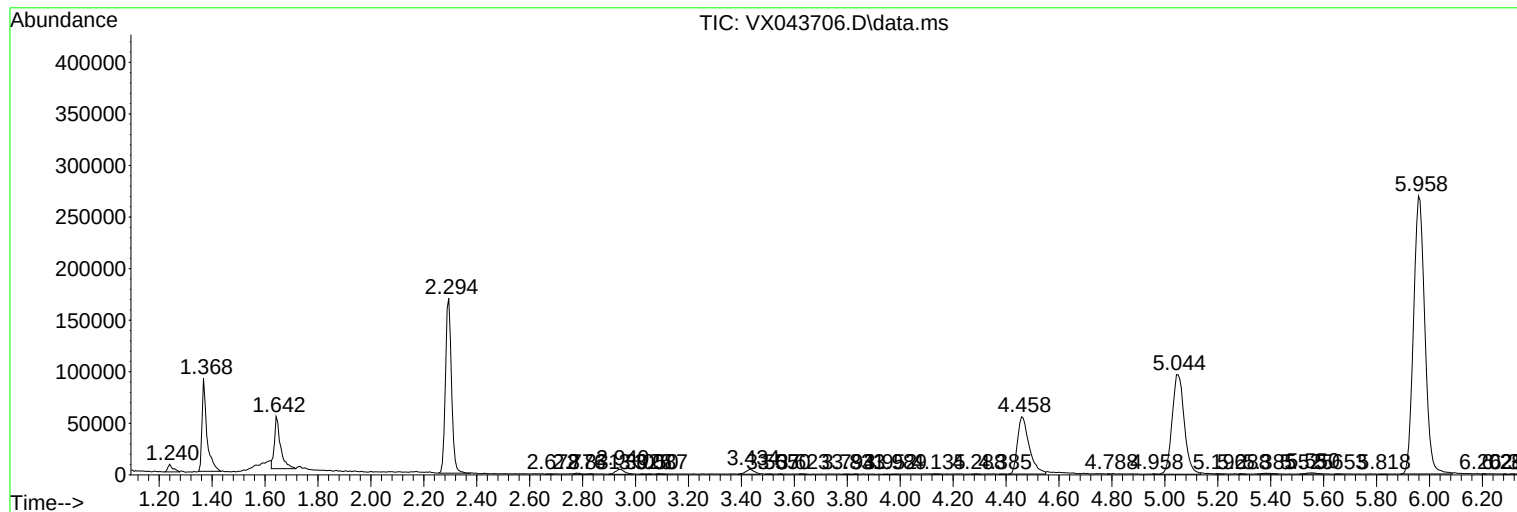

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043706.D
Acq On : 05 Nov 2024 11:13
Operator : JC/MD
Sample : VIBLK673
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK673

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043706.D
Acq On : 05 Nov 2024 11:13
Operator : JC/MD
Sample : VIBLK673
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK673

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
