

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043707.D
 Acq On : 05 Nov 2024 11:36
 Operator : JC/MD
 Sample : P4670-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COSY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M

Title : VOC Analysis

Signal : TIC: VX043707.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	27	rBV	4663	5070	0.60%	0.081%
2	1.295	31	34	38	rVB2	3808	4253	0.50%	0.068%
3	1.368	43	46	60	rVB	88374	113072	13.34%	1.796%
4	1.642	88	91	102	rVB	48559	72540	8.56%	1.152%
5	2.294	192	198	211	rVB	165907	261155	30.81%	4.148%
6	2.489	228	230	231	rBV	529	292	0.03%	0.005%
7	2.782	274	278	283	rVB2	992	1554	0.18%	0.025%
8	2.941	295	304	312	rBV2	2497	6390	0.75%	0.101%
9	3.227	348	351	353	rBV2	397	395	0.05%	0.006%
10	3.331	365	368	370	rVB2	293	287	0.03%	0.005%
11	3.355	370	372	375	rBV2	283	404	0.05%	0.006%
12	3.434	380	385	390	rVB4	2943	6322	0.75%	0.100%
13	3.605	412	413	415	rBV	377	284	0.03%	0.005%
14	3.867	454	456	457	rBV	508	377	0.04%	0.006%
15	3.886	457	459	461	rVV2	354	344	0.04%	0.005%
16	4.014	478	480	483	rBV	337	451	0.05%	0.007%
17	4.404	542	544	546	rBV2	288	344	0.04%	0.005%
18	4.465	546	554	572	rBV2	56750	182231	21.50%	2.894%
19	4.940	628	632	633	rBV2	245	280	0.03%	0.004%
20	5.050	639	650	670	rBV	102872	328230	38.73%	5.213%
21	5.471	717	719	721	rVV	460	346	0.04%	0.005%
22	5.641	745	747	748	rVB	277	196	0.02%	0.003%
23	5.672	751	752	755	rBV	514	601	0.07%	0.010%
24	5.739	761	763	766	rVB2	364	390	0.05%	0.006%
25	5.763	766	767	771	rBV2	361	369	0.04%	0.006%
26	5.964	789	800	819	rVV2	286215	847560	100.00%	13.461%
27	6.233	842	844	846	rVB2	360	264	0.03%	0.004%
28	6.361	861	865	868	rBV4	434	801	0.09%	0.013%
29	6.757	921	930	944	rBV	207867	508118	59.95%	8.070%
30	7.019	971	973	974	rVB	454	253	0.03%	0.004%
31	7.043	974	977	980	rBV4	428	618	0.07%	0.010%
32	7.111	984	988	989	rBV3	838	885	0.10%	0.014%
33	7.196	1001	1002	1004	rBV2	385	258	0.03%	0.004%
34	7.306	1011	1020	1035	rBV	168381	377261	44.51%	5.992%
35	7.476	1046	1048	1050	rBV2	449	580	0.07%	0.009%
36	7.501	1050	1052	1053	rVB	696	377	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043707.D
 Acq On : 05 Nov 2024 11:36
 Operator : JC/MD
 Sample : P4670-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0SY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	7.909	1118	1119	1123	rBV2	328	286	0.03%	0.005%
38	8.123	1150	1154	1156	rVB2	292	330	0.04%	0.005%
39	8.159	1158	1160	1161	rBV	325	220	0.03%	0.003%
40	8.324	1181	1187	1202	rBV	106301	189324	22.34%	3.007%
41	8.531	1220	1221	1224	rBV2	490	461	0.05%	0.007%
42	8.574	1226	1228	1229	rVB	584	340	0.04%	0.005%
43	8.647	1233	1240	1251	rBV	418478	668889	78.92%	10.623%
44	8.915	1282	1284	1285	rBV	334	283	0.03%	0.004%
45	8.952	1285	1290	1302	rVV	77557	121665	14.35%	1.932%
46	9.135	1318	1320	1325	rVB2	530	556	0.07%	0.009%
47	9.196	1327	1330	1333	rBV	294	516	0.06%	0.008%
48	9.275	1337	1343	1347	rVB2	2638	3981	0.47%	0.063%
49	9.385	1356	1361	1381	rBV	252818	410888	48.48%	6.526%
50	9.641	1402	1403	1406	rBV2	382	306	0.04%	0.005%
51	9.720	1413	1416	1418	rBV	345	393	0.05%	0.006%
52	9.799	1427	1429	1431	rBV	313	232	0.03%	0.004%
53	9.909	1444	1447	1449	rBV3	578	616	0.07%	0.010%
54	10.055	1465	1471	1485	rBV	430026	611465	72.14%	9.711%
55	10.336	1515	1517	1520	rBV2	449	325	0.04%	0.005%
56	10.573	1552	1556	1559	rVV3	196	292	0.03%	0.005%
57	10.811	1593	1595	1599	rBV2	433	670	0.08%	0.011%
58	10.939	1615	1616	1619	rVB	467	408	0.05%	0.006%
59	10.970	1619	1621	1623	rBV	319	360	0.04%	0.006%
60	11.092	1640	1641	1646	rVB	307	366	0.04%	0.006%
61	11.140	1646	1649	1650	rBV	501	419	0.05%	0.007%
62	11.189	1652	1657	1672	rVV	328777	438775	51.77%	6.968%
63	11.311	1673	1677	1683	rVB3	2320	3320	0.39%	0.053%
64	11.354	1683	1684	1686	rBV	324	251	0.03%	0.004%
65	11.396	1690	1691	1692	rBV	499	267	0.03%	0.004%
66	11.537	1712	1714	1716	rVB	415	350	0.04%	0.006%
67	11.573	1719	1720	1723	rVV2	413	343	0.04%	0.005%
68	11.683	1736	1738	1740	rVV2	197	196	0.02%	0.003%
69	11.707	1740	1742	1744	rVB2	360	281	0.03%	0.004%
70	11.878	1768	1770	1771	rVB	518	333	0.04%	0.005%
71	11.896	1771	1773	1775	rBV2	357	385	0.05%	0.006%
72	11.969	1784	1785	1788	rBV2	490	303	0.04%	0.005%
73	12.018	1788	1793	1802	rBV	391059	526673	62.14%	8.364%
74	12.219	1820	1826	1835	rBV3	7402	13642	1.61%	0.217%
75	12.317	1837	1842	1853	rVB	440621	563458	66.48%	8.949%
76	12.658	1895	1898	1901	rBV2	478	677	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043707.D
 Acq On : 05 Nov 2024 11:36
 Operator : JC/MD
 Sample : P4670-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0SY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	12.707	1905	1906	1908	rBV	299	228	0.03%	0.004%
78	12.762	1912	1915	1918	rVB2	619	707	0.08%	0.011%
79	12.841	1927	1928	1930	rVB	461	238	0.03%	0.004%
80	12.872	1930	1933	1936	rBV3	393	607	0.07%	0.010%
81	12.920	1939	1941	1943	rBV2	298	353	0.04%	0.006%
82	13.097	1968	1970	1971	rBV2	379	236	0.03%	0.004%
83	13.237	1992	1993	1994	rBV	410	227	0.03%	0.004%
84	13.298	2002	2003	2006	rBV2	395	305	0.04%	0.005%
85	13.414	2020	2022	2025	rBV2	432	472	0.06%	0.007%
86	13.445	2025	2027	2029	rBV2	232	273	0.03%	0.004%
87	13.536	2040	2042	2044	rBV2	326	419	0.05%	0.007%
88	13.658	2060	2062	2065	rBV2	355	425	0.05%	0.007%
89	13.707	2068	2070	2073	rBV	262	356	0.04%	0.006%
90	13.878	2095	2098	2100	rBV3	337	394	0.05%	0.006%
91	13.920	2102	2105	2107	rBV2	400	538	0.06%	0.009%
92	14.012	2118	2120	2123	rVB2	281	325	0.04%	0.005%
93	14.036	2123	2124	2125	rBV	397	221	0.03%	0.004%
94	14.121	2135	2138	2143	rVB4	1111	1769	0.21%	0.028%
95	14.310	2166	2169	2171	rBV2	384	430	0.05%	0.007%
96	14.658	2224	2226	2228	rVB	570	305	0.04%	0.005%
97	14.841	2253	2256	2258	rBV2	369	481	0.06%	0.008%
98	16.085	2459	2460	2463	rBV3	821	669	0.08%	0.011%
99	16.206	2478	2480	2482	rVB2	619	282	0.03%	0.004%
100	16.536	2533	2534	2536	rBV	720	338	0.04%	0.005%

Sum of corrected areas: 6296595




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043707.D
Acq On : 05 Nov 2024 11:36
Operator : JC/MD
Sample : P4670-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0SY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

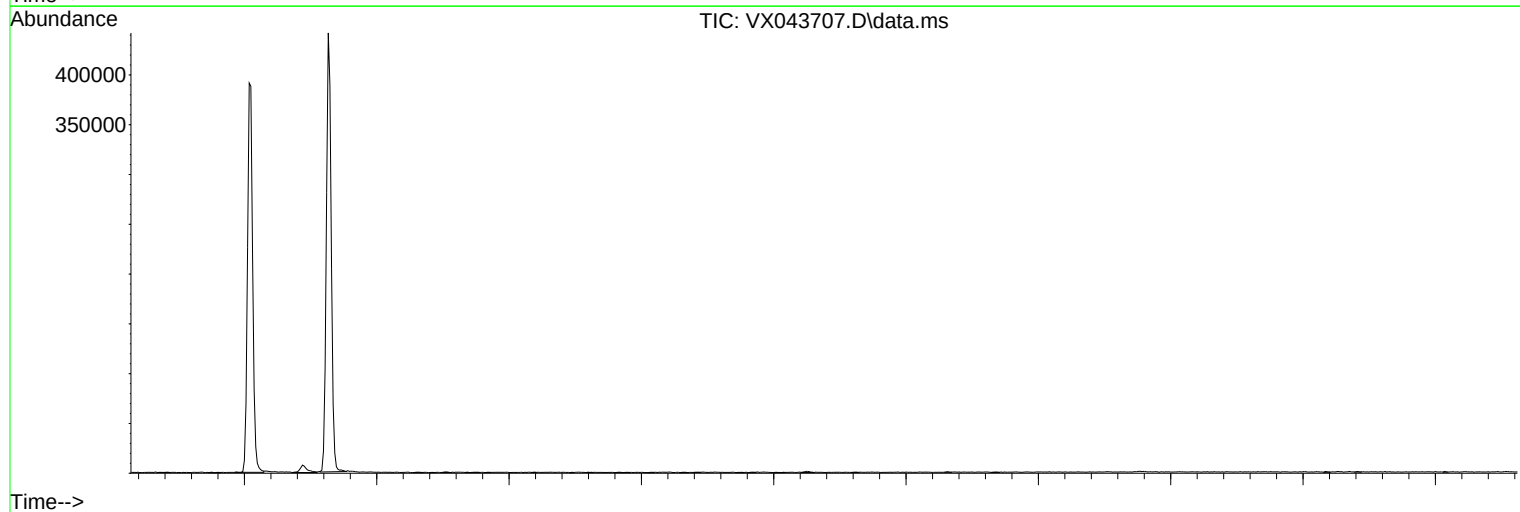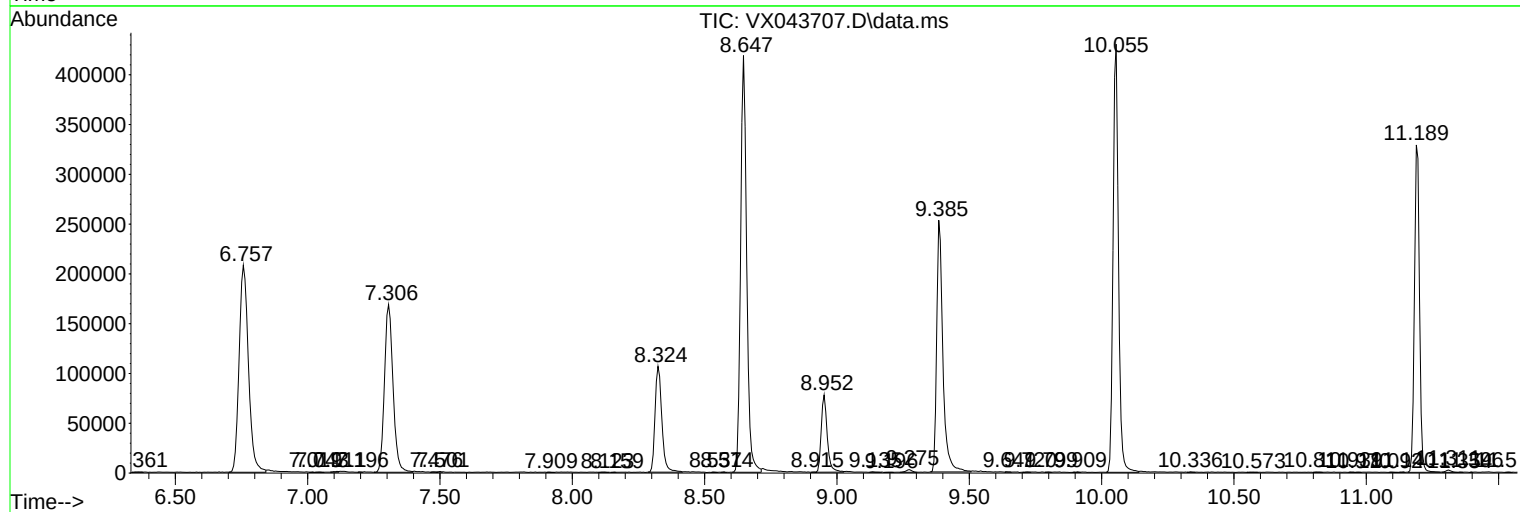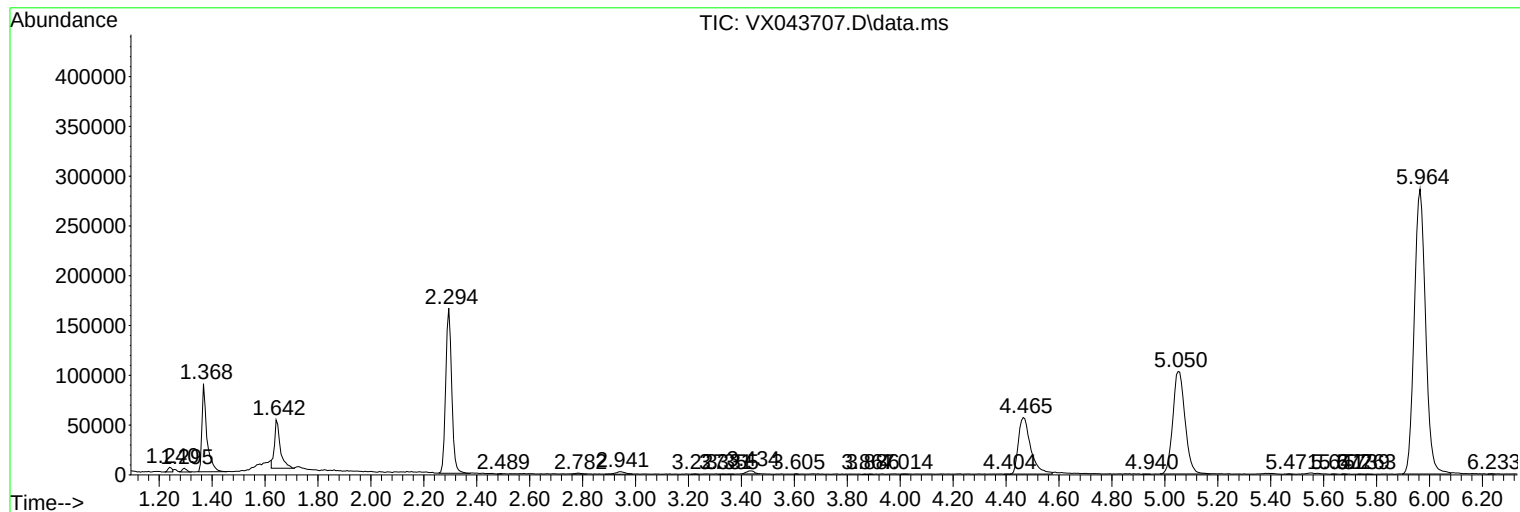

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043707.D
Acq On : 05 Nov 2024 11:36
Operator : JC/MD
Sample : P4670-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0SY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043707.D
Acq On : 05 Nov 2024 11:36
Operator : JC/MD
Sample : P4670-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0SY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
