

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043708.D
 Acq On : 05 Nov 2024 11:59
 Operator : JC/MD
 Sample : P4670-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0SY1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043708.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	28	rBV	4238	5266	0.18%	0.052%
2	1.368	43	46	57	rVB	92066	115537	3.96%	1.132%
3	1.642	88	91	103	rVB	50515	84131	2.88%	0.825%
4	2.294	192	198	208	rBV	168403	268249	9.19%	2.629%
5	2.386	209	213	224	rVB2	10172	19505	0.67%	0.191%
6	2.581	239	245	251	rVB3	2109	3800	0.13%	0.037%
7	2.745	271	272	274	rBV	617	407	0.01%	0.004%
8	2.782	274	278	279	rVV2	826	947	0.03%	0.009%
9	2.867	290	292	293	rVV	565	403	0.01%	0.004%
10	2.941	297	304	319	rVB	32653	78414	2.69%	0.769%
11	3.099	328	330	333	rVB2	303	336	0.01%	0.003%
12	3.288	359	361	364	rVV2	260	313	0.01%	0.003%
13	3.325	366	367	371	rBV	292	332	0.01%	0.003%
14	3.428	379	384	385	rBV4	3316	4517	0.15%	0.044%
15	3.587	407	410	411	rBV2	543	587	0.02%	0.006%
16	3.611	411	414	418	rVB2	355	330	0.01%	0.003%
17	3.721	429	432	435	rBV2	397	380	0.01%	0.004%
18	3.800	442	445	450	rVB3	374	505	0.02%	0.005%
19	3.995	475	477	484	rVV2	337	481	0.02%	0.005%
20	4.465	547	554	568	rBV	54093	168128	5.76%	1.648%
21	4.855	616	618	620	rVB	583	398	0.01%	0.004%
22	5.056	640	651	665	rBV2	105898	329057	11.28%	3.225%
23	5.312	690	693	696	rBV	317	334	0.01%	0.003%
24	5.379	699	704	706	rBV2	963	1238	0.04%	0.012%
25	5.550	726	732	733	rBV	745	1011	0.03%	0.010%
26	5.739	760	763	766	rVB2	326	428	0.01%	0.004%
27	5.964	787	800	819	rBV2	297304	879440	30.14%	8.620%
28	6.300	853	855	857	rBV	402	328	0.01%	0.003%
29	6.464	879	882	883	rBV	291	355	0.01%	0.003%
30	6.665	911	915	918	rVB3	253	372	0.01%	0.004%
31	6.757	921	930	951	rBV	208477	515669	17.67%	5.054%
32	7.019	971	973	976	rBV2	558	433	0.01%	0.004%
33	7.111	985	988	990	rBV3	578	715	0.02%	0.007%
34	7.306	1012	1020	1035	rBV	170879	383088	13.13%	3.755%
35	7.482	1047	1049	1050	rBV	538	376	0.01%	0.004%
36	7.531	1054	1057	1058	rBV2	439	452	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043708.D
 Acq On : 05 Nov 2024 11:59
 Operator : JC/MD
 Sample : P4670-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0SY1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	7.641	1072	1075	1078	rBV2	283	433	0.01%	0.004%
38	7.763	1094	1095	1097	rBV	406	284	0.01%	0.003%
39	7.842	1106	1108	1110	rVB2	381	303	0.01%	0.003%
40	7.860	1110	1111	1114	rBV2	317	320	0.01%	0.003%
41	7.976	1128	1130	1132	rVB2	340	295	0.01%	0.003%
42	8.080	1146	1147	1152	rBV2	357	350	0.01%	0.003%
43	8.238	1171	1173	1176	rVB	401	387	0.01%	0.004%
44	8.324	1181	1187	1200	rBV	115233	192775	6.61%	1.889%
45	8.519	1216	1219	1220	rBV	348	325	0.01%	0.003%
46	8.555	1224	1225	1227	rBV	597	462	0.02%	0.005%
47	8.647	1234	1240	1252	rBV	432659	700020	23.99%	6.861%
48	8.952	1285	1290	1300	rBV	78544	122313	4.19%	1.199%
49	9.275	1339	1343	1349	rVB	3840	6321	0.22%	0.062%
50	9.324	1349	1351	1353	rBV2	418	328	0.01%	0.003%
51	9.385	1356	1361	1383	rBV	247877	410836	14.08%	4.027%
52	10.055	1465	1471	1487	rBV2	464795	804316	27.57%	7.883%
53	10.238	1499	1501	1503	rVV	608	356	0.01%	0.003%
54	10.311	1510	1513	1516	rBV2	586	739	0.03%	0.007%
55	10.342	1516	1518	1520	rVB2	539	349	0.01%	0.003%
56	10.384	1520	1525	1527	rBV2	336	594	0.02%	0.006%
57	10.445	1534	1535	1538	rBV	499	535	0.02%	0.005%
58	10.476	1538	1540	1541	rVB	483	334	0.01%	0.003%
59	10.604	1557	1561	1564	rVB2	326	498	0.02%	0.005%
60	10.768	1585	1588	1590	rBV2	306	340	0.01%	0.003%
61	10.835	1594	1599	1602	rBV3	351	487	0.02%	0.005%
62	10.903	1609	1610	1613	rBV	329	301	0.01%	0.003%
63	11.000	1624	1626	1629	rVB	378	323	0.01%	0.003%
64	11.031	1629	1631	1633	rBV2	394	332	0.01%	0.003%
65	11.189	1652	1657	1666	rBV	349666	442014	15.15%	4.332%
66	11.311	1672	1677	1683	rVB3	4415	6927	0.24%	0.068%
67	11.445	1697	1699	1702	rBV2	425	524	0.02%	0.005%
68	11.969	1779	1785	1789	rBV	53952	70223	2.41%	0.688%
69	12.018	1789	1793	1807	rVB2	454022	668304	22.90%	6.550%
70	12.225	1820	1827	1833	rBV6	2145	4757	0.16%	0.047%
71	12.335	1837	1845	1857	rBV2	1820457	2917819	100.00%	28.598%
72	12.707	1903	1906	1909	rBV3	571	773	0.03%	0.008%
73	12.762	1910	1915	1919	rBV2	1119	1617	0.06%	0.016%
74	12.896	1934	1937	1939	rBV2	343	387	0.01%	0.004%
75	12.975	1949	1950	1955	rVB2	387	399	0.01%	0.004%
76	13.012	1955	1956	1961	rBV2	499	530	0.02%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043708.D
 Acq On : 05 Nov 2024 11:59
 Operator : JC/MD
 Sample : P4670-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0SY1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	13.061	1961	1964	1965	rBV2	296	347	0.01%	0.003%
78	13.103	1967	1971	1979	rVV	14922	21770	0.75%	0.213%
79	13.195	1983	1986	1993	rVV2	4076	5710	0.20%	0.056%
80	13.298	1999	2003	2007	rVB3	444	793	0.03%	0.008%
81	13.518	2037	2039	2043	rBV2	310	513	0.02%	0.005%
82	13.585	2045	2050	2061	rBV	425641	523458	17.94%	5.130%
83	13.701	2067	2069	2071	rVB	384	298	0.01%	0.003%
84	13.725	2071	2073	2077	rVB2	348	430	0.01%	0.004%
85	13.786	2079	2083	2087	rVB4	1545	1888	0.06%	0.019%
86	13.835	2089	2091	2093	rVB	438	344	0.01%	0.003%
87	13.859	2093	2095	2099	rBV3	400	392	0.01%	0.004%
88	13.957	2106	2111	2119	rBV	251404	320675	10.99%	3.143%
89	14.128	2135	2139	2143	rBV2	938	1616	0.06%	0.016%
90	14.262	2156	2161	2168	rBV	8909	12359	0.42%	0.121%
91	14.310	2168	2169	2172	rVV2	349	379	0.01%	0.004%
92	14.432	2185	2189	2191	rBV2	321	518	0.02%	0.005%
93	14.609	2216	2218	2220	rVB3	461	314	0.01%	0.003%
94	14.664	2225	2227	2228	rBV2	289	293	0.01%	0.003%
95	14.780	2242	2246	2253	rVV2	7338	10184	0.35%	0.100%
96	15.121	2300	2302	2304	rBV3	453	553	0.02%	0.005%
97	15.249	2317	2323	2332	rVB2	47762	72736	2.49%	0.713%
98	15.572	2374	2376	2377	rBV2	784	434	0.01%	0.004%
99	16.255	2486	2488	2491	rBV2	571	521	0.02%	0.005%
100	16.304	2493	2496	2498	rBV2	466	574	0.02%	0.006%

Sum of corrected areas: 10202891




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043708.D
Acq On : 05 Nov 2024 11:59
Operator : JC/MD
Sample : P4670-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0SY1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

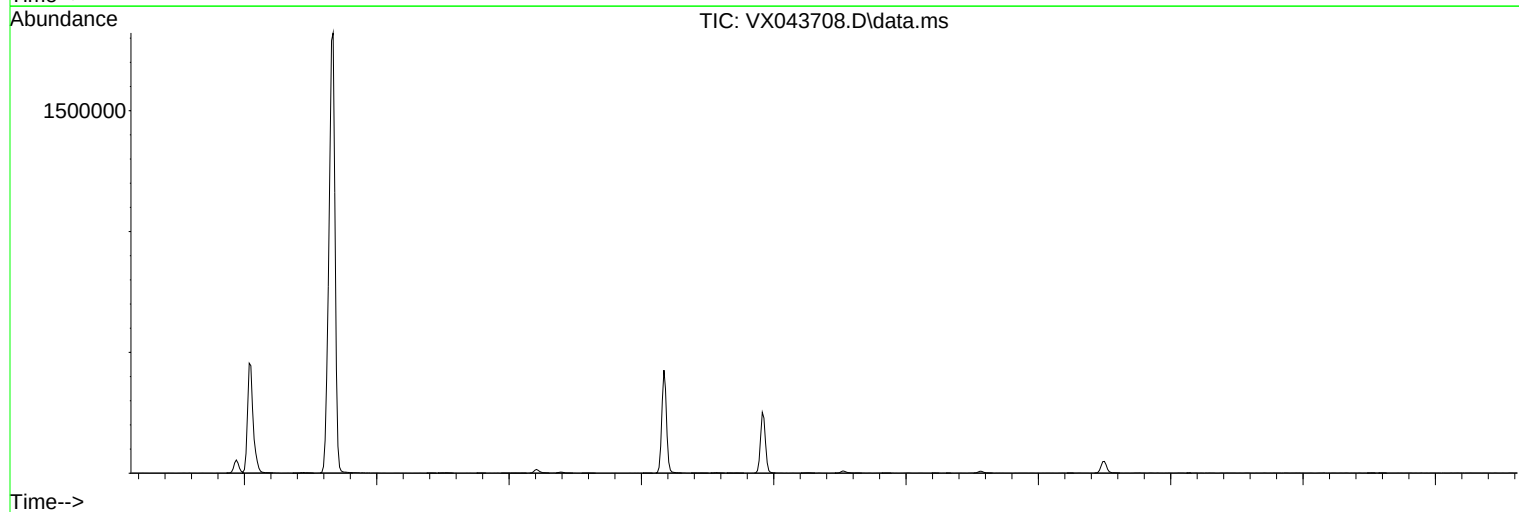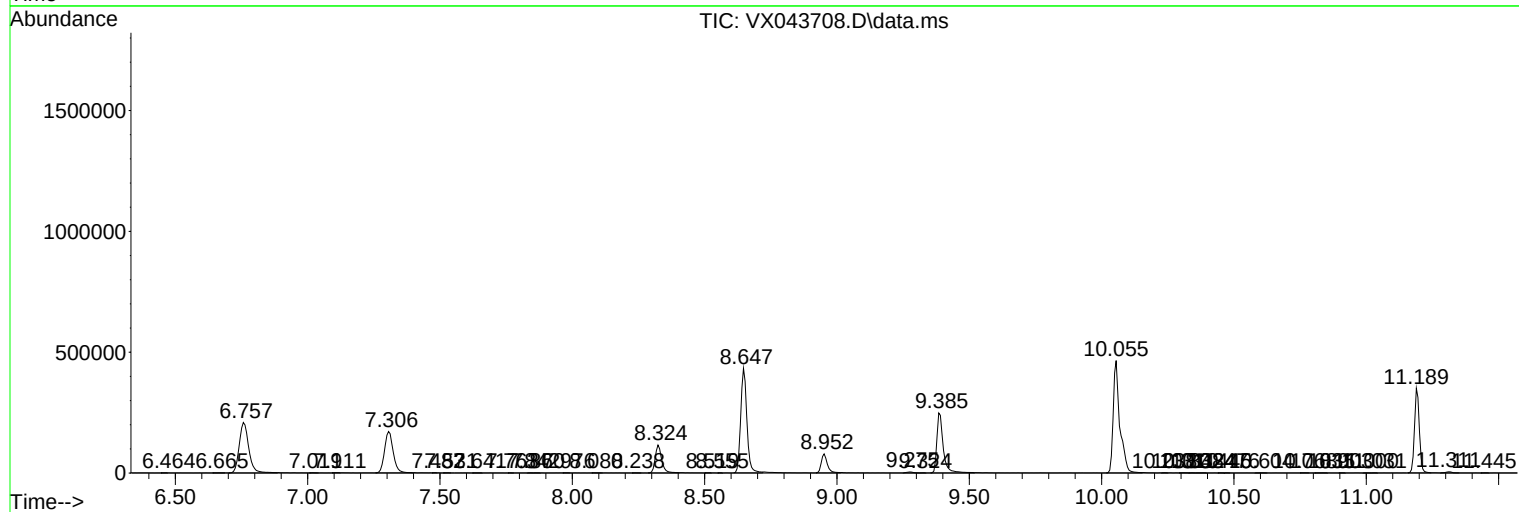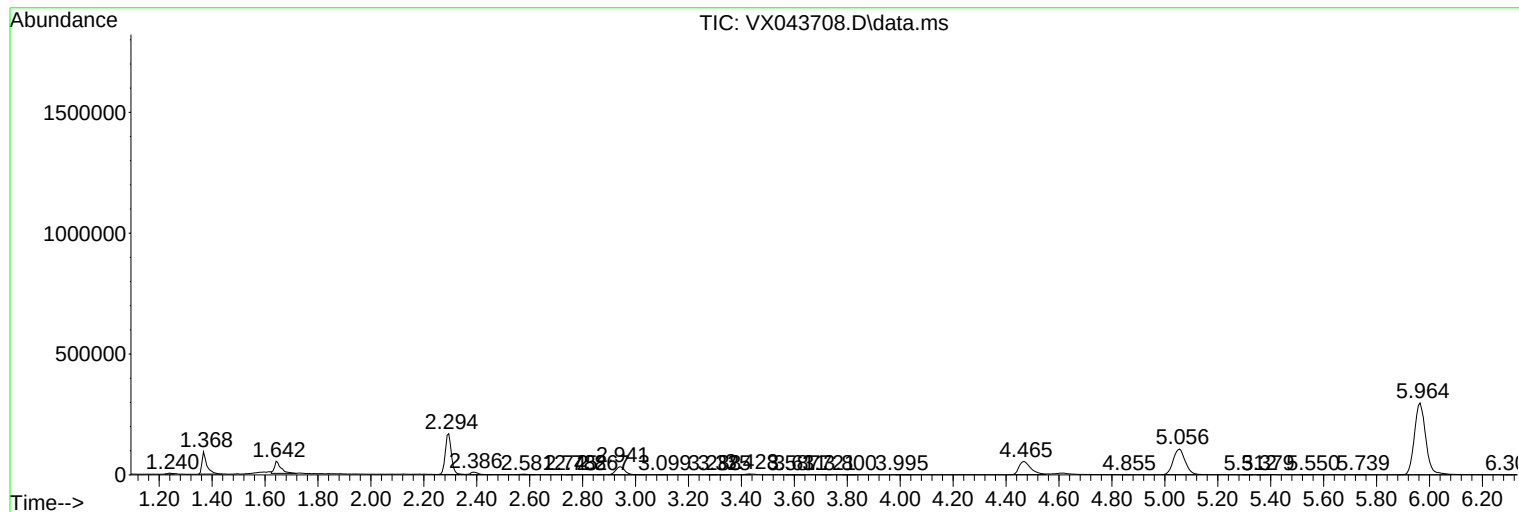

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043708.D
Acq On : 05 Nov 2024 11:59
Operator : JC/MD
Sample : P4670-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0SY1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043708.D
Acq On : 05 Nov 2024 11:59
Operator : JC/MD
Sample : P4670-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0SY1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
