

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043712.D
 Acq On : 05 Nov 2024 13:40
 Operator : JC/MD
 Sample : P4621-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6M9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M

Title : VOC Analysis

Signal : TIC: VX043712.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	31	rBV2	6772	10605	1.32%	0.168%
2	1.368	43	46	58	rBV	81552	106908	13.35%	1.698%
3	1.642	88	91	104	rVB	43259	76017	9.50%	1.208%
4	2.294	191	198	211	rVB	156670	243861	30.46%	3.874%
5	2.459	224	225	226	rBV	403	258	0.03%	0.004%
6	2.782	273	278	288	rVB4	2984	6019	0.75%	0.096%
7	2.940	297	304	310	rBV	6231	13560	1.69%	0.215%
8	3.044	319	321	323	rBV2	266	266	0.03%	0.004%
9	3.117	332	333	336	rBV2	524	519	0.06%	0.008%
10	3.172	341	342	345	rVB	480	317	0.04%	0.005%
11	3.440	377	386	393	rBV5	3015	7742	0.97%	0.123%
12	3.495	393	395	398	rVV2	328	342	0.04%	0.005%
13	3.544	401	403	406	rBV2	293	283	0.04%	0.004%
14	3.617	412	415	416	rBV2	239	236	0.03%	0.004%
15	3.690	425	427	429	rVB2	495	469	0.06%	0.007%
16	3.733	429	434	435	rBV2	633	864	0.11%	0.014%
17	4.215	511	513	514	rBV2	296	248	0.03%	0.004%
18	4.233	514	516	519	rVB3	443	497	0.06%	0.008%
19	4.269	521	522	526	rBV2	402	422	0.05%	0.007%
20	4.465	546	554	571	rBV	54432	168705	21.07%	2.680%
21	4.897	623	625	627	rBV	270	230	0.03%	0.004%
22	4.964	634	636	638	rBV2	248	252	0.03%	0.004%
23	5.050	638	650	668	rVV	101590	313629	39.18%	4.982%
24	5.306	689	692	693	rBV2	362	400	0.05%	0.006%
25	5.355	696	700	703	rBV2	335	459	0.06%	0.007%
26	5.379	703	704	706	rBV2	416	385	0.05%	0.006%
27	5.446	713	715	717	rBV	573	406	0.05%	0.006%
28	5.544	728	731	735	rBV3	462	811	0.10%	0.013%
29	5.641	745	747	751	rBV2	428	499	0.06%	0.008%
30	5.964	788	800	827	rBV2	263504	800520	100.00%	12.716%
31	6.287	849	853	855	rVB	247	287	0.04%	0.005%
32	6.342	860	862	863	rBV	373	233	0.03%	0.004%
33	6.476	881	884	888	rVB3	397	522	0.07%	0.008%
34	6.507	888	889	893	rBV2	287	361	0.05%	0.006%
35	6.757	920	930	949	rBV	226211	556360	69.50%	8.838%
36	7.068	979	981	984	rBV2	488	521	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043712.D
 Acq On : 05 Nov 2024 13:40
 Operator : JC/MD
 Sample : P4621-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6M9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	7.117	984	989	992	rBV6	946	1654	0.21%	0.026%
38	7.306	1011	1020	1032	rBV	163169	359427	44.90%	5.710%
39	7.531	1056	1057	1059	rBV2	345	303	0.04%	0.005%
40	7.848	1108	1109	1111	rBV2	336	234	0.03%	0.004%
41	7.921	1118	1121	1125	rBV3	398	761	0.10%	0.012%
42	8.074	1144	1146	1147	rVB2	447	255	0.03%	0.004%
43	8.263	1174	1177	1180	rBV2	333	496	0.06%	0.008%
44	8.324	1181	1187	1201	rBV	104945	177119	22.13%	2.814%
45	8.647	1233	1240	1257	rBV	388178	635043	79.33%	10.088%
46	8.817	1266	1268	1273	rVB	750	591	0.07%	0.009%
47	8.952	1285	1290	1305	rBV	72179	114212	14.27%	1.814%
48	9.269	1339	1342	1346	rBV5	724	1005	0.13%	0.016%
49	9.384	1356	1361	1378	rBV	237358	393677	49.18%	6.254%
50	9.647	1402	1404	1406	rBV	290	229	0.03%	0.004%
51	9.817	1429	1432	1433	rBV2	409	407	0.05%	0.006%
52	9.842	1433	1436	1441	rVV3	400	885	0.11%	0.014%
53	10.055	1465	1471	1484	rBV	470401	677702	84.66%	10.765%
54	10.195	1493	1494	1499	rVB3	465	385	0.05%	0.006%
55	10.476	1535	1540	1543	rBV2	371	588	0.07%	0.009%
56	10.646	1565	1568	1573	rBV3	512	791	0.10%	0.013%
57	10.701	1576	1577	1581	rBV	316	308	0.04%	0.005%
58	10.945	1613	1617	1619	rBV2	360	414	0.05%	0.007%
59	11.006	1625	1627	1630	rBV2	337	311	0.04%	0.005%
60	11.055	1634	1635	1640	rBV3	402	563	0.07%	0.009%
61	11.104	1640	1643	1646	rBV2	221	347	0.04%	0.006%
62	11.189	1652	1657	1665	rBV	313926	410323	51.26%	6.518%
63	11.445	1697	1699	1702	rBV3	252	350	0.04%	0.006%
64	11.567	1716	1719	1720	rBV2	330	354	0.04%	0.006%
65	11.707	1741	1742	1744	rVB2	387	242	0.03%	0.004%
66	11.945	1777	1781	1782	rVV2	341	375	0.05%	0.006%
67	12.018	1788	1793	1807	rBV	469617	619185	77.35%	9.836%
68	12.244	1828	1830	1833	rVB3	422	394	0.05%	0.006%
69	12.274	1833	1835	1837	rBV	343	334	0.04%	0.005%
70	12.317	1837	1842	1852	rBV	434766	565920	70.69%	8.990%
71	12.549	1878	1880	1883	rBV2	318	302	0.04%	0.005%
72	12.652	1895	1897	1899	rBV	375	337	0.04%	0.005%
73	12.762	1908	1915	1919	rBV4	1285	2372	0.30%	0.038%
74	12.798	1919	1921	1924	rVV2	336	362	0.05%	0.006%
75	12.859	1929	1931	1935	rVV2	499	462	0.06%	0.007%
76	12.914	1938	1940	1942	rVB	553	441	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043712.D
 Acq On : 05 Nov 2024 13:40
 Operator : JC/MD
 Sample : P4621-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6M9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	12.939	1942	1944	1947	rBV	409	573	0.07%	0.009%
78	12.981	1949	1951	1953	rBV2	365	240	0.03%	0.004%
79	13.122	1972	1974	1977	rVB2	481	355	0.04%	0.006%
80	13.207	1987	1988	1989	rBV	432	258	0.03%	0.004%
81	13.359	2010	2013	2015	rBV2	276	311	0.04%	0.005%
82	13.518	2037	2039	2041	rVB	366	294	0.04%	0.005%
83	13.536	2041	2042	2043	rBV	395	262	0.03%	0.004%
84	13.603	2050	2053	2055	rBV	536	572	0.07%	0.009%
85	13.664	2061	2063	2067	rBV	395	504	0.06%	0.008%
86	13.725	2070	2073	2074	rBV	445	364	0.05%	0.006%
87	13.743	2074	2076	2079	rVB2	397	395	0.05%	0.006%
88	13.969	2111	2113	2114	rBV	468	391	0.05%	0.006%
89	14.067	2127	2129	2131	rVB	442	279	0.03%	0.004%
90	14.134	2136	2140	2144	rVB2	1142	1829	0.23%	0.029%
91	14.396	2181	2183	2184	rBV2	285	253	0.03%	0.004%
92	14.658	2222	2226	2227	rBV2	454	726	0.09%	0.012%
93	14.737	2237	2239	2243	rBV2	357	495	0.06%	0.008%
94	14.780	2244	2246	2247	rVB	662	340	0.04%	0.005%
95	14.798	2247	2249	2251	rBV2	502	524	0.07%	0.008%
96	15.396	2346	2347	2349	rBV	598	319	0.04%	0.005%
97	15.542	2369	2371	2375	rBV3	556	748	0.09%	0.012%
98	15.597	2379	2380	2383	rVB2	612	380	0.05%	0.006%
99	15.920	2431	2433	2435	rBV2	530	560	0.07%	0.009%
100	16.023	2448	2450	2453	rBV3	664	696	0.09%	0.011%

Sum of corrected areas: 6295141




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043712.D
Acq On : 05 Nov 2024 13:40
Operator : JC/MD
Sample : P4621-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6M9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

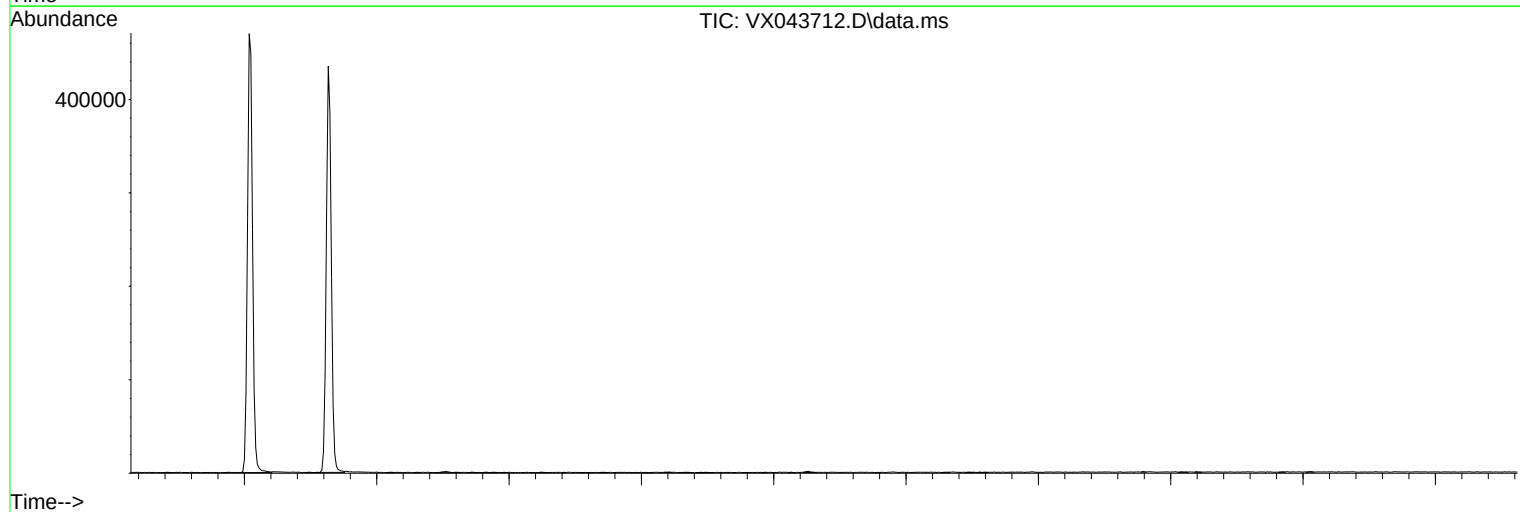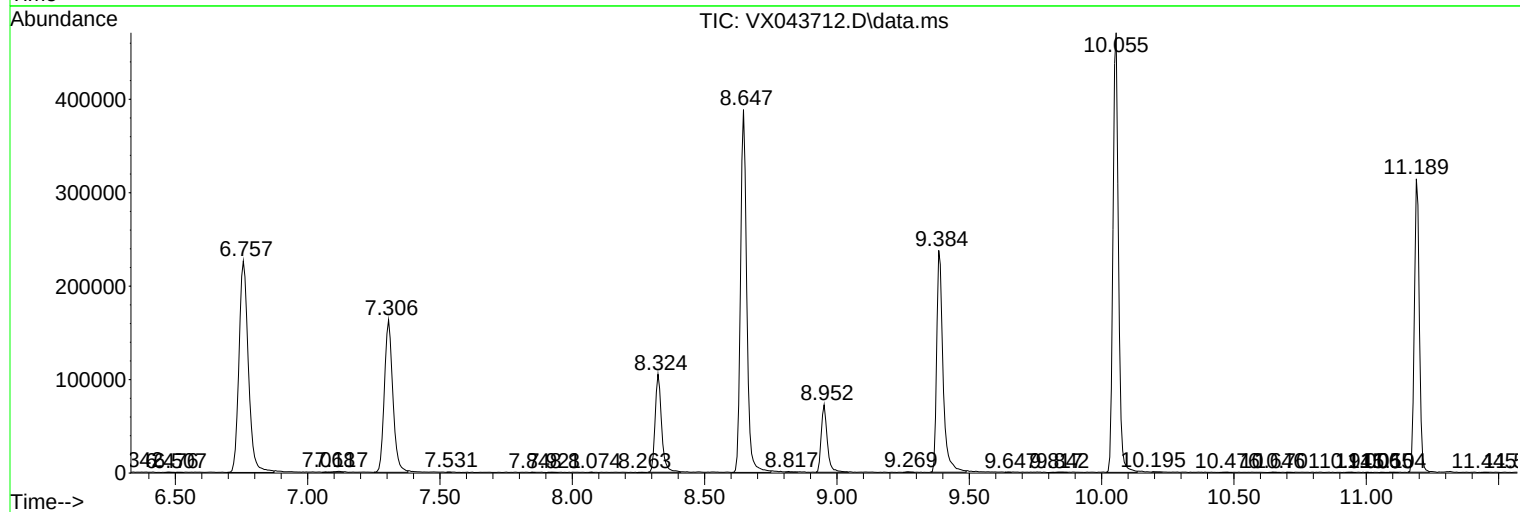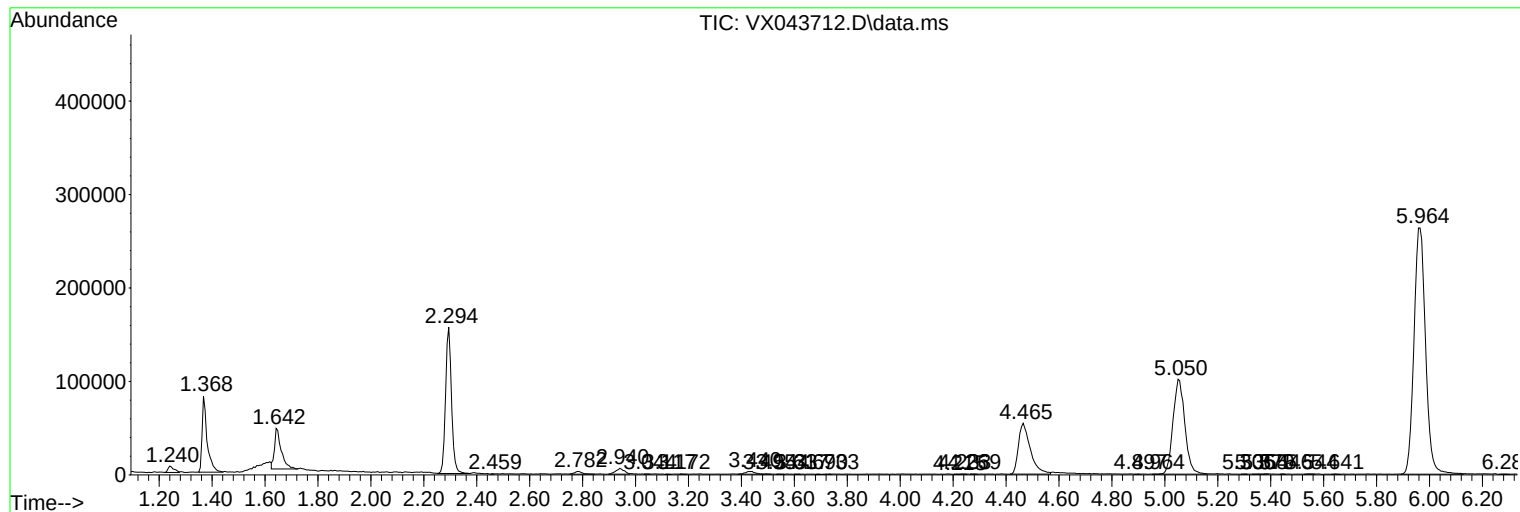

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043712.D
Acq On : 05 Nov 2024 13:40
Operator : JC/MD
Sample : P4621-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6M9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043712.D
Acq On : 05 Nov 2024 13:40
Operator : JC/MD
Sample : P4621-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6M9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
