

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043716.D
 Acq On : 05 Nov 2024 15:13
 Operator : JC/MD
 Sample : P4621-09RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6N5RE

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043716.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	22	25	27	rBV	5959	6015	1.15%	0.159%
2	1.367	43	46	58	rVB	57002	70456	13.48%	1.860%
3	1.648	89	92	103	rVB	37224	56622	10.83%	1.495%
4	2.294	192	198	210	rVB	99268	156030	29.84%	4.120%
5	2.782	274	278	284	rBV4	1852	3426	0.66%	0.090%
6	2.861	289	291	294	rVB	428	357	0.07%	0.009%
7	2.946	297	305	313	rBV	4440	10452	2.00%	0.276%
8	3.160	336	340	341	rBV2	300	365	0.07%	0.010%
9	3.434	379	385	387	rBV4	2021	3622	0.69%	0.096%
10	3.532	398	401	402	rBV2	345	295	0.06%	0.008%
11	3.721	429	432	434	rVB2	352	347	0.07%	0.009%
12	3.751	434	437	440	rBV2	324	525	0.10%	0.014%
13	4.044	484	485	488	rBV2	292	291	0.06%	0.008%
14	4.172	504	506	508	rBV	469	343	0.07%	0.009%
15	4.190	508	509	512	rVB2	407	388	0.07%	0.010%
16	4.282	522	524	527	rBV3	329	475	0.09%	0.013%
17	4.404	542	544	546	rBV	324	267	0.05%	0.007%
18	4.471	547	555	569	rBV	33548	102011	19.51%	2.694%
19	4.861	618	619	621	rBV	307	282	0.05%	0.007%
20	4.922	627	629	631	rBV2	282	350	0.07%	0.009%
21	5.056	638	651	667	rBV3	65945	207824	39.75%	5.488%
22	5.239	678	681	682	rVB2	325	338	0.06%	0.009%
23	5.556	730	733	736	rVB3	671	887	0.17%	0.023%
24	5.586	736	738	742	rBV3	506	713	0.14%	0.019%
25	5.629	742	745	746	rBV	407	447	0.09%	0.012%
26	5.964	789	800	819	rBV2	177539	522839	100.00%	13.806%
27	6.324	856	859	861	rBV2	219	278	0.05%	0.007%
28	6.574	898	900	902	rVV	478	319	0.06%	0.008%
29	6.757	921	930	945	rBV	115616	294312	56.29%	7.771%
30	6.952	960	962	965	rVB3	411	360	0.07%	0.010%
31	7.055	977	979	982	rBV2	326	291	0.06%	0.008%
32	7.116	982	989	998	rBV5	4344	10859	2.08%	0.287%
33	7.208	1002	1004	1007	rBV3	280	289	0.06%	0.008%
34	7.305	1012	1020	1032	rBV	103982	234395	44.83%	6.189%
35	7.458	1043	1045	1047	rBV	682	535	0.10%	0.014%
36	7.482	1047	1049	1053	rVV3	492	673	0.13%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043716.D
 Acq On : 05 Nov 2024 15:13
 Operator : JC/MD
 Sample : P4621-09RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6N5RE

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	7.586	1064	1066	1067	rBV	512	350	0.07%	0.009%
38	7.629	1072	1073	1075	rVB2	441	304	0.06%	0.008%
39	7.671	1077	1080	1083	rBV3	298	444	0.08%	0.012%
40	7.696	1083	1084	1087	rVV2	298	324	0.06%	0.009%
41	7.915	1118	1120	1122	rBV2	302	335	0.06%	0.009%
42	8.147	1154	1158	1159	rBV	329	334	0.06%	0.009%
43	8.324	1181	1187	1200	rBV	61938	111237	21.28%	2.937%
44	8.452	1206	1208	1209	rVB	513	282	0.05%	0.007%
45	8.561	1225	1226	1228	rBV	367	300	0.06%	0.008%
46	8.647	1234	1240	1256	rBV	253935	413697	79.13%	10.924%
47	8.951	1285	1290	1299	rBV	42882	66723	12.76%	1.762%
48	9.061	1306	1308	1309	rBV	411	365	0.07%	0.010%
49	9.177	1325	1327	1330	rVB2	550	466	0.09%	0.012%
50	9.201	1330	1331	1334	rVB2	355	360	0.07%	0.010%
51	9.262	1337	1341	1343	rBV3	389	457	0.09%	0.012%
52	9.342	1352	1354	1356	rBV2	399	378	0.07%	0.010%
53	9.390	1357	1362	1378	rBV	144025	232342	44.44%	6.135%
54	9.616	1398	1399	1402	rBV3	316	311	0.06%	0.008%
55	9.738	1417	1419	1424	rVB3	255	323	0.06%	0.009%
56	9.775	1424	1425	1430	rVB2	318	432	0.08%	0.011%
57	10.055	1465	1471	1489	rVV	252394	355187	67.93%	9.379%
58	10.317	1512	1514	1519	rVB3	408	371	0.07%	0.010%
59	10.409	1527	1529	1532	rVB2	290	268	0.05%	0.007%
60	10.610	1560	1562	1564	rBV	357	286	0.05%	0.008%
61	10.726	1577	1581	1584	rBV2	338	582	0.11%	0.015%
62	10.799	1590	1593	1594	rVB	515	470	0.09%	0.012%
63	10.939	1613	1616	1617	rBV2	321	267	0.05%	0.007%
64	11.006	1625	1627	1630	rVB	384	330	0.06%	0.009%
65	11.189	1652	1657	1665	rBV	184466	241401	46.17%	6.374%
66	11.299	1673	1675	1677	rVB2	468	316	0.06%	0.008%
67	11.329	1677	1680	1683	rBV	456	452	0.09%	0.012%
68	11.414	1691	1694	1697	rBV3	297	320	0.06%	0.008%
69	11.585	1721	1722	1725	rBV	337	267	0.05%	0.007%
70	12.024	1789	1794	1806	rBV	236713	307692	58.85%	8.125%
71	12.317	1837	1842	1858	rBV	266442	347573	66.48%	9.178%
72	12.524	1875	1876	1880	rVB2	497	387	0.07%	0.010%
73	12.561	1880	1882	1884	rVB	370	289	0.06%	0.008%
74	12.615	1890	1891	1894	rBV2	387	448	0.09%	0.012%
75	12.768	1912	1916	1919	rVB3	578	895	0.17%	0.024%
76	12.841	1927	1928	1931	rVB2	389	295	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043716.D
 Acq On : 05 Nov 2024 15:13
 Operator : JC/MD
 Sample : P4621-09RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6N5RE

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	13.006	1950	1955	1956	rBV2	222	334	0.06%	0.009%
78	13.225	1987	1991	1992	rBV2	279	353	0.07%	0.009%
79	13.262	1995	1997	2001	rVB2	390	411	0.08%	0.011%
80	13.298	2001	2003	2006	rBV2	292	296	0.06%	0.008%
81	13.463	2028	2030	2033	rBV2	245	323	0.06%	0.009%
82	13.597	2048	2052	2054	rVB2	517	435	0.08%	0.011%
83	13.646	2056	2060	2061	rBV2	278	298	0.06%	0.008%
84	13.664	2061	2063	2064	rBV	474	282	0.05%	0.007%
85	13.743	2073	2076	2078	rBV	522	447	0.09%	0.012%
86	13.768	2078	2080	2082	rVB2	486	339	0.06%	0.009%
87	14.127	2136	2139	2141	rBV2	734	961	0.18%	0.025%
88	14.231	2153	2156	2158	rVB2	314	328	0.06%	0.009%
89	14.329	2171	2172	2175	rVB2	440	386	0.07%	0.010%
90	14.451	2190	2192	2194	rVB2	603	528	0.10%	0.014%
91	14.743	2237	2240	2243	rVB2	484	503	0.10%	0.013%
92	14.816	2250	2252	2254	rBV	496	355	0.07%	0.009%
93	14.908	2266	2267	2269	rBV2	418	307	0.06%	0.008%
94	15.243	2318	2322	2323	rBV2	473	643	0.12%	0.017%
95	15.584	2376	2378	2379	rBV2	683	614	0.12%	0.016%
96	15.749	2401	2405	2407	rBV3	653	703	0.13%	0.019%
97	15.828	2416	2418	2421	rBV3	622	658	0.13%	0.017%
98	15.859	2421	2423	2426	rVV3	567	465	0.09%	0.012%
99	16.218	2480	2482	2484	rBV2	360	435	0.08%	0.011%
100	16.603	2543	2545	2548	rBV2	592	563	0.11%	0.015%

Sum of corrected areas: 3787105




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043716.D
Acq On : 05 Nov 2024 15:13
Operator : JC/MD
Sample : P4621-09RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6N5RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

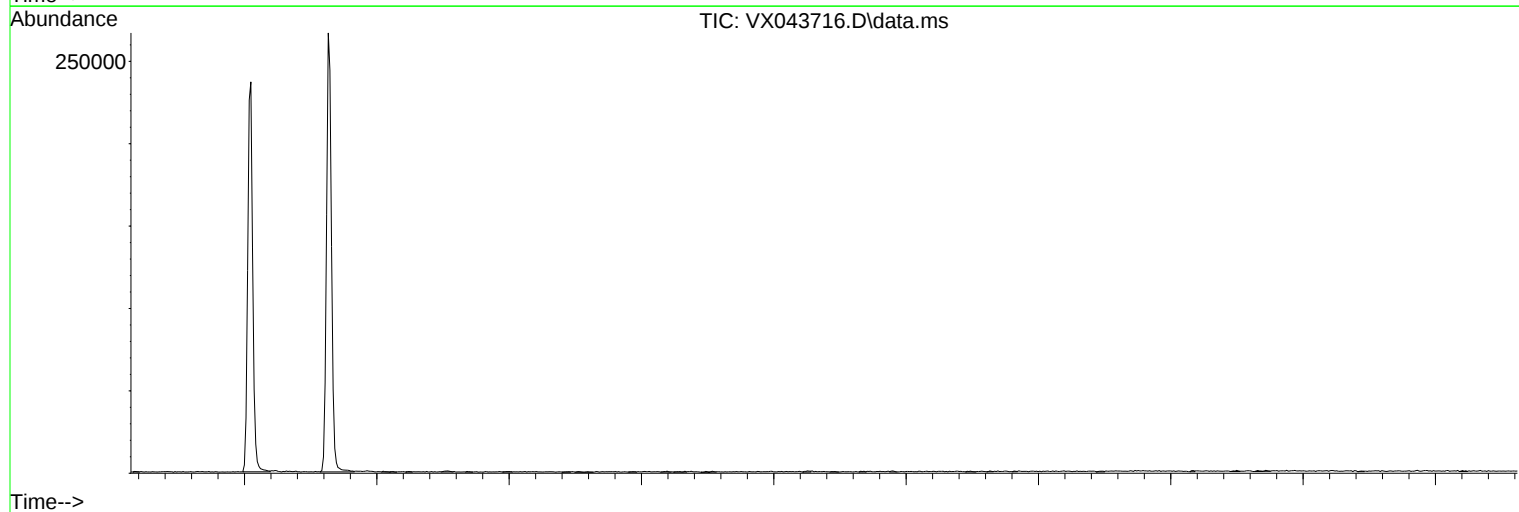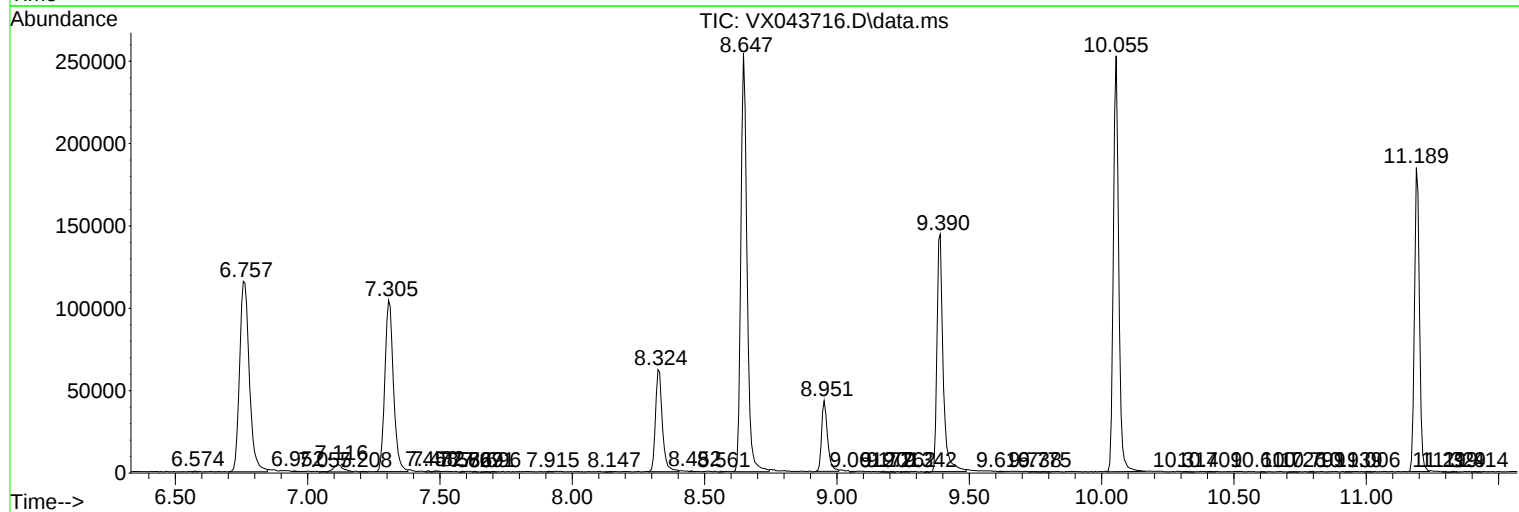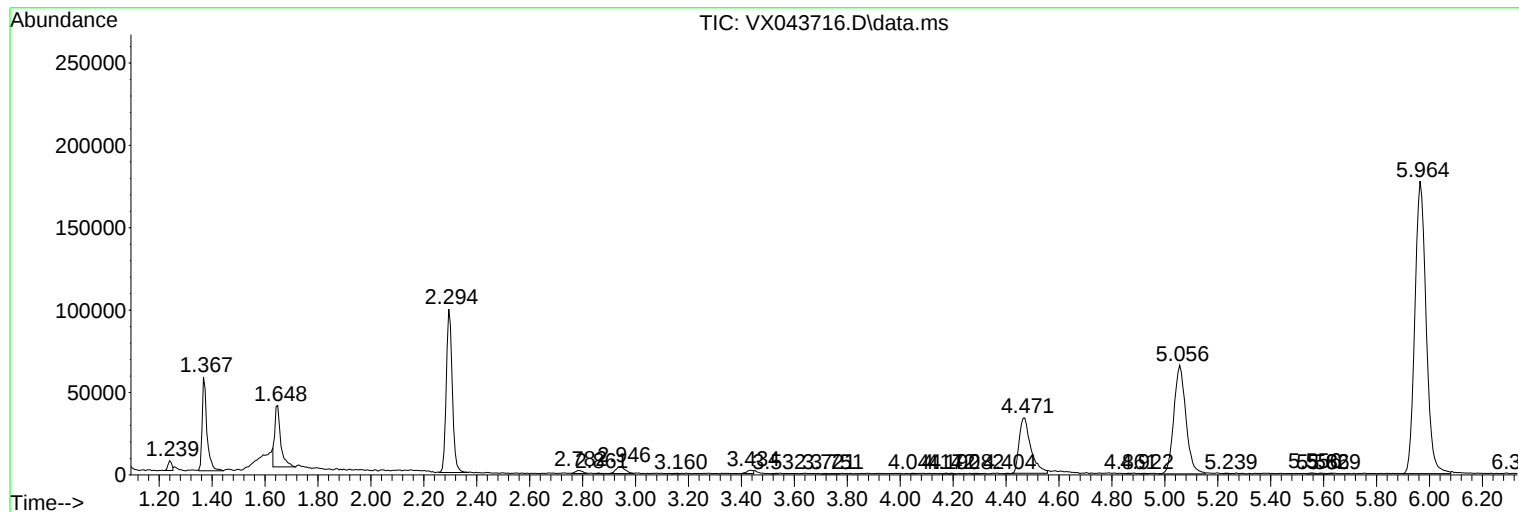

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043716.D
Acq On : 05 Nov 2024 15:13
Operator : JC/MD
Sample : P4621-09RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6N5RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043716.D
Acq On : 05 Nov 2024 15:13
Operator : JC/MD
Sample : P4621-09RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6N5RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
