

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043717.D
 Acq On : 05 Nov 2024 15:36
 Operator : JC/MD
 Sample : P4621-10RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6N6RE

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043717.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	22	25	32	rBV2	6831	9400	1.32%	0.183%
2	1.368	43	46	59	rBV	78066	90056	12.69%	1.752%
3	1.648	89	92	103	rVB	48092	70108	9.88%	1.364%
4	2.294	192	198	210	rBV	132787	208231	29.33%	4.052%
5	2.477	224	228	230	rBV2	378	544	0.08%	0.011%
6	2.501	230	232	234	rVV	321	279	0.04%	0.005%
7	2.575	241	244	245	rBV	468	390	0.05%	0.008%
8	2.660	255	258	259	rBV2	704	698	0.10%	0.014%
9	2.788	273	279	283	rBV3	2415	4064	0.57%	0.079%
10	2.940	297	304	313	rVV	5571	13380	1.88%	0.260%
11	3.062	321	324	330	rVB2	359	763	0.11%	0.015%
12	3.105	330	331	333	rBV	356	267	0.04%	0.005%
13	3.251	354	355	357	rVB2	419	273	0.04%	0.005%
14	3.282	357	360	362	rVB2	369	378	0.05%	0.007%
15	3.300	362	363	364	rBV	404	260	0.04%	0.005%
16	3.434	380	385	393	rVV2	2381	5650	0.80%	0.110%
17	3.507	395	397	401	rBV3	621	873	0.12%	0.017%
18	3.727	431	433	434	rVB	534	268	0.04%	0.005%
19	3.800	439	445	446	rBV	471	623	0.09%	0.012%
20	3.830	448	450	453	rVB2	367	342	0.05%	0.007%
21	4.007	477	479	482	rVV	497	414	0.06%	0.008%
22	4.093	489	493	496	rVV2	197	308	0.04%	0.006%
23	4.160	503	504	507	rVB	524	347	0.05%	0.007%
24	4.196	507	510	511	rBV2	323	302	0.04%	0.006%
25	4.239	516	517	521	rBV2	288	278	0.04%	0.005%
26	4.465	546	554	567	rBV	47788	147401	20.76%	2.868%
27	4.824	611	613	614	rBV	537	436	0.06%	0.008%
28	4.842	614	616	620	rVB2	289	282	0.04%	0.005%
29	4.922	628	629	632	rBV2	235	258	0.04%	0.005%
30	5.056	639	651	669	rBV2	87242	281095	39.60%	5.470%
31	5.312	691	693	697	rVB3	383	476	0.07%	0.009%
32	5.513	723	726	729	rBV3	377	668	0.09%	0.013%
33	5.544	729	731	734	rBV2	314	410	0.06%	0.008%
34	5.574	734	736	738	rBV2	373	286	0.04%	0.006%
35	5.702	755	757	759	rBV	282	264	0.04%	0.005%
36	5.739	759	763	767	rBV3	332	451	0.06%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043717.D
 Acq On : 05 Nov 2024 15:36
 Operator : JC/MD
 Sample : P4621-10RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6N6RE

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	5.836	776	779	782	rBV3	404	644	0.09%	0.013%
38	5.964	790	800	822	rBV2	238300	709913	100.00%	13.814%
39	6.202	835	839	842	rBV2	468	788	0.11%	0.015%
40	6.440	876	878	880	rVB	383	280	0.04%	0.005%
41	6.623	905	908	912	rBV	430	544	0.08%	0.011%
42	6.757	921	930	948	rBV	149313	373866	52.66%	7.275%
43	6.903	953	954	959	rVB3	1202	1033	0.15%	0.020%
44	7.110	983	988	998	rBV5	5204	13476	1.90%	0.262%
45	7.208	1002	1004	1005	rBV	685	423	0.06%	0.008%
46	7.305	1012	1020	1033	rBV	145135	324100	45.65%	6.307%
47	7.494	1046	1051	1053	rBV2	807	1640	0.23%	0.032%
48	7.616	1069	1071	1074	rVV2	372	266	0.04%	0.005%
49	7.708	1083	1086	1087	rBV	434	282	0.04%	0.005%
50	7.836	1104	1107	1109	rVB2	812	882	0.12%	0.017%
51	7.903	1117	1118	1121	rVB2	377	266	0.04%	0.005%
52	8.147	1154	1158	1161	rBV2	311	436	0.06%	0.008%
53	8.324	1181	1187	1200	rBV	90613	152013	21.41%	2.958%
54	8.647	1234	1240	1256	rBV	356982	565104	79.60%	10.996%
55	8.952	1285	1290	1305	rBV	62324	96897	13.65%	1.886%
56	9.177	1326	1327	1329	rVV	521	295	0.04%	0.006%
57	9.269	1340	1342	1345	rBV2	321	404	0.06%	0.008%
58	9.323	1349	1351	1356	rVB	468	357	0.05%	0.007%
59	9.384	1356	1361	1380	rBV	213790	338831	47.73%	6.593%
60	9.653	1403	1405	1406	rBV	387	284	0.04%	0.006%
61	9.835	1433	1435	1437	rVV2	315	268	0.04%	0.005%
62	9.872	1440	1441	1444	rBV	294	316	0.04%	0.006%
63	9.903	1444	1446	1448	rVV2	341	292	0.04%	0.006%
64	9.976	1456	1458	1460	rBV2	325	315	0.04%	0.006%
65	10.055	1464	1471	1486	rBV	326563	462415	65.14%	8.998%
66	10.415	1529	1530	1533	rVB	403	288	0.04%	0.006%
67	10.634	1565	1566	1570	rVV	422	346	0.05%	0.007%
68	10.719	1579	1580	1584	rBV	468	529	0.07%	0.010%
69	10.896	1608	1609	1613	rBV3	386	367	0.05%	0.007%
70	11.085	1638	1640	1644	rBV2	245	262	0.04%	0.005%
71	11.122	1644	1646	1649	rBV2	326	354	0.05%	0.007%
72	11.189	1651	1657	1668	rBV	268765	345417	48.66%	6.721%
73	11.299	1673	1675	1679	rVB3	401	521	0.07%	0.010%
74	11.847	1761	1765	1766	rBV	458	593	0.08%	0.012%
75	11.933	1777	1779	1782	rVB2	500	312	0.04%	0.006%
76	12.018	1788	1793	1805	rBV	299641	402870	56.75%	7.839%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043717.D
 Acq On : 05 Nov 2024 15:36
 Operator : JC/MD
 Sample : P4621-10RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH6N6RE

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	12.250	1829	1831	1832	rVB2	432	261	0.04%	0.005%
78	12.317	1837	1842	1853	rBV	368919	488041	68.75%	9.497%
79	12.530	1876	1877	1879	rBV2	450	297	0.04%	0.006%
80	12.762	1912	1915	1918	rVV	1031	1295	0.18%	0.025%
81	12.823	1921	1925	1927	rVV2	452	422	0.06%	0.008%
82	12.914	1936	1940	1943	rVB2	361	565	0.08%	0.011%
83	13.012	1954	1956	1957	rBV	319	272	0.04%	0.005%
84	13.054	1960	1963	1964	rBV	398	286	0.04%	0.006%
85	13.103	1967	1971	1972	rBV2	361	424	0.06%	0.008%
86	13.792	2082	2084	2086	rBV2	382	386	0.05%	0.008%
87	13.890	2099	2100	2103	rBV2	367	343	0.05%	0.007%
88	13.914	2103	2104	2107	rVB	423	341	0.05%	0.007%
89	13.945	2107	2109	2111	rBV2	410	339	0.05%	0.007%
90	14.073	2127	2130	2133	rBV3	408	476	0.07%	0.009%
91	14.134	2135	2140	2142	rBV4	781	1211	0.17%	0.024%
92	14.511	2198	2202	2203	rBV2	402	520	0.07%	0.010%
93	14.944	2271	2273	2275	rBV2	338	290	0.04%	0.006%
94	15.170	2309	2310	2313	rBV3	520	584	0.08%	0.011%
95	15.359	2340	2341	2342	rBV	705	262	0.04%	0.005%
96	15.383	2342	2345	2349	rBV4	948	1690	0.24%	0.033%
97	15.432	2352	2353	2355	rBV	689	324	0.05%	0.006%
98	15.572	2374	2376	2379	rBV3	518	486	0.07%	0.009%
99	15.658	2388	2390	2392	rBV	742	531	0.07%	0.010%
100	16.700	2559	2561	2562	rVB2	664	361	0.05%	0.007%

Sum of corrected areas: 5139019




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043717.D
Acq On : 05 Nov 2024 15:36
Operator : JC/MD
Sample : P4621-10RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6N6RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

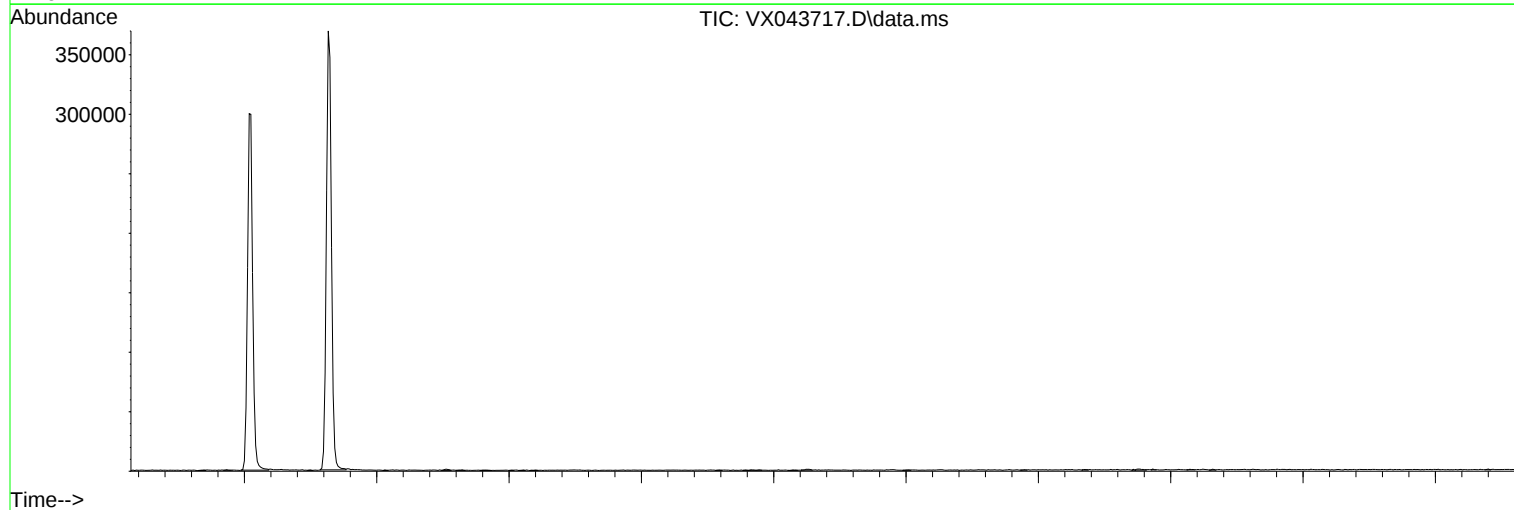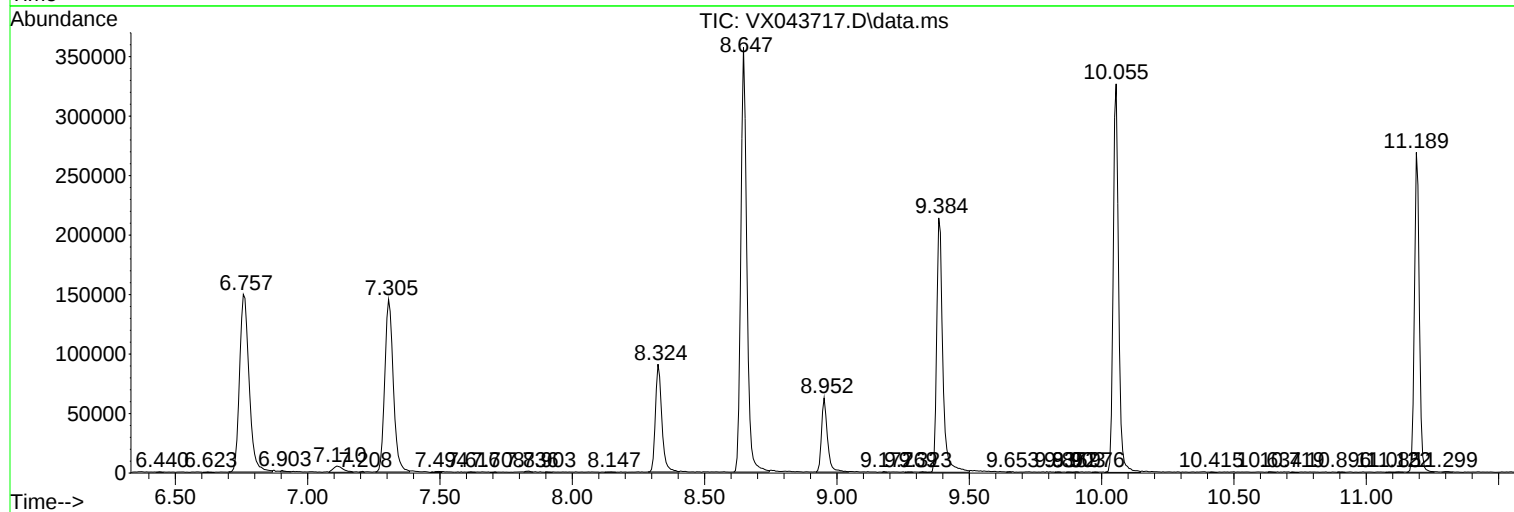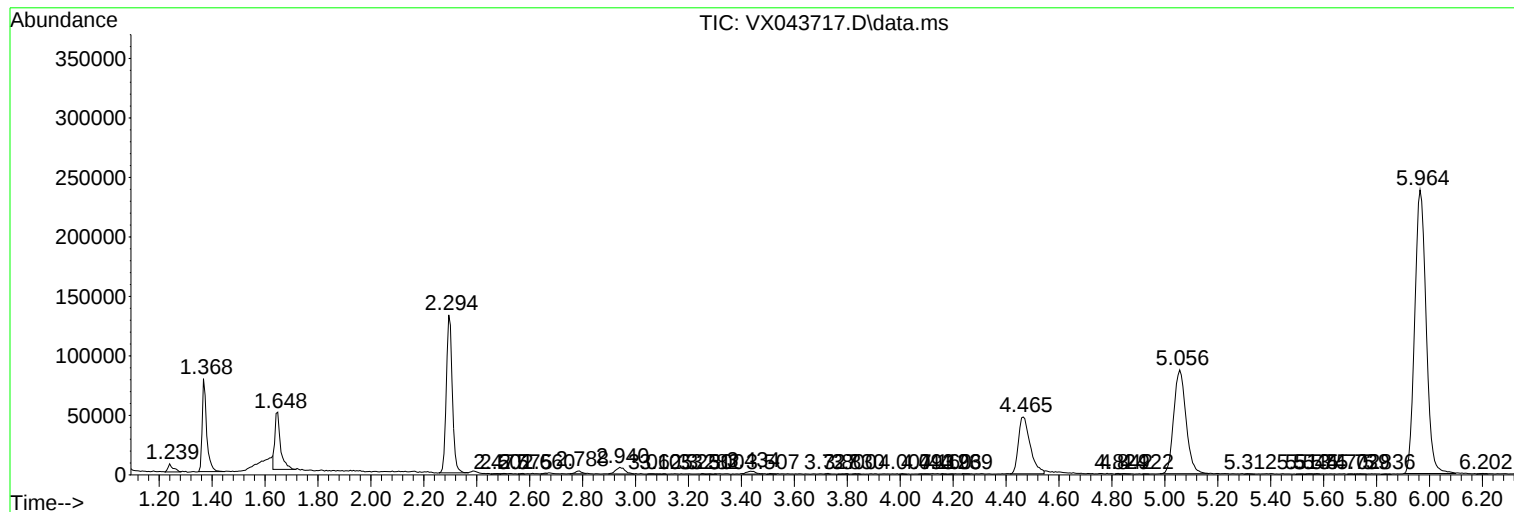

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043717.D
Acq On : 05 Nov 2024 15:36
Operator : JC/MD
Sample : P4621-10RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6N6RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043717.D
Acq On : 05 Nov 2024 15:36
Operator : JC/MD
Sample : P4621-10RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH6N6RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
