

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043719.D
 Acq On : 05 Nov 2024 16:22
 Operator : JC/MD
 Sample : P4621-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH8M6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043719.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	33	rBV3	6817	10568	1.57%	0.209%
2	1.368	43	46	58	rVB	65093	77569	11.53%	1.531%
3	1.648	89	92	103	rVB	42520	61436	9.13%	1.213%
4	2.294	192	198	211	rVV	112427	177929	26.46%	3.512%
5	2.410	215	217	218	rBV2	557	390	0.06%	0.008%
6	2.538	237	238	240	rVB	561	279	0.04%	0.006%
7	2.581	243	245	249	rVB3	867	994	0.15%	0.020%
8	2.617	249	251	254	rBV2	489	626	0.09%	0.012%
9	2.672	256	260	264	rVV2	1392	2130	0.32%	0.042%
10	2.788	273	279	286	rVB2	3060	5661	0.84%	0.112%
11	2.947	296	305	311	rBV2	5026	11466	1.70%	0.226%
12	3.032	317	319	322	rBV2	278	345	0.05%	0.007%
13	3.056	322	323	326	rVV	375	282	0.04%	0.006%
14	3.233	350	352	355	rVB2	417	370	0.06%	0.007%
15	3.434	379	385	386	rBV3	2202	3047	0.45%	0.060%
16	3.507	395	397	399	rVB2	417	311	0.05%	0.006%
17	3.721	430	432	435	rBV2	365	467	0.07%	0.009%
18	4.160	499	504	505	rBV3	358	608	0.09%	0.012%
19	4.202	509	511	512	rVV	312	274	0.04%	0.005%
20	4.355	535	536	540	rVB2	302	275	0.04%	0.005%
21	4.465	546	554	573	rBV	47841	149909	22.29%	2.959%
22	4.879	620	622	625	rBV3	457	557	0.08%	0.011%
23	4.922	628	629	632	rBV	354	270	0.04%	0.005%
24	4.965	634	636	638	rBV	283	297	0.04%	0.006%
25	5.050	639	650	668	rBV	83064	272015	40.44%	5.369%
26	5.367	700	702	705	rBV2	339	520	0.08%	0.010%
27	5.550	729	732	733	rBV3	455	433	0.06%	0.009%
28	5.964	788	800	824	rBV2	223771	672556	100.00%	13.274%
29	6.245	844	846	847	rBV	421	334	0.05%	0.007%
30	6.312	855	857	862	rVB3	391	612	0.09%	0.012%
31	6.757	922	930	948	rBV	174596	441738	65.68%	8.719%
32	7.104	982	987	999	rVB3	5501	13762	2.05%	0.272%
33	7.306	1012	1020	1033	rBV	137801	309916	46.08%	6.117%
34	7.556	1059	1061	1063	rVB2	487	397	0.06%	0.008%
35	7.580	1063	1065	1068	rVB2	303	299	0.04%	0.006%
36	7.610	1068	1070	1073	rBV2	278	284	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043719.D
 Acq On : 05 Nov 2024 16:22
 Operator : JC/MD
 Sample : P4621-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH8M6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	7.635	1073	1074	1077	rVB2	315	288	0.04%	0.006%
38	7.684	1079	1082	1085	rBV2	439	444	0.07%	0.009%
39	7.757	1092	1094	1097	rVB	355	326	0.05%	0.006%
40	7.793	1097	1100	1101	rBV2	351	331	0.05%	0.007%
41	7.830	1101	1106	1112	rVB6	1175	2414	0.36%	0.048%
42	8.092	1147	1149	1152	rVB	333	297	0.04%	0.006%
43	8.135	1152	1156	1158	rVB2	334	457	0.07%	0.009%
44	8.177	1161	1163	1166	rBV2	246	289	0.04%	0.006%
45	8.324	1181	1187	1198	rVV	81828	144163	21.44%	2.845%
46	8.446	1205	1207	1209	rBV2	373	318	0.05%	0.006%
47	8.537	1217	1222	1223	rBV	569	660	0.10%	0.013%
48	8.555	1223	1225	1228	rBV2	391	383	0.06%	0.008%
49	8.647	1234	1240	1255	rBV	310823	504167	74.96%	9.951%
50	8.952	1285	1290	1302	rBV	58886	93188	13.86%	1.839%
51	9.080	1308	1311	1315	rVB	490	451	0.07%	0.009%
52	9.147	1318	1322	1324	rBV3	252	353	0.05%	0.007%
53	9.384	1356	1361	1373	rBV	198118	309722	46.05%	6.113%
54	9.750	1419	1421	1422	rVB	484	252	0.04%	0.005%
55	9.769	1422	1424	1425	rBV	323	254	0.04%	0.005%
56	9.854	1436	1438	1443	rVB3	432	654	0.10%	0.013%
57	9.897	1443	1445	1446	rBV2	287	269	0.04%	0.005%
58	10.055	1465	1471	1487	rBV	378520	540153	80.31%	10.661%
59	10.890	1605	1608	1610	rBV	542	387	0.06%	0.008%
60	11.189	1652	1657	1666	rBV	252781	334972	49.81%	6.611%
61	11.323	1677	1679	1681	rBV2	395	354	0.05%	0.007%
62	11.488	1704	1706	1709	rBV	336	345	0.05%	0.007%
63	11.597	1722	1724	1726	rBV2	370	286	0.04%	0.006%
64	11.683	1735	1738	1741	rBV2	465	684	0.10%	0.014%
65	11.762	1749	1751	1753	rBV3	260	290	0.04%	0.006%
66	11.829	1759	1762	1765	rVB2	454	489	0.07%	0.010%
67	12.018	1788	1793	1804	rBV	350524	457049	67.96%	9.021%
68	12.195	1820	1822	1823	rVB2	526	296	0.04%	0.006%
69	12.219	1824	1826	1827	rBV2	344	253	0.04%	0.005%
70	12.317	1837	1842	1854	rBV	334966	437786	65.09%	8.641%
71	12.433	1860	1861	1862	rBV	550	282	0.04%	0.006%
72	12.738	1906	1911	1912	rBV2	489	753	0.11%	0.015%
73	12.762	1912	1915	1920	rVB2	920	1151	0.17%	0.023%
74	13.006	1953	1955	1959	rVB2	282	295	0.04%	0.006%
75	13.048	1959	1962	1964	rBV2	317	435	0.06%	0.009%
76	13.122	1973	1974	1976	rBV	565	391	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043719.D
 Acq On : 05 Nov 2024 16:22
 Operator : JC/MD
 Sample : P4621-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH8M6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	13.189	1983	1985	1989	rBV	332	426	0.06%	0.008%
78	13.341	2008	2010	2011	rBV	537	310	0.05%	0.006%
79	13.414	2020	2022	2023	rBV2	367	318	0.05%	0.006%
80	13.689	2065	2067	2070	rBV2	356	407	0.06%	0.008%
81	13.762	2077	2079	2082	rVB3	305	325	0.05%	0.006%
82	13.847	2089	2093	2095	rBV	452	543	0.08%	0.011%
83	14.030	2120	2123	2126	rBV2	209	394	0.06%	0.008%
84	14.134	2136	2140	2143	rVB3	1090	1460	0.22%	0.029%
85	14.280	2162	2164	2167	rVB2	281	259	0.04%	0.005%
86	14.359	2174	2177	2179	rBV2	475	575	0.09%	0.011%
87	14.457	2189	2193	2195	rBV4	774	1157	0.17%	0.023%
88	14.487	2195	2198	2201	rBV2	312	439	0.07%	0.009%
89	14.512	2201	2202	2205	rVB2	379	266	0.04%	0.005%
90	14.627	2220	2221	2223	rBV	621	462	0.07%	0.009%
91	14.774	2242	2245	2246	rVB3	391	336	0.05%	0.007%
92	14.829	2252	2254	2255	rBV2	563	397	0.06%	0.008%
93	14.993	2279	2281	2284	rVB2	619	725	0.11%	0.014%
94	15.060	2291	2292	2295	rBV2	342	374	0.06%	0.007%
95	15.847	2419	2421	2422	rBV	610	317	0.05%	0.006%
96	15.883	2426	2427	2430	rVB2	669	422	0.06%	0.008%
97	15.993	2444	2445	2448	rVB3	498	313	0.05%	0.006%
98	16.024	2448	2450	2451	rBV2	482	356	0.05%	0.007%
99	16.389	2508	2510	2512	rBV	407	374	0.06%	0.007%
100	16.584	2540	2542	2543	rBV2	646	448	0.07%	0.009%

Sum of corrected areas: 5066660




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043719.D
Acq On : 05 Nov 2024 16:22
Operator : JC/MD
Sample : P4621-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH8M6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

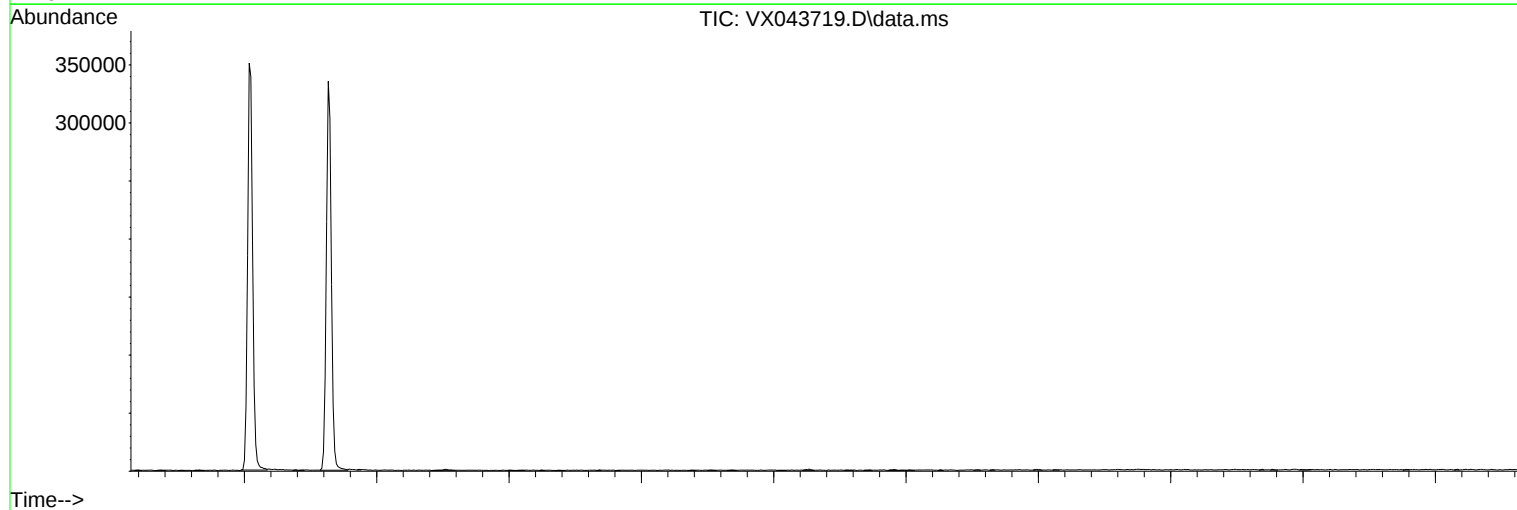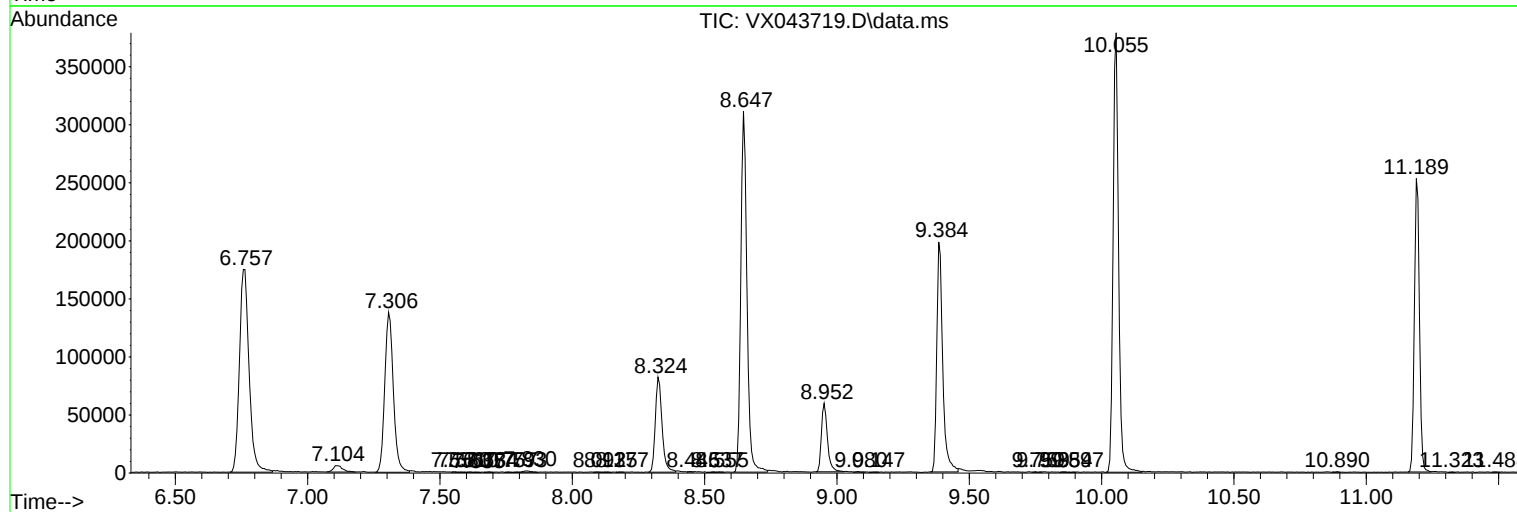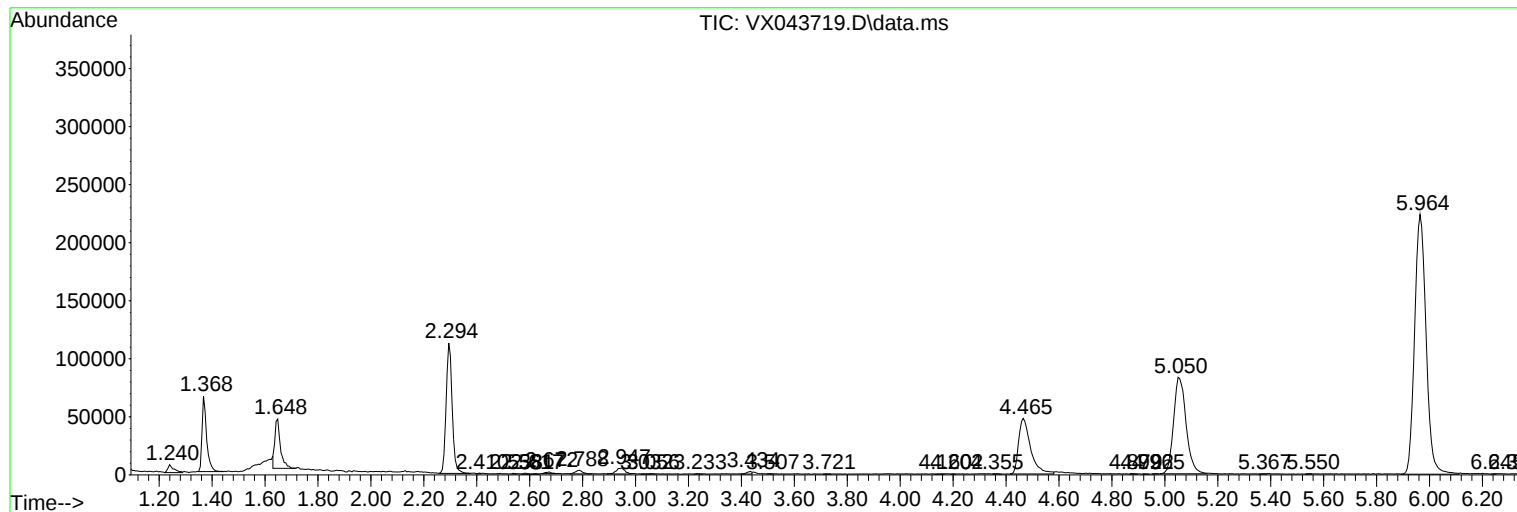

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043719.D
Acq On : 05 Nov 2024 16:22
Operator : JC/MD
Sample : P4621-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH8M6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043719.D
Acq On : 05 Nov 2024 16:22
Operator : JC/MD
Sample : P4621-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH8M6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
