

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043721.D
 Acq On : 05 Nov 2024 17:09
 Operator : JC/MD
 Sample : P4670-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COSY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043721.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	32	rBV2	6519	9074	1.68%	0.219%
2	1.368	43	46	57	rVB	60981	67704	12.56%	1.632%
3	1.648	89	92	103	rVB	41688	62565	11.61%	1.508%
4	2.294	192	198	211	rBV	97904	154526	28.67%	3.724%
5	2.386	211	213	220	rVV3	1475	2256	0.42%	0.054%
6	2.453	223	224	227	rBV2	450	380	0.07%	0.009%
7	2.569	238	243	248	rBV	3847	6647	1.23%	0.160%
8	2.788	276	279	281	rVV2	828	758	0.14%	0.018%
9	2.947	298	305	310	rBV3	6734	15533	2.88%	0.374%
10	3.130	332	335	337	rVB2	501	670	0.12%	0.016%
11	3.148	337	338	340	rBV2	319	295	0.05%	0.007%
12	3.373	373	375	377	rVV	478	321	0.06%	0.008%
13	3.440	378	386	394	rVB4	2421	6518	1.21%	0.157%
14	3.715	428	431	433	rVB	371	335	0.06%	0.008%
15	3.812	444	447	450	rBV2	363	486	0.09%	0.012%
16	3.855	452	454	455	rVV	364	297	0.06%	0.007%
17	3.873	455	457	460	rVV	525	571	0.11%	0.014%
18	3.971	470	473	476	rBV2	399	514	0.10%	0.012%
19	4.001	476	478	479	rBV	530	312	0.06%	0.008%
20	4.129	496	499	502	rBV2	280	326	0.06%	0.008%
21	4.257	517	520	525	rBV3	323	585	0.11%	0.014%
22	4.465	546	554	569	rBV2	37657	109142	20.25%	2.630%
23	5.056	638	651	669	rBV2	68197	215532	39.98%	5.194%
24	5.379	700	704	706	rBV3	375	588	0.11%	0.014%
25	5.672	750	752	756	rBV3	399	375	0.07%	0.009%
26	5.714	756	759	762	rBV2	244	323	0.06%	0.008%
27	5.867	782	784	785	rBV	351	313	0.06%	0.008%
28	5.964	789	800	819	rBV2	180731	539057	100.00%	12.990%
29	6.300	851	855	858	rBV2	576	710	0.13%	0.017%
30	6.757	921	930	949	rBV	142362	359276	66.65%	8.658%
31	7.074	979	982	984	rBV4	349	535	0.10%	0.013%
32	7.111	986	988	989	rBV2	602	481	0.09%	0.012%
33	7.208	1002	1004	1005	rBV2	517	489	0.09%	0.012%
34	7.306	1012	1020	1035	rBV	106143	242618	45.01%	5.847%
35	7.476	1046	1048	1051	rVB3	702	628	0.12%	0.015%
36	7.604	1067	1069	1071	rVB2	565	441	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043721.D
 Acq On : 05 Nov 2024 17:09
 Operator : JC/MD
 Sample : P4670-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0SY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	7.671	1078	1080	1083	rBV	256	320	0.06%	0.008%
38	7.732	1088	1090	1092	rBV	347	312	0.06%	0.008%
39	7.806	1099	1102	1104	rBV2	271	380	0.07%	0.009%
40	7.903	1116	1118	1119	rBV2	308	317	0.06%	0.008%
41	8.324	1182	1187	1200	rBV	63807	115945	21.51%	2.794%
42	8.537	1220	1222	1225	rVB2	368	335	0.06%	0.008%
43	8.647	1234	1240	1259	rBV	251141	417233	77.40%	10.054%
44	8.952	1286	1290	1302	rVV	44197	70571	13.09%	1.701%
45	9.275	1337	1343	1348	rBV3	1671	3087	0.57%	0.074%
46	9.385	1356	1361	1376	rBV	154983	248760	46.15%	5.995%
47	9.555	1387	1389	1393	rVB3	420	410	0.08%	0.010%
48	9.683	1409	1410	1412	rBV	545	399	0.07%	0.010%
49	10.055	1465	1471	1485	rVV	318926	449129	83.32%	10.823%
50	10.451	1534	1536	1539	rBV2	356	390	0.07%	0.009%
51	10.525	1544	1548	1549	rBV	452	516	0.10%	0.012%
52	10.689	1573	1575	1577	rVB	456	339	0.06%	0.008%
53	10.854	1600	1602	1605	rBV2	300	350	0.06%	0.008%
54	10.927	1612	1614	1616	rBV2	302	290	0.05%	0.007%
55	10.951	1616	1618	1621	rVB2	396	302	0.06%	0.007%
56	11.189	1652	1657	1671	rVV	205279	272140	50.48%	6.558%
57	11.317	1674	1678	1682	rVB4	1573	2265	0.42%	0.055%
58	11.354	1682	1684	1685	rBV	315	294	0.05%	0.007%
59	11.549	1715	1716	1719	rVB3	435	294	0.05%	0.007%
60	11.835	1762	1763	1766	rVV	242	338	0.06%	0.008%
61	11.860	1766	1767	1770	rVB2	439	291	0.05%	0.007%
62	12.024	1788	1794	1802	rBV	285737	382116	70.89%	9.208%
63	12.219	1822	1826	1830	rBV3	4072	6019	1.12%	0.145%
64	12.317	1837	1842	1851	rBV	284351	359301	66.65%	8.658%
65	12.567	1881	1883	1886	rBV2	399	313	0.06%	0.008%
66	12.616	1888	1891	1892	rBV2	384	390	0.07%	0.009%
67	12.756	1912	1914	1917	rBV2	514	716	0.13%	0.017%
68	12.823	1922	1925	1927	rBV3	375	346	0.06%	0.008%
69	12.872	1931	1933	1935	rVB2	319	301	0.06%	0.007%
70	12.933	1940	1943	1945	rVB2	316	373	0.07%	0.009%
71	13.012	1953	1956	1959	rBV	450	468	0.09%	0.011%
72	13.055	1959	1963	1967	rBV3	298	527	0.10%	0.013%
73	13.457	2027	2029	2032	rVB2	303	387	0.07%	0.009%
74	13.597	2050	2052	2056	rVB	355	294	0.05%	0.007%
75	13.652	2059	2061	2063	rVV	429	379	0.07%	0.009%
76	13.701	2066	2069	2074	rVB2	389	525	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043721.D
 Acq On : 05 Nov 2024 17:09
 Operator : JC/MD
 Sample : P4670-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0SY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	13.744	2074	2076	2079	rVB2	533	565	0.10%	0.014%
78	13.847	2088	2093	2095	rVB2	305	488	0.09%	0.012%
79	13.878	2095	2098	2100	rBV2	377	492	0.09%	0.012%
80	13.939	2106	2108	2111	rBV2	347	453	0.08%	0.011%
81	14.054	2126	2127	2129	rBV2	585	401	0.07%	0.010%
82	14.128	2137	2139	2140	rBV	429	337	0.06%	0.008%
83	14.335	2171	2173	2174	rBV	387	312	0.06%	0.008%
84	14.560	2208	2210	2212	rBV2	319	302	0.06%	0.007%
85	14.701	2231	2233	2236	rBV2	361	392	0.07%	0.009%
86	14.853	2256	2258	2261	rBV3	486	569	0.11%	0.014%
87	15.036	2286	2288	2292	rBV3	539	762	0.14%	0.018%
88	15.085	2294	2296	2298	rBV	469	325	0.06%	0.008%
89	15.146	2305	2306	2308	rBV2	497	450	0.08%	0.011%
90	15.182	2311	2312	2313	rBV	509	369	0.07%	0.009%
91	15.444	2352	2355	2356	rBV2	476	401	0.07%	0.010%
92	15.536	2368	2370	2373	rBV2	683	788	0.15%	0.019%
93	16.072	2455	2458	2459	rBV2	1034	1022	0.19%	0.025%
94	16.280	2491	2492	2493	rBV	618	381	0.07%	0.009%
95	16.316	2496	2498	2500	rVV	517	324	0.06%	0.008%
96	16.444	2517	2519	2521	rVV2	514	302	0.06%	0.007%
97	16.517	2529	2531	2532	rBV	755	620	0.12%	0.015%
98	16.621	2547	2548	2549	rBV	534	302	0.06%	0.007%
99	16.688	2557	2559	2563	rVB3	586	426	0.08%	0.010%
100	16.731	2565	2566	2567	rBV	568	298	0.06%	0.007%

Sum of corrected areas: 4149724




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043721.D
Acq On : 05 Nov 2024 17:09
Operator : JC/MD
Sample : P4670-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0SY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

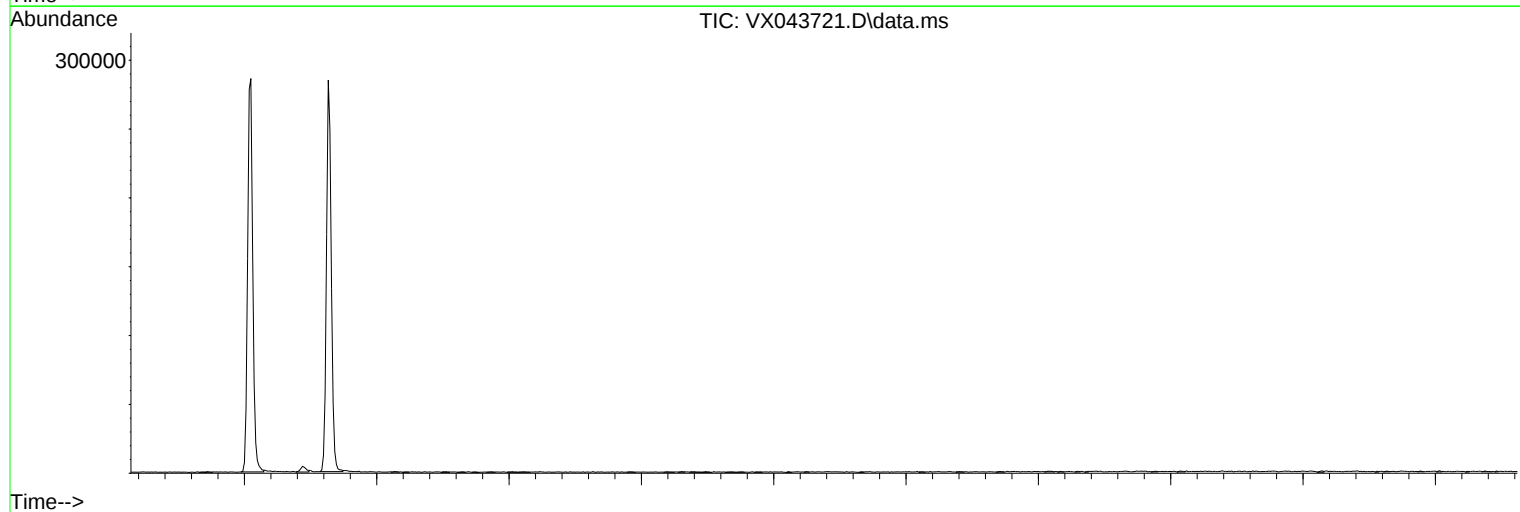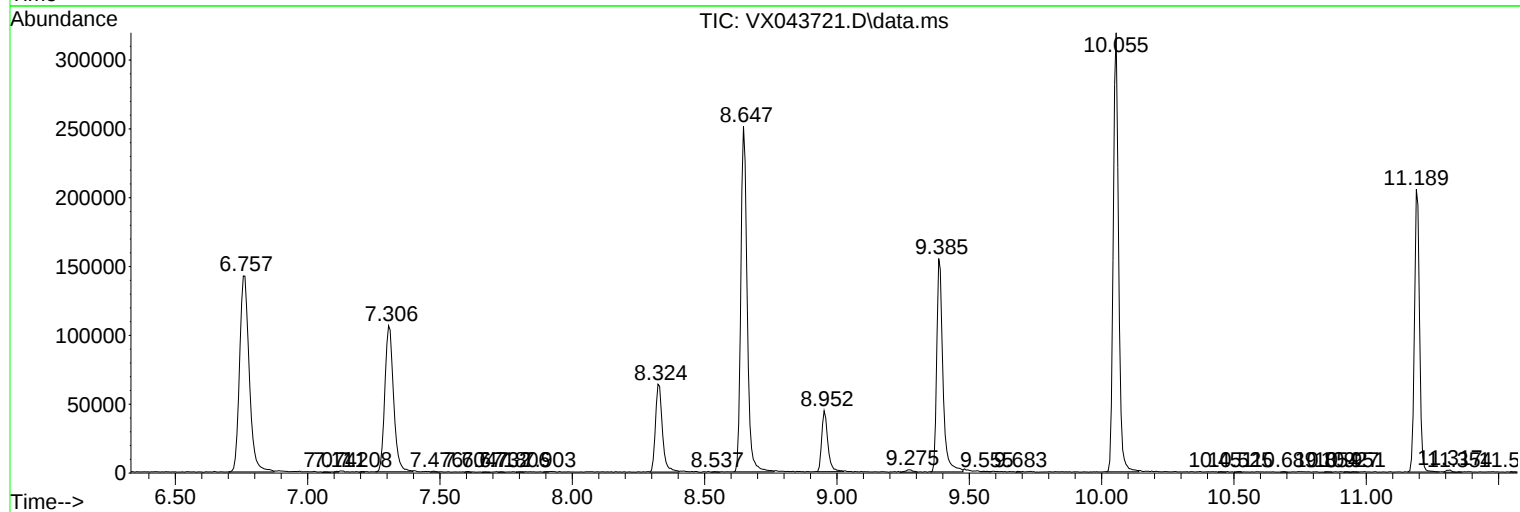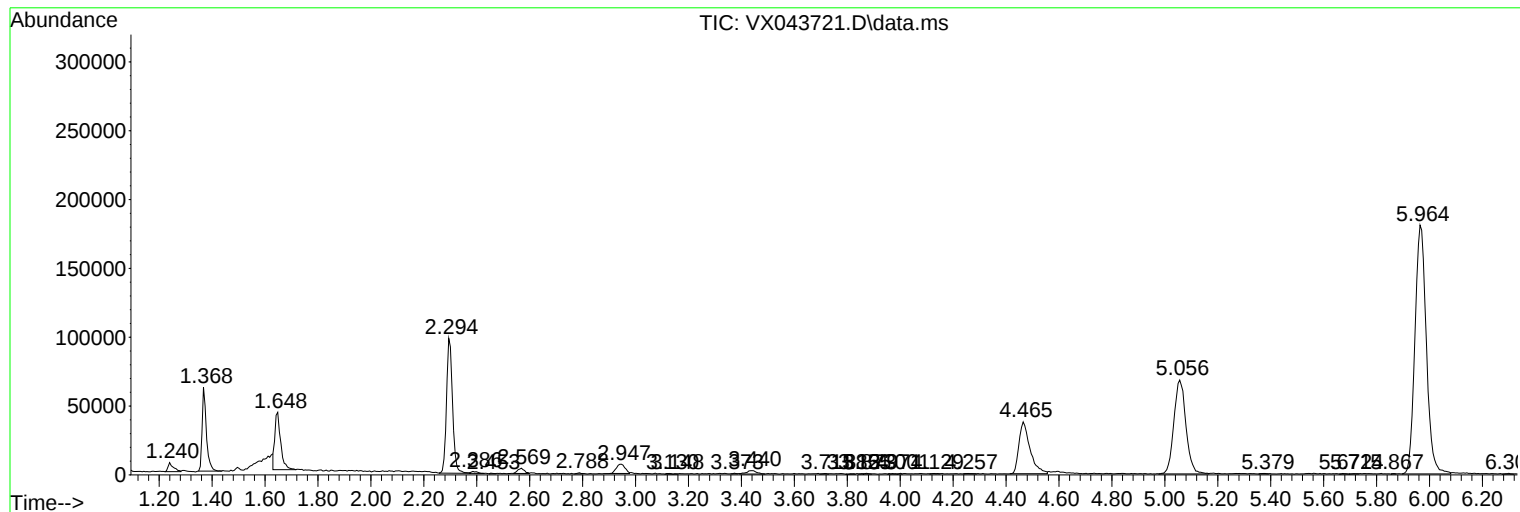

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043721.D
Acq On : 05 Nov 2024 17:09
Operator : JC/MD
Sample : P4670-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0SY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043721.D
Acq On : 05 Nov 2024 17:09
Operator : JC/MD
Sample : P4670-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0SY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc