

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043722.D
 Acq On : 05 Nov 2024 17:32
 Operator : JC/MD
 Sample : P4670-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043722.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	22	25	34	rBV	6408	10164	2.08%	0.263%
2	1.367	43	46	54	rBV	52132	60010	12.26%	1.554%
3	1.648	89	92	101	rVB	42485	54399	11.11%	1.409%
4	2.300	193	199	210	rVB	91450	145653	29.75%	3.772%
5	2.574	242	244	249	rVV2	400	450	0.09%	0.012%
6	2.782	275	278	279	rBV2	451	513	0.10%	0.013%
7	2.940	298	304	316	rVB3	3748	8825	1.80%	0.229%
8	3.032	316	319	322	rVB3	315	376	0.08%	0.010%
9	3.074	322	326	329	rBV2	309	343	0.07%	0.009%
10	3.190	343	345	347	rBV2	292	272	0.06%	0.007%
11	3.215	347	349	353	rVB2	574	619	0.13%	0.016%
12	3.251	353	355	356	rBV	405	295	0.06%	0.008%
13	3.440	378	386	395	rVB5	4575	10787	2.20%	0.279%
14	3.519	397	399	402	rBV2	456	288	0.06%	0.007%
15	3.574	406	408	411	rBV	362	386	0.08%	0.010%
16	3.897	460	461	464	rBV2	324	358	0.07%	0.009%
17	4.117	496	497	502	rVB2	540	710	0.15%	0.018%
18	4.464	546	554	567	rBV2	29417	90852	18.56%	2.353%
19	4.696	591	592	595	rBV2	323	369	0.08%	0.010%
20	4.855	617	618	620	rBV2	296	276	0.06%	0.007%
21	4.897	623	625	627	rVB	356	270	0.06%	0.007%
22	4.934	627	631	635	rBV2	363	528	0.11%	0.014%
23	5.056	640	651	668	rVV2	64964	194470	39.72%	5.036%
24	5.245	680	682	683	rBV2	514	451	0.09%	0.012%
25	5.275	686	687	691	rVV2	523	438	0.09%	0.011%
26	5.306	691	692	694	rVB2	407	274	0.06%	0.007%
27	5.452	715	716	719	rVB	416	307	0.06%	0.008%
28	5.482	719	721	723	rBV2	336	371	0.08%	0.010%
29	5.556	731	733	735	rBV2	346	401	0.08%	0.010%
30	5.964	790	800	818	rBV2	165330	489563	100.00%	12.678%
31	6.269	848	850	852	rBV2	302	364	0.07%	0.009%
32	6.482	883	885	888	rVB2	592	396	0.08%	0.010%
33	6.507	888	889	893	rBV2	270	274	0.06%	0.007%
34	6.543	893	895	898	rVB2	429	370	0.08%	0.010%
35	6.763	922	931	949	rBV	151082	377976	77.21%	9.788%
36	7.116	987	989	992	rBV4	583	476	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043722.D
 Acq On : 05 Nov 2024 17:32
 Operator : JC/MD
 Sample : P4670-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	7.305	1012	1020	1034	rBV	98969	220846	45.11%	5.719%
38	7.458	1043	1045	1046	rVB	399	287	0.06%	0.007%
39	7.494	1050	1051	1053	rVB2	488	326	0.07%	0.008%
40	7.610	1068	1070	1073	rVB2	390	304	0.06%	0.008%
41	7.689	1082	1083	1087	rVB	453	430	0.09%	0.011%
42	7.726	1087	1089	1090	rBV	374	276	0.06%	0.007%
43	7.781	1095	1098	1101	rVB2	417	445	0.09%	0.012%
44	7.939	1120	1124	1125	rBV2	411	525	0.11%	0.014%
45	7.982	1128	1131	1133	rBV2	372	340	0.07%	0.009%
46	8.055	1140	1143	1146	rBV2	277	365	0.07%	0.009%
47	8.281	1178	1180	1182	rVV2	445	432	0.09%	0.011%
48	8.323	1182	1187	1201	rVV	57015	100528	20.53%	2.603%
49	8.519	1216	1219	1220	rBV2	354	266	0.05%	0.007%
50	8.579	1227	1229	1233	rVB3	479	304	0.06%	0.008%
51	8.647	1234	1240	1252	rBV	239999	387411	79.13%	10.033%
52	8.951	1285	1290	1299	rBV	39227	60784	12.42%	1.574%
53	9.128	1317	1319	1322	rVB	471	307	0.06%	0.008%
54	9.183	1325	1328	1329	rBV	308	289	0.06%	0.007%
55	9.274	1340	1343	1344	rBV2	508	438	0.09%	0.011%
56	9.323	1350	1351	1354	rVB2	370	327	0.07%	0.008%
57	9.348	1354	1355	1356	rBV	497	281	0.06%	0.007%
58	9.384	1356	1361	1380	rVV	133495	216830	44.29%	5.615%
59	9.604	1394	1397	1399	rBV3	374	420	0.09%	0.011%
60	9.695	1410	1412	1416	rBV3	885	1247	0.25%	0.032%
61	9.945	1452	1453	1457	rBV2	365	482	0.10%	0.012%
62	10.055	1465	1471	1488	rBV	320756	461102	94.19%	11.941%
63	10.256	1501	1504	1506	rBV2	311	458	0.09%	0.012%
64	10.347	1517	1519	1521	rVB3	393	305	0.06%	0.008%
65	10.640	1564	1567	1568	rVB3	331	301	0.06%	0.008%
66	10.872	1602	1605	1607	rBV2	325	430	0.09%	0.011%
67	10.908	1609	1611	1613	rBV2	331	350	0.07%	0.009%
68	11.006	1624	1627	1629	rBV2	469	490	0.10%	0.013%
69	11.067	1634	1637	1640	rBV2	399	508	0.10%	0.013%
70	11.128	1644	1647	1648	rBV2	241	274	0.06%	0.007%
71	11.189	1652	1657	1666	rBV	174853	230960	47.18%	5.981%
72	11.305	1673	1676	1678	rBV	433	550	0.11%	0.014%
73	11.433	1694	1697	1701	rVB2	310	426	0.09%	0.011%
74	11.536	1713	1714	1717	rBV	382	301	0.06%	0.008%
75	11.713	1741	1743	1746	rVV2	352	388	0.08%	0.010%
76	11.768	1750	1752	1757	rVB2	331	394	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043722.D
 Acq On : 05 Nov 2024 17:32
 Operator : JC/MD
 Sample : P4670-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	11.841	1761	1764	1767	rBV3	442	583	0.12%	0.015%
78	12.018	1788	1793	1802	rBV	286302	384256	78.49%	9.951%
79	12.317	1837	1842	1853	rBV	244774	322288	65.83%	8.346%
80	12.487	1868	1870	1874	rBV2	462	530	0.11%	0.014%
81	12.743	1910	1912	1914	rBV2	315	394	0.08%	0.010%
82	13.036	1958	1960	1963	rBV	381	507	0.10%	0.013%
83	13.213	1986	1989	1992	rBV3	366	408	0.08%	0.011%
84	13.438	2025	2026	2029	rVB2	428	275	0.06%	0.007%
85	13.463	2029	2030	2033	rVB2	401	331	0.07%	0.009%
86	13.493	2033	2035	2037	rBV	295	368	0.08%	0.010%
87	13.536	2041	2042	2045	rBV2	292	321	0.07%	0.008%
88	13.725	2072	2073	2076	rBV2	393	411	0.08%	0.011%
89	14.060	2126	2128	2133	rBV3	316	473	0.10%	0.012%
90	14.133	2136	2140	2142	rBV4	395	526	0.11%	0.014%
91	14.249	2157	2159	2163	rVB2	401	429	0.09%	0.011%
92	14.292	2163	2166	2167	rBV3	370	366	0.07%	0.009%
93	14.597	2214	2216	2218	rBV2	424	324	0.07%	0.008%
94	14.700	2231	2233	2235	rVB	499	318	0.06%	0.008%
95	15.609	2380	2382	2384	rBV2	536	524	0.11%	0.014%
96	15.718	2398	2400	2403	rVB2	539	501	0.10%	0.013%
97	15.895	2426	2429	2431	rVB	651	553	0.11%	0.014%
98	16.310	2493	2497	2501	rBV4	710	1480	0.30%	0.038%
99	16.420	2514	2515	2518	rBV3	541	299	0.06%	0.008%
100	16.669	2554	2556	2558	rBB2	592	469	0.10%	0.012%

Sum of corrected areas: 3861535




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043722.D
Acq On : 05 Nov 2024 17:32
Operator : JC/MD
Sample : P4670-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

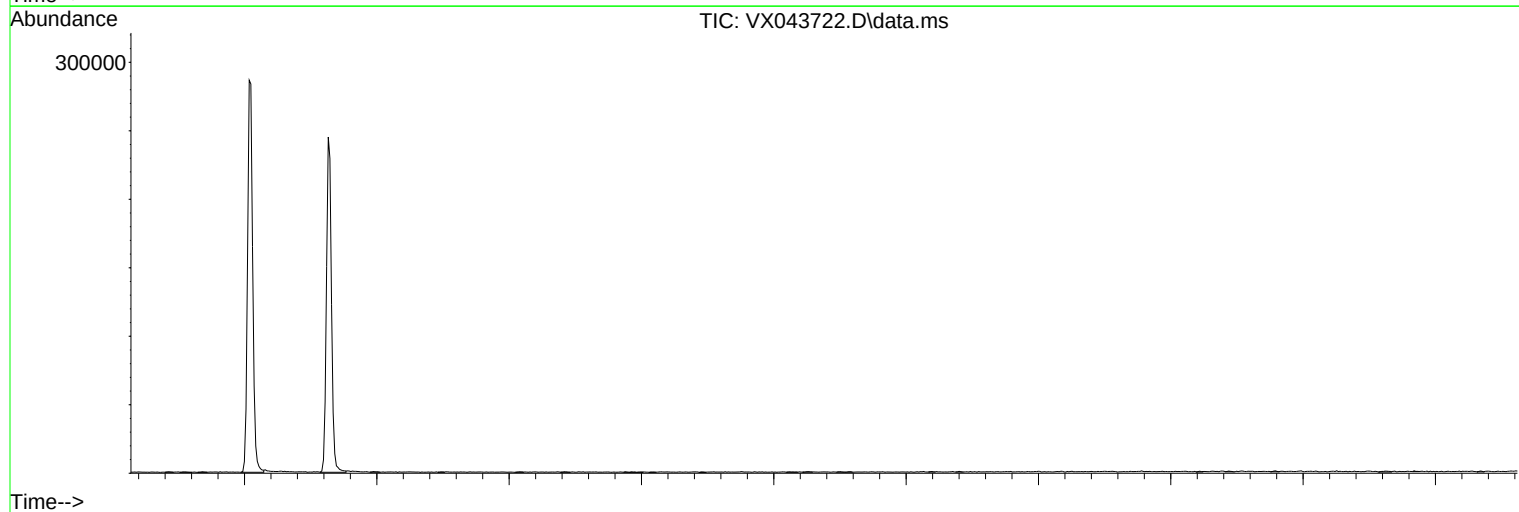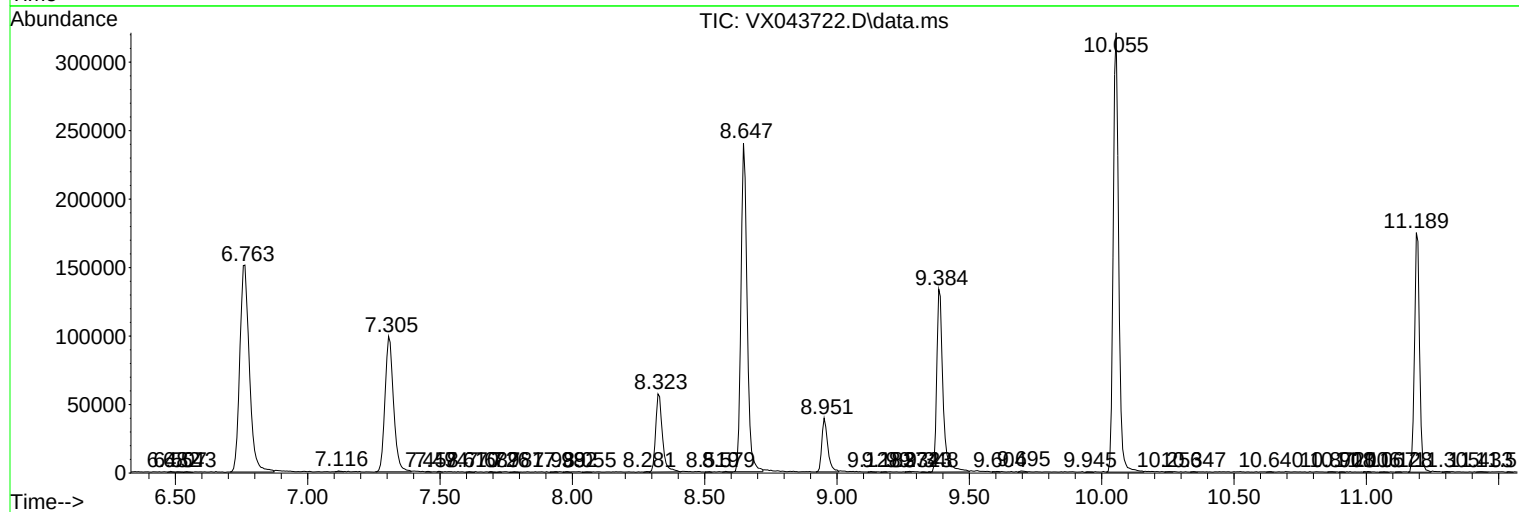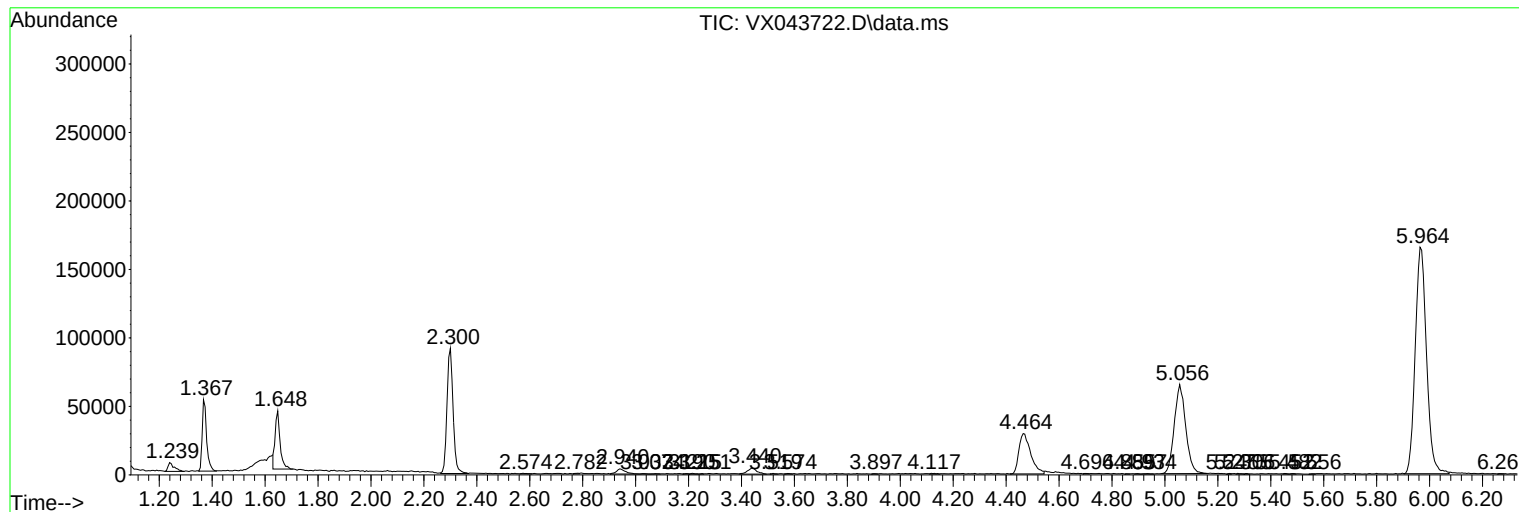

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043722.D
Acq On : 05 Nov 2024 17:32
Operator : JC/MD
Sample : P4670-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043722.D
Acq On : 05 Nov 2024 17:32
Operator : JC/MD
Sample : P4670-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
