

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043723.D
 Acq On : 05 Nov 2024 17:55
 Operator : JC/MD
 Sample : VIBLK675
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK675

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043723.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	32	rVB2	6379	9835	2.18%	0.272%
2	1.368	43	46	56	rVB	47146	53563	11.85%	1.480%
3	1.648	89	92	102	rVB2	34814	51552	11.40%	1.424%
4	2.300	192	199	209	rBV	79991	130275	28.82%	3.598%
5	2.520	234	235	238	rVB2	480	360	0.08%	0.010%
6	2.544	238	239	241	rBV2	768	568	0.13%	0.016%
7	2.562	241	242	248	rVV4	821	1148	0.25%	0.032%
8	2.782	275	278	282	rBV4	802	1122	0.25%	0.031%
9	2.940	301	304	311	rVB3	1109	2016	0.45%	0.056%
10	2.995	311	313	316	rVB2	349	323	0.07%	0.009%
11	3.026	316	318	321	rBV3	257	273	0.06%	0.008%
12	3.257	352	356	358	rVV2	337	327	0.07%	0.009%
13	3.343	368	370	375	rVB2	402	510	0.11%	0.014%
14	3.434	379	385	394	rVB5	2204	4757	1.05%	0.131%
15	3.507	395	397	399	rVB2	396	279	0.06%	0.008%
16	3.910	461	463	465	rVB	356	269	0.06%	0.007%
17	4.148	500	502	503	rBV	621	481	0.11%	0.013%
18	4.410	543	545	546	rBV2	338	253	0.06%	0.007%
19	4.465	547	554	572	rBV2	26889	86349	19.10%	2.385%
20	4.903	624	626	627	rBV	299	249	0.06%	0.007%
21	5.056	640	651	668	rBV	58255	180742	39.98%	4.992%
22	5.391	704	706	708	rVB2	367	265	0.06%	0.007%
23	5.501	720	724	725	rVV2	241	310	0.07%	0.009%
24	5.550	731	732	736	rBV2	490	508	0.11%	0.014%
25	5.605	739	741	742	rVV2	387	296	0.07%	0.008%
26	5.659	748	750	752	rVV3	252	236	0.05%	0.007%
27	5.684	752	754	757	rVV2	255	320	0.07%	0.009%
28	5.794	770	772	774	rBV2	341	330	0.07%	0.009%
29	5.879	780	786	787	rBV2	296	415	0.09%	0.011%
30	5.964	790	800	820	rBV2	148920	452094	100.00%	12.488%
31	6.409	871	873	875	rBV	311	323	0.07%	0.009%
32	6.440	877	878	881	rVV2	423	255	0.06%	0.007%
33	6.495	884	887	888	rBV	402	257	0.06%	0.007%
34	6.592	902	903	905	rVB2	395	238	0.05%	0.007%
35	6.757	922	930	945	rBV	142038	360307	79.70%	9.952%
36	6.934	957	959	963	rVB3	639	678	0.15%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043723.D
 Acq On : 05 Nov 2024 17:55
 Operator : JC/MD
 Sample : VIBLK675
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK675

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	7.068	979	981	982	rVB	442	240	0.05%	0.007%
38	7.305	1012	1020	1037	rBV	92985	208462	46.11%	5.758%
39	7.513	1053	1054	1058	rBV2	364	254	0.06%	0.007%
40	7.677	1079	1081	1085	rBV2	310	283	0.06%	0.008%
41	7.769	1095	1096	1099	rBV	233	284	0.06%	0.008%
42	7.854	1108	1110	1111	rBV	402	258	0.06%	0.007%
43	7.940	1121	1124	1127	rBV2	396	410	0.09%	0.011%
44	8.000	1132	1134	1137	rVB	478	501	0.11%	0.014%
45	8.074	1144	1146	1150	rBV2	349	479	0.11%	0.013%
46	8.110	1150	1152	1154	rVB	337	225	0.05%	0.006%
47	8.129	1154	1155	1157	rBV2	437	274	0.06%	0.008%
48	8.165	1160	1161	1163	rBV	302	275	0.06%	0.008%
49	8.324	1182	1187	1196	rBV	54390	92692	20.50%	2.560%
50	8.647	1234	1240	1251	rBV	215518	354422	78.40%	9.790%
51	8.891	1276	1280	1282	rVB2	453	665	0.15%	0.018%
52	8.952	1282	1290	1304	rBV	37470	59856	13.24%	1.653%
53	9.275	1340	1343	1349	rBV4	1263	1962	0.43%	0.054%
54	9.384	1356	1361	1372	rBV	130582	202018	44.68%	5.580%
55	9.689	1410	1411	1415	rBV	329	396	0.09%	0.011%
56	9.744	1419	1420	1421	rBV	525	253	0.06%	0.007%
57	9.787	1426	1427	1429	rBV	331	236	0.05%	0.007%
58	9.872	1437	1441	1442	rBV2	317	413	0.09%	0.011%
59	9.951	1452	1454	1458	rVB3	358	345	0.08%	0.010%
60	9.994	1460	1461	1463	rVB	437	242	0.05%	0.007%
61	10.055	1465	1471	1484	rBV	309639	447798	99.05%	12.369%
62	10.256	1502	1504	1506	rVB2	310	225	0.05%	0.006%
63	10.726	1580	1581	1582	rBV	380	255	0.06%	0.007%
64	10.982	1620	1623	1624	rBV2	382	368	0.08%	0.010%
65	11.073	1636	1638	1640	rVB2	330	266	0.06%	0.007%
66	11.104	1641	1643	1646	rVB2	275	303	0.07%	0.008%
67	11.152	1649	1651	1652	rBV2	312	302	0.07%	0.008%
68	11.189	1652	1657	1667	rVV	168348	219713	48.60%	6.069%
69	11.311	1673	1677	1684	rBV4	893	1414	0.31%	0.039%
70	11.500	1706	1708	1712	rBV2	374	547	0.12%	0.015%
71	11.530	1712	1713	1718	rVV2	360	484	0.11%	0.013%
72	11.610	1723	1726	1727	rBV	304	288	0.06%	0.008%
73	11.683	1737	1738	1741	rBV2	367	277	0.06%	0.008%
74	11.811	1758	1759	1761	rVB	531	251	0.06%	0.007%
75	11.921	1775	1777	1778	rBV	299	238	0.05%	0.007%
76	12.024	1789	1794	1805	rBV	275546	371398	82.15%	10.259%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
 Data File : VX043723.D
 Acq On : 05 Nov 2024 17:55
 Operator : JC/MD
 Sample : VIBLK675
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK675

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	12.195	1820	1822	1825	rBV3	322	367	0.08%	0.010%
78	12.274	1833	1835	1837	rVB2	446	333	0.07%	0.009%
79	12.317	1837	1842	1855	rBV	229863	299145	66.17%	8.263%
80	12.646	1895	1896	1898	rVB2	395	244	0.05%	0.007%
81	12.725	1907	1909	1910	rBV	575	319	0.07%	0.009%
82	12.798	1920	1921	1923	rBV	287	242	0.05%	0.007%
83	12.890	1934	1936	1939	rVB2	439	526	0.12%	0.015%
84	12.920	1939	1941	1944	rBV2	324	418	0.09%	0.012%
85	12.957	1944	1947	1948	rBV2	316	376	0.08%	0.010%
86	13.243	1992	1994	1996	rBV2	436	400	0.09%	0.011%
87	13.378	2014	2016	2018	rVV	295	257	0.06%	0.007%
88	13.573	2046	2048	2052	rVV2	391	369	0.08%	0.010%
89	13.615	2053	2055	2061	rVB3	327	414	0.09%	0.011%
90	13.798	2082	2085	2088	rBV3	413	522	0.12%	0.014%
91	13.914	2102	2104	2108	rBV3	370	387	0.09%	0.011%
92	14.188	2148	2149	2153	rBV	433	435	0.10%	0.012%
93	14.268	2161	2162	2163	rBV	424	239	0.05%	0.007%
94	14.548	2206	2208	2212	rBV3	377	572	0.13%	0.016%
95	14.871	2260	2261	2263	rBV2	454	291	0.06%	0.008%
96	15.243	2320	2322	2324	rBV2	453	452	0.10%	0.012%
97	15.536	2368	2370	2374	rBV4	690	909	0.20%	0.025%
98	16.444	2517	2519	2520	rBV2	531	361	0.08%	0.010%
99	16.645	2550	2552	2553	rBV	621	548	0.12%	0.015%
100	16.694	2558	2560	2562	rVV2	701	501	0.11%	0.014%

Sum of corrected areas: 3620282




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043723.D
Acq On : 05 Nov 2024 17:55
Operator : JC/MD
Sample : VIBLK675
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK675

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

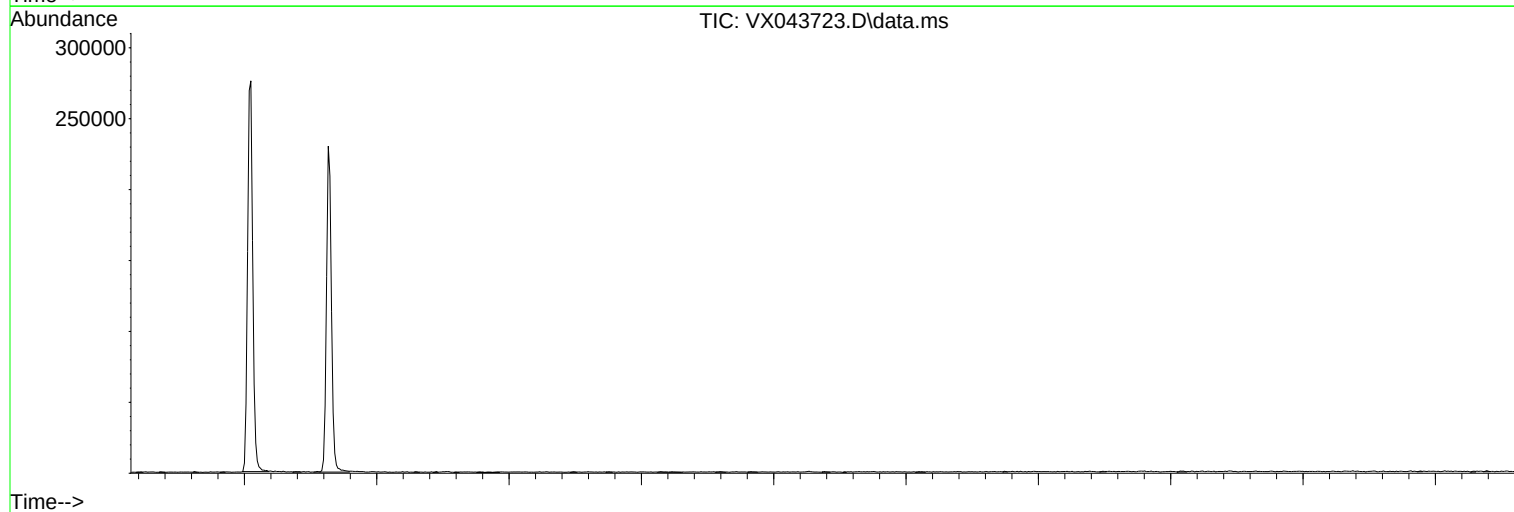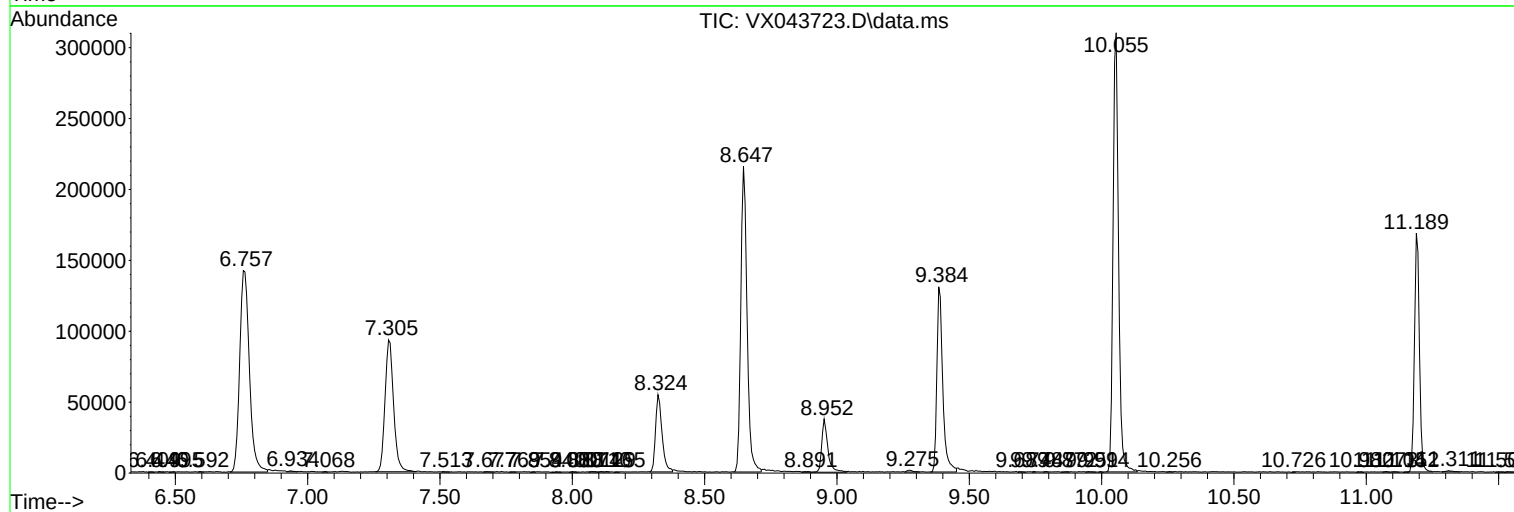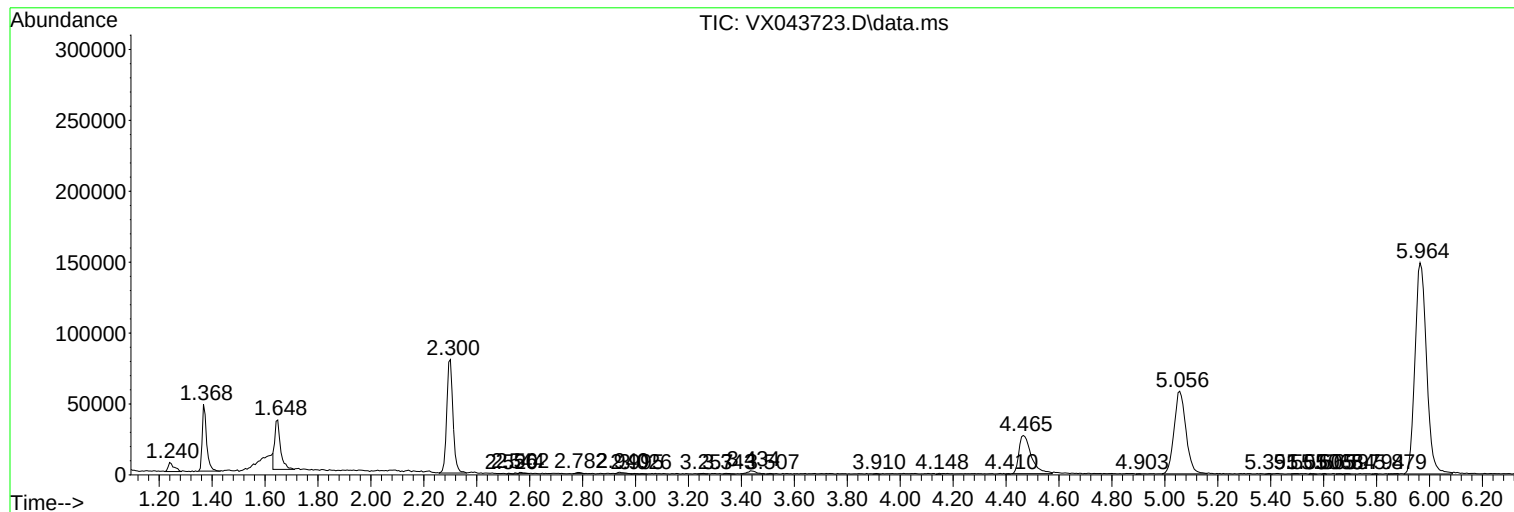

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043723.D
Acq On : 05 Nov 2024 17:55
Operator : JC/MD
Sample : VIBLK675
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK675

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043723.D
Acq On : 05 Nov 2024 17:55
Operator : JC/MD
Sample : VIBLK675
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK675

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
