
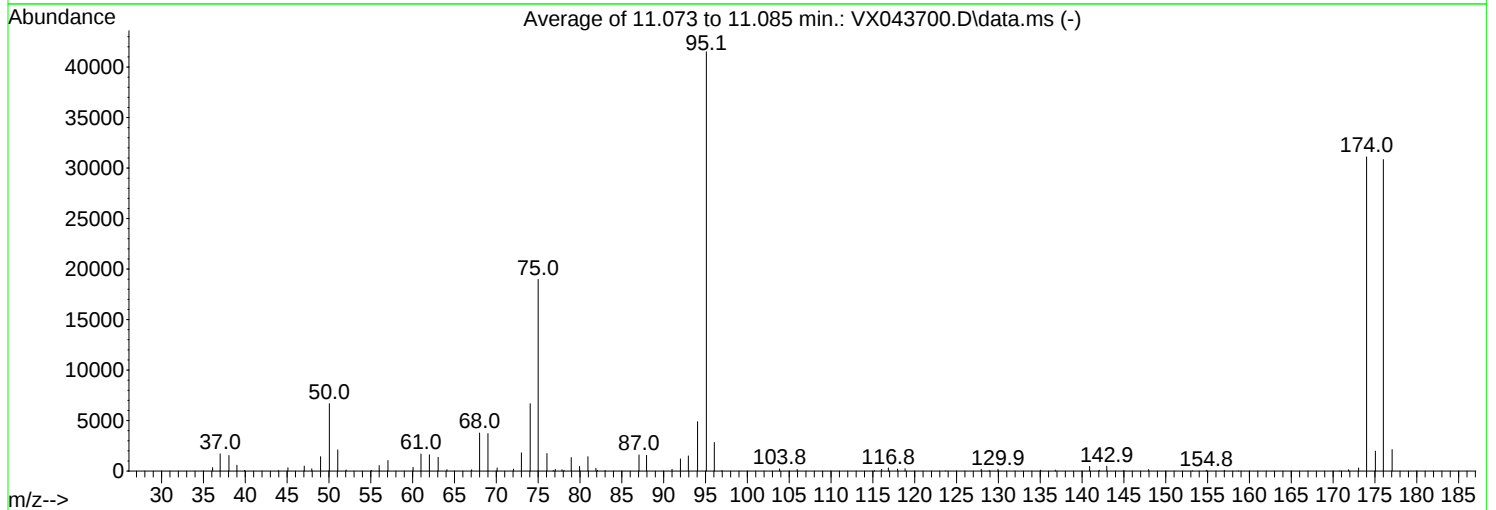


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110524\
Data File : VX043700.D
Acq On : 05 Nov 2024 07:57
Operator : JC/MD
Sample : BFB694
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB694

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXL110424WMA.M
Title : VOC Analysis
Last Update : Wed Nov 06 01:38:34 2024

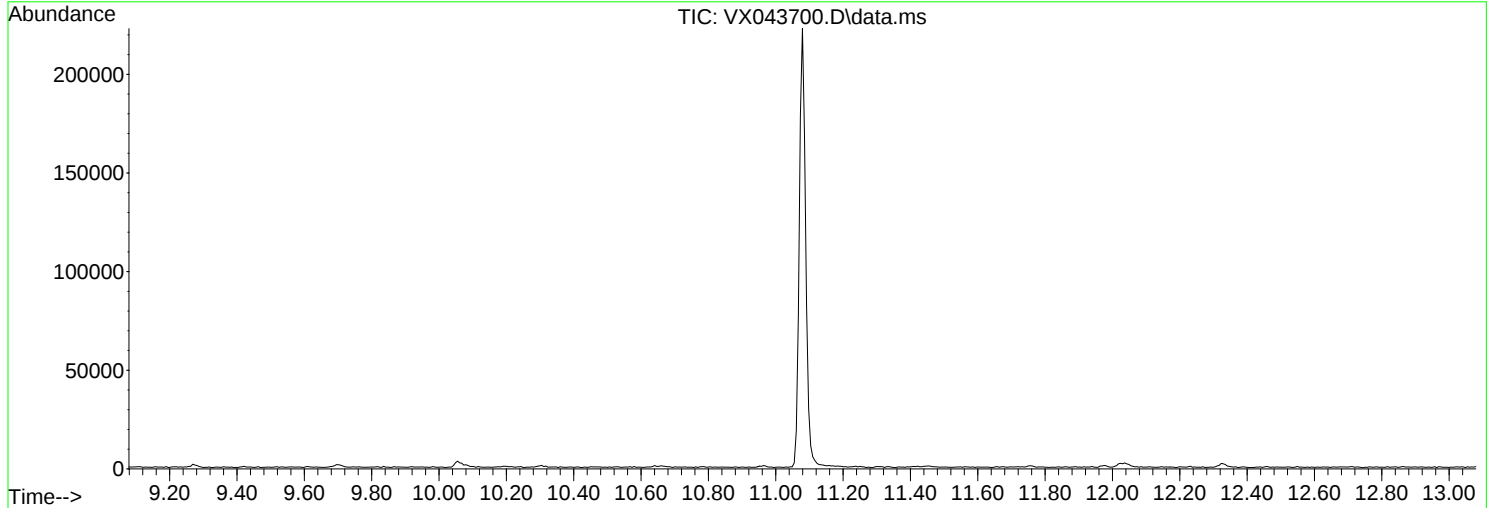

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	6679	PASS
75	95	30	80	45.7	18983	PASS
95	95	100	100	100.0	41517	PASS
96	95	5	9	6.8	2831	PASS
173	174	0.00	2	1.0	315	PASS
174	95	50	120	74.9	31107	PASS
175	174	5	9	6.3	1972	PASS
176	174	95	101	99.2	30845	PASS
177	176	5	9	6.9	2135	PASS

m/z	Abundance
39.90	565.0
43.00	82.0
44.00	414.0

Instrument :
MSVOA_X
ClientSampleId :
BFB694

m/z	Abundance
36.10	285.0
37.00	1668.0
38.10	1675.0
39.00	678.0
39.90	540.0
44.00	524.0
45.10	444.0
47.10	470.0
48.00	238.0
49.00	1639.0
50.10	7222.0
51.00	2247.0
52.20	101.0
55.00	61.0
56.00	731.0
57.00	1082.0
60.00	377.0
61.00	1921.0
62.10	1626.0
63.00	1460.0
64.10	113.0
67.00	120.0
68.00	4002.0
69.00	3778.0
70.10	412.0
72.10	215.0
73.00	1898.0
74.00	6770.0
75.00	19168.0
76.00	1616.0
77.10	212.0
77.90	153.0
78.90	1310.0
80.00	396.0
80.90	1447.0
82.00	394.0
83.00	74.0
87.10	1546.0
87.90	1480.0
91.00	151.0
92.00	1185.0
93.00	1493.0
94.10	4759.0
95.10	40480.0
96.00	3217.0
96.90	62.0
103.90	190.0
105.90	111.0
116.10	167.0
116.90	248.0
118.00	141.0
118.80	263.0
127.90	85.0
128.90	67.0
130.00	107.0
135.10	68.0
136.70	74.0
140.90	518.0
142.00	67.0
142.90	476.0
145.00	56.0
148.00	233.0
153.20	54.0
154.80	69.0
157.00	65.0
171.90	158.0
173.00	278.0
174.00	25304.0
175.00	1648.0
176.00	25184.0
177.00	1824.0

Instrument :
MSVOA_X
ClientSampleId :
BFB694

m/z	Abundance
36.10	515.0
37.00	2258.0
38.00	1788.0
39.00	543.0
40.00	619.0
43.90	449.0
45.10	370.0
47.10	695.0
48.00	271.0
49.00	1655.0
50.00	7764.0
51.10	2097.0
52.00	138.0
55.10	66.0
56.10	595.0
57.00	1196.0
60.00	430.0
61.00	1983.0
62.00	1911.0
63.10	1569.0
64.10	234.0
67.10	119.0
68.00	4365.0
69.00	4601.0
70.10	344.0
72.10	187.0
73.00	2012.0
74.10	7600.0
75.00	22560.0
76.10	2094.0
77.00	308.0
77.80	246.0
78.90	1688.0
79.90	553.0
81.00	1630.0
81.80	454.0
83.00	68.0
87.00	2081.0
88.00	2006.0
90.90	163.0
92.00	1314.0
93.00	1651.0
94.10	5833.0
95.10	48744.0
96.10	2927.0
97.00	65.0
103.80	261.0
106.00	300.0
116.00	192.0
116.80	334.0
117.90	224.0
118.90	255.0
123.70	61.0
128.00	185.0
128.90	78.0
130.00	295.0
135.10	130.0
136.80	154.0
141.00	543.0
142.00	85.0
143.00	543.0
145.00	87.0
147.90	105.0
154.90	82.0
157.00	73.0
158.70	51.0
170.80	63.0
171.80	105.0
173.00	308.0
174.00	36800.0
175.00	2376.0
176.00	36280.0
177.10	2437.0

Instrument :
MSVOA_X
ClientSampleId :
BFB694

m/z	Abundance
36.00	240.0
37.10	1196.0
38.10	1168.0
39.00	526.0
40.00	715.0
44.00	422.0
45.00	189.0
46.90	320.0
47.90	184.0
49.00	986.0
50.10	5051.0
51.00	1956.0
51.90	95.0
55.20	63.0
55.90	307.0
57.10	858.0
60.10	306.0
61.10	1180.0
61.90	1313.0
63.00	1061.0
64.20	86.0
67.00	147.0
68.00	2942.0
69.10	2777.0
70.10	191.0
71.90	207.0
73.00	1525.0
74.00	5647.0
75.00	15220.0
76.00	1508.0
76.80	182.0
78.10	151.0
79.00	1005.0
79.90	435.0
80.90	1202.0
82.10	195.0
87.00	1184.0
87.90	1185.0
91.10	222.0
92.00	1115.0
92.90	1355.0
94.00	4072.0
95.10	35328.0
96.10	2348.0
103.80	191.0
105.90	67.0
115.20	109.0
116.00	155.0
116.80	313.0
117.90	228.0
118.90	213.0
127.90	267.0
129.90	154.0
135.00	84.0
136.90	94.0
140.80	342.0
142.10	92.0
143.00	426.0
147.90	116.0
154.80	89.0
157.00	102.0
171.90	159.0
173.10	360.0
174.00	31216.0
175.10	1892.0
176.00	31072.0
177.00	2144.0

Instrument :
MSVOA_X
ClientSampleId :
BFB694