


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX110618\
Data File : VX005797.D
Acq On : 06 Nov 2018 09:46
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X103118W.M
Title : SW846 8260
Last Update : Wed Oct 31 18:23:06 2018

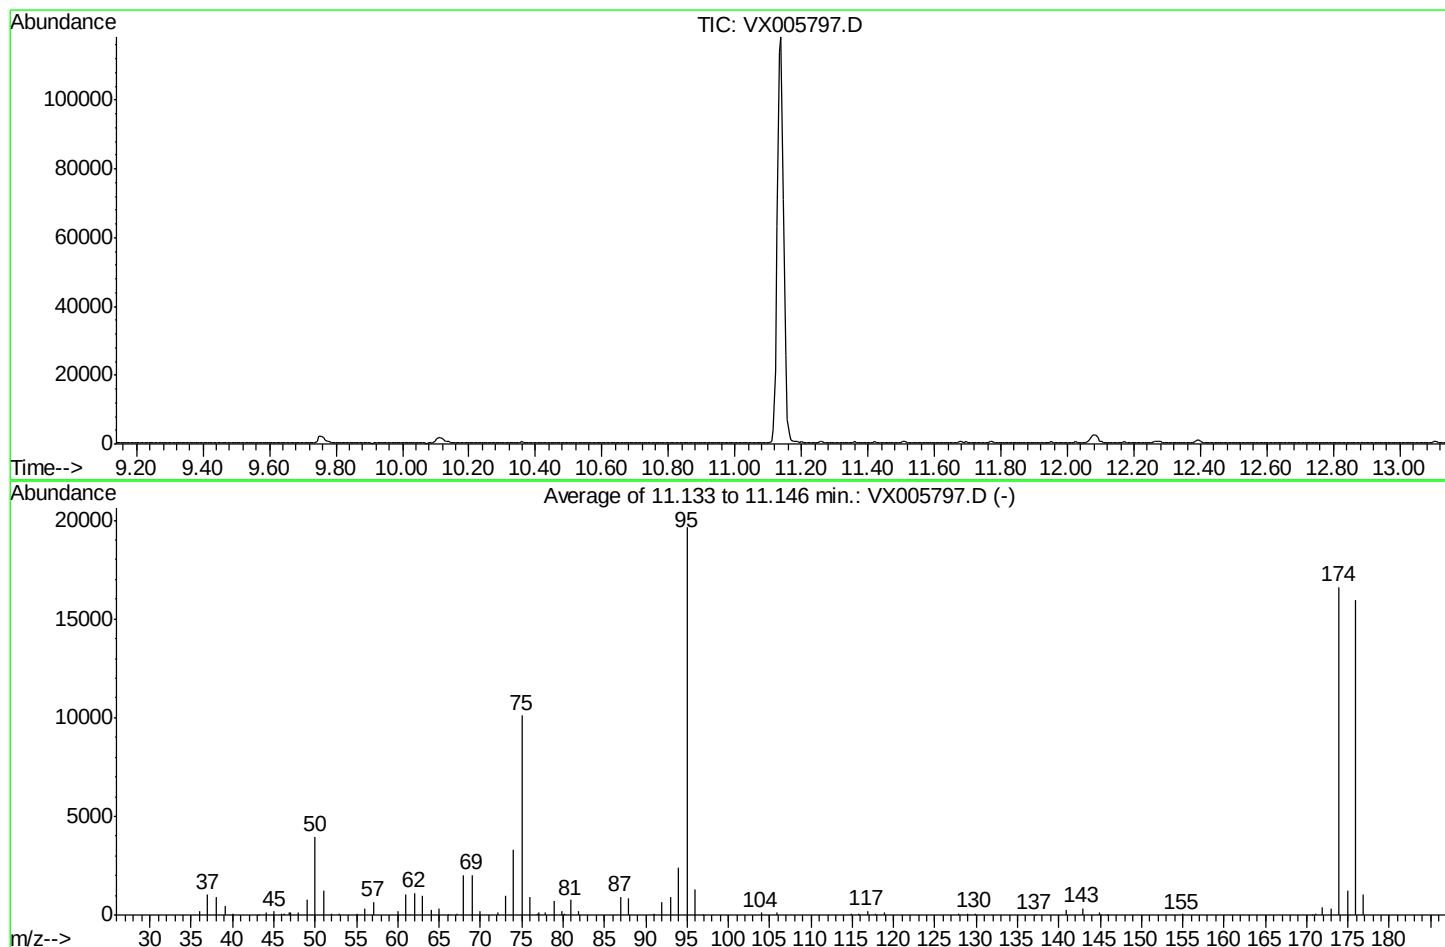

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	3969	PASS
75	95	30	60	51.4	10091	PASS
95	95	100	100	100.0	19641	PASS
96	95	5	9	6.7	1317	PASS
173	174	0.00	2	1.8	298	PASS
174	95	50	100	84.6	16617	PASS
175	174	5	9	7.6	1265	PASS
176	174	95	101	96.1	15966	PASS
177	176	5	9	6.6	1057	PASS