


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110619\
 Data File : VX013332.D
 Acq On : 06 Nov 2019 09:09
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
 Title : SW846 8260
 Last Update : Sat Nov 02 07:06:38 2019

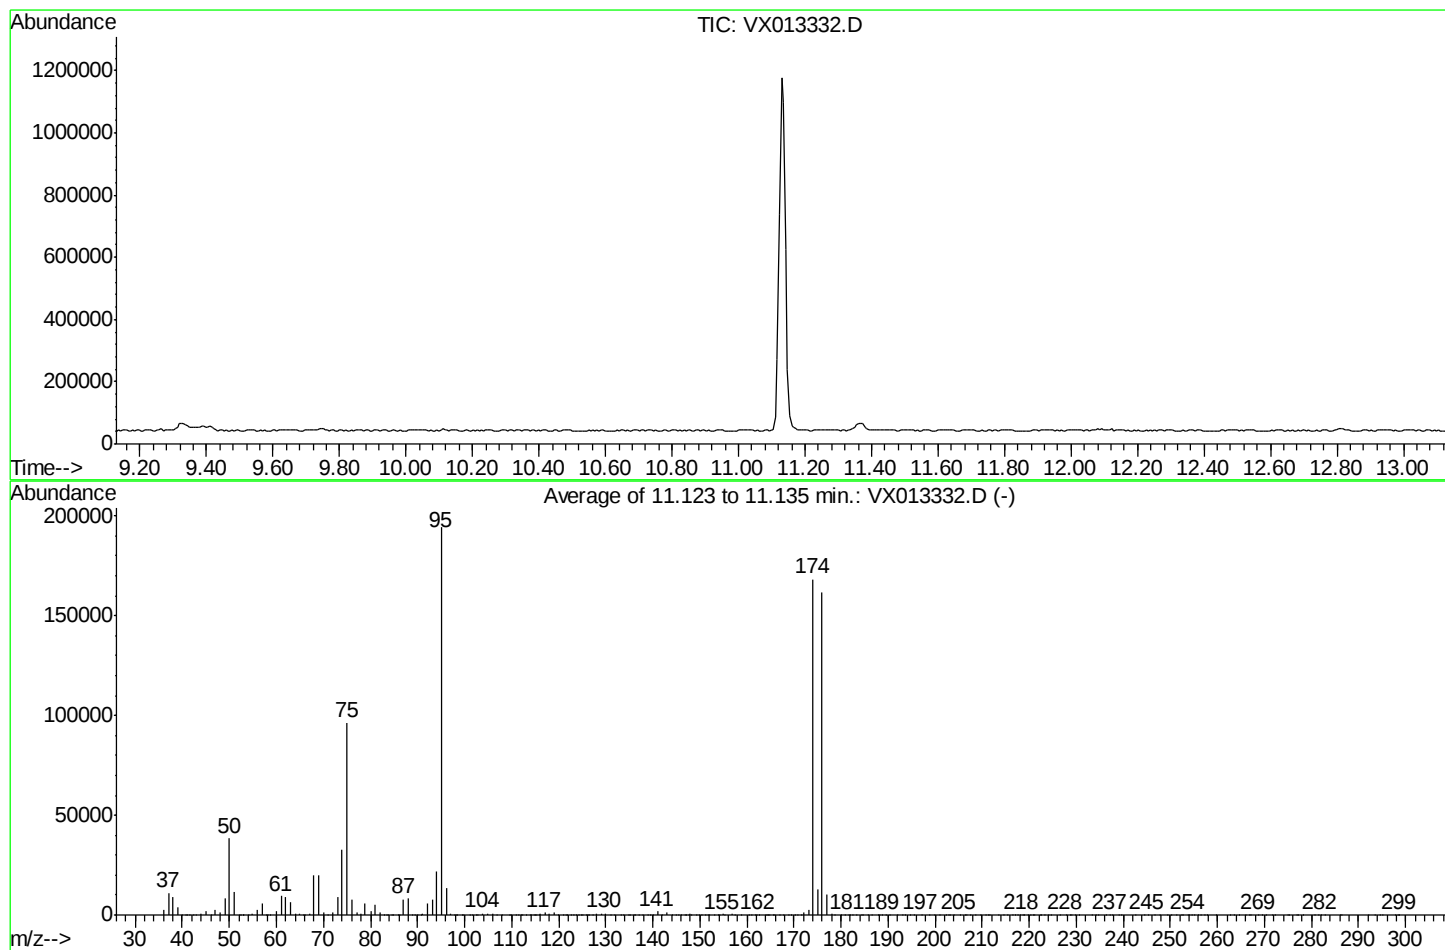

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	38333	PASS
75	95	30	60	49.7	96544	PASS
95	95	100	100	100.0	194330	PASS
96	95	5	9	7.0	13614	PASS
173	174	0.00	2	1.4	2416	PASS
174	95	50	100	86.7	168401	PASS
175	174	5	9	7.5	12596	PASS
176	174	95	101	95.9	161445	PASS
177	176	5	9	6.6	10576	PASS