

Data File : VX019278.D
Acq On : 04 Nov 2020 18:57
Operator : JC/MD
Sample : VX1106WBSD01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1106WBSD01

Manual Integrations
APPROVED

MMDadoda
11/5/2020 7:02:28 PM

Quant Time: Nov 05 02:53:14 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102720W.M
Quant Title : SW846 8260
QLast Update : Tue Oct 27 13:55:07 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	247725	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	423226	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	378857	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	190589	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.03	65	162523	50.87	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.74%	
35) Dibromofluoromethane	5.46	113	125702	47.28	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.56%	
50) Toluene-d8	8.70	98	480758	47.97	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.94%	
62) 4-Bromofluorobenzene	11.12	95	179312	47.25	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.50%	

Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.18	85	39252	19.006	ug/l	97
3) Chloromethane	1.31	50	47227	20.469	ug/l	100
4) Vinyl Chloride	1.39	62	53970	20.170	ug/l	100
5) Bromomethane	1.64	94	40573	22.203	ug/l	100
6) Chloroethane	1.72	64	36137	21.153	ug/l	97
7) Trichlorofluoromethane	1.92	101	82811	19.700	ug/l	99
8) Diethyl Ether	2.17	74	33854	20.984	ug/l	95
9) 1,1,2-Trichlorotrifluoroet	2.37	101	45657	19.595	ug/l	98
10) Methyl Iodide	2.49	142	48268	21.690	ug/l	98
11) Tert butyl alcohol	3.02	59	64422	102.095	ug/l	100
12) 1,1-Dichloroethene	2.36	96	46402	19.326	ug/l	98
13) Acrolein	2.28	56	22551	83.775	ug/l	98
14) Allyl chloride	2.71	41	72523	19.942	ug/l	99
15) Acrylonitrile	3.12	53	138245	104.260	ug/l	99
16) Acetone	2.42	43	114225	103.641	ug/l	99
17) Carbon Disulfide	2.55	76	123183	18.485	ug/l	99
18) Methyl Acetate	2.75	43	56309	21.010	ug/l	99
19) Methyl tert-butyl Ether	3.17	73	165825	19.933	ug/l	98
20) Methylene Chloride	2.83	84	53959	19.502	ug/l	95
21) trans-1,2-Dichloroethene	3.14	96	52709	19.075	ug/l	96
22) Diisopropyl ether	3.82	45	153001	21.103	ug/l	95
23) Vinyl Acetate	3.78	43	671630	103.882	ug/l	98
24) 1,1-Dichloroethane	3.67	63	92868	20.516	ug/l	100
25) 2-Butanone	4.64	43	182457	105.044	ug/l	96
26) 2,2-Dichloropropane	4.55	77	81327	19.111	ug/l	99
27) cis-1,2-Dichloroethene	4.57	96	59765	19.355	ug/l	97
28) Bromochloromethane	4.98	49	42579	20.691	ug/l	92
29) Tetrahydrofuran	5.09	42	116616	106.536	ug/l	98
30) Chloroform	5.18	83	96981	20.128	ug/l	99
31) Cyclohexane	5.55	56	79611	19.714	ug/l	99
32) 1,1,1-Trichloroethane	5.46	97	87813	20.102	ug/l	98
36) 1,1-Dichloropropene	5.77	75	73809	18.886	ug/l	98
37) Ethyl Acetate	4.79	43	71343	19.661	ug/l	99
38) Carbon Tetrachloride	5.76	117	73310	18.403	ug/l	99

Data File : VX019278.D
Acq On : 04 Nov 2020 18:57
Operator : JC/MD
Sample : VX1106WBSD01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1106WBSD01

Manual Integrations
APPROVED

MMDadoda
11/5/2020 7:02:28 PM

Quant Time: Nov 05 02:53:14 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102720W.M
Quant Title : SW846 8260
QLast Update : Tue Oct 27 13:55:07 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
39) Methylcyclohexane	7.44	83	85401	18.275	ug/l	97
40) Benzene	6.11	78	214198	19.330	ug/l	99
41) Methacrylonitrile	5.00	41	38545	19.725	ug/l	98
42) 1,2-Dichloroethane	6.17	62	80904	19.811	ug/l	100
43) Isopropyl Acetate	6.41	43	117311	19.308	ug/l	99
44) Trichloroethene	7.19	130	57605	18.152	ug/l	92
45) 1,2-Dichloropropane	7.49	63	54955	20.248	ug/l	100
46) Dibromomethane	7.63	93	37979	18.923	ug/l	95
47) Bromodichloromethane	7.87	83	75972	19.205	ug/l	97
48) Methyl methacrylate	7.74	41	57162	19.547	ug/l	98
49) 1,4-Dioxane	7.73	88	24991	384.270	ug/l	97
51) 4-Methyl-2-Pentanone	8.62	43	360439	103.215	ug/l	99
52) Toluene	8.76	92	135478	18.983	ug/l	98
53) t-1,3-Dichloropropene	9.02	75	80612	17.841	ug/l	99
54) cis-1,3-Dichloropropene	8.42	75	87864	18.493	ug/l	99
55) 1,1,2-Trichloroethane	9.20	97	54651	19.381	ug/l	97
56) Ethyl methacrylate	9.16	69	80380	18.872	ug/l	97
57) 1,3-Dichloropropane	9.35	76	92567	19.470	ug/l	100
58) 2-Chloroethyl Vinyl ether	8.29	63	228238	95.817	ug/l	96
59) 2-Hexanone	9.47	43	274134	103.126	ug/l	98
60) Dibromochloromethane	9.56	129	55958	18.285	ug/l	100
61) 1,2-Dibromoethane	9.65	107	56994	18.901	ug/l	98
64) Tetrachloroethene	9.32	164	54073	18.733	ug/l	94
65) Chlorobenzene	10.12	112	142905	18.455	ug/l	100
66) 1,1,1,2-Tetrachloroethane	10.20	131	51551	18.492	ug/l	100
67) Ethyl Benzene	10.23	91	258505	18.735	ug/l	100
68) m/p-Xylenes	10.34	106	194838	37.623	ug/l	99
69) o-Xylene	10.68	106	91214	18.570	ug/l	98
70) Styrene	10.70	104	155860	18.597	ug/l	99
71) Bromoform	10.84	173	37198	16.830	ug/l #	99
73) Isopropylbenzene	11.00	105	251395	18.634	ug/l	100
74) N-amyl acetate	10.88	43	93932	19.043	ug/l	98
75) 1,1,2,2-Tetrachloroethane	11.25	83	82785	19.635	ug/l	99
76) 1,2,3-Trichloropropane	11.28	75	77143m	19.603	ug/l	
77) Bromobenzene	11.24	156	59582	17.795	ug/l	93
78) n-propylbenzene	11.34	91	287475	18.667	ug/l	100
79) 2-Chlorotoluene	11.40	91	171241	18.887	ug/l	99
80) 1,3,5-Trimethylbenzene	11.49	105	210992	18.513	ug/l	100
81) trans-1,4-Dichloro-2-buten	11.06	75	24516	16.403	ug/l	93
82) 4-Chlorotoluene	11.49	91	203530	18.383	ug/l	98
83) tert-Butylbenzene	11.76	119	198898	18.226	ug/l	97
84) 1,2,4-Trimethylbenzene	11.79	105	214451	18.638	ug/l	100
85) sec-Butylbenzene	11.93	105	246563	18.839	ug/l	99
86) p-Isopropyltoluene	12.05	119	222006	18.377	ug/l	99
87) 1,3-Dichlorobenzene	12.01	146	112000	17.962	ug/l	99
88) 1,4-Dichlorobenzene	12.08	146	114781	17.684	ug/l	97
89) n-Butylbenzene	12.37	91	206065	18.147	ug/l	98
90) Hexachloroethane	12.58	117	35960	17.513	ug/l	96
91) 1,2-Dichlorobenzene	12.37	146	109169	18.233	ug/l	99
92) 1,2-Dibromo-3-Chloropropan	12.98	75	18524	17.947	ug/l	93

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX110620\
Quantitation Report (QT Reviewed)

Data File : VX019278.D
Acq On : 04 Nov 2020 18:57
Operator : JC/MD
Sample : VX1106WBSD01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1106WBSD01

Manual Integrations
APPROVED

MMDadoda
11/5/2020 7:02:28 PM

Quant Time: Nov 05 02:53:14 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102720W.M
Quant Title : SW846 8260
QLast Update : Tue Oct 27 13:55:07 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
93) 1,2,4-Trichlorobenzene	13.63	180	73344	16.308	ug/l	100
94) Hexachlorobutadiene	13.76	225	31647	15.985	ug/l	97
95) Naphthalene	13.82	128	238905	16.867	ug/l	100
96) 1,2,3-Trichlorobenzene	14.00	180	73036	16.740	ug/l	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VX019278.D


```
Acq On       : 04 Nov 2020   18:57
Operator     : JC/MD
Sample       : VX1106WBSD01
Misc         : 5.0mL/MSV0A_X/WATER
ALS Vial     : 6      Sample Multiplier: 1
```


Instrument :
MSVOA_X
ClientSampleId :
VX1106WBSD01

Manual Integrations
APPROVED

MMDadoda
11/5/2020 7:02:28 PM

Quant Time: Nov 05 02:53:14 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102720W.M
Quant Title : SW846 8260
QLast Update : Tue Oct 27 13:55:07 2020
Response via : Initial Calibration

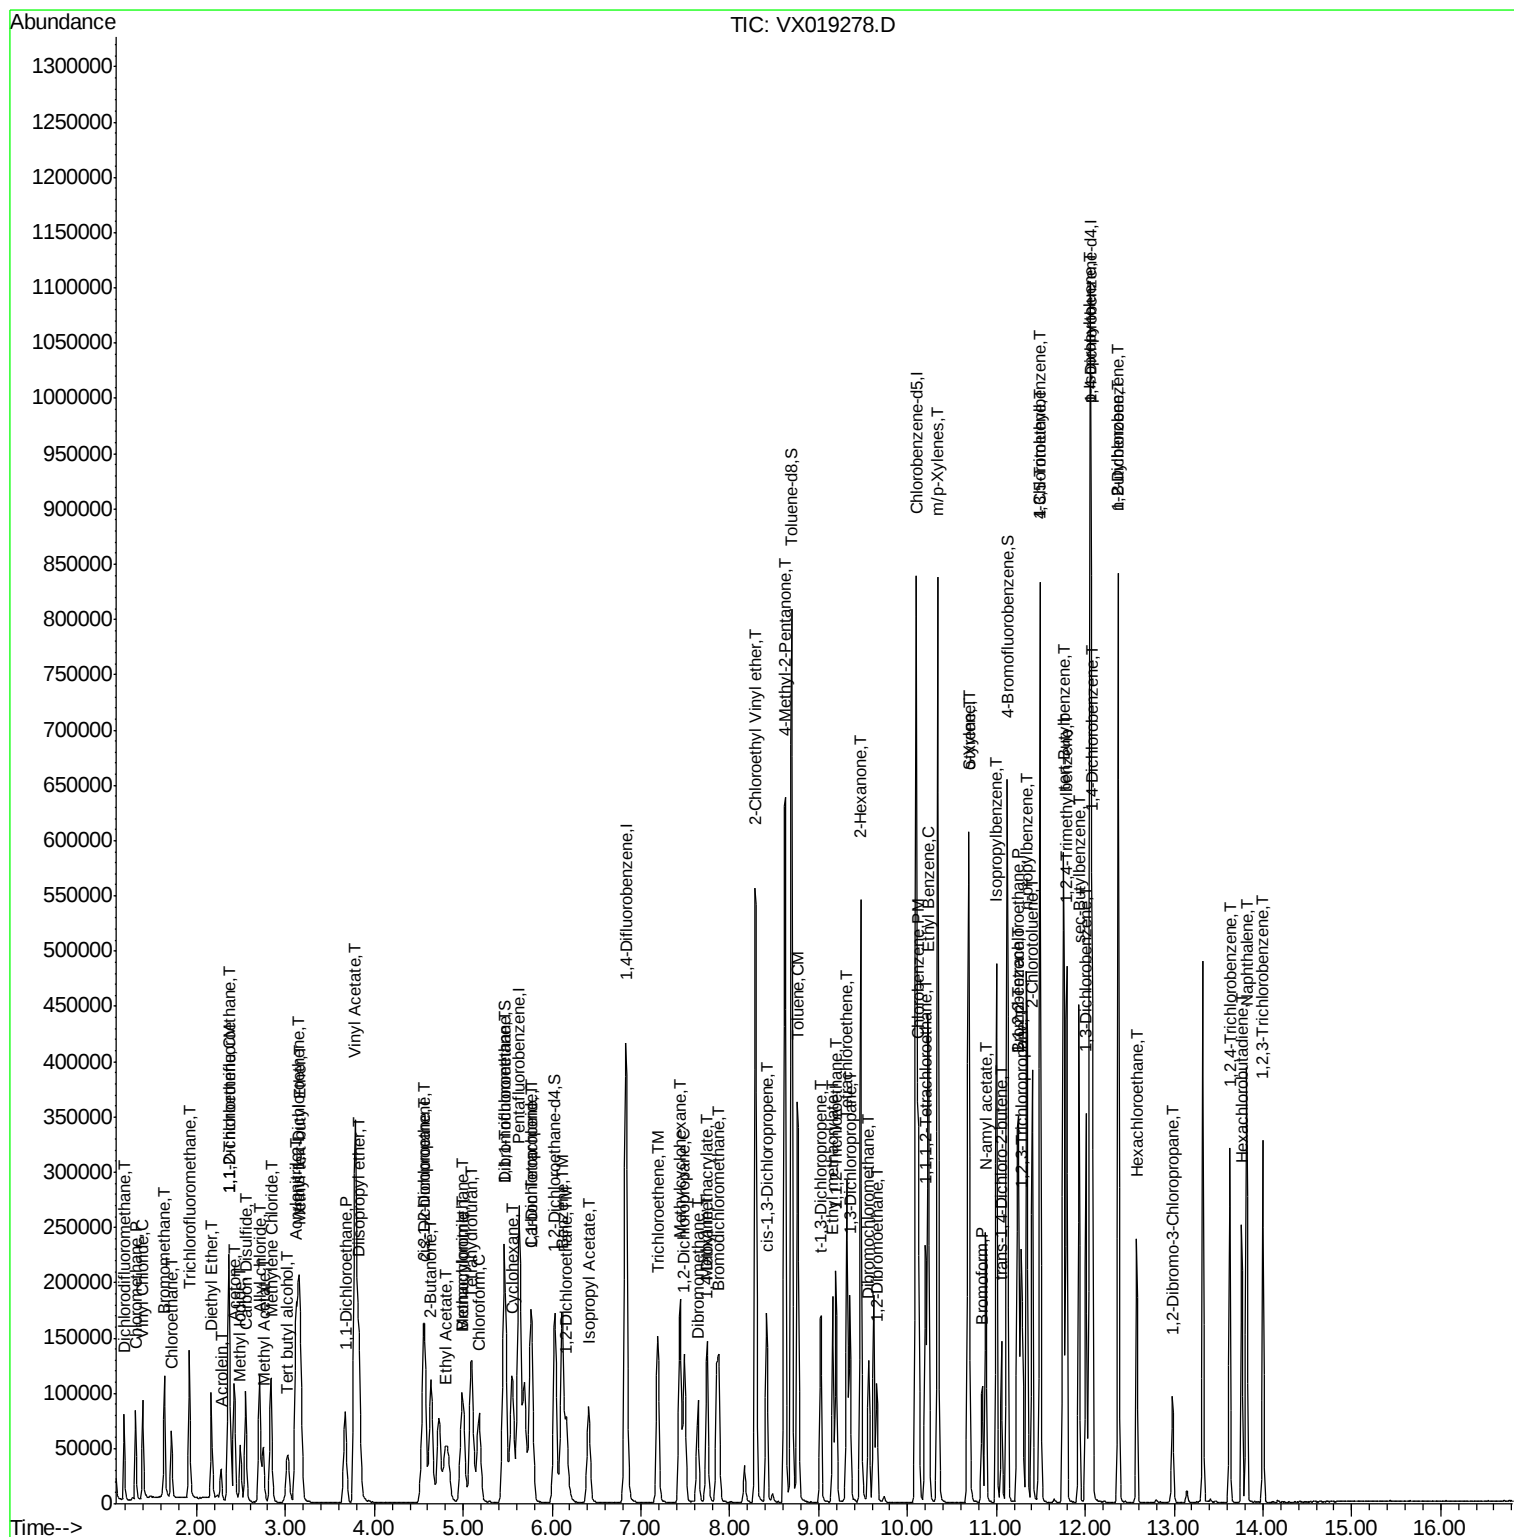



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. 0.00 min

Lab File: VX019278.D

Acq: 04 Nov 2020 18:57

Instrument :

MSVOA_X

ClientSampleId :

VX1106WBSD01

Tgt Ion:168 Resp: 247725

Ion Ratio Lower Upper

168 100


99 57.3 46.6 69.8

Manual Integrations

APPROVED

MMDadoda

11/5/2020 7:02:28 PM



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.63

100000

80000

60000



40000

20000

0

5.50 5.60 5.70

Time-->



#2

Dichlorodifluoromethane

Concen: 19.006 ug/l

RT: 1.18 min Scan# 16

Delta R.T. 0.00 min

Lab File: VX019278.D


Acq: 04 Nov 2020 18:57

Tgt Ion: 85 Resp: 39252

Ion Ratio Lower Upper

85 100

87 31.4 16.6 49.7



Abundance Ion 84.90 (84.60 to 85.60): VX0

Ion 86.90 (86.60 to 87.60): VX0

1.18

50000

40000

30000


20000


10000

0

1.15 1.20 1.25

Time-->





#3

Chloromethane

Concen: 20.469 ug/l

RT: 1.31 min Scan# 37

Delta R.T. 0.00 min

Lab File: VX019278.D

Acq: 04 Nov 2020 18:57

Instrument :

MSVOA_X

ClientSampleId :

VX1106WBSD01

Tgt Ion: 50 Resp: 47227

Ion Ratio Lower Upper

50 100





52 33.4 26.8 40.2

Manual Integrations

APPROVED

MMDadoda

11/5/2020 7:02:28 PM



#4

Vinyl Chloride

Concen: 20.170 ug/l

RT: 1.39 min Scan# 50

Delta R.T. 0.00 min

Lab File: VX019278.D




Acq: 04 Nov 2020 18:57


Tgt Ion: 62 Resp: 53970

Ion Ratio Lower Upper

62 100

64 31.6 25.4 38.0





#5

Bromomethane

Concen: 22.203 ug/l

RT: 1.64 min Scan# 90

Delta R.T. 0.00 min

Lab File: VX019278.D

Acq: 04 Nov 2020 18:57

Instrument :

MSVOA_X

ClientSampleId :

VX1106WBSD01

Tgt Ion: 94 Resp: 40573

Ion Ratio Lower Upper

94 100





96 95.0 76.0 114.0

Manual Integrations

APPROVED

MMDadoda

11/5/2020 7:02:28 PM

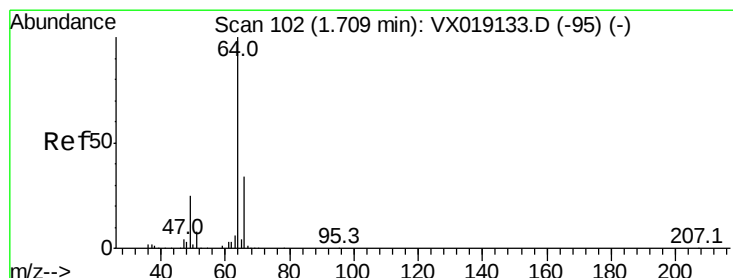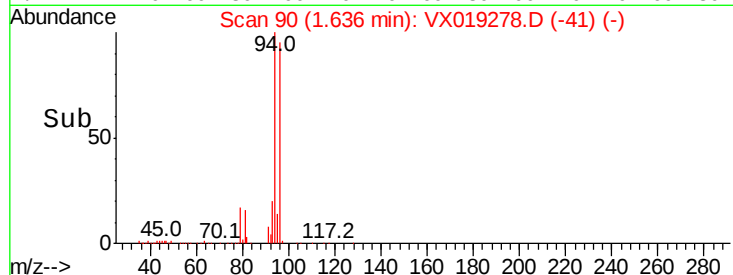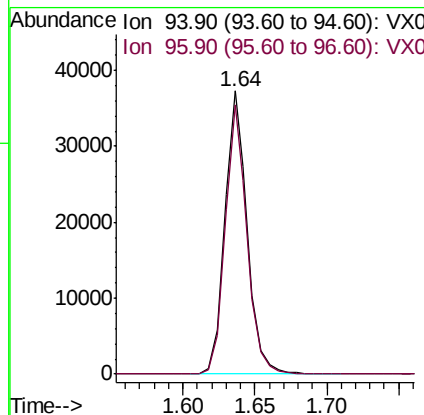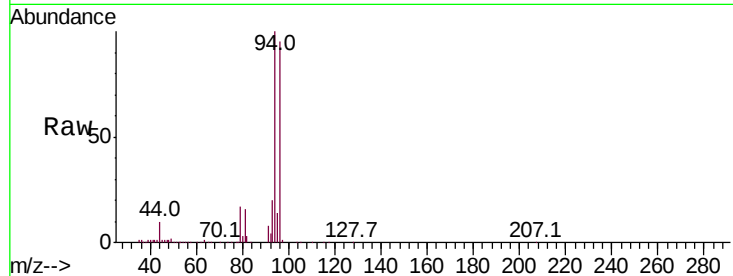

#6

Chloroethane

Concen: 21.153 ug/l

RT: 1.72 min Scan# 103

Delta R.T. 0.01 min

Lab File: VX019278.D




Acq: 04 Nov 2020 18:57


Tgt Ion: 64 Resp: 36137

Ion Ratio Lower Upper

64 100

66 32.3 27.1 40.7

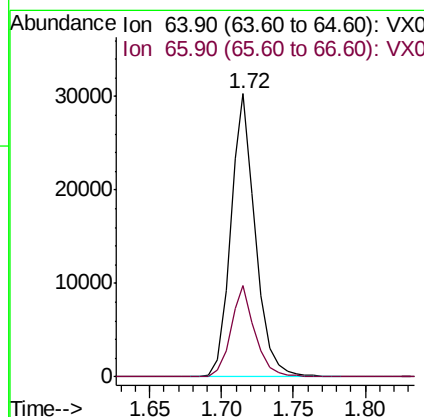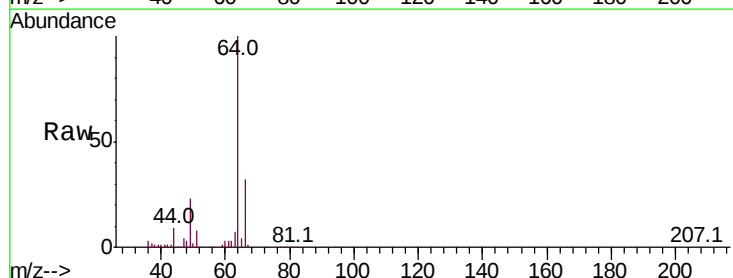



#7





Trichlorofluoromethane
Concen: 19.700 ug/l
RT: 1.92 min Scan# 136
Delta R.T. 0.00 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Instrument :
MSVOA_X
ClientSampleId :
VX1106WBSD01

Tgt Ion	Ratio	Lower	Upper
101	100		
103	61.9	50.0	75.0

Manual Integrations
APPROVED




MMDadoda
11/5/2020 7:02:28 PM

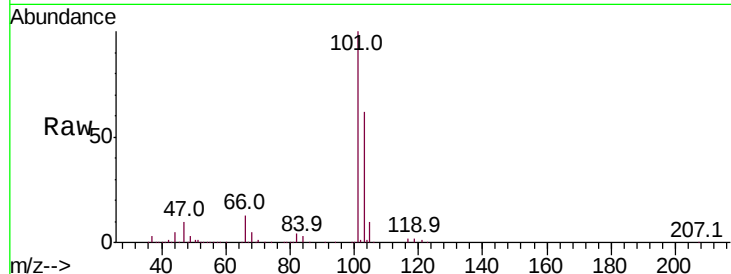


#8

Diethyl Ether
Concen: 20.984 ug/l
RT: 2.17 min Scan# 177
Delta R.T. 0.00 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Tgt Ion	Ratio	Lower	Upper
74	100		
45	86.1	41.0	123.0





#9

1,1,2-Trichlorotrifluoroethane

Concen: 19.595 ug/l

RT: 2.37 min Scan# 210

Delta R.T. 0.00 min

Lab File: VX019278.D

Acq: 04 Nov 2020 18:57

Instrument :

MSVOA_X





ClientSampleId :

VX1106WBSD01

Tgt Ion:	101	Resp:	45657
Ion Ratio	Lower	Upper	
101	100		
85	45.1	35.0	52.4
151	75.5	61.4	92.2

Manual Integrations
APPROVED

MMDadoda
11/5/2020 7:02:28 PM



#10

Methyl Iodide

Concen: 21.690 ug/l




RT: 2.49 min Scan# 230


Delta R.T. 0.00 min

Lab File: VX019278.D

Acq: 04 Nov 2020 18:57

Tgt Ion:	142	Resp:	48268
Ion Ratio	Lower	Upper	
142	100		
127	46.3	36.1	54.1
141	14.3	11.3	16.9





#11





Tert butyl alcohol
Concen: 102.095 ug/l
RT: 3.02 min Scan# 317
Delta R.T. 0.00 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Instrument :
MSVOA_X
ClientSampleId :
VX1106WBSD01

Tgt Ion: 59 Resp: 64422
Ion Ratio Lower Upper
59 100
57 10.5 8.4 12.6

Manual Integrations
APPROVED




MMDadoda
11/5/2020 7:02:28 PM




#12

1,1-Dichloroethene
Concen: 19.326 ug/l
RT: 2.36 min Scan# 208
Delta R.T. 0.00 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Tgt Ion: 96 Resp: 46402
Ion Ratio Lower Upper
96 100
61 160.4 127.7 191.5
98 61.8 52.1 78.1

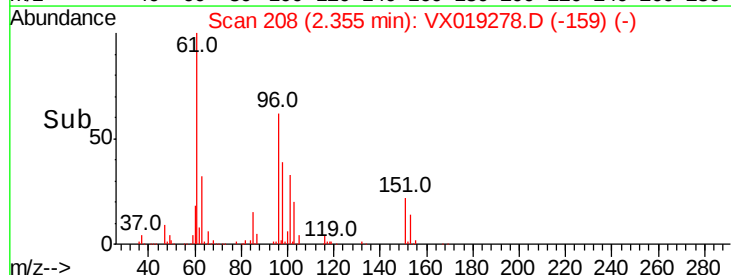

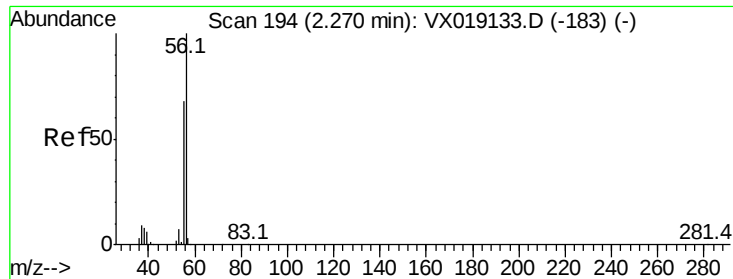

#13

Acrolein

Concen: 83.775 ug/l

RT: 2.28 min Scan# 195

Delta R.T. 0.01 min

Lab File: VX019278.D

Acq: 04 Nov 2020 18:57

Instrument :

MSVOA_X

ClientSampleId :

VX1106WBSD01

Tgt Ion: 56 Resp: 22551





Ion Ratio Lower Upper

56 100

55 69.7 54.7 82.1

Manual Integrations
APPROVED

MMDadoda
11/5/2020 7:02:28 PM

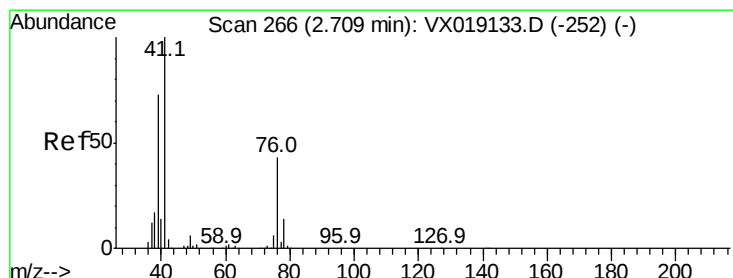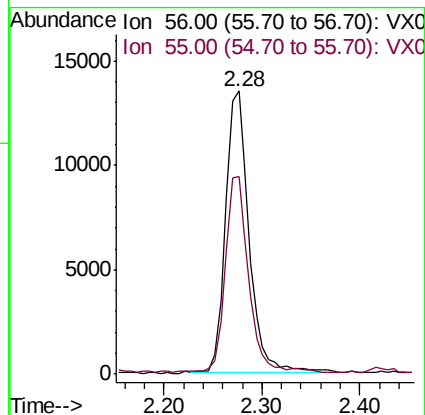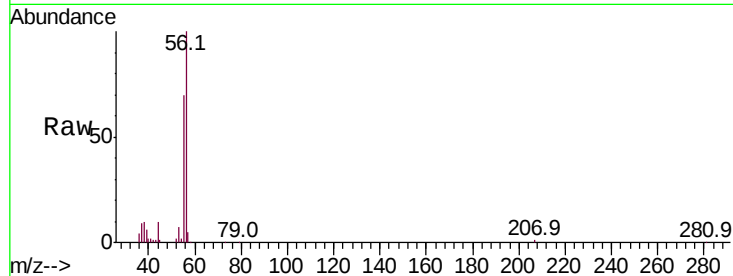

#14

Allyl chloride

Concen: 19.942 ug/l

RT: 2.71 min Scan# 266

Delta R.T. 0.00 min

Lab File: VX019278.D

Acq: 04 Nov 2020 18:57




Tgt Ion: 41 Resp: 72523


Ion Ratio Lower Upper

41 100

39 69.3 55.2 82.8

76 37.6 31.5 47.3

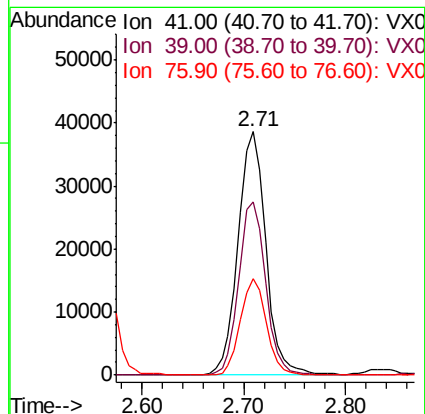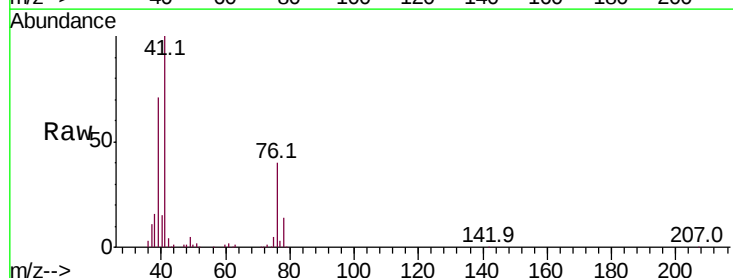



#15

Acrylonitrile

Concen: 104.260 ug/l

RT: 3.12 min Scan# 333

Delta R.T. 0.00 min

Lab File: VX019278.D

Acq: 04 Nov 2020 18:57

Instrument :

MSVOA_X





ClientSampleId :

VX1106WBSD01

Tgt Ion	Ratio	Lower	Upper
53	100		
52	82.2	65.7	98.5
51	36.5	28.4	42.6

Manual Integrations
APPROVED

MMDadoda
11/5/2020 7:02:28 PM



#16

Acetone

Concen: 103.641 ug/l




RT: 2.42 min Scan# 219


Delta R.T. 0.00 min

Lab File: VX019278.D

Acq: 04 Nov 2020 18:57

Tgt Ion	Ratio	Lower	Upper
43	100		
58	33.4	26.3	39.5









#17
Carbon Disulfide
Concen: 18.485 ug/l
RT: 2.55 min Scan# 240
Delta R.T. 0.00 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Instrument :
MSVOA_X
ClientSampleId :
VX1106WBSD01

Tgt Ion	Ratio	Lower	Upper
76	100		
78	9.4	7.3	10.9




Manual Integrations
APPROVED


MMDadoda
11/5/2020 7:02:28 PM

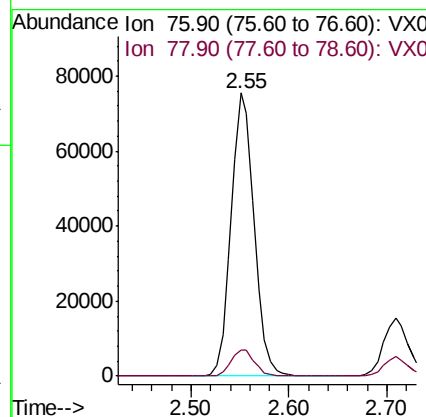

#18
Methyl Acetate
Concen: 21.010 ug/l
RT: 2.75 min Scan# 273
Delta R.T. 0.01 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Tgt Ion	Ratio	Lower	Upper
43	100		
74	27.9	22.6	33.8

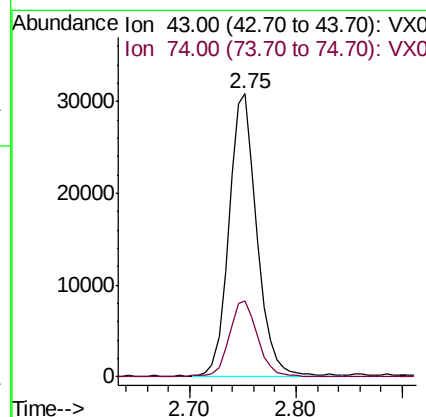







#19
Methyl tert-butyl Ether
Concen: 19.933 ug/l
RT: 3.17 min Scan# 341
Delta R.T. 0.00 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Instrument :
MSVOA_X
ClientSampleId :
VX1106WBSD01

Tgt Ion: 73 Resp: 165825
Ion Ratio Lower Upper
73 100
57 21.6 16.6 25.0




Manual Integrations
APPROVED


MMDadoda
11/5/2020 7:02:28 PM



#20
Methylene Chloride
Concen: 19.502 ug/l
RT: 2.83 min Scan# 286
Delta R.T. -0.01 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Tgt Ion: 84 Resp: 53959
Ion Ratio Lower Upper
84 100
49 117.8 86.8 130.2
51 35.8 27.3 40.9
86 63.9 50.6 76.0





#21

trans-1,2-Dichloroethene

Concen: 19.075 ug/l

RT: 3.14 min Scan# 337

Delta R.T. 0.00 min

Lab File: VX019278.D

Acq: 04 Nov 2020 18:57

Instrument :

MSVOA_X





ClientSampleId :

VX1106WBSD01

Tgt Ion:	96	Resp:	52709
Ion Ratio	Lower	Upper	
96	100		
61	134.6	104.2	156.4
98	60.6	51.3	76.9

Manual Integrations
APPROVED

MMDadoda
11/5/2020 7:02:28 PM

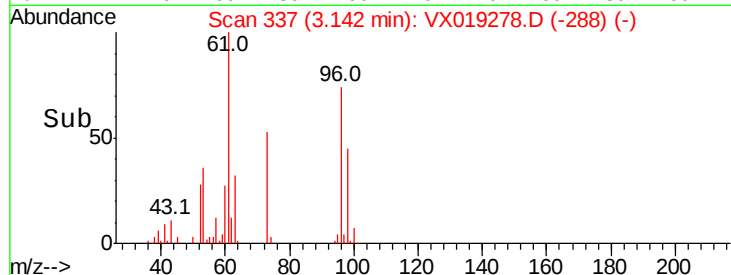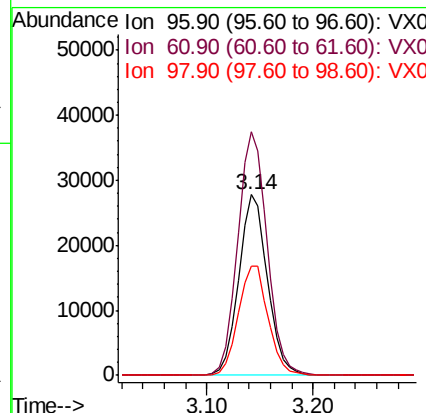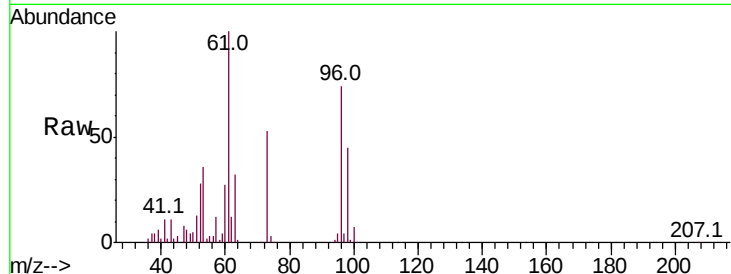

#22

Diisopropyl ether

Concen: 21.103 ug/l




RT: 3.82 min Scan# 449


Delta R.T. 0.00 min

Lab File: VX019278.D

Acq: 04 Nov 2020 18:57

Tgt Ion:	45	Resp:	153001
Ion Ratio	Lower	Upper	
45	100		
43	76.3	56.2	84.4
87	30.9	26.2	39.2
59	13.0	10.1	15.1

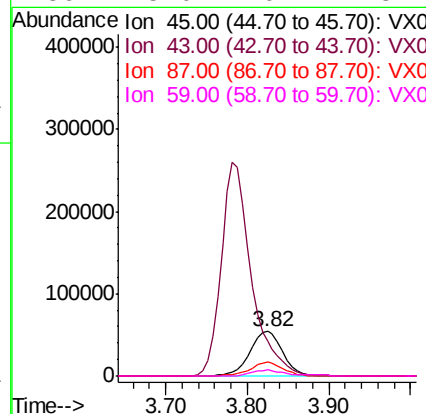

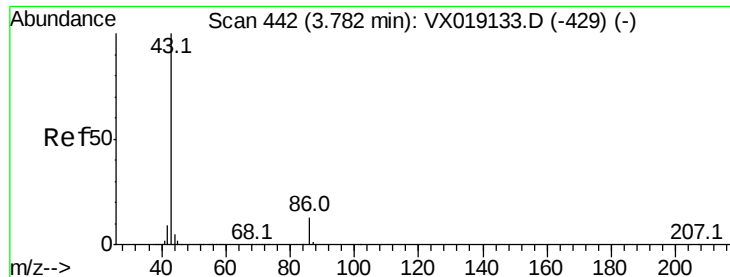

#23

Vinyl Acetate

Concen: 103.882 ug/l

RT: 3.78 min Scan# 442

Delta R.T. 0.00 min

Lab File: VX019278.D

Acq: 04 Nov 2020 18:57

Instrument :

MSVOA_X

ClientSampleId :

VX1106WBSD01

Tgt Ion: 43 Resp: 671630

Ion Ratio Lower Upper

43 100


86 12.3 10.4 15.6

Manual Integrations

APPROVED

MMDadoda

11/5/2020 7:02:28 PM

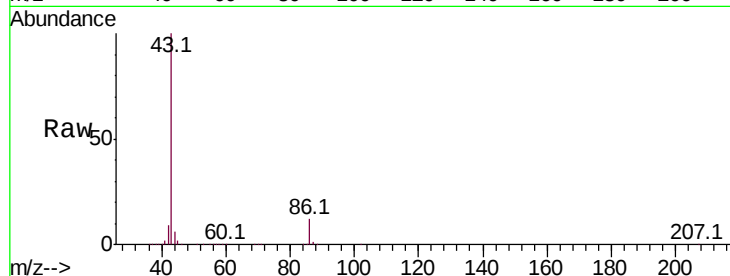

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 86.00 (85.70 to 86.70): VX0

300000

250000

200000

150000



100000

50000

0

3.60 3.70 3.80 3.90 4.00

Time-->

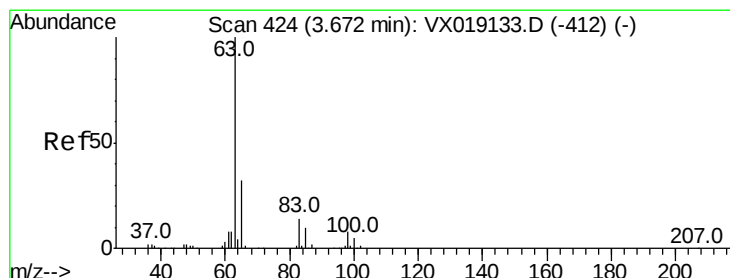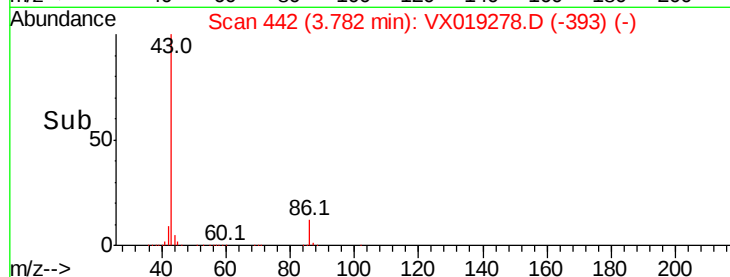

#24

1,1-Dichloroethane

Concen: 20.516 ug/l

RT: 3.67 min Scan# 424

Delta R.T. 0.00 min

Lab File: VX019278.D

Acq: 04 Nov 2020 18:57


Tgt Ion: 63 Resp: 92868

Ion Ratio Lower Upper

63 100

98 7.6 3.8 11.4

100 4.8 2.4 7.2

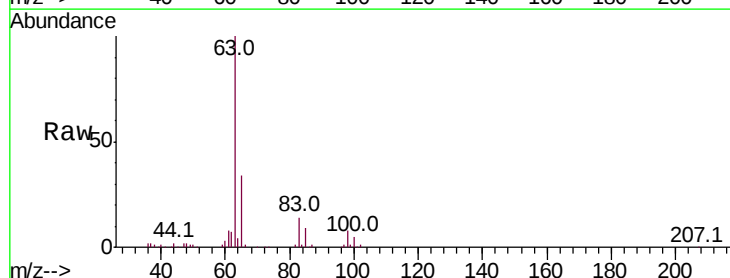

Abundance Ion 62.90 (62.60 to 63.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

Ion 99.90 (99.60 to 100.60): VX0

50000

40000

30000


20000


10000

0

3.60 3.70 3.80

Time-->

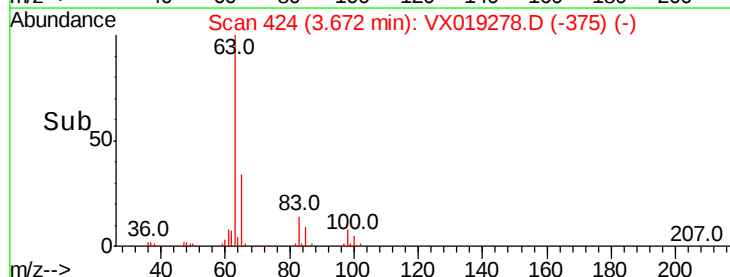



#25

2-Butanone

Concen: 105.044 ug/l

RT: 4.64 min Scan# 582

Delta R.T. 0.00 min

Lab File: VX019278.D

Acq: 04 Nov 2020 18:57

Instrument :

MSVOA_X

ClientSampleId :

VX1106WBSD01

Tgt Ion: 43 Resp: 182457

Ion Ratio Lower Upper

43 100





72 28.6 24.6 36.8

Manual Integrations

APPROVED

MMDadoda

11/5/2020 7:02:28 PM



#26

2,2-Dichloropropane

Concen: 19.111 ug/l

RT: 4.55 min Scan# 568

Delta R.T. 0.00 min

Lab File: VX019278.D




Acq: 04 Nov 2020 18:57


Tgt Ion: 77 Resp: 81327

Ion Ratio Lower Upper

77 100

97 22.4 11.4 34.1









#27
 cis-1,2-Dichloroethene
 Concen: 19.355 ug/l
 RT: 4.57 min Scan# 571
 Delta R.T. 0.01 min
 Lab File: VX019278.D
 Acq: 04 Nov 2020 18:57

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1106WBSD01

Tgt Ion	Ratio	Resp	Lower	Upper
96	100	59765		
61	144.3	0.0	278.8	
98	64.1	0.0	130.2	




Manual Integrations
 APPROVED


MMDadoda
 11/5/2020 7:02:28 PM

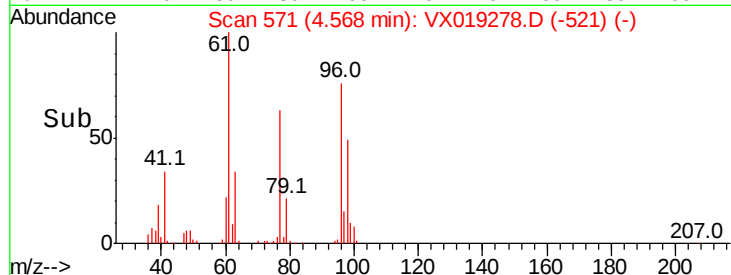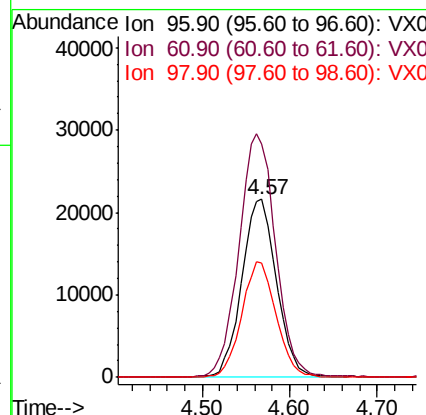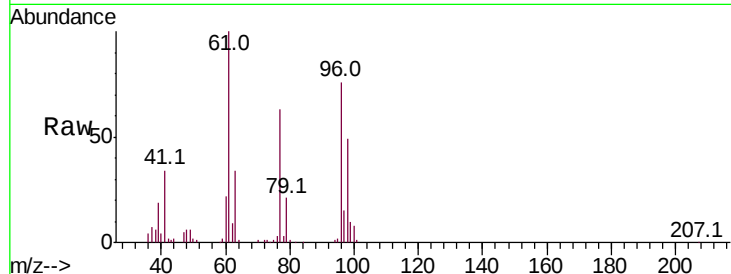

#28
 Bromochloromethane
 Concen: 20.691 ug/l
 RT: 4.98 min Scan# 639
 Delta R.T. 0.00 min
 Lab File: VX019278.D
 Acq: 04 Nov 2020 18:57

Tgt Ion	Ratio	Resp	Lower	Upper
49	100	42579		
129	1.8	0.0	4.4	
130	81.1	71.3	106.9	

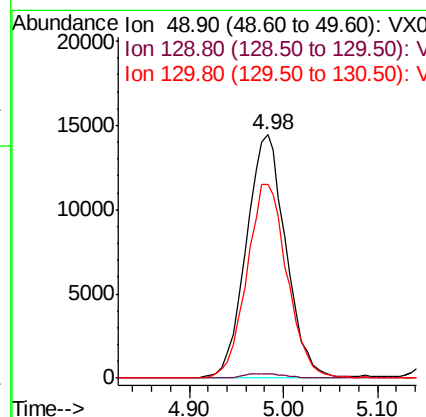







#29
Tetrahydrofuran
Concen: 106.536 ug/l
RT: 5.09 min Scan# 657
Delta R.T. 0.01 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Instrument :
MSVOA_X
ClientSampleId :
VX1106WBSD01

Tgt Ion	Ratio	Lower	Upper
42	100		
72	51.8	42.6	63.8
71	48.1	39.7	59.5




Manual Integrations
APPROVED


MMDadoda
11/5/2020 7:02:28 PM

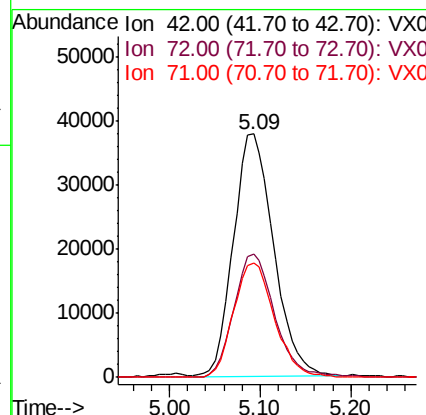

#30
Chloroform
Concen: 20.128 ug/l
RT: 5.18 min Scan# 671
Delta R.T. 0.00 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Tgt Ion	Ratio	Lower	Upper
83	100		
85	65.8	51.9	77.9

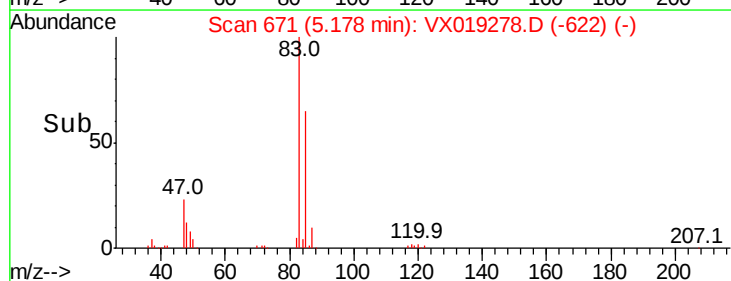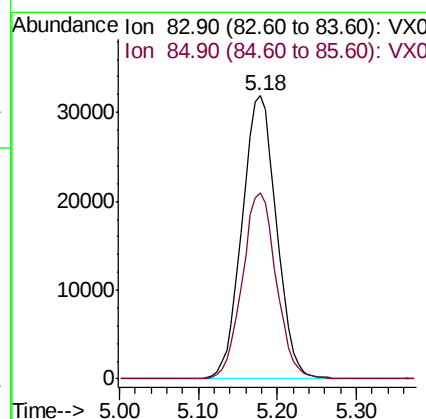







#31
Cyclohexane
Concen: 19.714 ug/l
RT: 5.55 min Scan# 732
Delta R.T. 0.00 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Instrument :
MSVOA_X
ClientSampleId :
VX1106WBSD01

Tgt Ion: 56 Resp: 79611
Ion Ratio Lower Upper
56 100
69 33.2 25.9 38.9
84 90.9 73.4 110.2




Manual Integrations
APPROVED


MMDadoda
11/5/2020 7:02:28 PM



#32
1,1,1-Trichloroethane
Concen: 20.102 ug/l
RT: 5.46 min Scan# 718
Delta R.T. 0.00 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Tgt Ion: 97 Resp: 87813
Ion Ratio Lower Upper
97 100
99 63.5 51.7 77.5
61 43.8 34.2 51.2









#33
 1,2-Dichloroethane-d4
 Concen: 50.872 ug/l
 RT: 6.03 min Scan# 811
 Delta R.T. 0.00 min
 Lab File: VX019278.D
 Acq: 04 Nov 2020 18:57

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1106WBSD01

Tgt Ion	Ratio	Resp	Lower	Upper
65	100	162523		
67	51.3	0.0	103.0	




Manual Integrations
 APPROVED


MMDadoda
 11/5/2020 7:02:28 PM

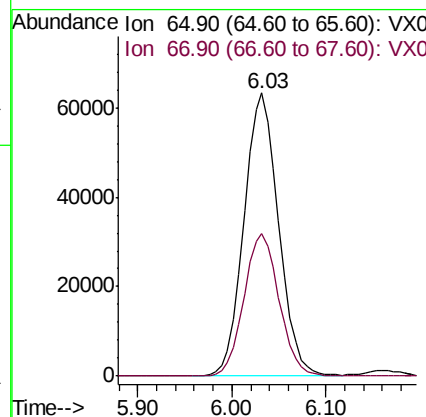

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.83 min Scan# 942
 Delta R.T. 0.00 min
 Lab File: VX019278.D
 Acq: 04 Nov 2020 18:57

Tgt Ion	Ratio	Resp	Lower	Upper
114	100	423226		
63	21.3	0.0	38.8	
88	16.3	0.0	34.2	

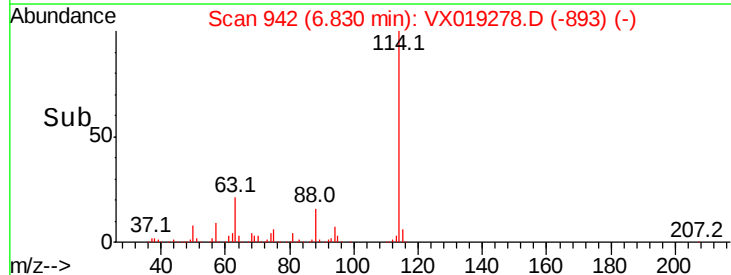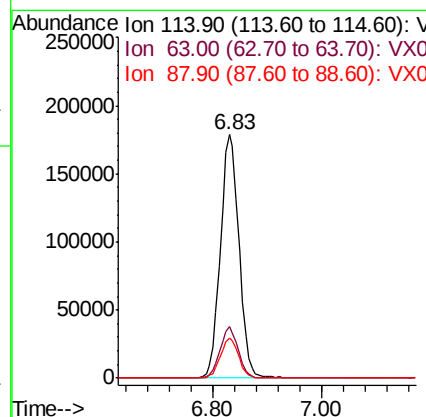

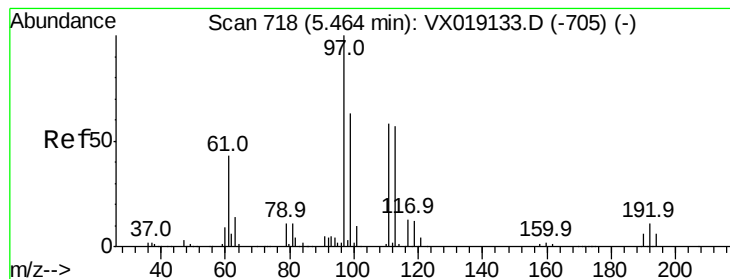

#35

Dibromofluoromethane

Concen: 47.284 ug/l

RT: 5.46 min Scan# 718

Delta R.T. 0.00 min

Lab File: VX019278.D

Acq: 04 Nov 2020 18:57

Instrument :

MSVOA_X


ClientSampleId :

VX1106WBSD01




Tgt Ion:	113	Resp:	125702
Ion Ratio	Lower	Upper	
113	100		
111	102.0	82.3	123.5
192	19.1	16.2	24.2

Manual Integrations
APPROVED

MMDadoda
11/5/2020 7:02:28 PM

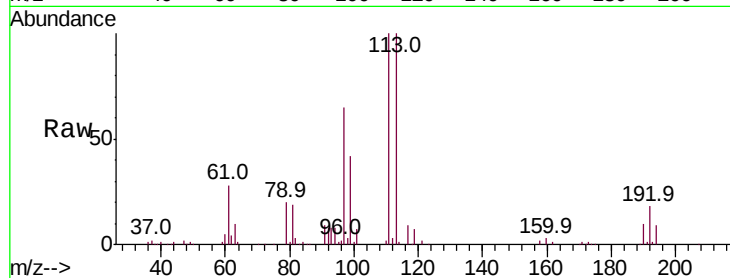

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V

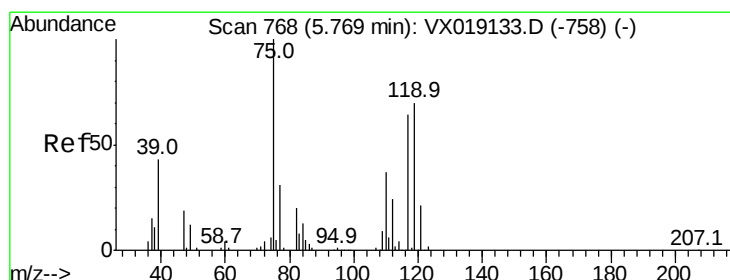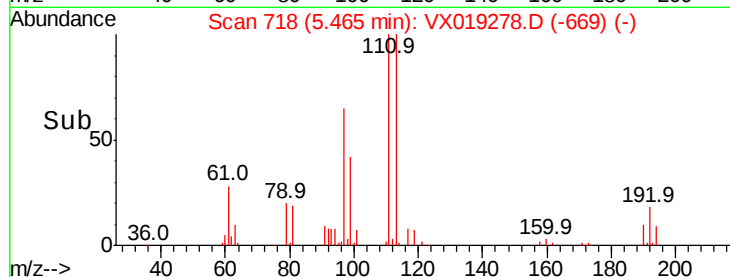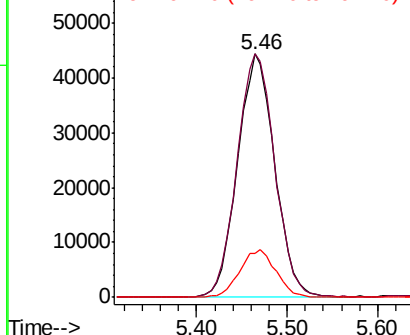

#36

1,1-Dichloropropene

Concen: 18.886 ug/l


RT: 5.77 min Scan# 768

Delta R.T. 0.00 min



Lab File: VX019278.D


Acq: 04 Nov 2020 18:57

Tgt Ion:	75	Resp:	73809
Ion Ratio	Lower	Upper	
75	100		
110	35.3	18.3	54.9
77	30.3	24.9	37.3

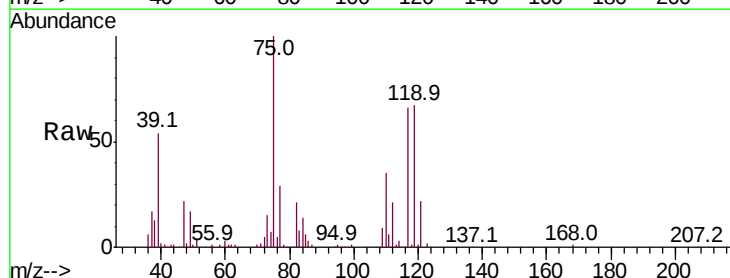

Abundance Ion 74.90 (74.60 to 75.60): VX0
Ion 109.90 (109.60 to 110.60): V
Ion 76.90 (76.60 to 77.60): VX0

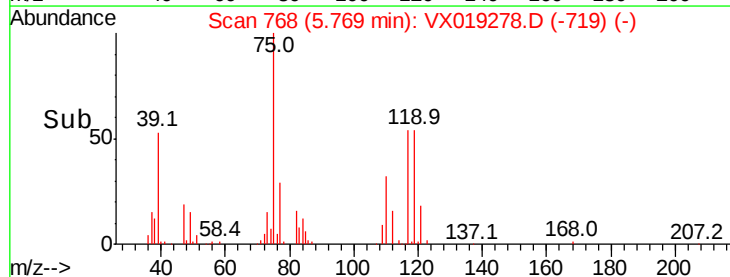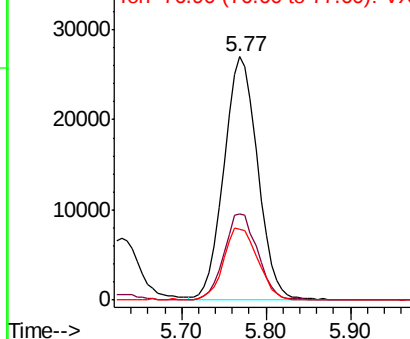

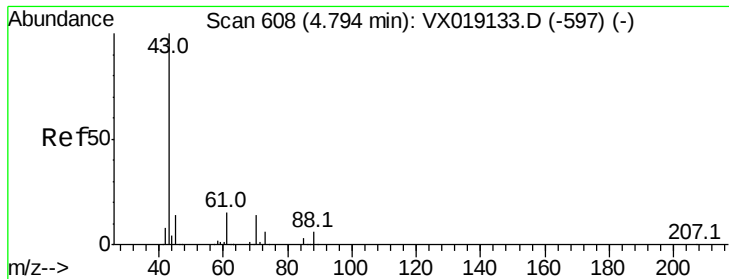





#37
Ethyl Acetate
Concen: 19.661 ug/l
RT: 4.79 min Scan# 608
Delta R.T. 0.00 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Instrument :
MSVOA_X
ClientSampleId :
VX1106WBSD01

Tgt Ion	Ratio	Lower	Upper
43	100		
61	15.2	12.5	18.7
70	12.5	10.5	15.7




Manual Integrations
APPROVED


MMDadoda
11/5/2020 7:02:28 PM

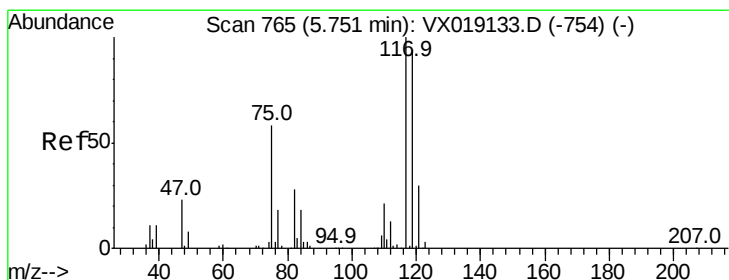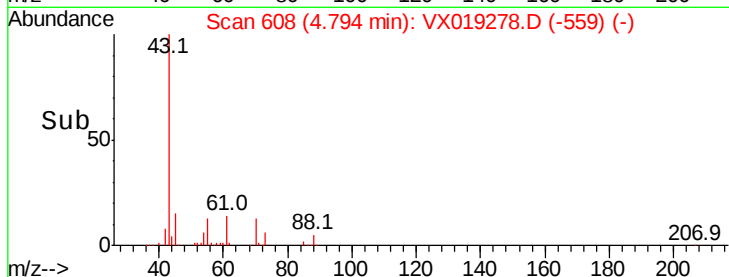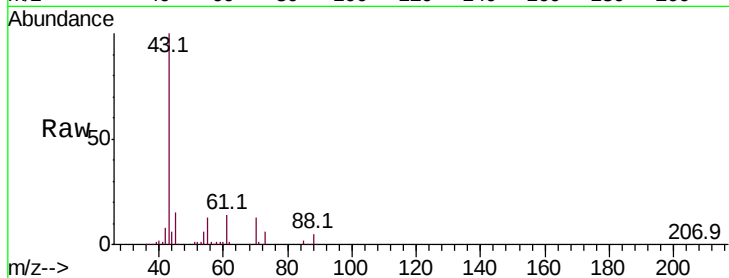

#38
Carbon Tetrachloride
Concen: 18.403 ug/l
RT: 5.76 min Scan# 766
Delta R.T. 0.01 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Tgt Ion	Ratio	Lower	Upper
117	100		
119	94.5	75.0	112.6
121	30.9	23.9	35.9

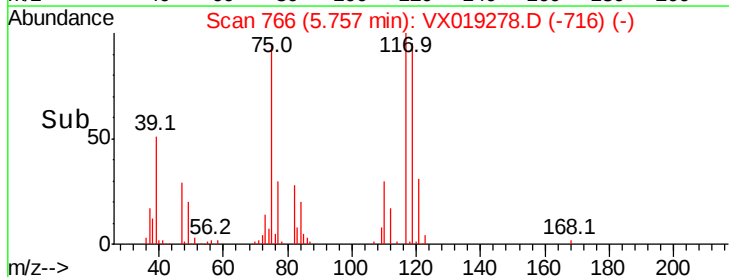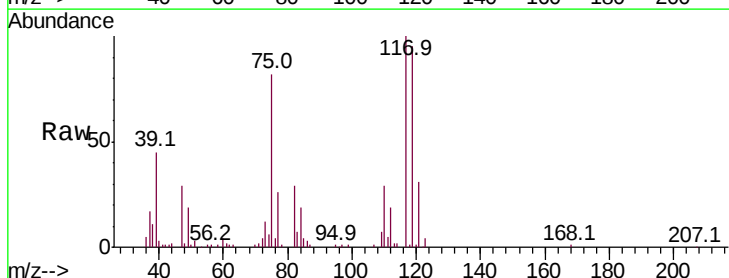







#39
Methylcyclohexane
Concen: 18.275 ug/l
RT: 7.44 min Scan# 1042
Delta R.T. 0.00 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Instrument :
MSVOA_X
ClientSampleId :
VX1106WBSD01

Tgt Ion	Ratio	Lower	Upper
83	100		
55	71.9	57.0	85.6
98	46.7	40.5	60.7




Manual Integrations
APPROVED


MMDadoda
11/5/2020 7:02:28 PM



#40
Benzene
Concen: 19.330 ug/l
RT: 6.11 min Scan# 824
Delta R.T. 0.00 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Tgt Ion	Ratio	Lower	Upper
78	100		
77	23.7	18.7	28.1









#41
Methacrylonitrile
Concen: 19.725 ug/l
RT: 5.00 min Scan# 642
Delta R.T. 0.00 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Instrument :
MSVOA_X
ClientSampleId :
VX1106WBSD01

Tgt Ion	Ion	Ratio	Lower	Upper
41	100			
39	55.4	44.4	66.6	
67	80.3	66.4	99.6	
52	33.5	26.2	39.4	




Manual Integrations
APPROVED


MMDadoda
11/5/2020 7:02:28 PM

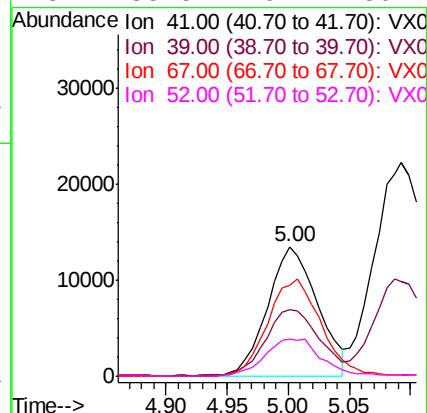

#42
1,2-Dichloroethane
Concen: 19.811 ug/l
RT: 6.17 min Scan# 833
Delta R.T. 0.01 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Tgt Ion	Ion	Ratio	Lower	Upper
62	100			
98	9.4	0.0	19.0	

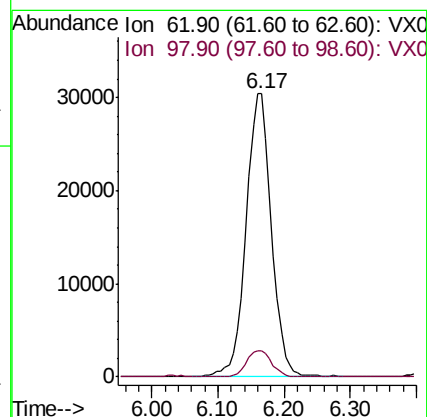







#43
Isopropyl Acetate
Concen: 19.308 ug/l
RT: 6.41 min Scan# 873
Delta R.T. 0.00 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Instrument :
MSVOA_X
ClientSampleId :
VX1106WBSD01

Tgt Ion	Ratio	Lower	Upper
43	100		
61	22.4	17.8	26.6
87	15.3	12.6	19.0




Manual Integrations
APPROVED


MMDadoda
11/5/2020 7:02:28 PM

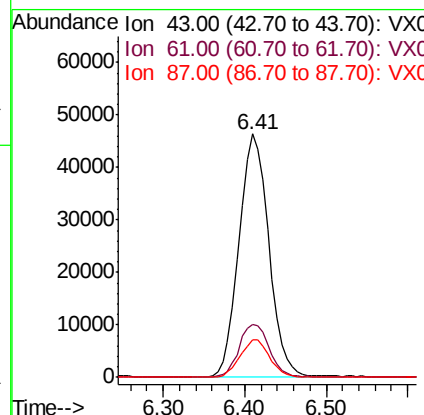

#44
Trichloroethene
Concen: 18.152 ug/l
RT: 7.19 min Scan# 1001
Delta R.T. 0.00 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Tgt Ion	Ratio	Lower	Upper
130	100		
95	103.8	0.0	192.0

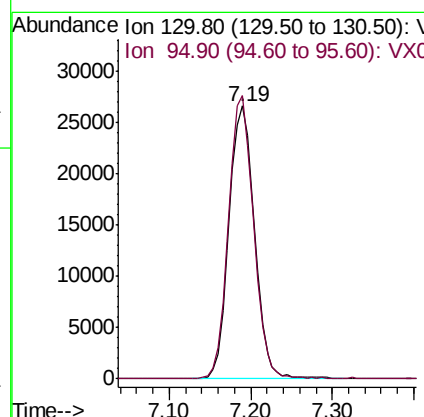







#45
 1,2-Dichloropropane
 Concen: 20.248 ug/l
 RT: 7.49 min Scan# 1050
 Delta R.T. 0.00 min
 Lab File: VX019278.D
 Acq: 04 Nov 2020 18:57

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1106WBSD01

Tgt Ion: 63 Resp: 54955
 Ion Ratio Lower Upper
 63 100
 65 31.7 25.2 37.8




Manual Integrations
 APPROVED


MMDadoda
 11/5/2020 7:02:28 PM



#46
 Dibromomethane
 Concen: 18.923 ug/l
 RT: 7.63 min Scan# 1074
 Delta R.T. -0.01 min
 Lab File: VX019278.D
 Acq: 04 Nov 2020 18:57

Tgt Ion: 93 Resp: 37979
 Ion Ratio Lower Upper
 93 100
 95 81.4 67.0 100.6
 174 95.3 81.7 122.5









#47
Bromodichloromethane
Concen: 19.205 ug/l
RT: 7.87 min Scan# 1113
Delta R.T. 0.00 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Instrument :
MSVOA_X
ClientSampleId :
VX1106WBSD01

Tgt Ion	Ratio	Lower	Upper
83	100		
85	61.8	51.2	76.8
127	8.1	7.1	10.7




Manual Integrations
APPROVED


MMDadoda
11/5/2020 7:02:28 PM



#48
Methyl methacrylate
Concen: 19.547 ug/l
RT: 7.74 min Scan# 1092
Delta R.T. 0.00 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Tgt Ion	Ratio	Lower	Upper
41	100		
69	91.6	75.5	113.3
39	60.6	48.9	73.3









#49
1,4-Dioxane
Concen: 384.270 ug/l
RT: 7.73 min Scan# 1090
Delta R.T. 0.01 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Instrument :
MSVOA_X
ClientSampleId :
VX1106WBSD01

Tgt Ion	Ratio	Lower	Upper
88	100		
43	29.7	23.0	34.6
58	67.5	52.2	78.2




Manual Integrations
APPROVED


MMDadoda
11/5/2020 7:02:28 PM

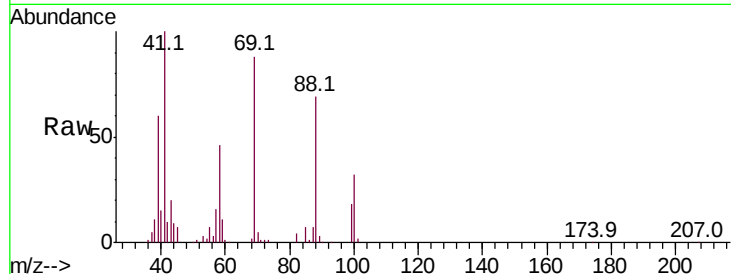

#50
Toluene-d8
Concen: 47.973 ug/l
RT: 8.70 min Scan# 1248
Delta R.T. 0.00 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Tgt Ion	Ratio	Lower	Upper
98	100		
100	65.7	53.0	79.6









#51
4-Methyl-2-Pentanone
Concen: 103.215 ug/l
RT: 8.62 min Scan# 1235
Delta R.T. -0.01 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Instrument :
MSVOA_X
ClientSampleId :
VX1106WBSD01

Tgt Ion: 43 Resp: 360439
Ion Ratio Lower Upper
43 100
58 43.0 35.0 52.4




Manual Integrations
APPROVED


MMDadoda
11/5/2020 7:02:28 PM

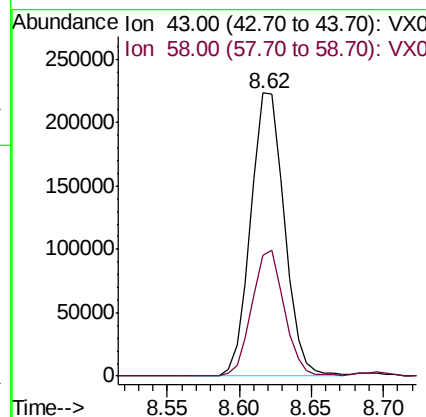

#52
Toluene
Concen: 18.983 ug/l
RT: 8.76 min Scan# 1259
Delta R.T. 0.00 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Tgt Ion: 92 Resp: 135478
Ion Ratio Lower Upper
92 100
91 173.7 136.3 204.5

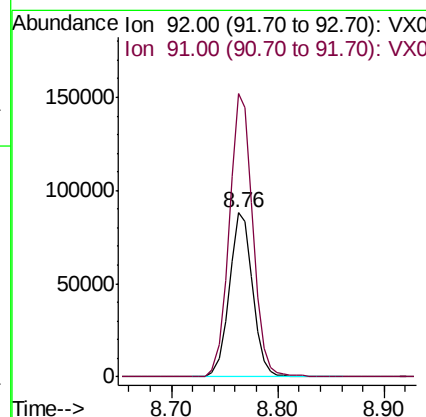







#53
t-1,3-Dichloropropene
Concen: 17.841 ug/l
RT: 9.02 min Scan# 1302
Delta R.T. 0.00 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Instrument :
MSVOA_X
ClientSampleId :
VX1106WBSD01

Tgt Ion: 75 Resp: 80612
Ion Ratio Lower Upper
75 100
77 32.3 25.4 38.0




Manual Integrations
APPROVED


MMDadoda
11/5/2020 7:02:28 PM

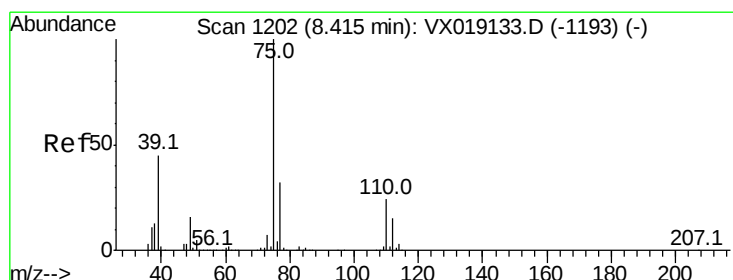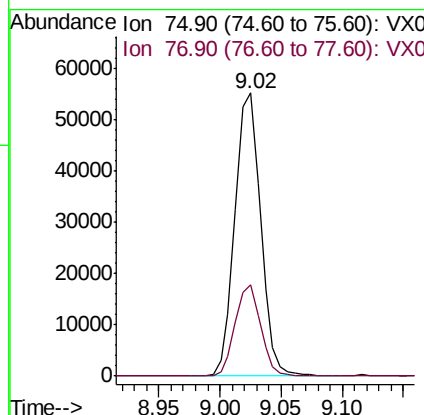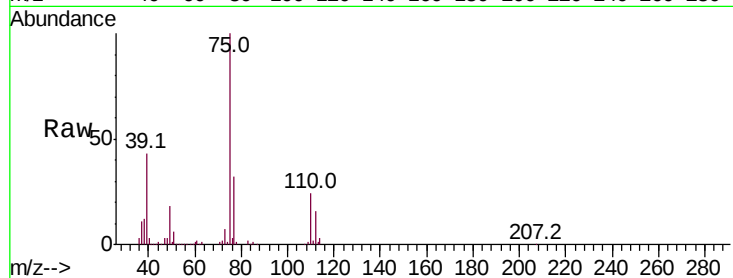

#54
cis-1,3-Dichloropropene
Concen: 18.493 ug/l
RT: 8.42 min Scan# 1202
Delta R.T. 0.00 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Tgt Ion: 75 Resp: 87864
Ion Ratio Lower Upper
75 100
77 32.0 25.5 38.3
39 46.4 36.2 54.2

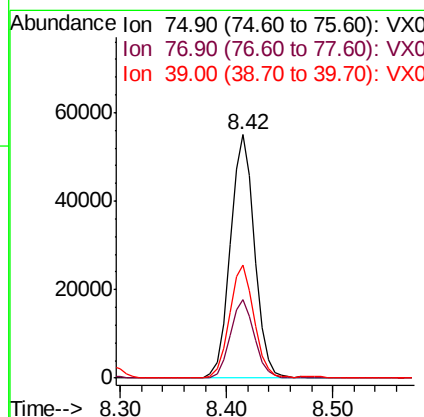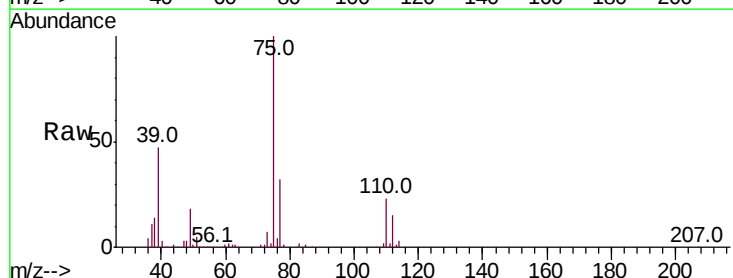







#55
 1,1,2-Trichloroethane
 Concen: 19.381 ug/l
 RT: 9.20 min Scan# 1330
 Delta R.T. 0.00 min
 Lab File: VX019278.D
 Acq: 04 Nov 2020 18:57

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1106WBSD01

Tgt Ion	Ratio	Lower	Upper
97	100		
83	83.8	67.2	100.8
85	52.3	44.6	67.0
99	64.5	49.4	74.0




Manual Integrations
 APPROVED


MMDadoda
 11/5/2020 7:02:28 PM

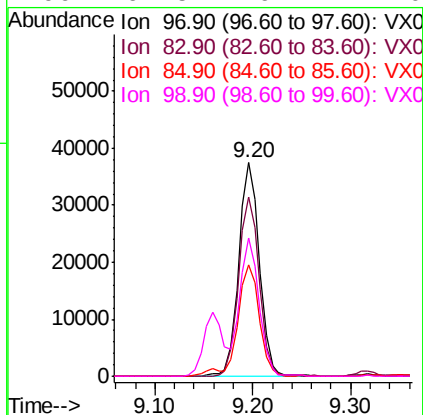

#56
 Ethyl methacrylate
 Concen: 18.872 ug/l
 RT: 9.16 min Scan# 1324
 Delta R.T. 0.00 min
 Lab File: VX019278.D
 Acq: 04 Nov 2020 18:57

Tgt Ion	Ratio	Lower	Upper
69	100		
41	60.9	46.5	69.7
39	36.1	27.6	41.4

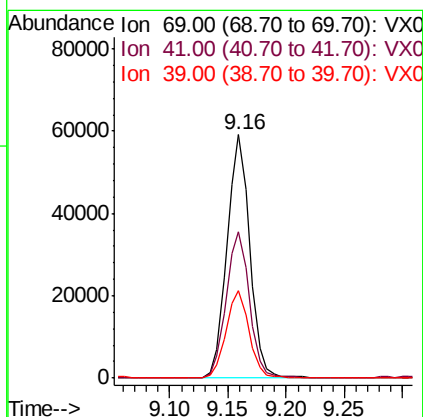



#57

1,3-Dichloropropane

Concen: 19.470 ug/l

RT: 9.35 min Scan# 1356

Delta R.T. 0.00 min

Lab File: VX019278.D

Acq: 04 Nov 2020 18:57

Instrument :

MSVOA_X

ClientSampleId :

VX1106WBSD01

Tgt Ion: 76 Resp: 92567

Ion Ratio Lower Upper

76 100


78 32.5 25.9 38.9

Manual Integrations

APPROVED

MMDadoda

11/5/2020 7:02:28 PM



Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0

9.35

60000



40000

20000

0

9.30 9.40 9.50

Time-->

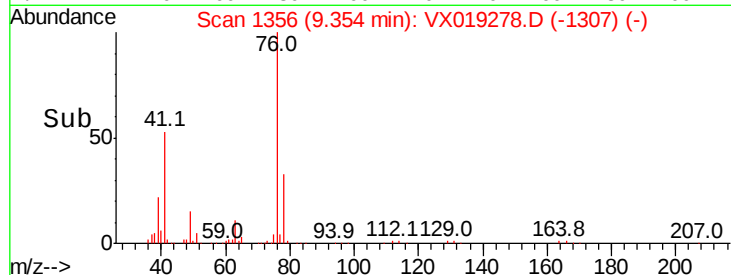

#58

2-Chloroethyl Vinyl ether

Concen: 95.817 ug/l

RT: 8.29 min Scan# 1181

Delta R.T. -0.01 min

Lab File: VX019278.D


Acq: 04 Nov 2020 18:57

Tgt Ion: 63 Resp: 228238

Ion Ratio Lower Upper

63 100

106 29.4 25.1 37.7



Abundance Ion 62.90 (62.60 to 63.60): VX0

Ion 105.90 (105.60 to 106.60): V

8.29

150000


100000


50000

0

8.20 8.30 8.40

Time-->









#59
2-Hexanone
Concen: 103.126 ug/l
RT: 9.47 min Scan# 1375
Delta R.T. 0.00 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Instrument :
MSVOA_X
ClientSampleId :
VX1106WBSD01

Tgt Ion: 43 Resp: 274134
Ion Ratio Lower Upper
43 100
58 59.4 30.5 91.5




Manual Integrations
APPROVED


MMDadoda
11/5/2020 7:02:28 PM

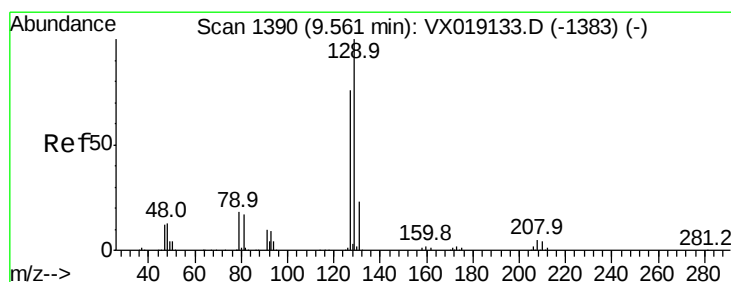

#60
Dibromochloromethane
Concen: 18.285 ug/l
RT: 9.56 min Scan# 1390
Delta R.T. 0.00 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Tgt Ion: 129 Resp: 55958
Ion Ratio Lower Upper
129 100
127 77.1 38.6 115.8





#61

1,2-Dibromoethane

Concen: 18.901 ug/l

RT: 9.65 min Scan# 1405

Delta R.T. 0.00 min

Lab File: VX019278.D

Acq: 04 Nov 2020 18:57

Instrument :

MSVOA_X

ClientSampleId :

VX1106WBSD01

Tgt Ion:107 Resp: 56994

Ion Ratio Lower Upper

107 100





109 93.4 75.9 113.9

Manual Integrations

APPROVED

MMDadoda

11/5/2020 7:02:28 PM

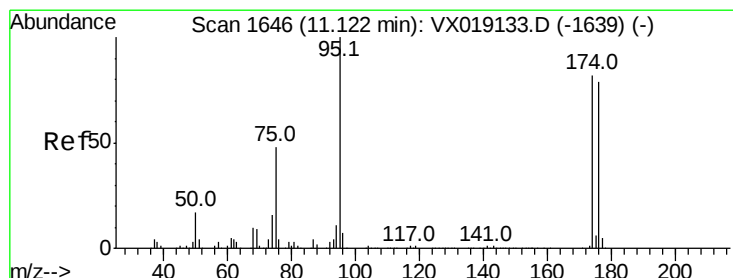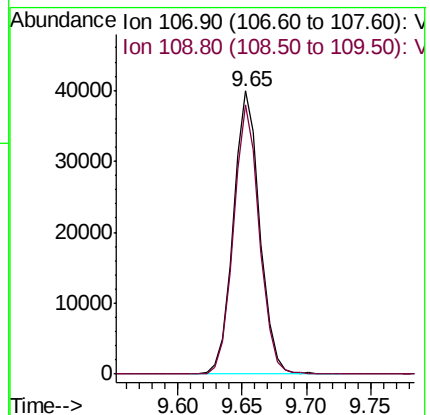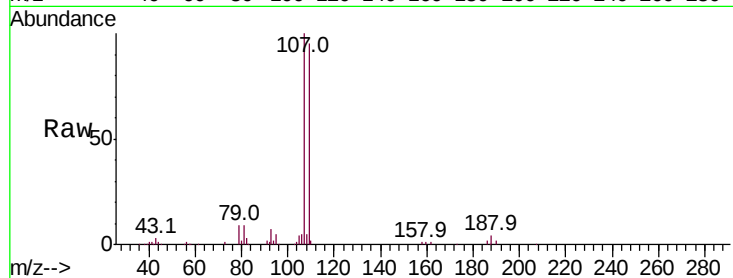

#62

4-Bromofluorobenzene

Concen: 47.248 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.00 min

Lab File: VX019278.D

Acq: 04 Nov 2020 18:57




Tgt Ion: 95 Resp: 179312


Ion Ratio Lower Upper

95 100

174 75.6 0.0 156.0

176 73.1 0.0 149.8

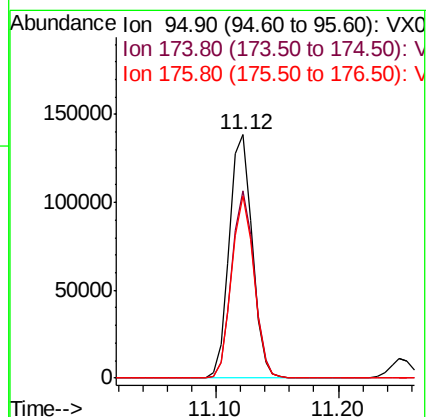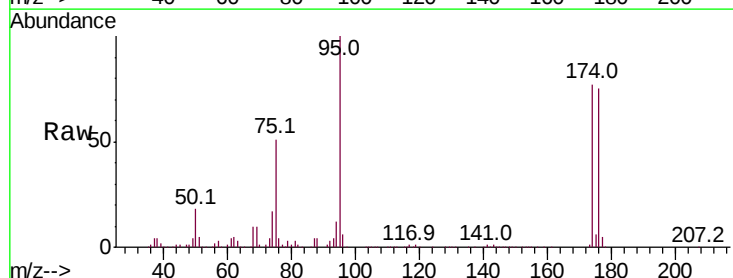







#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. 0.00 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Instrument :
MSVOA_X
ClientSampleId :
VX1106WBSD01

Tgt Ion	Ratio	Resp Lower	Resp Upper
117	100		
82	56.4	43.6	65.4
119	32.2	25.5	38.3

Manual Integrations
APPROVED

MMDadoda
11/5/2020 7:02:28 PM

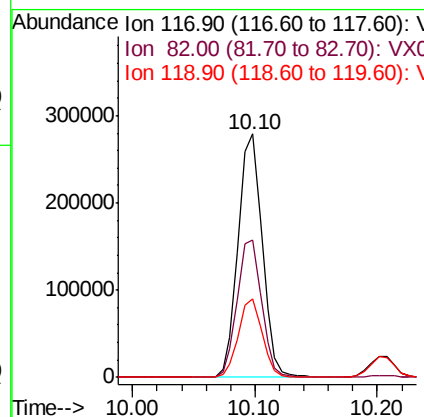

#64
Tetrachloroethene
Concen: 18.733 ug/l
RT: 9.32 min Scan# 1350
Delta R.T. 0.00 min
Lab File: VX019278.D
Acq: 04 Nov 2020 18:57

Tgt Ion	Ratio	Resp Lower	Resp Upper
164	100		
166	133.5	104.1	156.1
129	101.6	76.2	114.4
131	101.8	74.6	112.0

