

Data File : VX019279.D  
 Acq On : 04 Nov 2020 19:19  
 Operator : JC/MD  
 Sample : L4607-07  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 TRIP-BLANK

Quant Time: Nov 05 02:56:24 2020  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X102720W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue Oct 27 13:55:07 2020  
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.64	168	280654	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	496298	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	462286	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	234857	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.03	65	193466	53.45	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	106.90%	
35) Dibromofluoromethane	5.46	113	153122	49.12	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	98.24%	
50) Toluene-d8	8.70	98	607956	51.73	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	103.46%	
62) 4-Bromofluorobenzene	11.12	95	228139	51.26	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	102.52%	


Target Compounds Qvalue  
 -----


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VX019279.D  
Acq On : 04 Nov 2020 19:19  
Operator : JC/MD  
Sample : L4607-07  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampled :  
TRIP-BLANK

Quant Time: Nov 05 02:56:24 2020  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X102720W.M  
Quant Title : SW846 8260  
QLast Update : Tue Oct 27 13:55:07 2020  
Response via : Initial Calibration



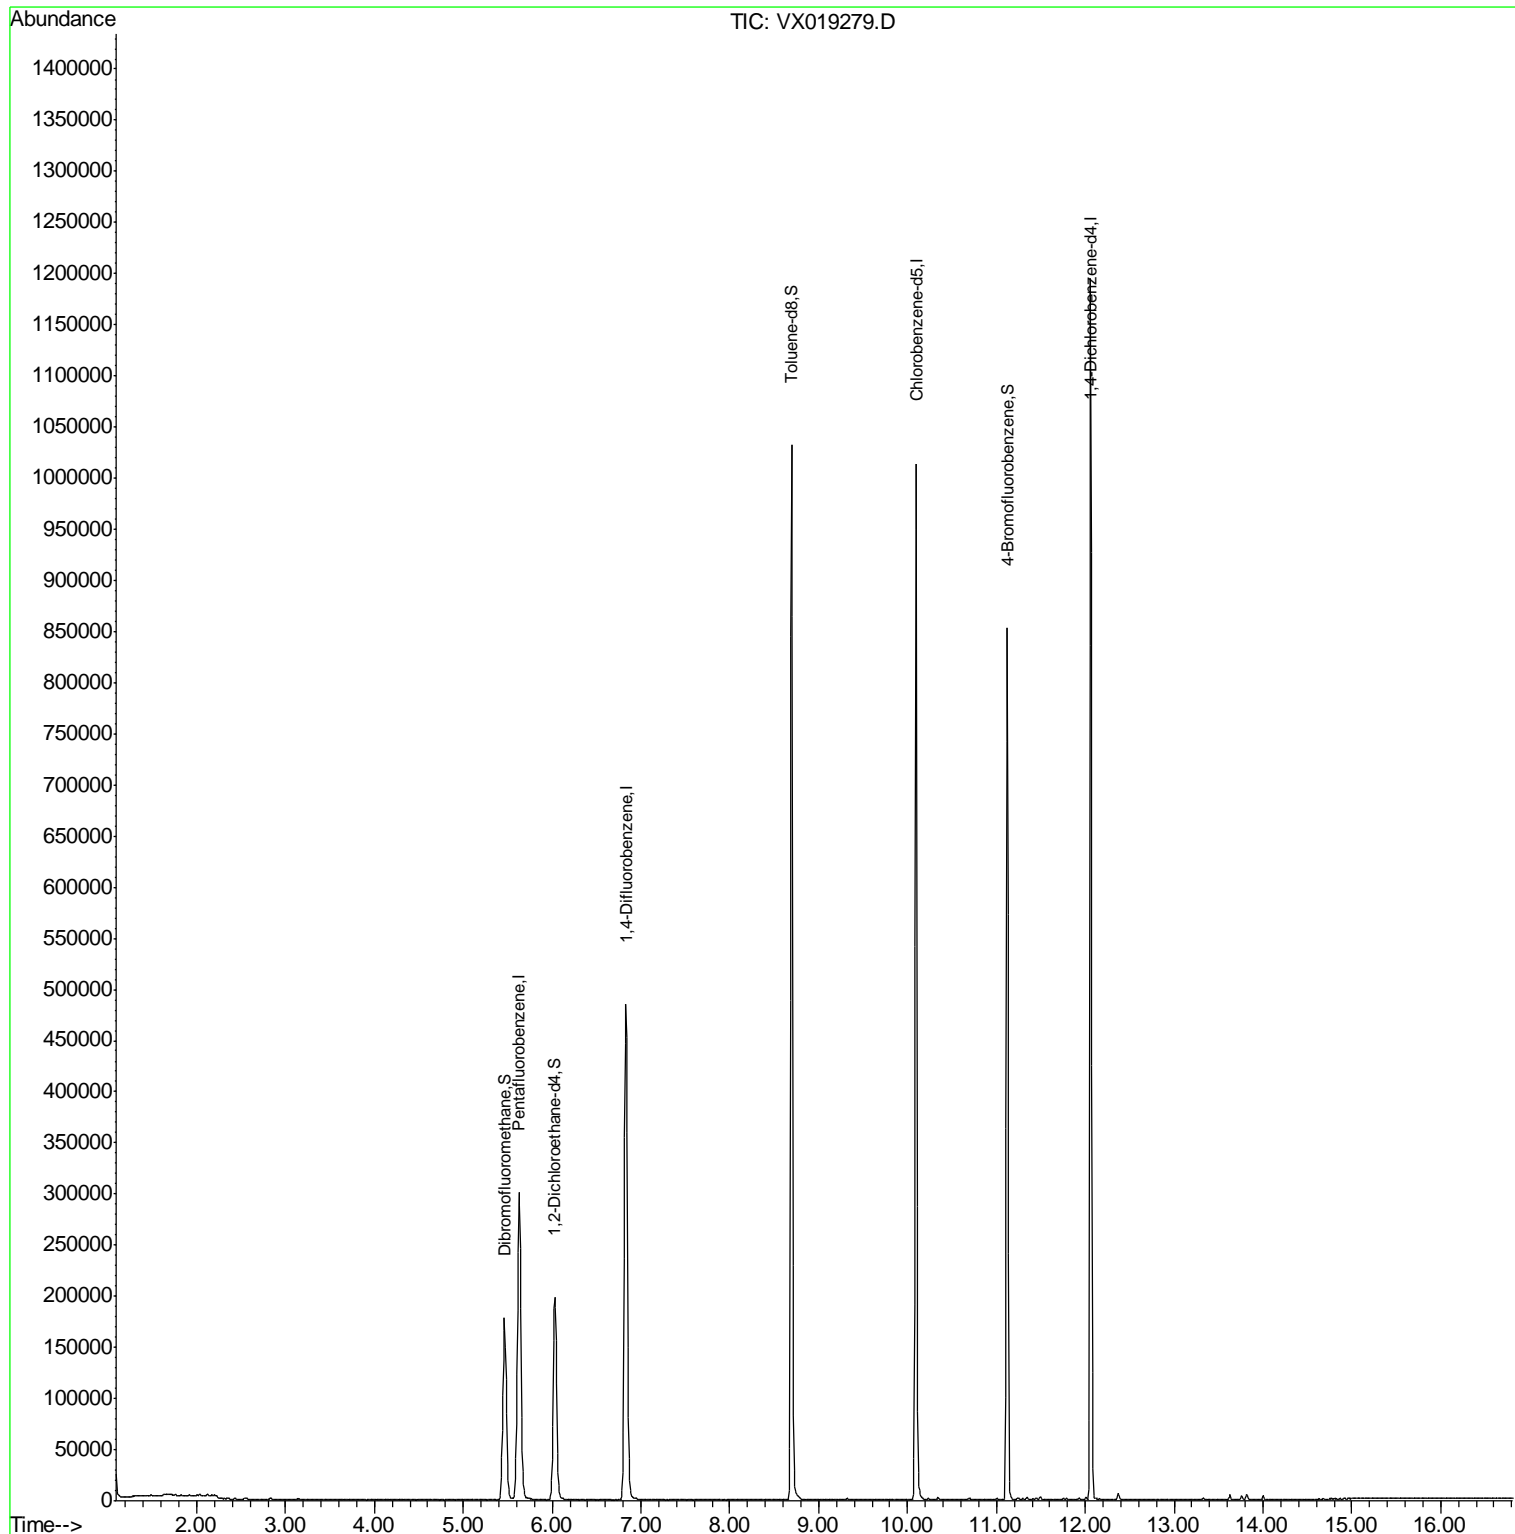


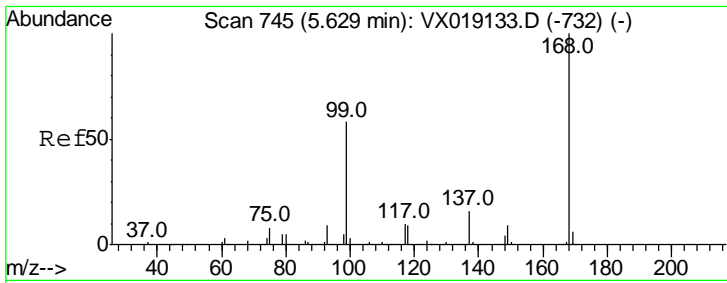

#1  
 Pentafluorobenzene  
 Concen: 50.000 ug/l  
 RT: 5.64 min Scan# 746  
 Delta R.T. 0.01 min  
 Lab File: VX019279.D  
 Acq: 04 Nov 2020 19:19




**Instrument :**  
 MSVOA\_X  
**ClientSampled :**  
 TRIP-BLANK


Tgt Ion	Resp	Lower	Upper
168	100		
99	58.6	46.6	69.8

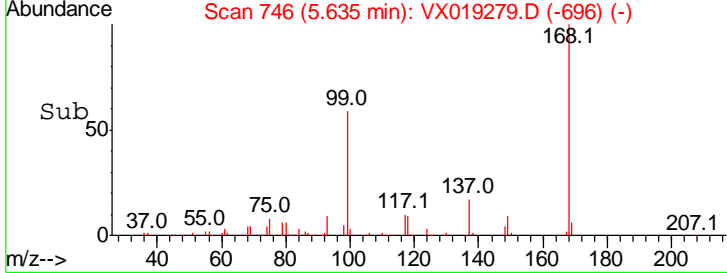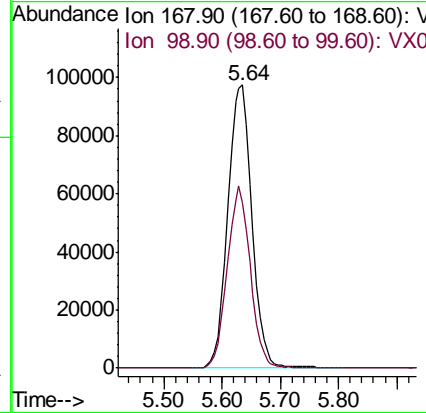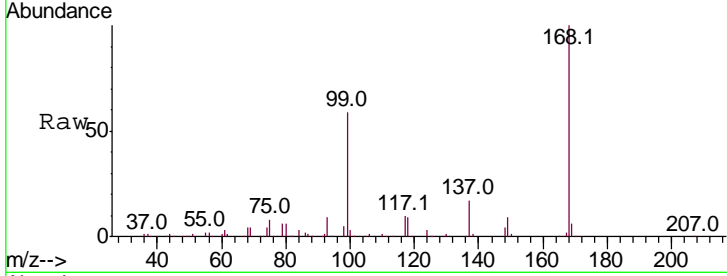

#33  
 1,2-Dichloroethane-d4  
 Concen: 53.453 ug/l  
 RT: 6.03 min Scan# 811  
 Delta R.T. -0.00 min  
 Lab File: VX019279.D  
 Acq: 04 Nov 2020 19:19

Tgt Ion	Resp	Lower	Upper
65	100		
67	51.6	0.0	103.0


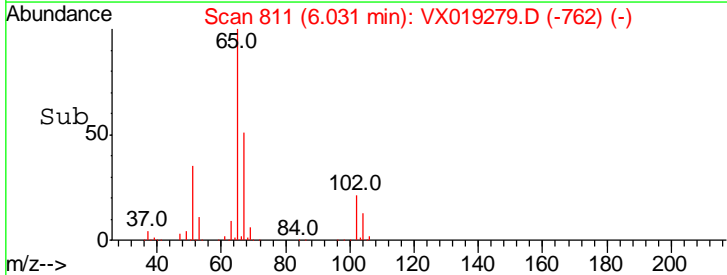
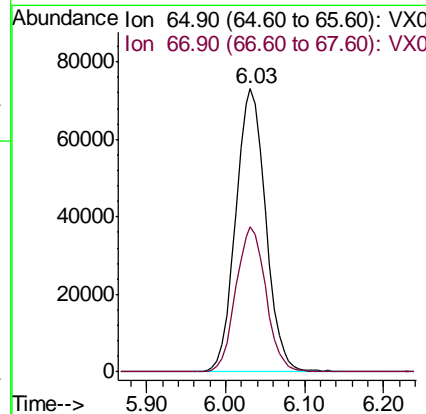
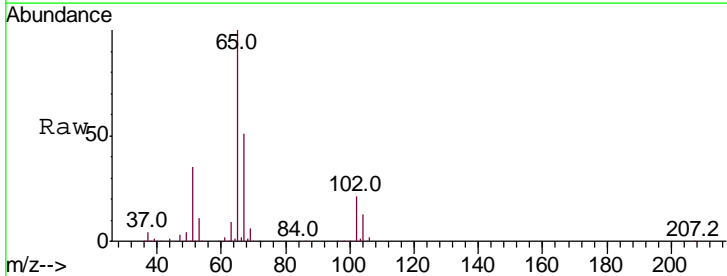


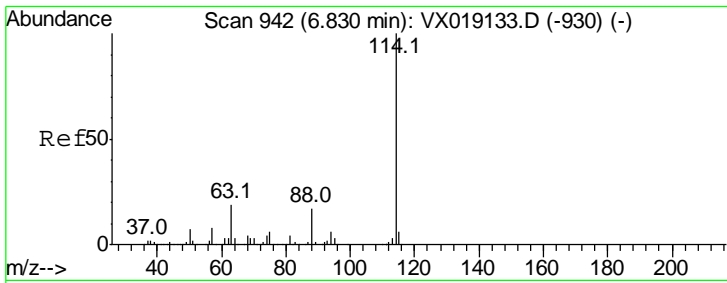

#34  
 1,4-Difluorobenzene  
 Concen: 50.000 ug/l  
 RT: 6.83 min Scan# 942  
 Delta R.T. -0.00 min  
 Lab File: VX019279.D  
 Acq: 04 Nov 2020 19:19




Instrument :  
 MSVOA\_X  
 ClientSampled :  
 TRIP-BLANK


Tgt Ion	Resp	Lower	Upper
114	100		
63	20.8	0.0	38.8
88	15.8	0.0	34.2

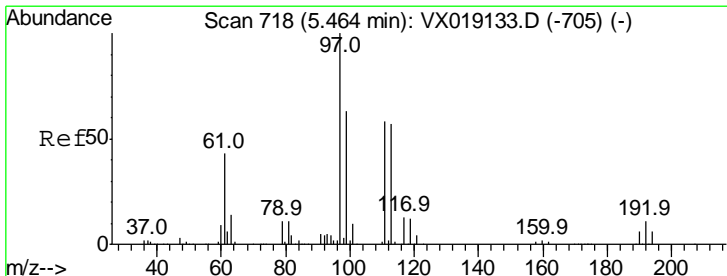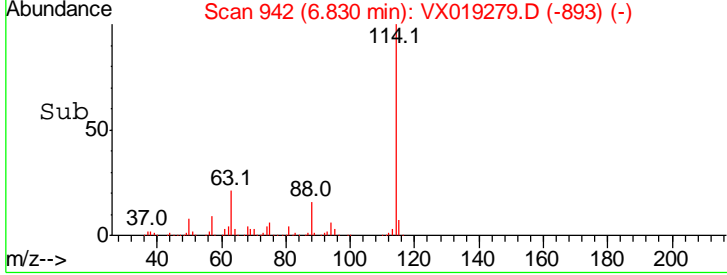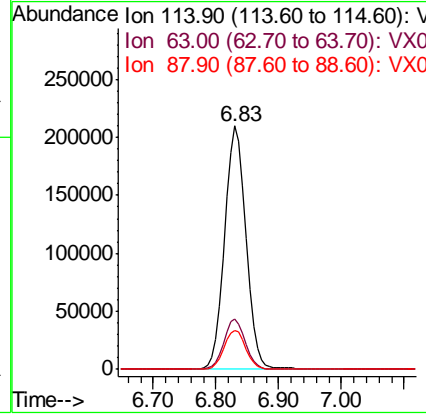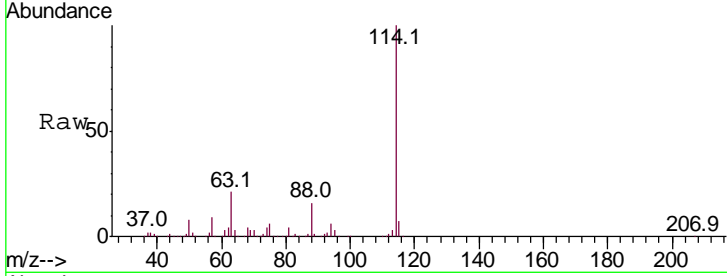

#35  
 Dibromofluoromethane  
 Concen: 49.118 ug/l  
 RT: 5.46 min Scan# 718  
 Delta R.T. -0.00 min  
 Lab File: VX019279.D  
 Acq: 04 Nov 2020 19:19

Tgt Ion	Resp	Lower	Upper
113	100		
111	102.2	82.3	123.5
192	19.3	16.2	24.2


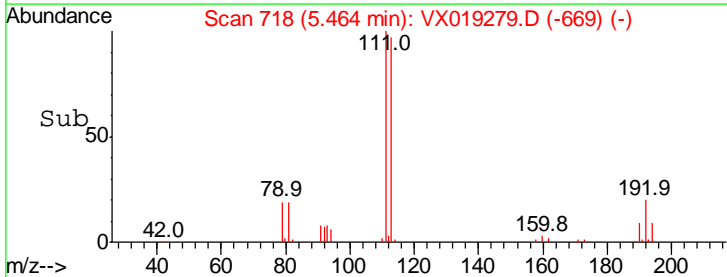
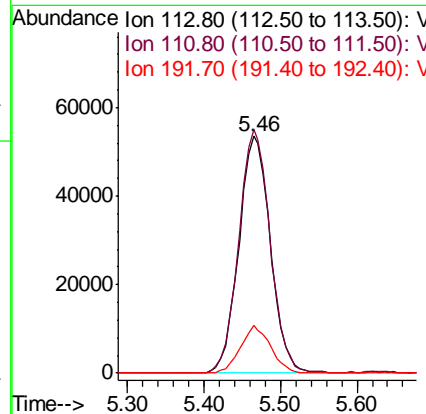
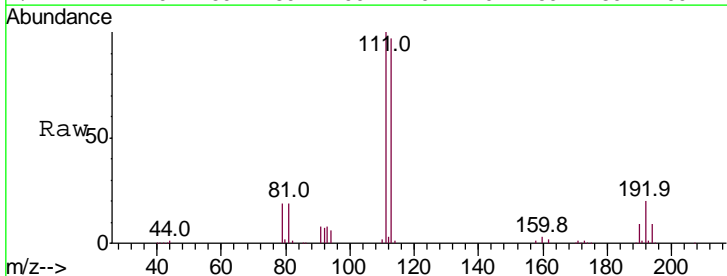


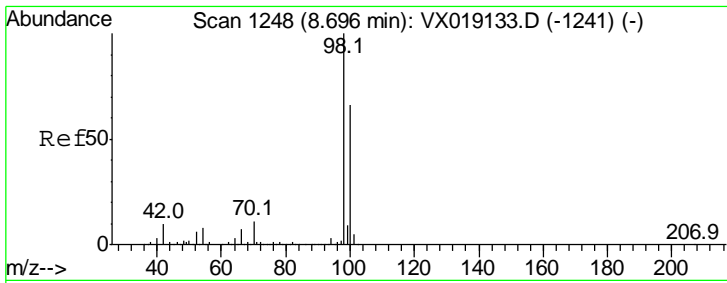

#50  
 Toluene-d8  
 Concen: 51.734 ug/l  
 RT: 8.70 min Scan# 1248  
 Delta R.T. -0.00 min  
 Lab File: VX019279.D  
 Acq: 04 Nov 2020 19:19




**Instrument :**  
 MSVOA\_X  
**ClientSampled :**  
 TRIP-BLANK


Tgt Ion	Resp	Lower	Upper
98	100		
100	66.2	53.0	79.6

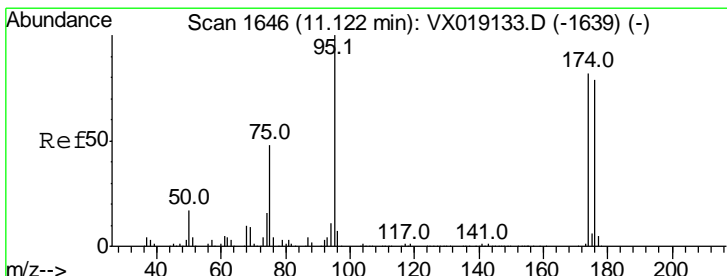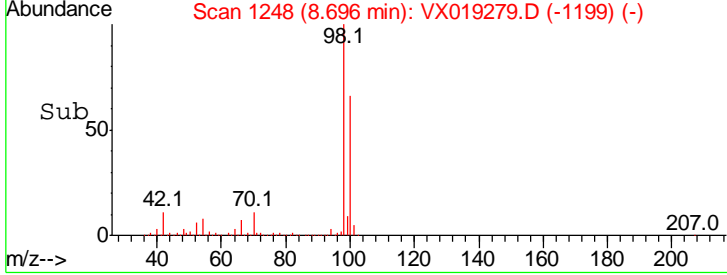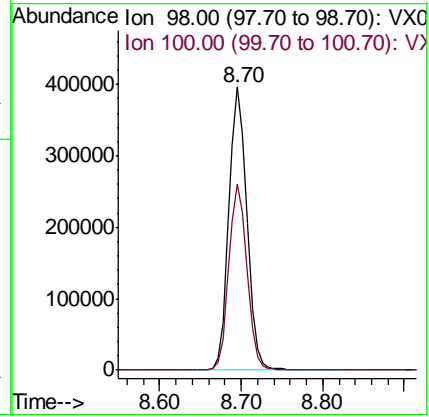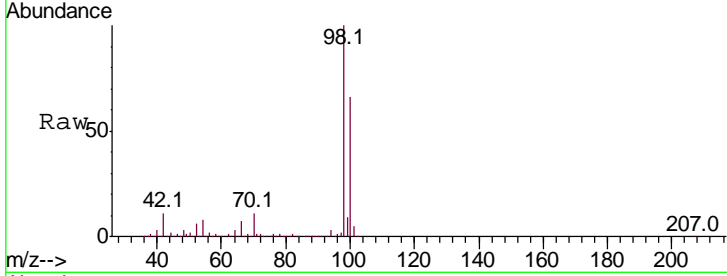

#62  
 4-Bromofluorobenzene  
 Concen: 51.262 ug/l  
 RT: 11.12 min Scan# 1646  
 Delta R.T. -0.00 min  
 Lab File: VX019279.D  
 Acq: 04 Nov 2020 19:19

Tgt Ion	Resp	Lower	Upper
95	100		
174	76.1	0.0	156.0
176	73.6	0.0	149.8


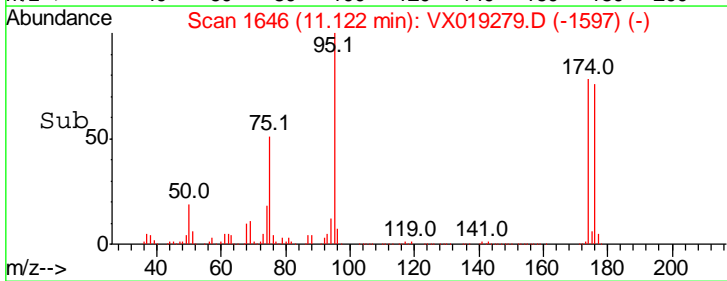
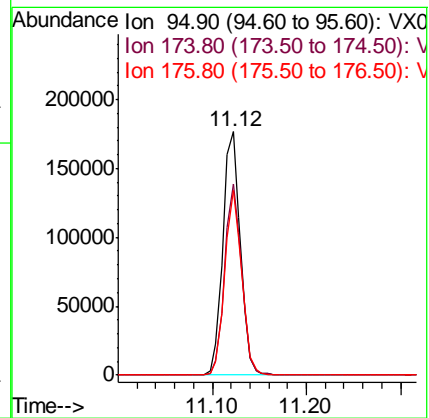
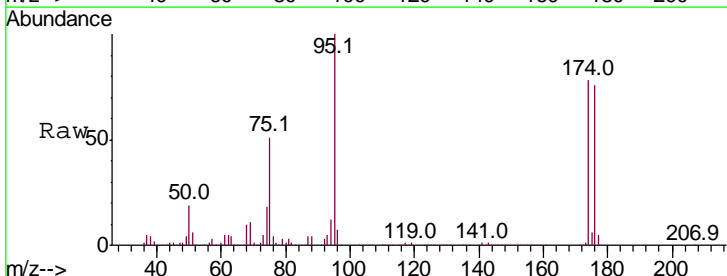


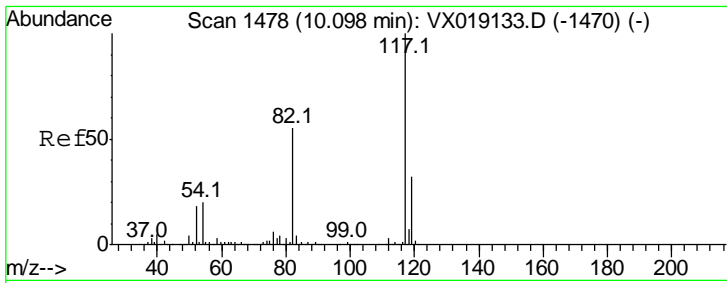

#63  
 Chlorobenzene-d5  
 Concen: 50.000 ug/l  
 RT: 10.10 min Scan# 1478  
 Delta R.T. -0.00 min  
 Lab File: VX019279.D  
 Acq: 04 Nov 2020 19:19

Instrument : MSVOA\_X  
 ClientSampled : TRIP-BLANK

Tgt Ion	Resp	Lower	Upper
117	100		
82	57.1	43.6	65.4
119	32.6	25.5	38.3

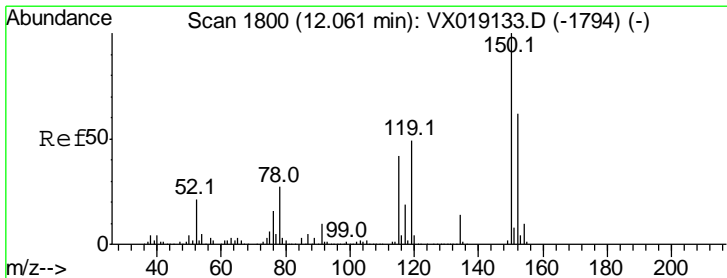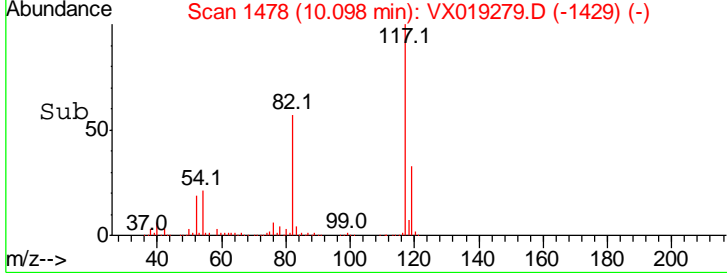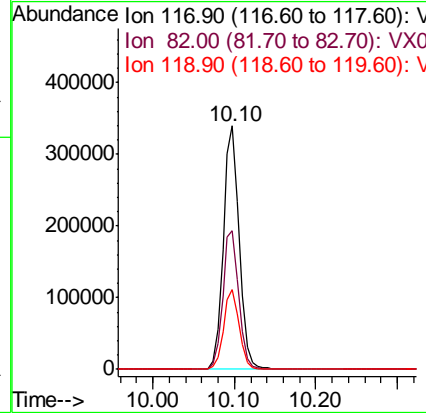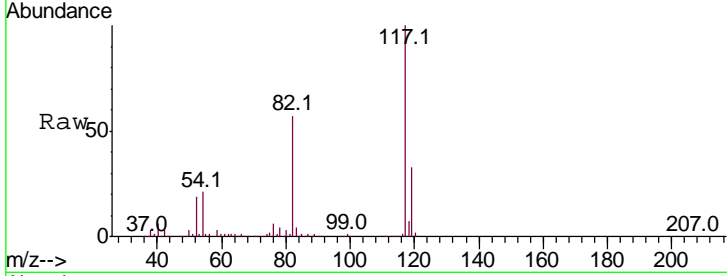

#72  
 1,4-Dichlorobenzene-d4  
 Concen: 50.000 ug/l  
 RT: 12.06 min Scan# 1800  
 Delta R.T. -0.00 min  
 Lab File: VX019279.D  
 Acq: 04 Nov 2020 19:19

Tgt Ion	Resp	Lower	Upper
152	100		
115	61.2	41.9	125.7
150	155.7	0.0	347.8

