

Data File : VX019297.D
Acq On : 05 Nov 2020 02:02
Operator : JC/MD
Sample : L4622-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PAV-B7-110220-DP

Quant Time: Nov 05 03:36:22 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102720W.M
Quant Title : SW846 8260
QLast Update : Tue Oct 27 13:55:07 2020
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	289685	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	517518	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	499151	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	243494	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.03	65	207789	55.62	ug/l	0.00
Spiked Amount 50.000			Recovery	=	111.24%	
35) Dibromofluoromethane	5.46	113	166305	51.16	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.32%	
50) Toluene-d8	8.70	98	652410	53.24	ug/l	0.00
Spiked Amount 50.000			Recovery	=	106.48%	
62) 4-Bromofluorobenzene	11.12	95	244283	52.64	ug/l	0.00
Spiked Amount 50.000			Recovery	=	105.28%	
Target Compounds						
16) Acetone	2.42	43	15891	12.330	ug/l	97
20) Methylene Chloride	2.84	84	6369	1.968	ug/l	97
43) Isopropyl Acetate	6.41	43	73003	9.826	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VX019297.D
Acq On : 05 Nov 2020 02:02
Operator : JC/MD
Sample : L4622-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PAV-B7-110220-DP

Quant Time: Nov 05 03:36:22 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102720W.M
Quant Title : SW846 8260
QLast Update : Tue Oct 27 13:55:07 2020
Response via : Initial Calibration

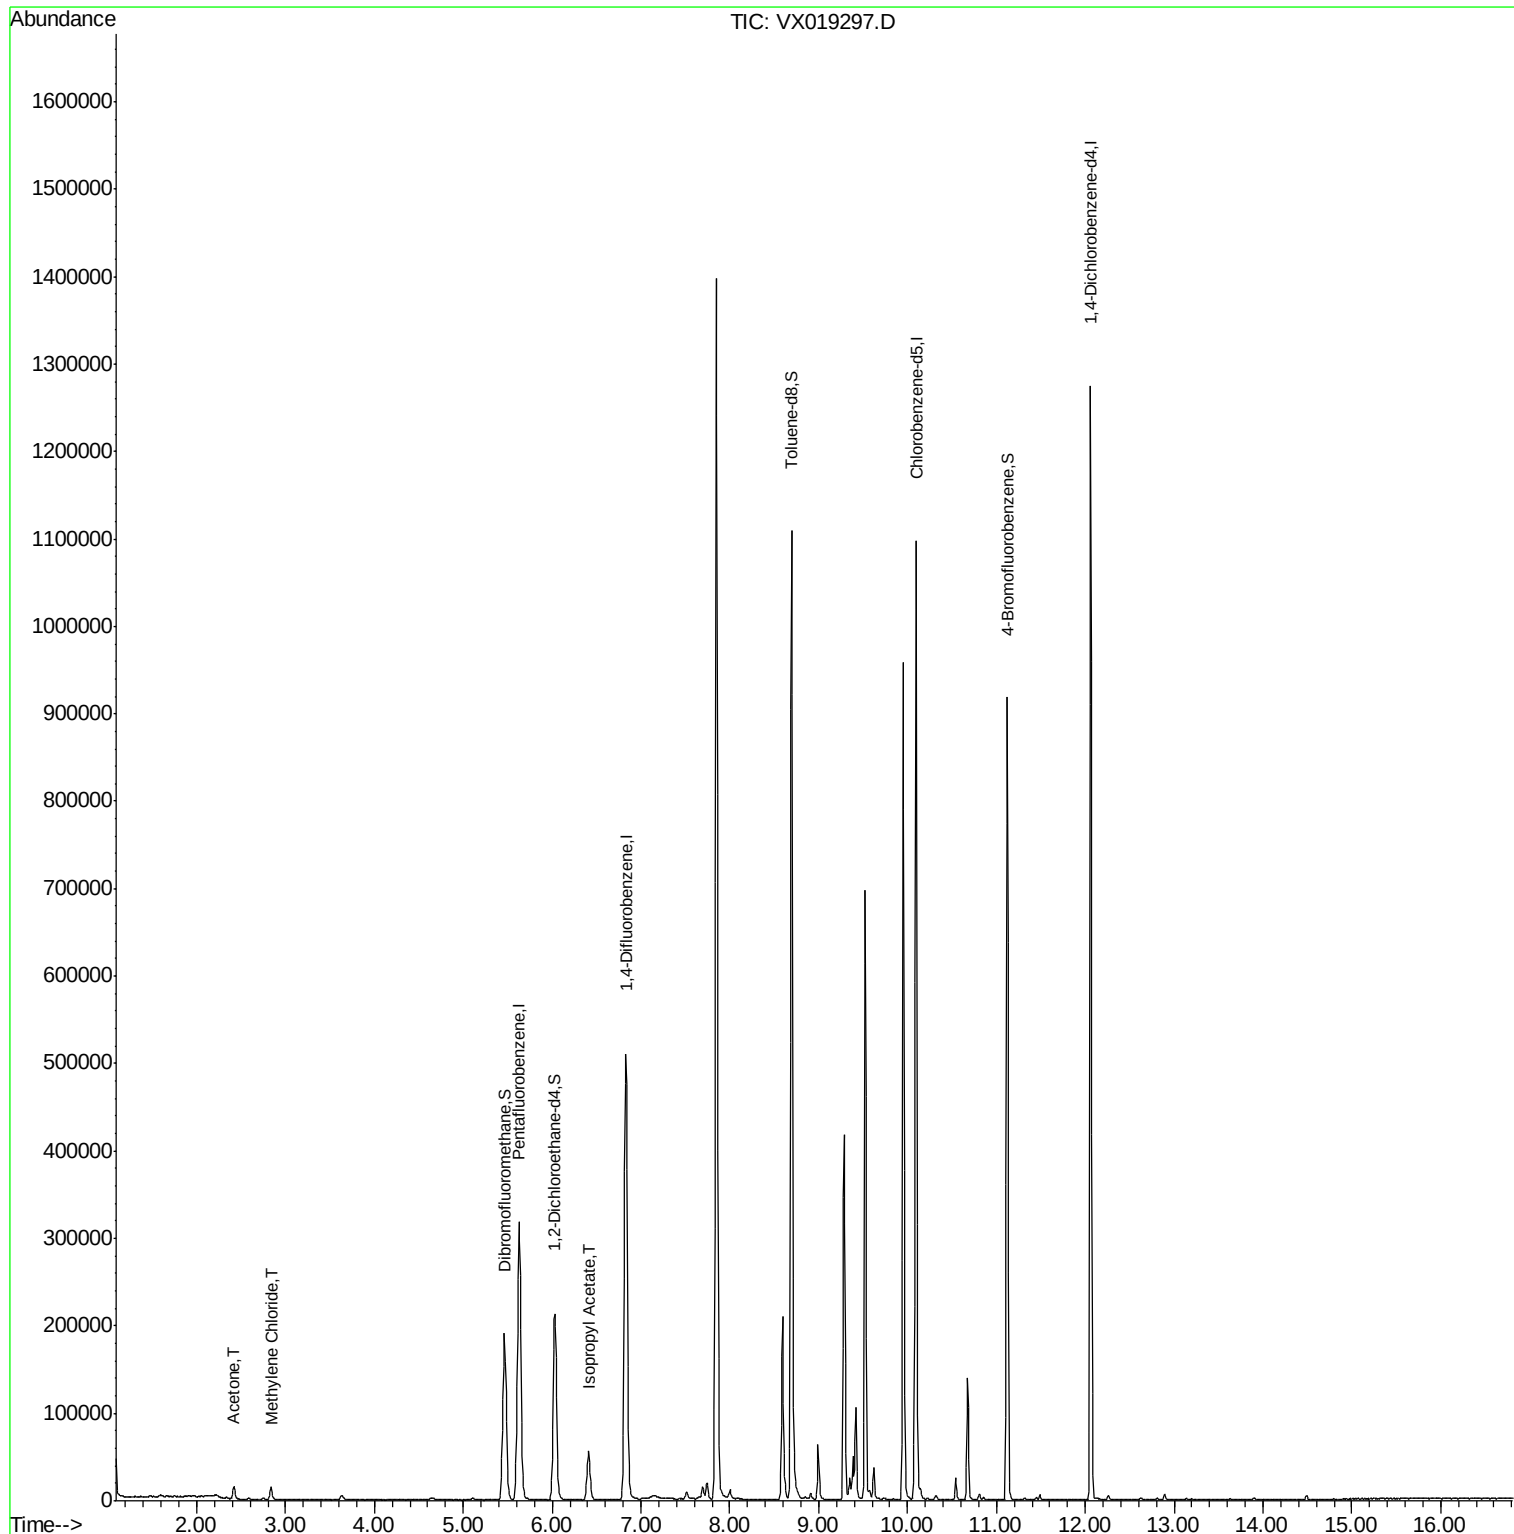

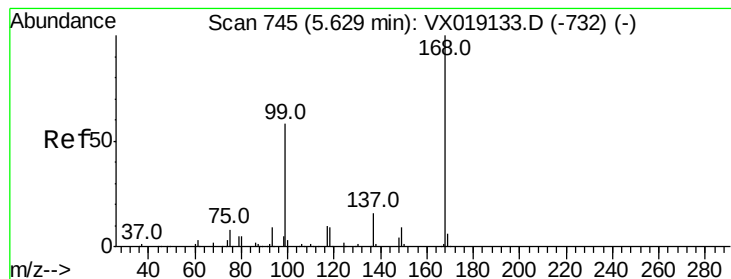

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.00 min

Lab File: VX019297.D

Acq: 05 Nov 2020 02:02


Instrument :
MSVOA_X
ClientSampleId :
PAV-B7-110220-DP

Tgt Ion:168 Resp: 289685

Ion Ratio Lower Upper

168 100

99 62.4 46.6 69.8

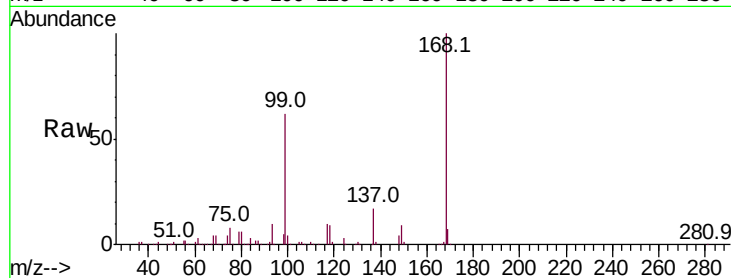

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

120000

100000

80000

60000

40000



20000

0

5.50 5.60 5.70 5.80

5.63

Time-->

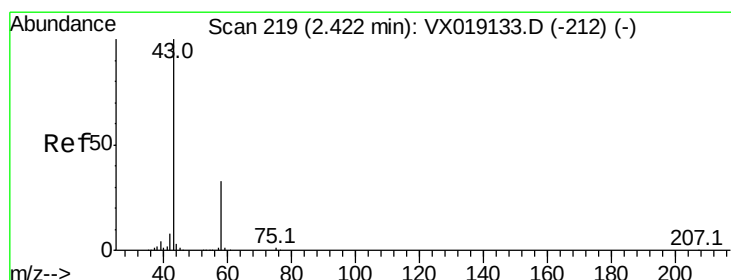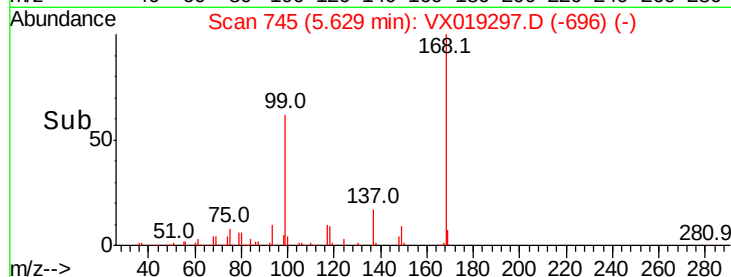

#16

Acetone

Concen: 12.330 ug/l

RT: 2.42 min Scan# 218

Delta R.T. -0.01 min

Lab File: VX019297.D


Acq: 05 Nov 2020 02:02

Tgt Ion: 43 Resp: 15891

Ion Ratio Lower Upper

43 100

58 30.9 26.3 39.5

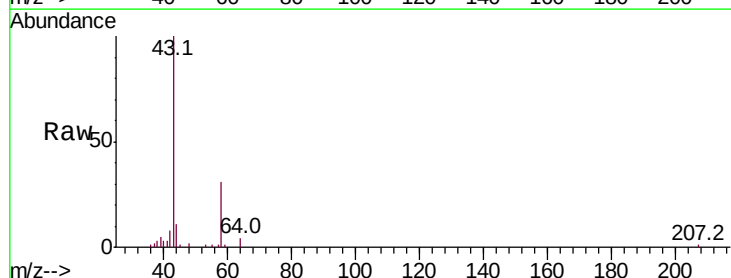

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

10000

8000

6000

4000


2000


0

2.40 2.50

2.42

Time-->




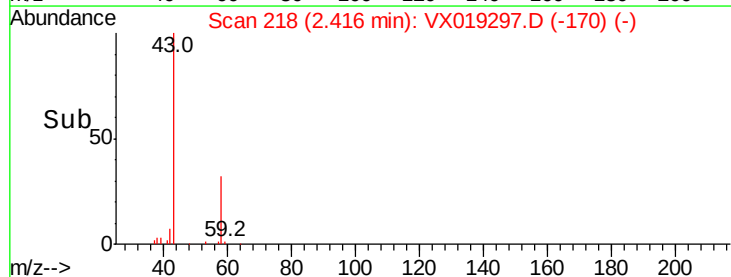


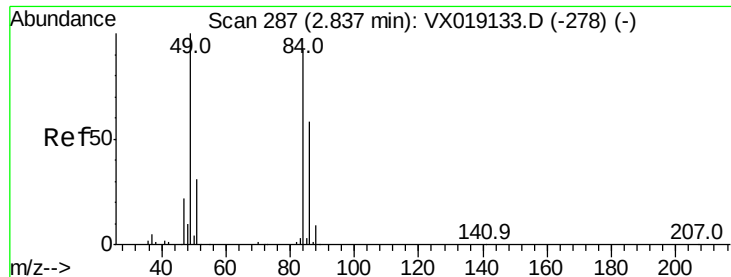

#20
Methylene Chloride
Concen: 1.968 ug/l
RT: 2.84 min Scan# 287
Delta R.T. -0.00 min
Lab File: VX019297.D
Acq: 05 Nov 2020 02:02




Instrument :
MSVOA_X
ClientSampleId :
PAV-B7-110220-DP


Tgt Ion:	84	Resp:	6369
Ion	Ratio	Lower	Upper
84	100		
49	111.2	86.8	130.2
51	35.7	27.3	40.9
86	60.0	50.6	76.0

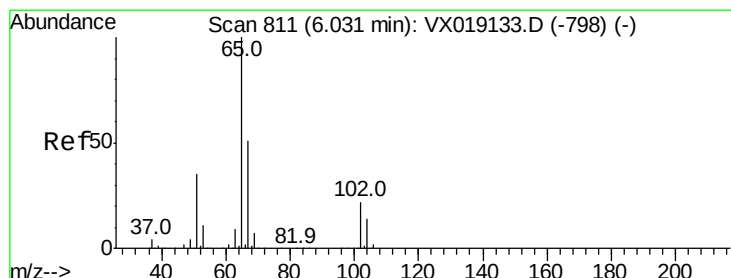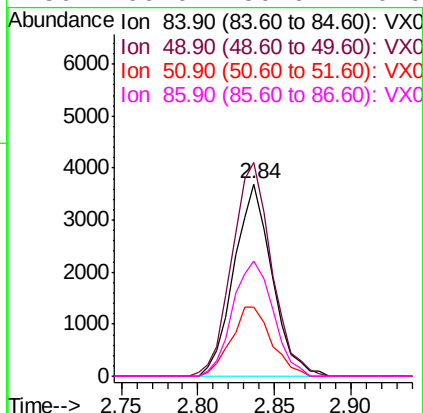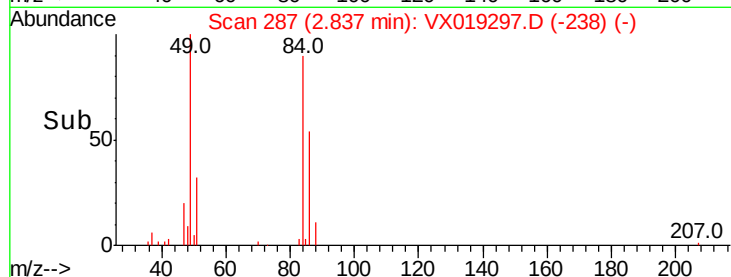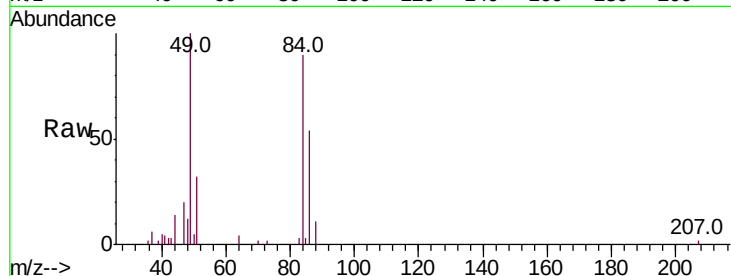

#33
1,2-Dichloroethane-d4
Concen: 55.620 ug/l
RT: 6.03 min Scan# 811
Delta R.T. -0.00 min
Lab File: VX019297.D
Acq: 05 Nov 2020 02:02

Tgt Ion:	65	Resp:	207789
Ion	Ratio	Lower	Upper
65	100		
67	51.8	0.0	103.0

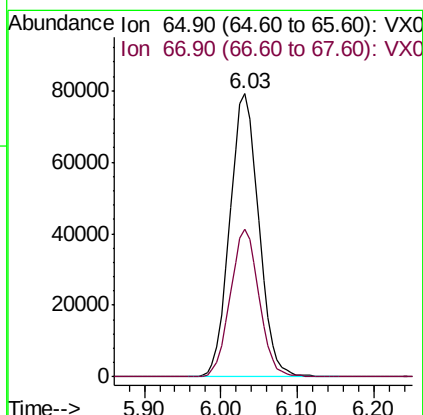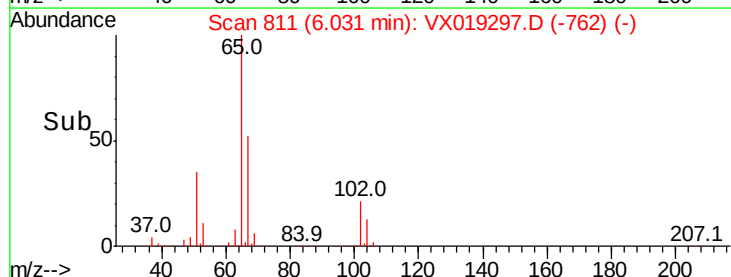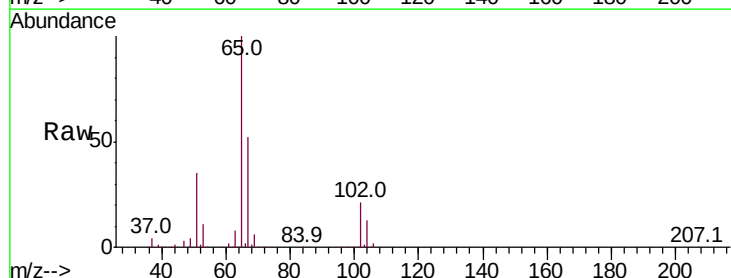

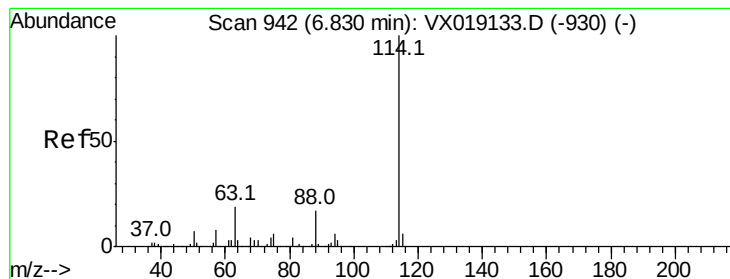

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.00 min

Lab File: VX019297.D

Acq: 05 Nov 2020 02:02

Instrument :

MSVOA_X

ClientSampleId :

PAV-B7-110220-DP


Tgt Ion:114 Resp: 517518

Ion Ratio Lower Upper

114 100

63 21.1 0.0 38.8




88 15.9 0.0 34.2

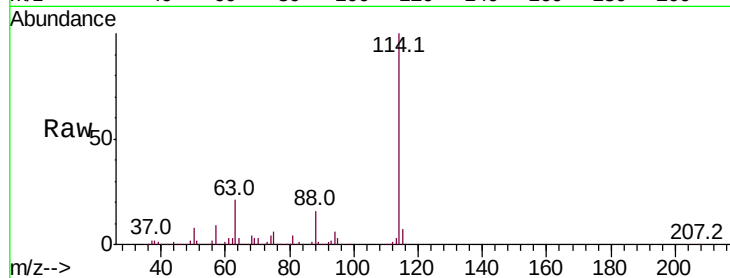

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

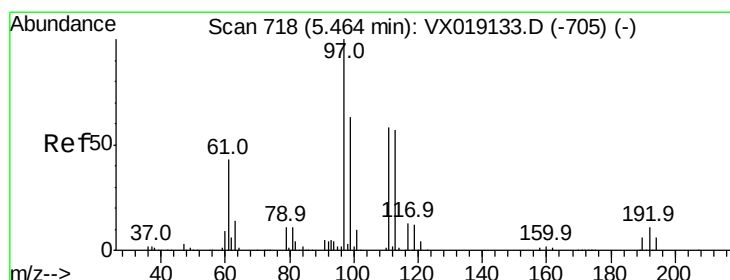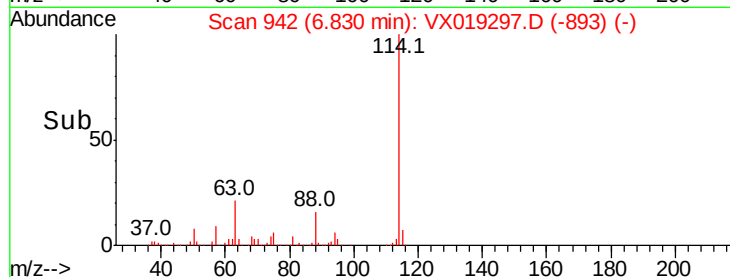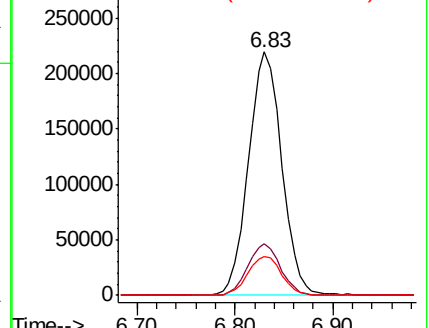

#35

Dibromofluoromethane

Concen: 51.159 ug/l

RT: 5.46 min Scan# 718

Delta R.T. -0.00 min

Lab File: VX019297.D

Acq: 05 Nov 2020 02:02


Tgt Ion:113 Resp: 166305

Ion Ratio Lower Upper

113 100

111 102.6 82.3 123.5



192 19.3 16.2 24.2

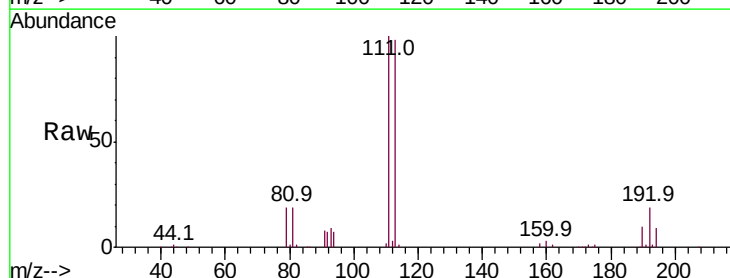


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

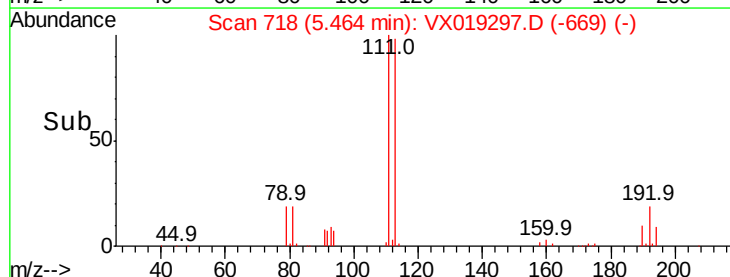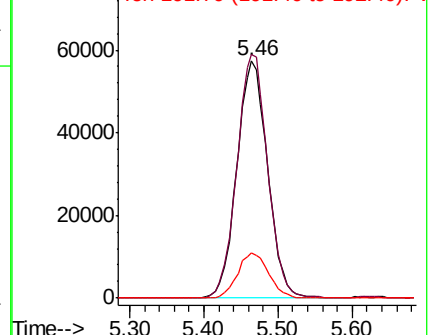

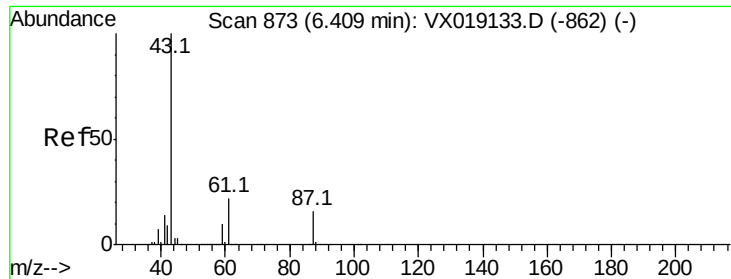

#43

Isopropyl Acetate

Concen: 9.826 ug/l

RT: 6.41 min Scan# 873

Delta R.T. -0.00 min

Lab File: VX019297.D

Acq: 05 Nov 2020 02:02

Instrument :

MSVOA_X

ClientSampleId :

PAV-B7-110220-DP


Tgt Ion: 43 Resp: 73003

Ion Ratio Lower Upper

43 100

61 21.4 17.8 26.6




87 14.9 12.6 19.0

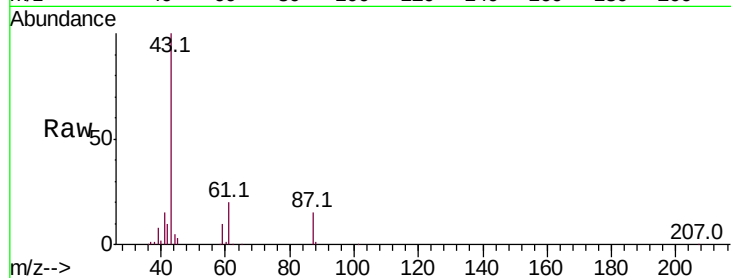

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

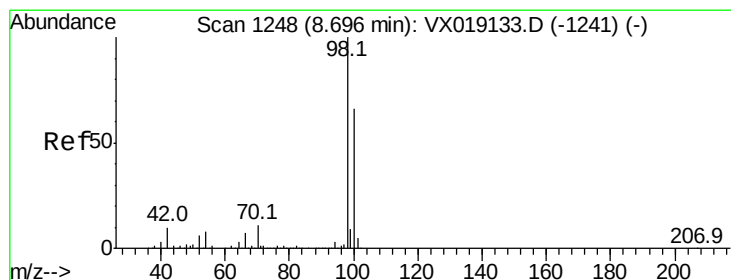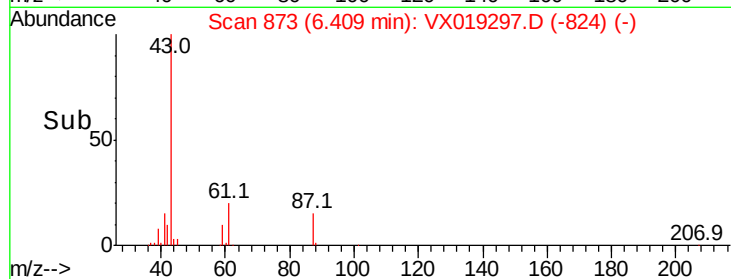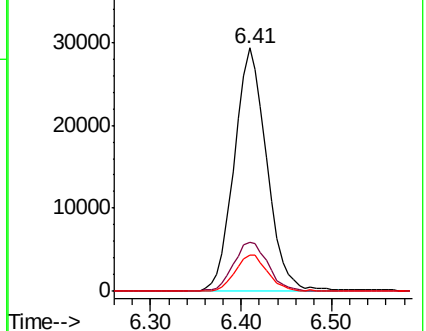

#50

Toluene-d8

Concen: 53.240 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. -0.00 min

Lab File: VX019297.D


Acq: 05 Nov 2020 02:02

Tgt Ion: 98 Resp: 652410

Ion Ratio Lower Upper



98 100


100 65.9 53.0 79.6

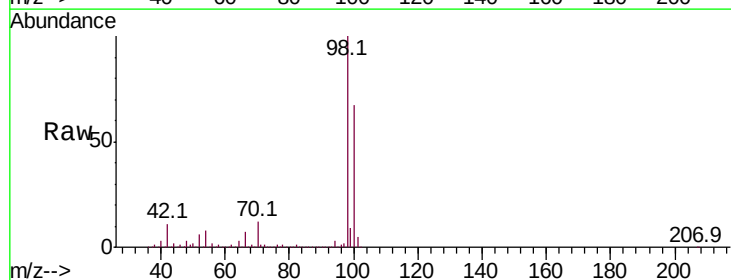

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

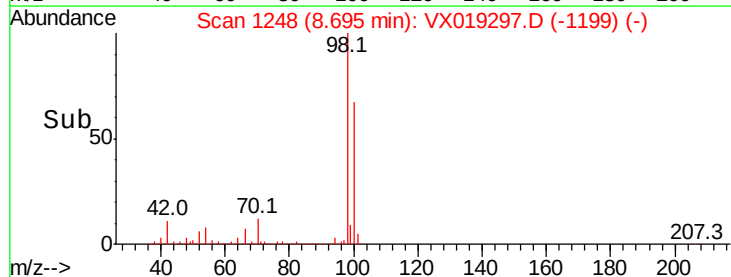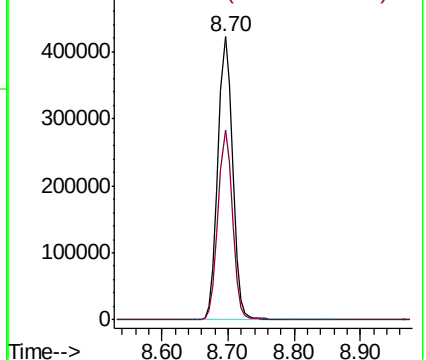

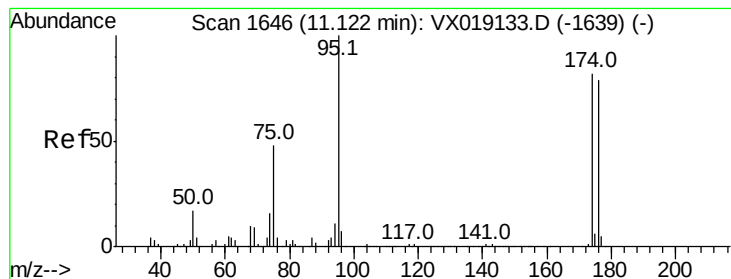

#62

4-Bromofluorobenzene

Concen: 52.639 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX019297.D

Acq: 05 Nov 2020 02:02

Instrument :

MSVOA_X

ClientSampleId :

PAV-B7-110220-DP


Tgt Ion: 95 Resp: 244283

Ion Ratio Lower Upper

95 100

174 75.4 0.0 156.0




176 72.2 0.0 149.8

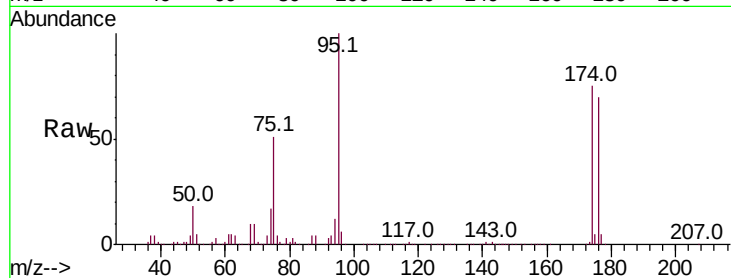

Abundance Ion 94.90 (94.60 to 95.60): VX019133.D (-1639) (-)

Ion 173.80 (173.50 to 174.50): VX019133.D (-1639) (-)

Ion 175.80 (175.50 to 176.50): VX019133.D (-1639) (-)

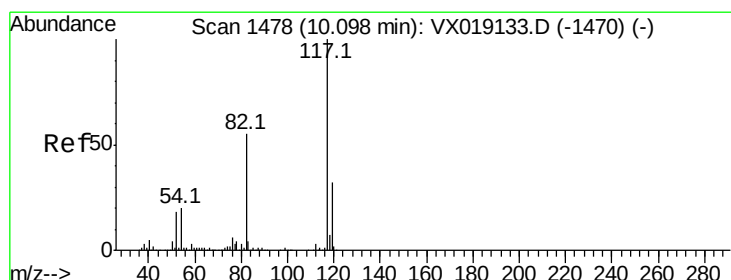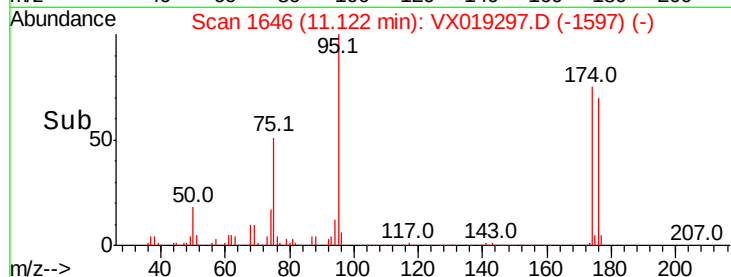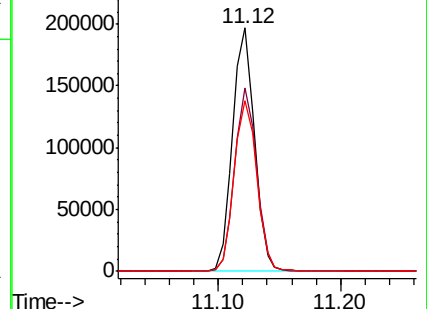

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.10 min Scan# 1478

Delta R.T. -0.00 min

Lab File: VX019297.D

Acq: 05 Nov 2020 02:02


Tgt Ion: 117 Resp: 499151

Ion Ratio Lower Upper

117 100

82 56.4 43.6 65.4



119 31.2 25.5 38.3

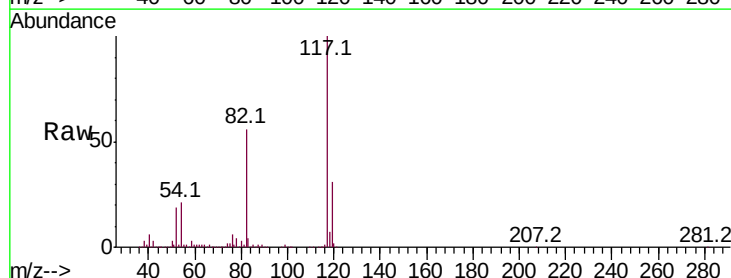


Abundance Ion 116.90 (116.60 to 117.60): VX019133.D (-1470) (-)

Ion 82.00 (81.70 to 82.70): VX019133.D (-1470) (-)

Ion 118.90 (118.60 to 119.60): VX019133.D (-1470) (-)

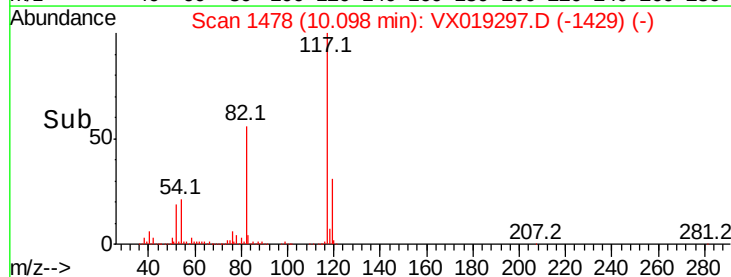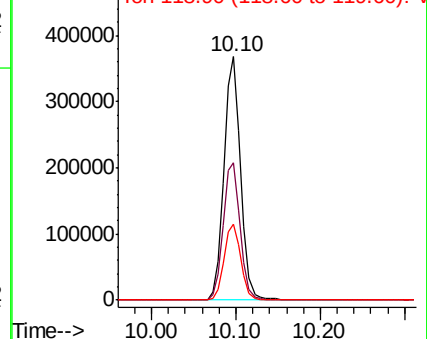

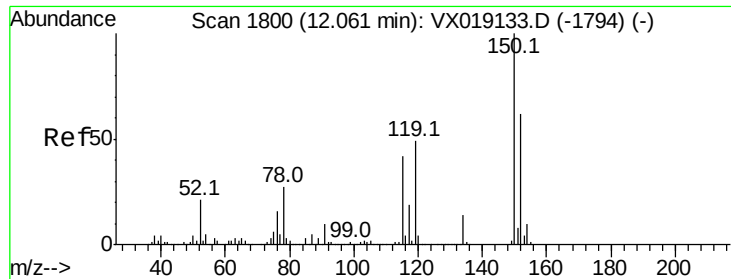

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. -0.00 min

Lab File: VX019297.D

Acq: 05 Nov 2020 02:02

Instrument :

MSVOA_X

ClientSampleId :

PAV-B7-110220-DP


Tgt Ion:152 Resp: 243494

Ion Ratio Lower Upper

152 100

115 62.0 41.9 125.7

150 159.3 0.0 347.8

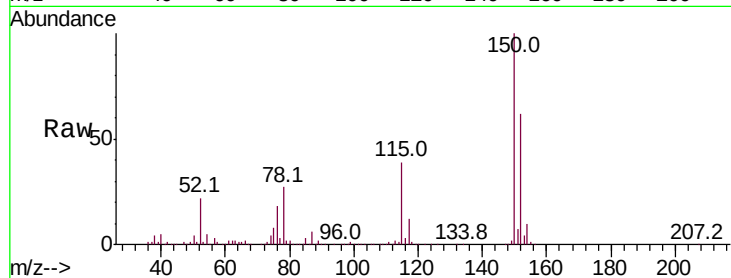

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

