



Acrolein

Response Ratio

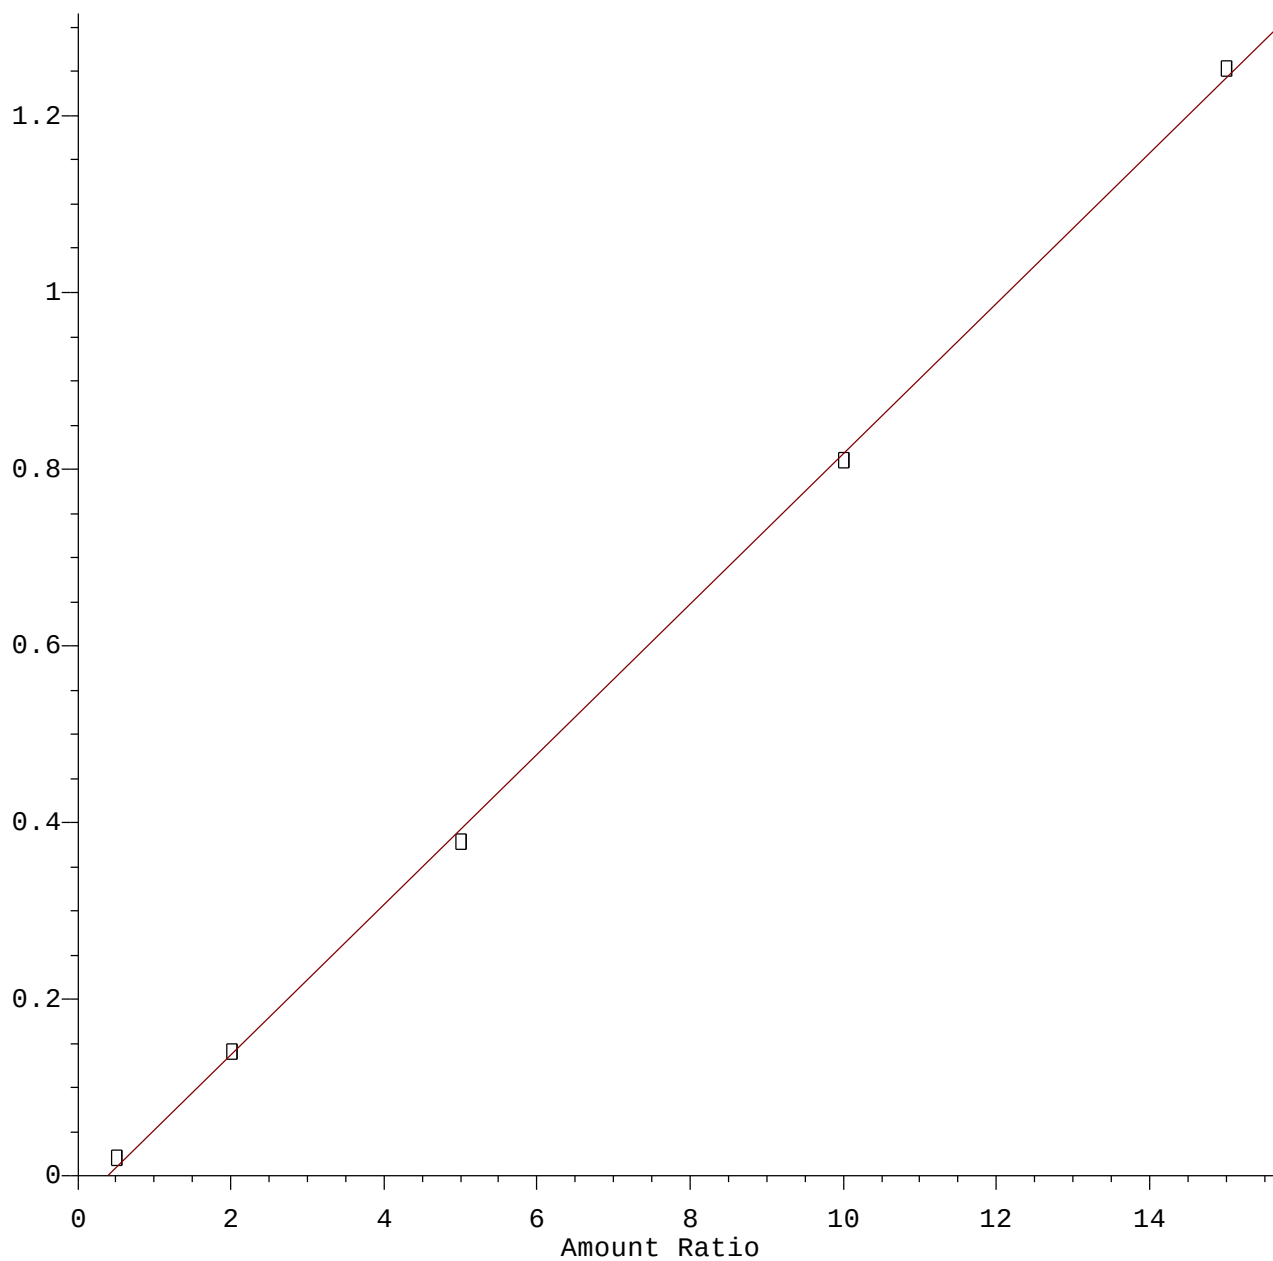

Resp Ratio = 8.50×10^{-2} * Amt - 3.26×10^{-2}
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X110718W.M
Calibration Table Last Updated: Fri Nov 09 14:02:25 2018

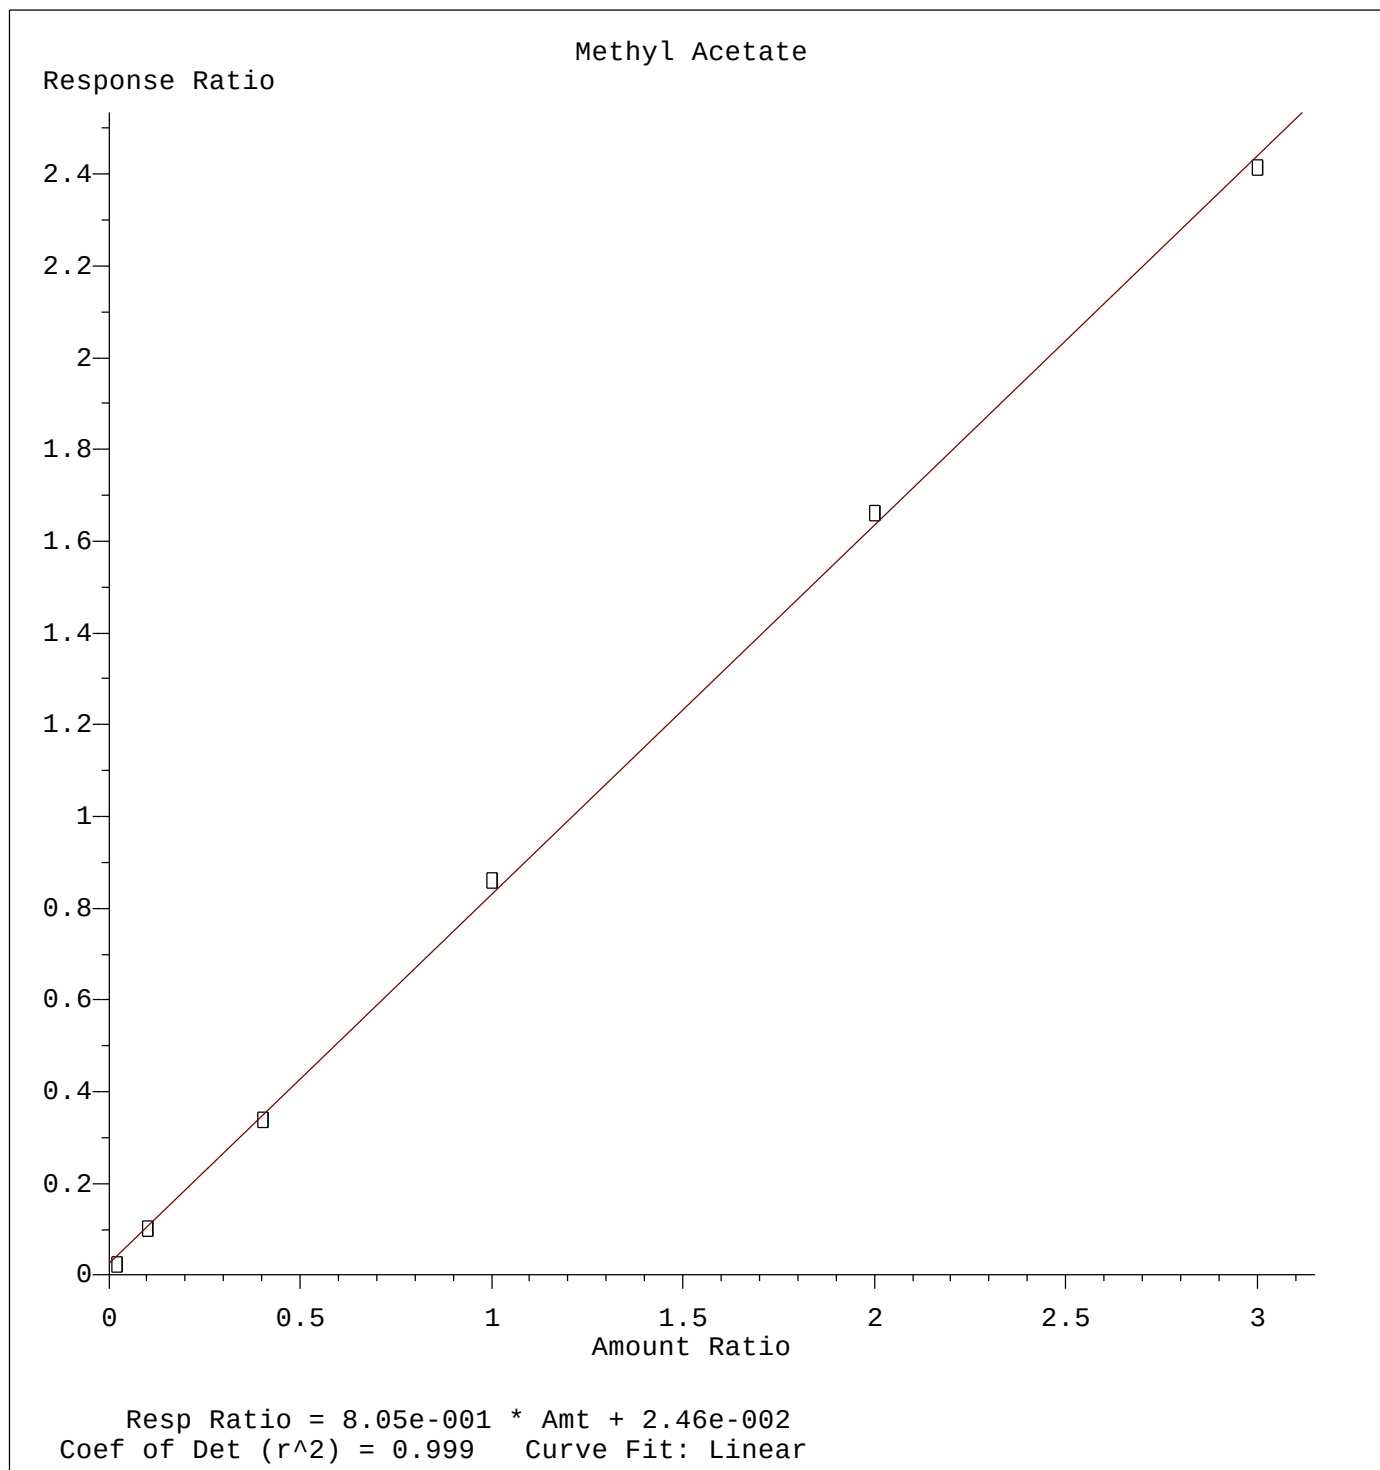

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X110718W.M
Calibration Table Last Updated: Fri Nov 09 14:02:25 2018


2-Chloroethyl Vinyl ether

Response Ratio

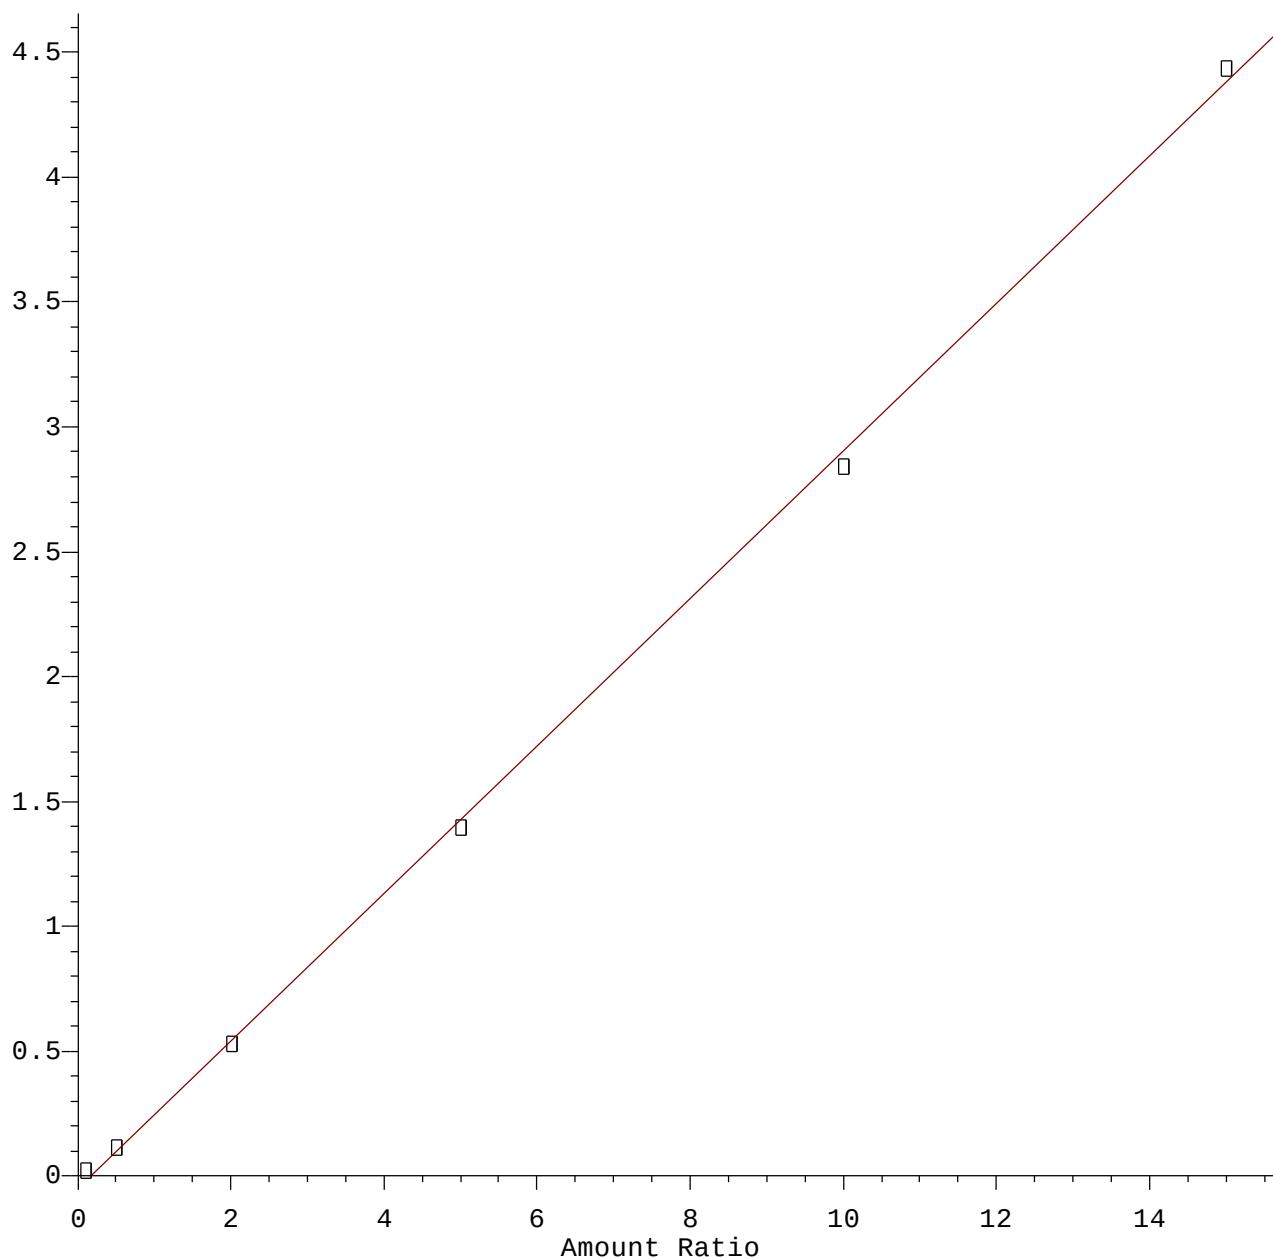

Resp Ratio = $2.95 \times 10^{-1} \times \text{Amt} - 4.89 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X110718W.M
Calibration Table Last Updated: Fri Nov 09 14:02:25 2018

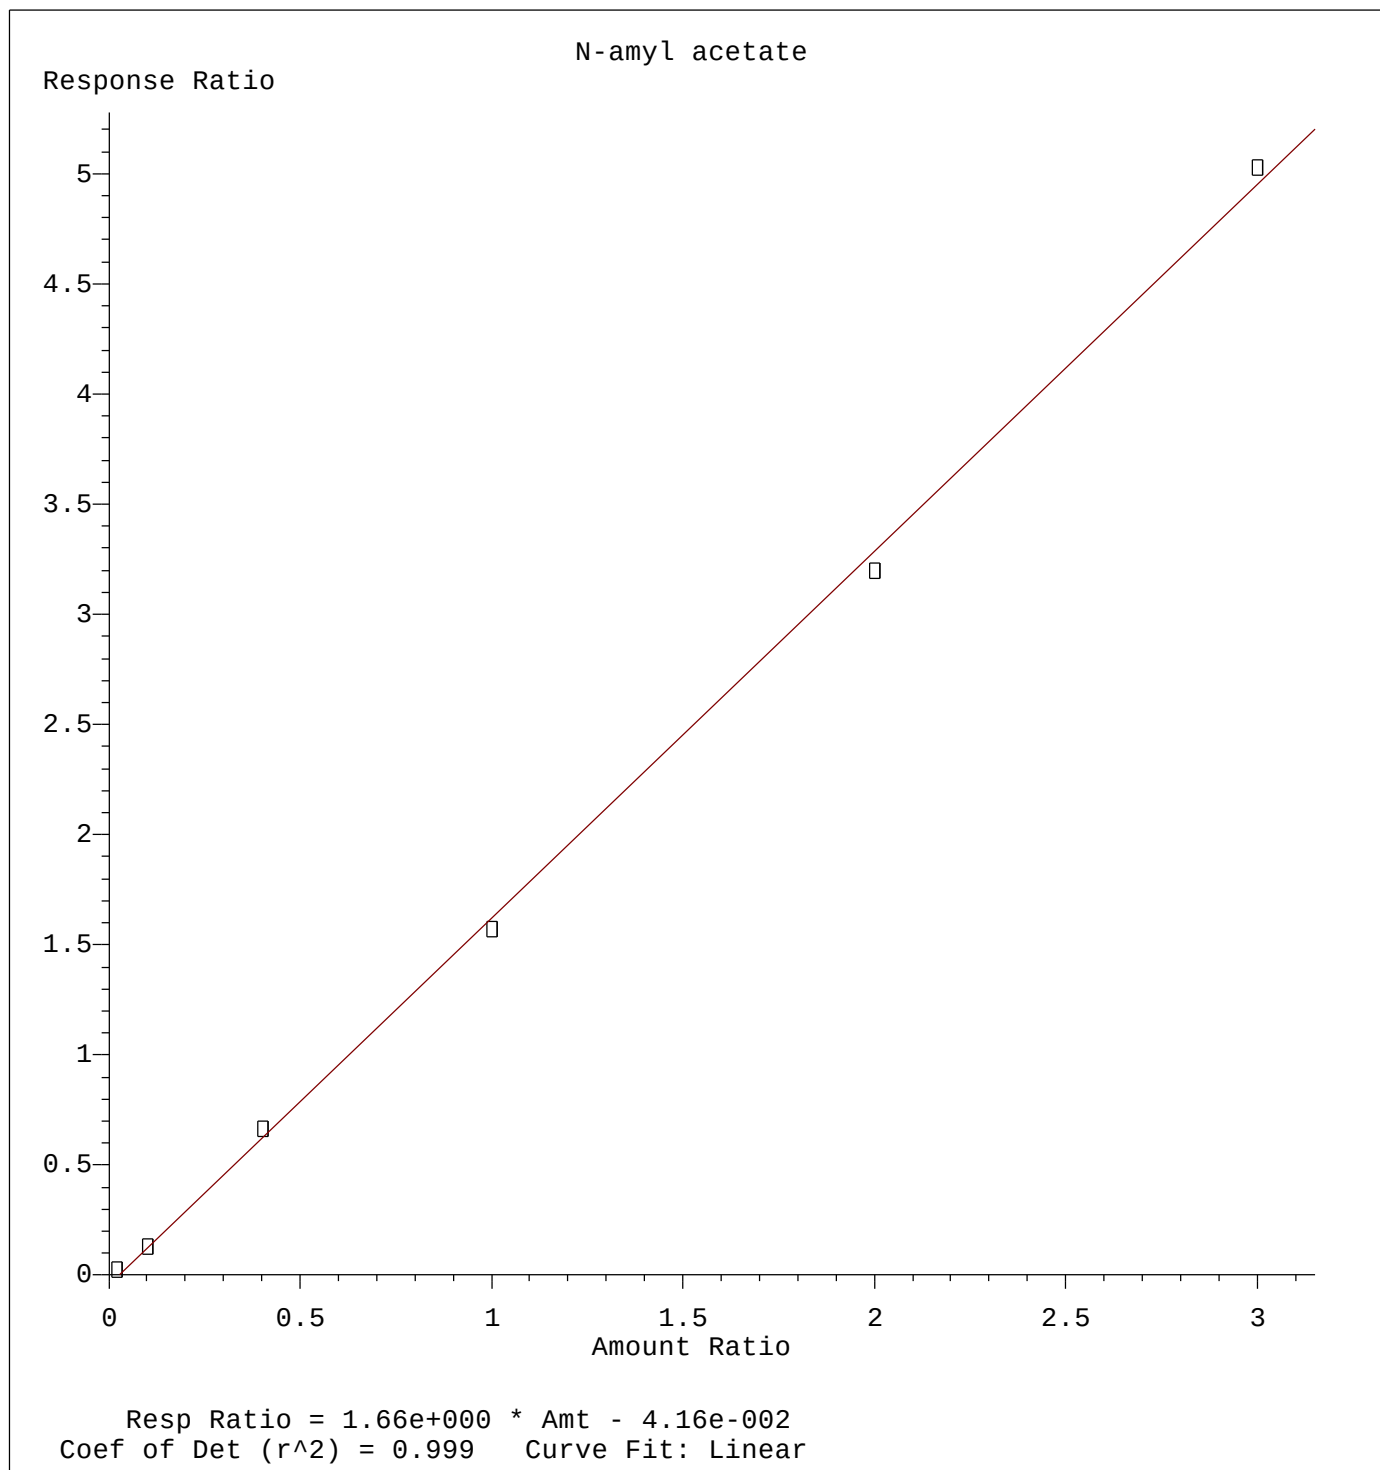

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X110718W.M
Calibration Table Last Updated: Fri Nov 09 14:02:25 2018

1,2,4-Trimethylbenzene

Response Ratio

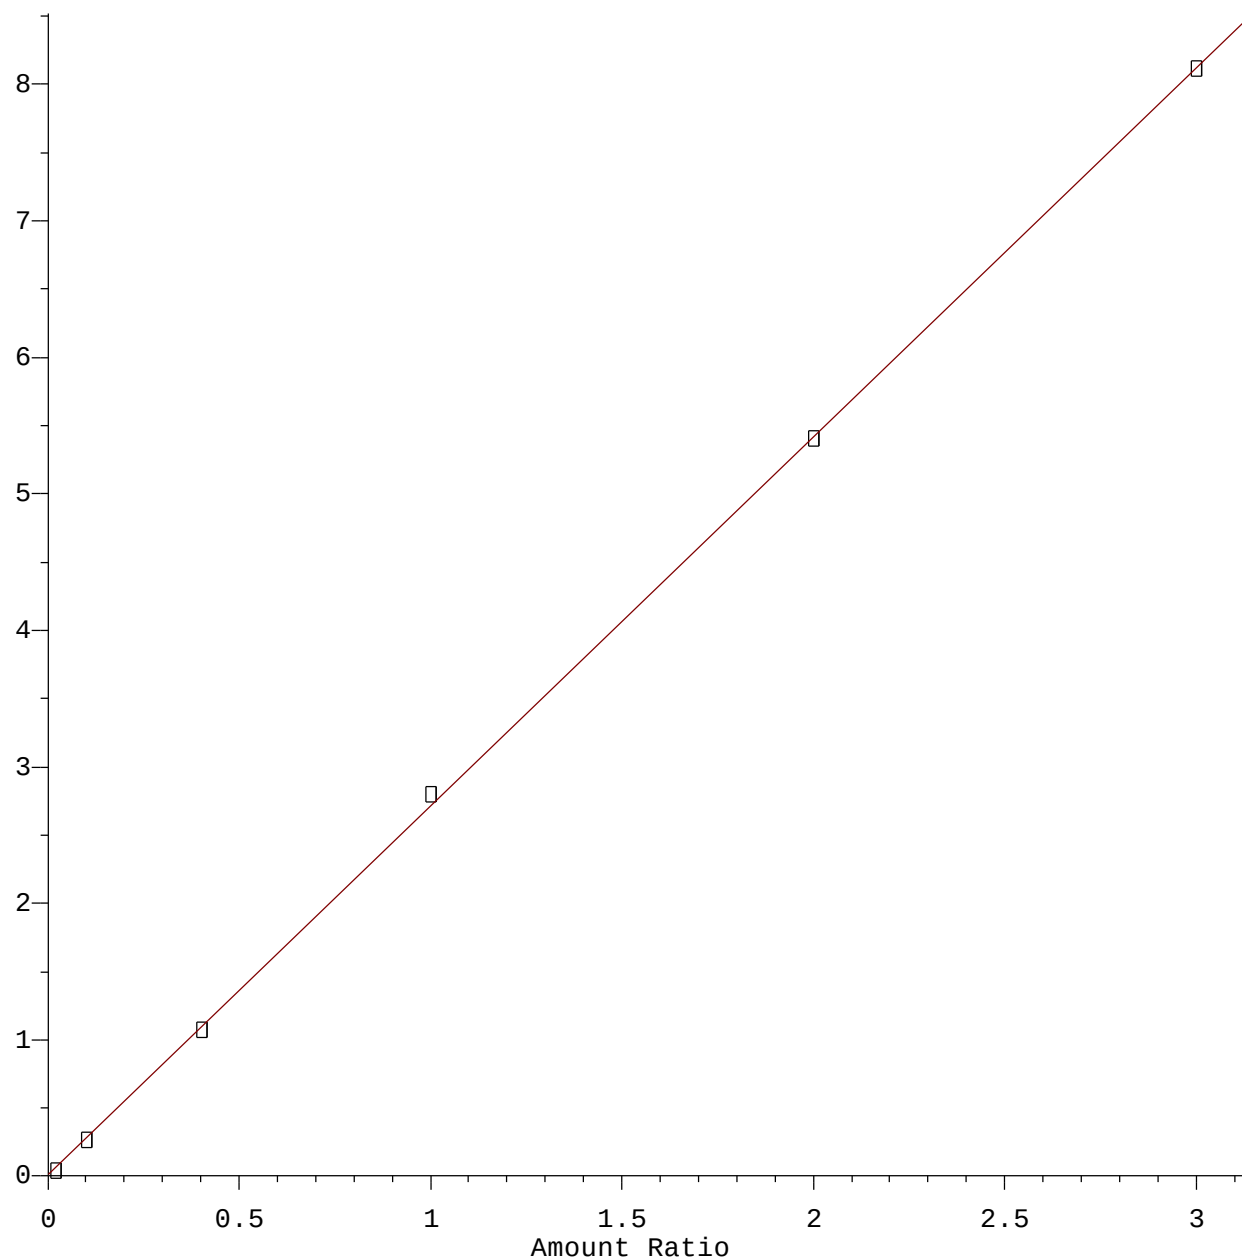


Resp Ratio = 2.71e+000 * Amt + 6.50e-003
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X110718W.M
Calibration Table Last Updated: Fri Nov 09 14:02:25 2018

Naphthalene

Response Ratio

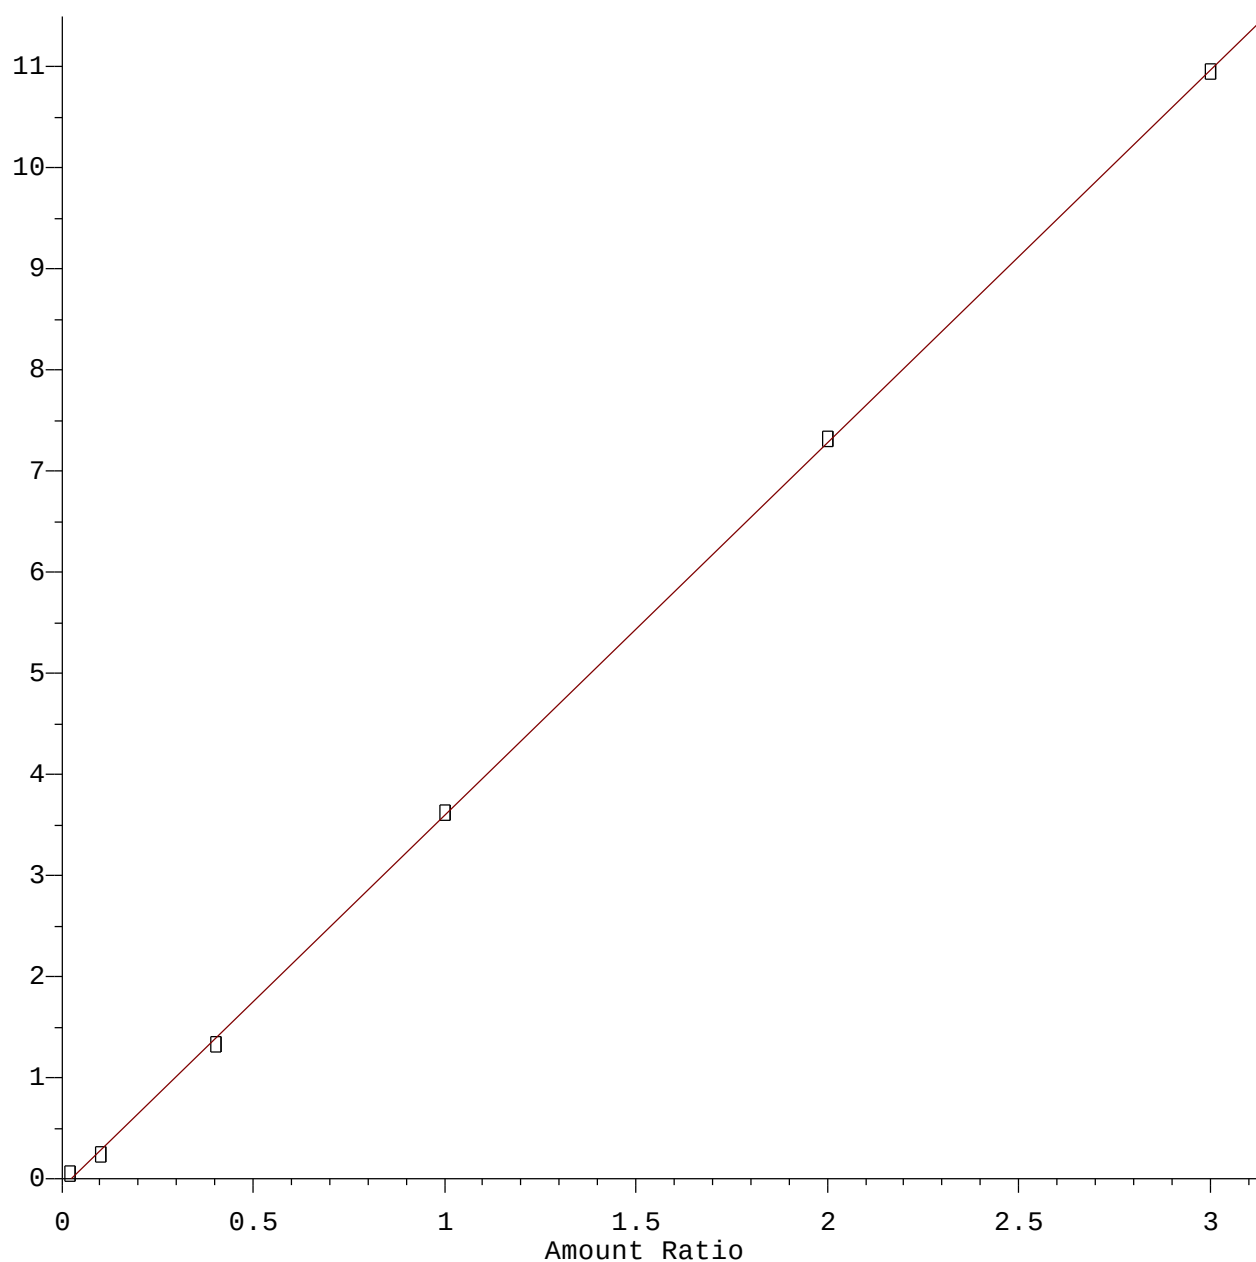

Resp Ratio = 3.68e+000 * Amt - 8.67e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X110718W.M
Calibration Table Last Updated: Fri Nov 09 14:02:25 2018