

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110718\
 Data File : VX005834.D
 Acq On : 07 Nov 2018 18:11
 Operator : JC/MD
 Sample : J5848-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S81-0100

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X110718W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.325	21	28	32	rBV3	47160	111925	22.84%	2.139%
2	1.581	68	70	76	rVB3	6567	10716	2.19%	0.205%
3	1.788	100	104	116	rVB2	21458	36026	7.35%	0.688%
4	2.001	135	139	149	rVB	18711	28438	5.80%	0.543%
5	2.398	197	204	207	rBV3	4797	9085	1.85%	0.174%
6	2.440	207	211	215	rVV	19675	32779	6.69%	0.626%
7	2.483	215	218	227	rVB	18768	31038	6.33%	0.593%
8	2.580	229	234	235	rBV2	3412	5248	1.07%	0.100%
9	2.617	235	240	250	rVB	15533	30850	6.30%	0.590%
10	2.843	271	277	280	rBV3	8254	16828	3.43%	0.322%
11	2.891	280	285	289	rVV	19080	41421	8.45%	0.792%
12	2.928	289	291	304	rVB2	12446	22934	4.68%	0.438%
13	3.166	323	330	343	rVB2	20942	51690	10.55%	0.988%
14	3.519	381	388	400	rVB	9669	22017	4.49%	0.421%
15	4.306	509	517	522	rBV3	1974	5393	1.10%	0.103%
16	4.397	522	532	545	rVB2	22703	66185	13.51%	1.265%
17	4.592	557	564	575	rVB4	4099	12155	2.48%	0.232%
18	5.232	655	669	680	rBV8	2055	8648	1.77%	0.165%
19	5.501	700	713	720	rBV3	66680	189895	38.76%	3.629%
20	5.580	720	726	731	rVV5	22610	67266	13.73%	1.285%
21	5.665	731	740	767	rVB	120808	359761	73.43%	6.875%
22	5.927	773	783	796	rVB5	10183	34367	7.01%	0.657%
23	6.068	796	806	814	rVV3	72231	191143	39.01%	3.653%
24	6.141	816	818	826	rVV3	5278	10579	2.16%	0.202%
25	6.257	829	837	845	rVV5	6851	23868	4.87%	0.456%
26	6.354	845	853	861	rVV6	11351	35989	7.35%	0.688%
27	6.452	861	869	880	rVB3	8261	23197	4.73%	0.443%
28	6.860	926	936	957	rBV2	149318	369894	75.50%	7.069%
29	7.464	1025	1035	1046	rVB3	43537	106055	21.65%	2.027%
30	7.732	1073	1079	1086	rVB2	4396	8904	1.82%	0.170%
31	7.848	1092	1098	1106	rVB3	3670	7292	1.49%	0.139%
32	8.049	1121	1131	1139	rVB3	6129	18039	3.68%	0.345%
33	8.177	1144	1152	1161	rBV3	9821	21506	4.39%	0.411%
34	8.390	1181	1187	1192	rVB3	3389	6427	1.31%	0.123%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110718\
 Data File : VX005834.D
 Acq On : 07 Nov 2018 18:11
 Operator : JC/MD
 Sample : J5848-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S81-0100

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X110718W.M
 Title : SW846 8260

35	8.665	1226	1232	1234	rBV3	10328	17139	3.50%	0.328%
36	8.713	1234	1240	1249	rVV	298424	489953	100.00%	9.363%
37	8.787	1249	1252	1256	rVV2	4983	8215	1.68%	0.157%
38	8.835	1256	1260	1265	rVV	7857	14174	2.89%	0.271%
39	8.909	1269	1272	1278	rVB4	3432	5508	1.12%	0.105%
40	9.037	1288	1293	1299	rVB2	14656	24056	4.91%	0.460%
41	9.165	1306	1314	1320	rBB2	7267	11637	2.38%	0.222%
42	9.567	1374	1380	1385	rBV4	5211	9558	1.95%	0.183%
43	9.622	1385	1389	1393	rVB	8893	12234	2.50%	0.234%
44	9.677	1393	1398	1402	rBV	10192	14525	2.96%	0.278%
45	10.116	1464	1470	1478	rBV	289782	396692	80.97%	7.581%
46	10.183	1478	1481	1486	rVB	5583	8365	1.71%	0.160%
47	10.250	1486	1492	1502	rBV	72529	98133	20.03%	1.875%
48	10.360	1502	1510	1516	rVB	26504	43054	8.79%	0.823%
49	10.640	1549	1556	1560	rBV6	4397	9951	2.03%	0.190%
50	10.701	1560	1566	1578	rVB	191416	258093	52.68%	4.932%
51	10.835	1578	1588	1596	rVB3	7838	13029	2.66%	0.249%
52	10.914	1596	1601	1605	rBV4	3374	6073	1.24%	0.116%
53	11.018	1613	1618	1622	rBV	8028	10746	2.19%	0.205%
54	11.140	1632	1638	1643	rBV	248785	323616	66.05%	6.184%
55	11.183	1643	1645	1651	rVB2	4557	5604	1.14%	0.107%
56	11.274	1657	1660	1665	rVB4	4714	7115	1.45%	0.136%
57	11.359	1670	1674	1678	rBV	9706	12364	2.52%	0.236%
58	11.457	1687	1690	1694	rVB	5179	6007	1.23%	0.115%
59	11.670	1719	1725	1732	rBV	87836	117514	23.98%	2.246%
60	11.804	1743	1747	1753	rVB	53637	69070	14.10%	1.320%
61	11.945	1767	1770	1775	rVB	4688	6099	1.24%	0.117%
62	12.024	1775	1783	1787	rBV	13679	17480	3.57%	0.334%
63	12.079	1787	1792	1798	rBV	332271	409946	83.67%	7.834%
64	12.140	1798	1802	1811	rVB	97735	125356	25.59%	2.396%
65	12.231	1811	1817	1821	rVB	4828	5980	1.22%	0.114%
66	12.298	1824	1828	1831	rBV	30915	41032	8.37%	0.784%
67	12.365	1836	1839	1849	rVB4	12094	22465	4.59%	0.429%
68	12.463	1849	1855	1859	rBV2	11939	16445	3.36%	0.314%
69	12.518	1859	1864	1870	rVV	30572	37630	7.68%	0.719%
70	12.585	1870	1875	1877	rVV	9845	11942	2.44%	0.228%
71	12.609	1877	1879	1882	rVV2	9715	11133	2.27%	0.213%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110718\
 Data File : VX005834.D
 Acq On : 07 Nov 2018 18:11
 Operator : JC/MD
 Sample : J5848-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S81-0100

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X110718W.M
 Title : SW846 8260

72	12.670	1885	1889	1892	rVV	13027	16983	3.47%	0.325%
73	12.701	1892	1894	1899	rVV2	6884	10117	2.06%	0.193%
74	12.755	1899	1903	1911	rVV4	22442	48393	9.88%	0.925%
75	12.853	1915	1919	1921	rVV2	5315	8020	1.64%	0.153%
76	12.902	1923	1927	1932	rVV2	22610	31565	6.44%	0.603%
77	12.975	1932	1939	1943	rVV2	20579	31809	6.49%	0.608%
78	13.018	1943	1946	1953	rVV2	15304	22958	4.69%	0.439%
79	13.085	1953	1957	1963	rVB2	7092	10580	2.16%	0.202%
80	13.194	1971	1975	1978	rBV3	9544	12750	2.60%	0.244%
81	13.225	1978	1980	1983	rVV	4760	5719	1.17%	0.109%
82	13.304	1989	1993	1995	rBV2	5989	7203	1.47%	0.138%
83	13.347	1995	2000	2005	rVV2	59364	88015	17.96%	1.682%
84	13.389	2005	2007	2011	rVV3	4076	5724	1.17%	0.109%
85	13.481	2015	2022	2031	rVB	23317	35089	7.16%	0.671%
86	13.560	2031	2035	2038	rBV3	4141	6024	1.23%	0.115%
87	13.603	2038	2042	2044	rVV	4631	6270	1.28%	0.120%
88	13.639	2044	2048	2053	rVV4	15749	29193	5.96%	0.558%
89	13.700	2055	2058	2059	rVV	6918	9115	1.86%	0.174%
90	13.719	2059	2061	2066	rVB2	11022	13932	2.84%	0.266%
91	13.835	2077	2080	2087	rVB2	12480	23355	4.77%	0.446%
92	13.914	2087	2093	2098	rVB3	7176	11074	2.26%	0.212%
93	13.987	2098	2105	2109	rBV2	11046	16710	3.41%	0.319%
94	14.030	2109	2112	2116	rBV3	4505	5501	1.12%	0.105%
95	14.133	2124	2129	2132	rBV3	3640	5273	1.08%	0.101%
96	14.273	2148	2152	2159	rVB3	9379	17365	3.54%	0.332%
97	14.432	2174	2178	2182	rVB3	5226	6165	1.26%	0.118%
98	14.542	2191	2196	2204	rVB2	12460	18210	3.72%	0.348%
99	14.840	2238	2245	2249	rBV2	5217	8601	1.76%	0.164%
100	15.249	2306	2312	2321	rVB6	3113	5704	1.16%	0.109%


Sum of corrected areas: 5232908

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110718\
Data File : VX005834.D
Acq On : 07 Nov 2018 18:11
Operator : JC/MD
Sample : J5848-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S81-0100

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X110718W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

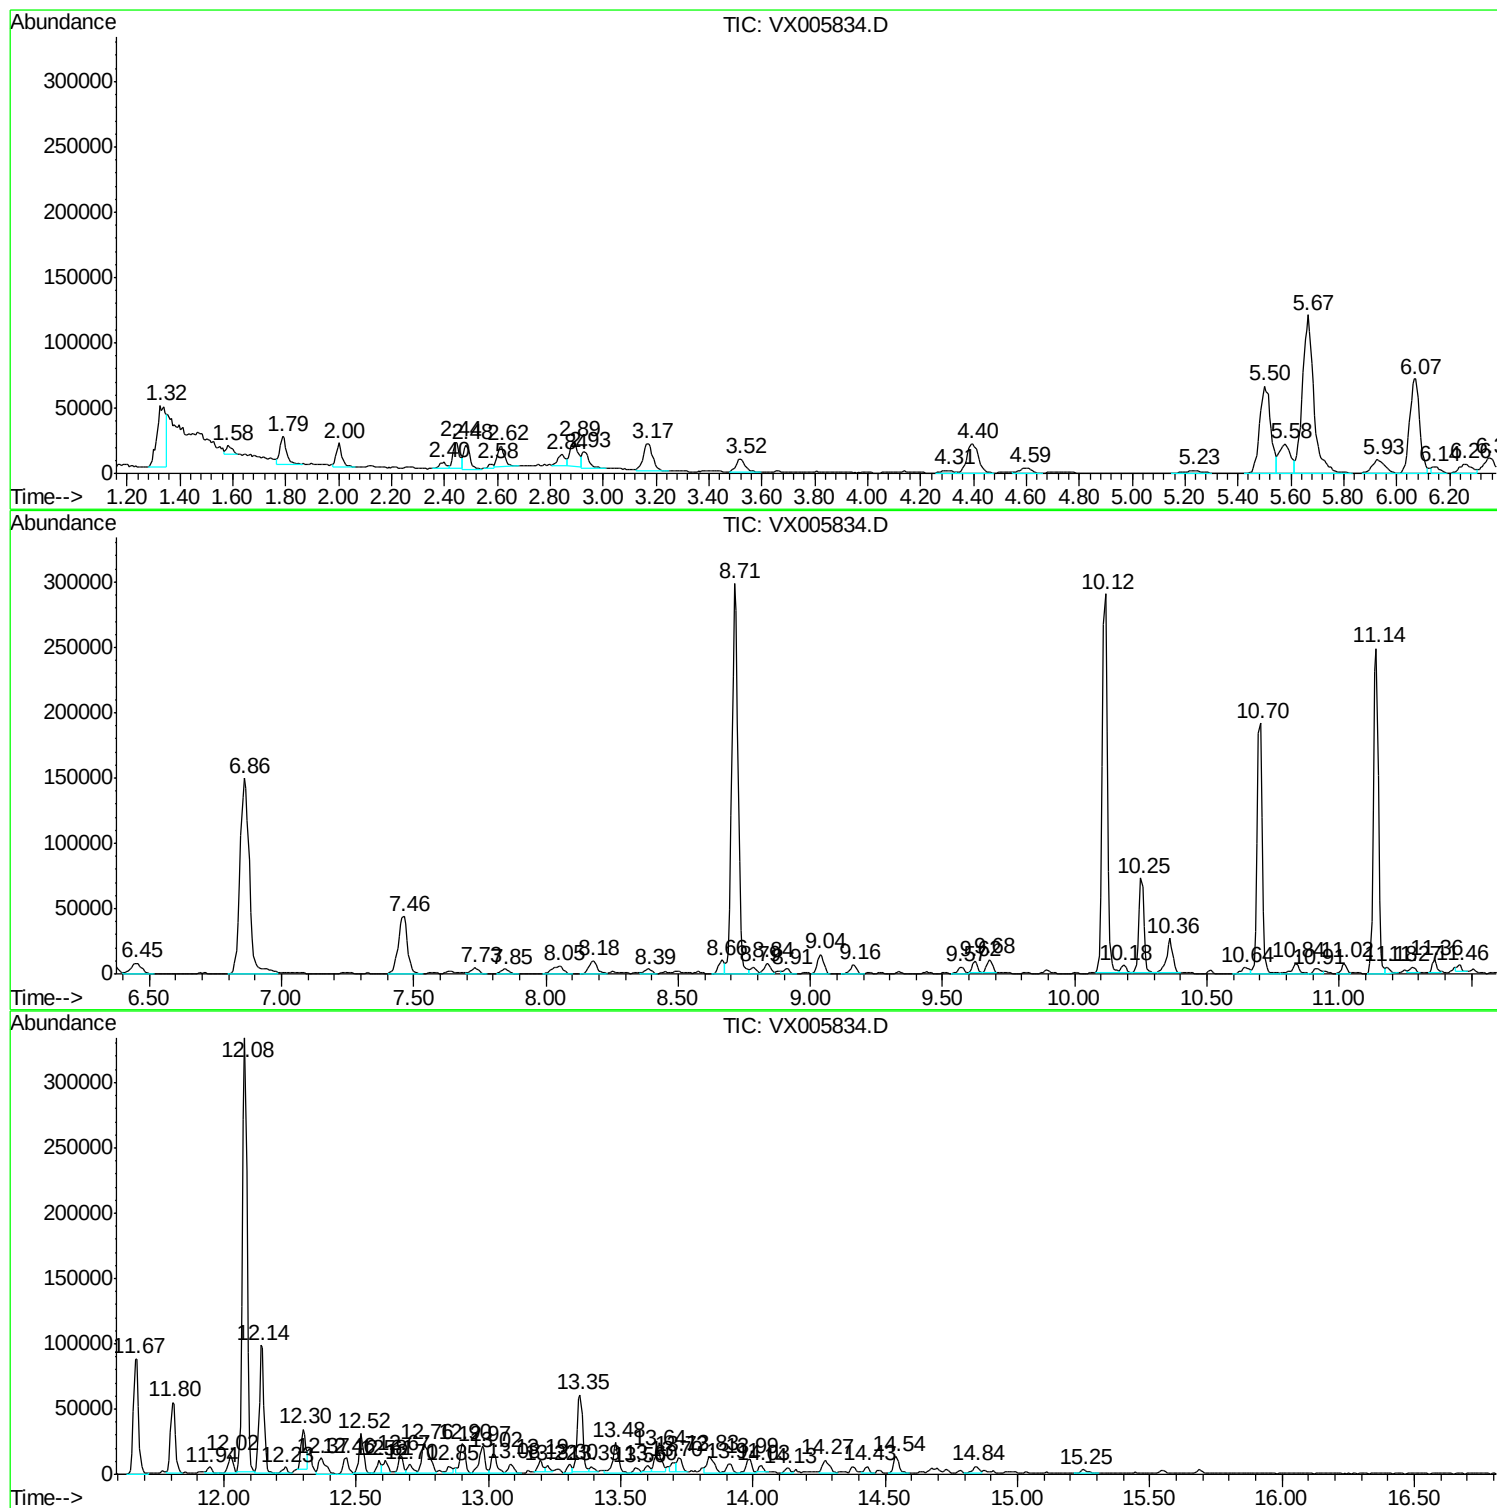

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110718\
Data File : VX005834.D
Acq On : 07 Nov 2018 18:11
Operator : JC/MD
Sample : J5848-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S81-0100

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X110718W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110718\
Data File : VX005834.D
Acq On : 07 Nov 2018 18:11
Operator : JC/MD
Sample : J5848-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S81-0100

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X110718W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc