

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX110719\
 Data File : VX013344.D
 Acq On : 07 Nov 2019 11:11
 Operator : JC/SP
 Sample : VX1107WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1107WBL01

Quant Time: Nov 07 16:27:38 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
 Quant Title : SW846 8260
 QLast Update : Sat Nov 02 07:06:38 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	878511	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.84	114	1349323	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	1176792	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	509794	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.05	65	483091	46.42	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.84%	
35) Dibromofluoromethane	5.48	113	408259	48.24	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.48%	
50) Toluene-d8	8.71	98	1595442	50.01	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.02%	
62) 4-Bromofluorobenzene	11.13	95	526388	45.71	ug/l	0.00
Spiked Amount	50.000		Recovery	=	91.42%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX110719\
Data File : VX013344.D
Acq On : 07 Nov 2019 11:11
Operator : JC/SP
Sample : VX1107WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1107WBL01

Quant Time: Nov 07 16:27:38 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
Quant Title : SW846 8260
QLast Update : Sat Nov 02 07:06:38 2019
Response via : Initial Calibration

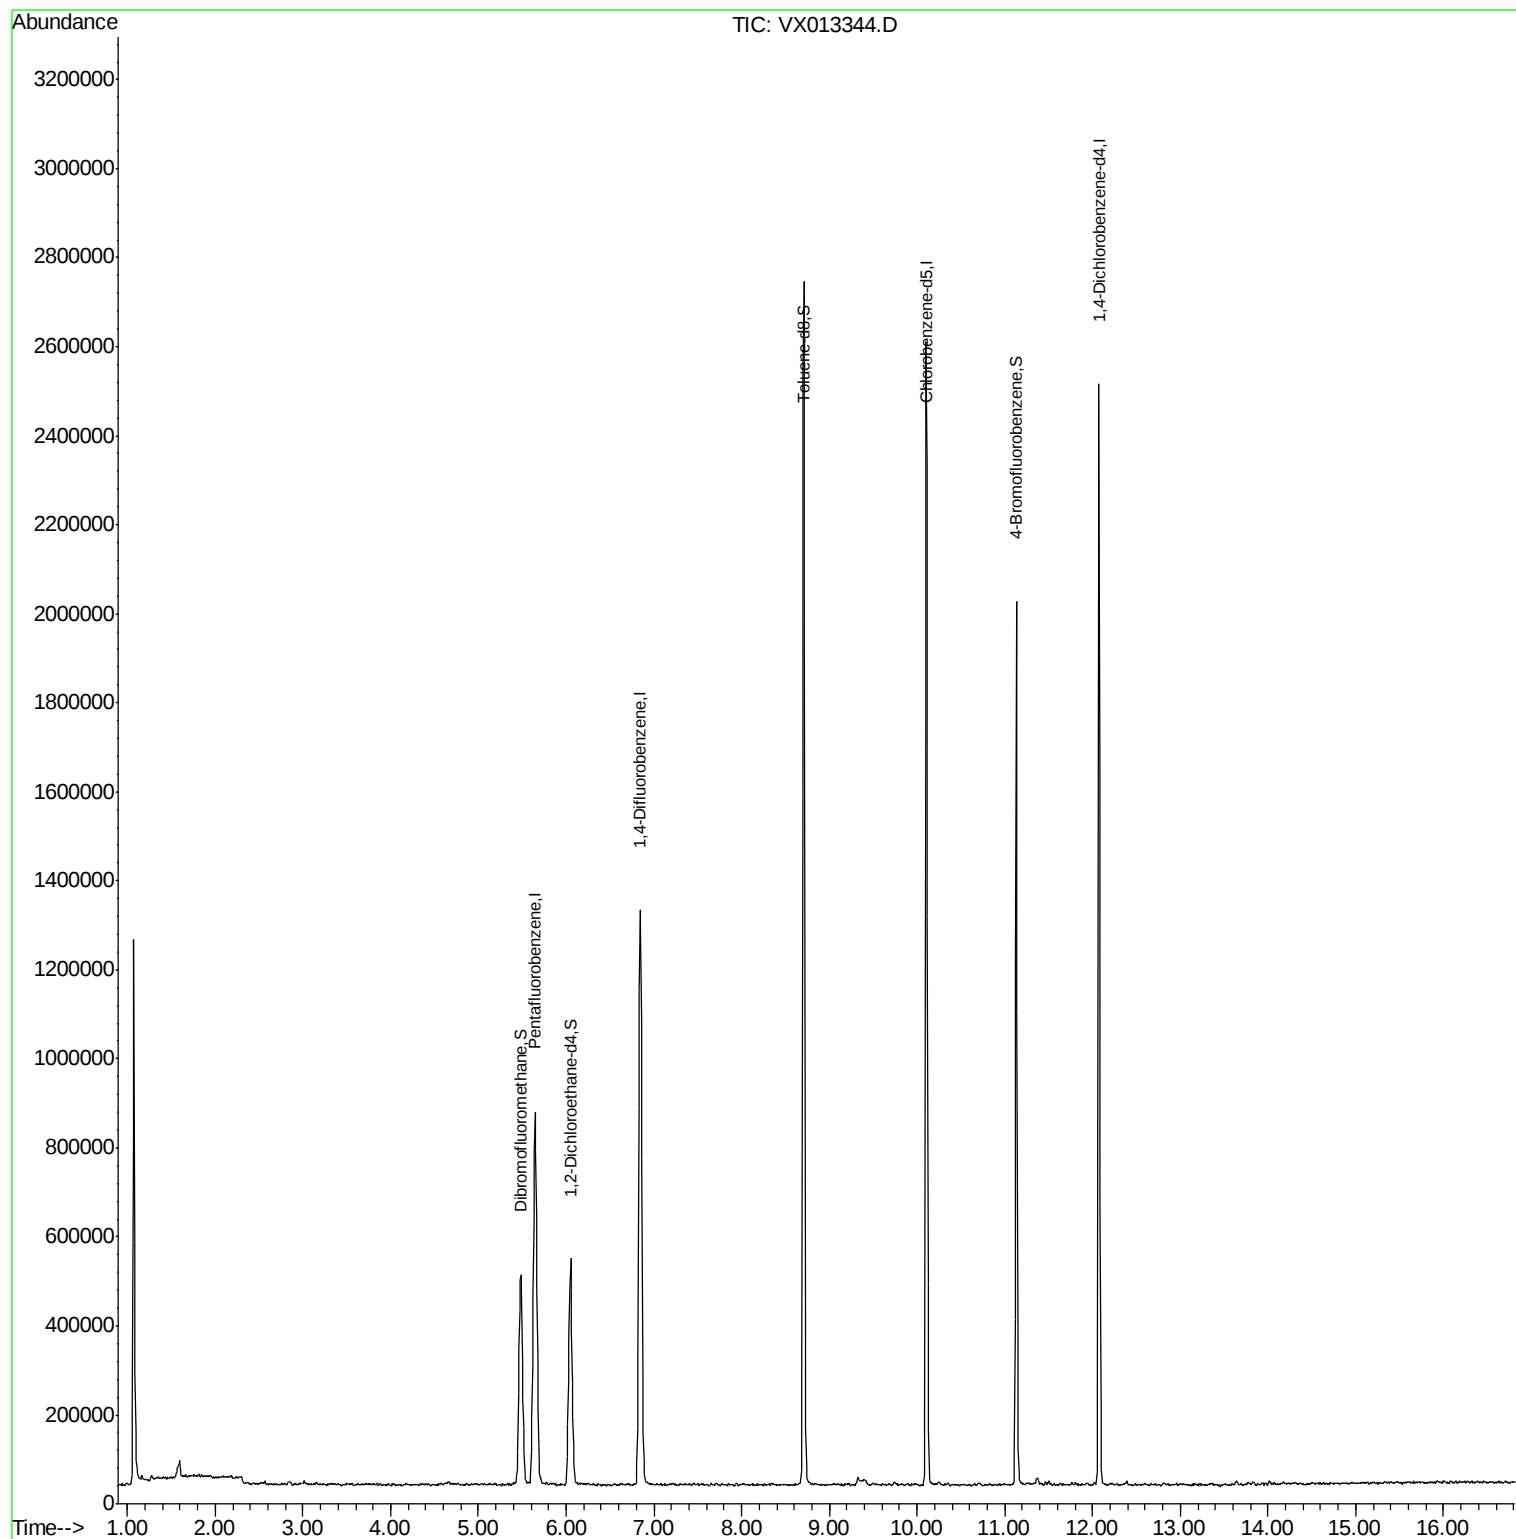

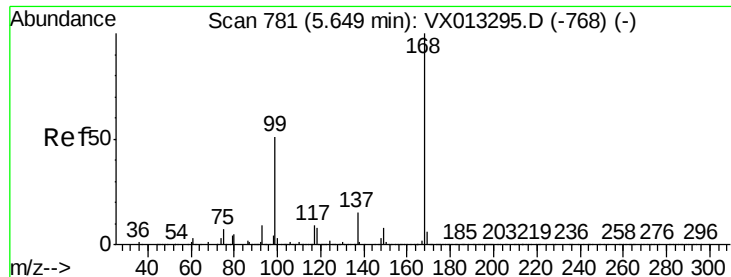

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 781

Delta R.T. -0.00 min

Lab File: VX013344.D

Acq: 07 Nov 2019 11:11

Instrument :

MSVOA_X

ClientSampleId :


VX1107WBL01

Tgt Ion:168 Resp: 878511

Ion Ratio Lower Upper




168 100

99 48.2 40.8 61.2

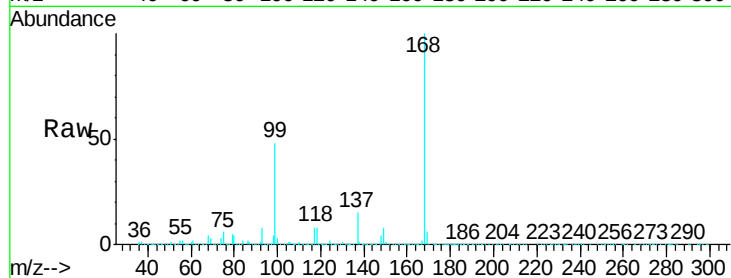

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

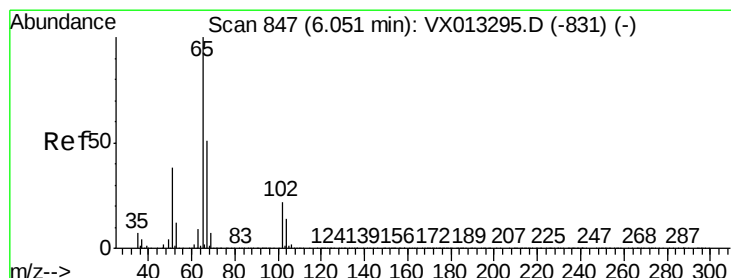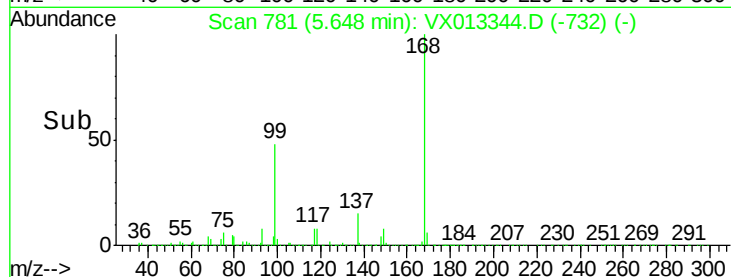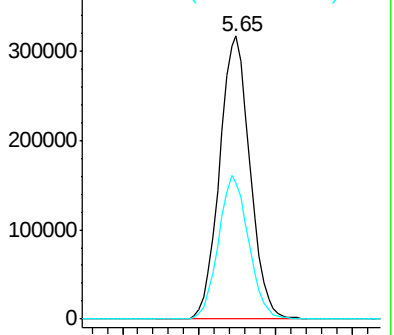

#33

1,2-Dichloroethane-d4

Concen: 46.416 ug/l

RT: 6.05 min Scan# 847

Delta R.T. -0.00 min

Lab File: VX013344.D


Acq: 07 Nov 2019 11:11

Tgt Ion: 65 Resp: 483091

Ion Ratio Lower Upper



65 100


67 52.7 0.0 104.2

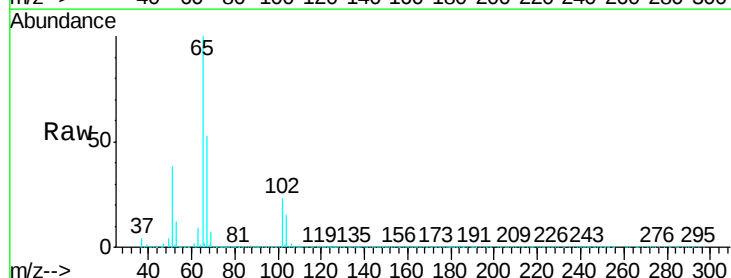

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

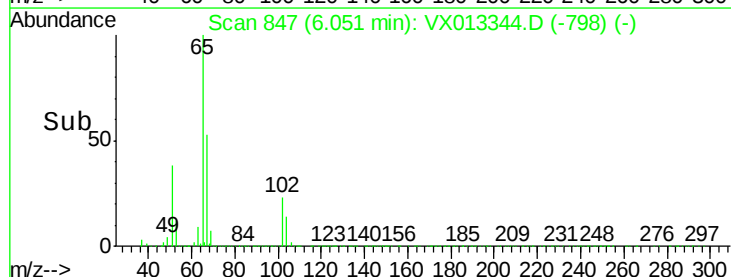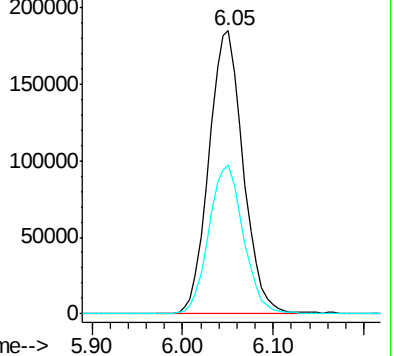

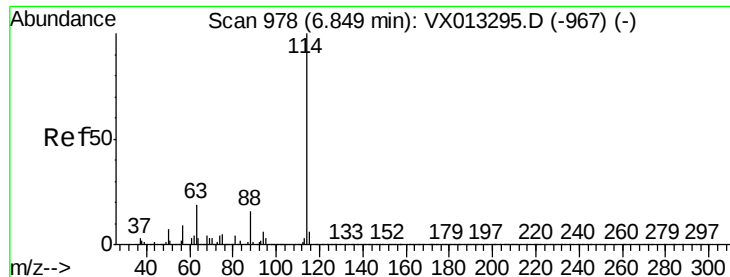

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.84 min Scan# 977

Delta R.T. -0.01 min

Lab File: VX013344.D

Acq: 07 Nov 2019 11:11

Instrument :

MSVOA_X

ClientSampleId :

VX1107WBL01


Tgt Ion:114 Resp: 1349323

Ion Ratio Lower Upper

114 100

63 20.4 0.0 38.4




88 15.5 0.0 32.2

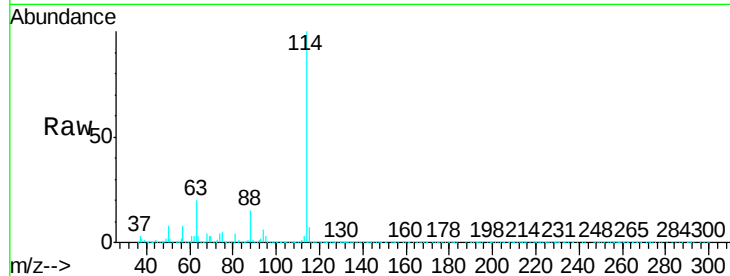

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

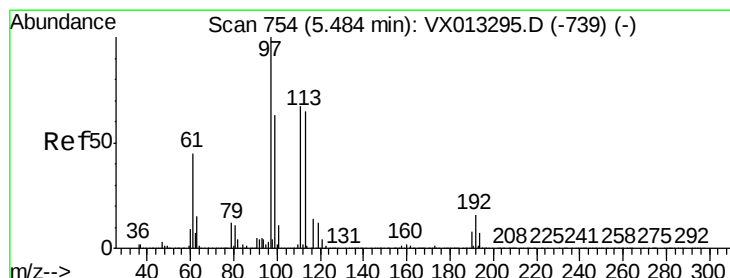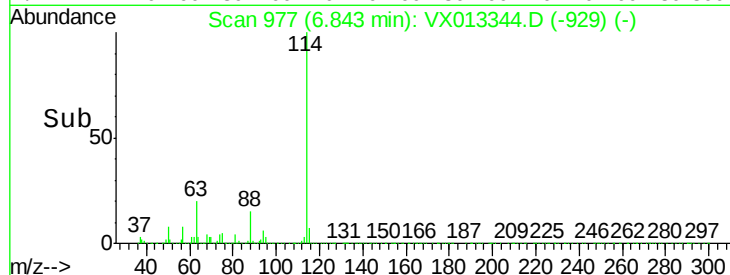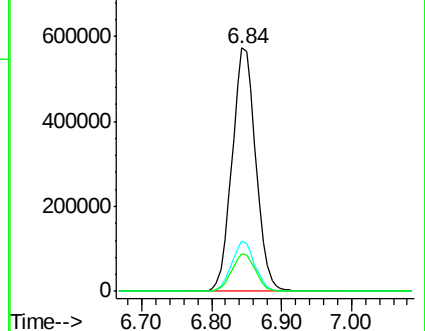

#35

Dibromofluoromethane

Concen: 48.240 ug/l

RT: 5.48 min Scan# 754

Delta R.T. -0.00 min

Lab File: VX013344.D

Acq: 07 Nov 2019 11:11


Tgt Ion:113 Resp: 408259

Ion Ratio Lower Upper

113 100

111 100.6 81.9 122.9



192 23.2 19.1 28.7

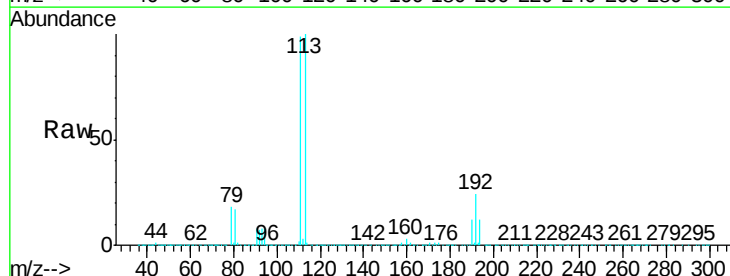


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

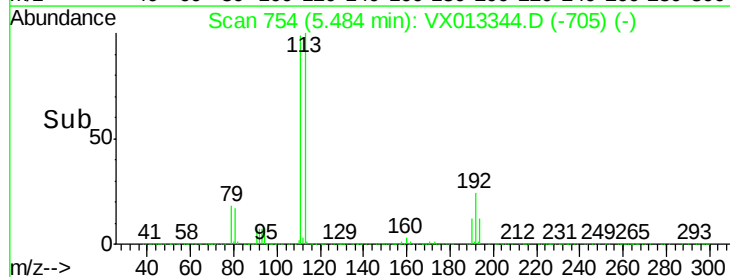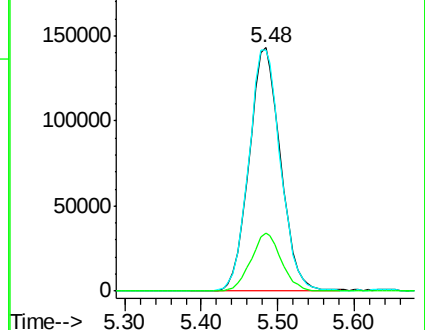

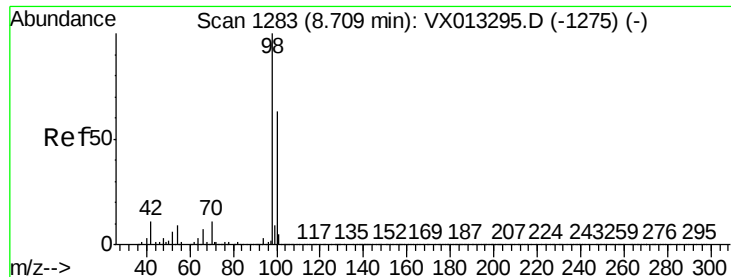

#50

Toluene-d8

Concen: 50.006 ug/l

RT: 8.71 min Scan# 1283

Delta R.T. -0.00 min

Lab File: VX013344.D

Acq: 07 Nov 2019 11:11

Instrument :

MSVOA_X

ClientSampleId :





VX1107WBL01

Tgt Ion: 98 Resp: 1595442

Ion Ratio Lower Upper

98 100

100 64.8 52.2 78.2

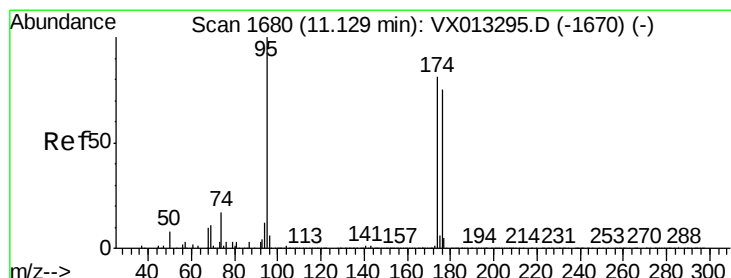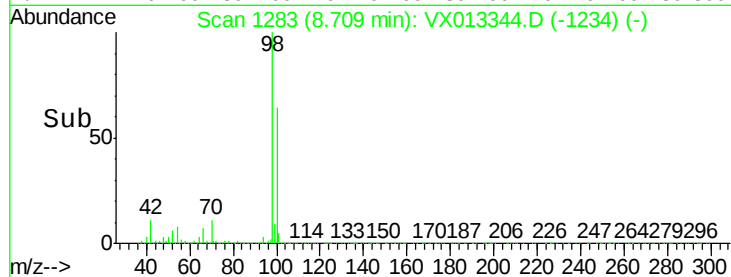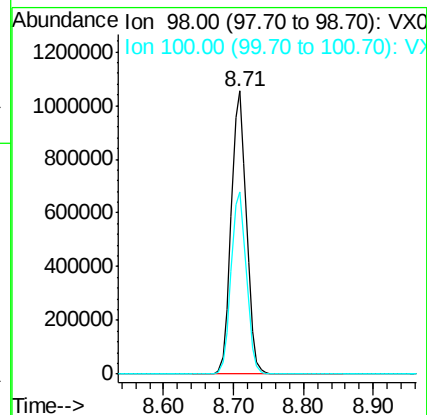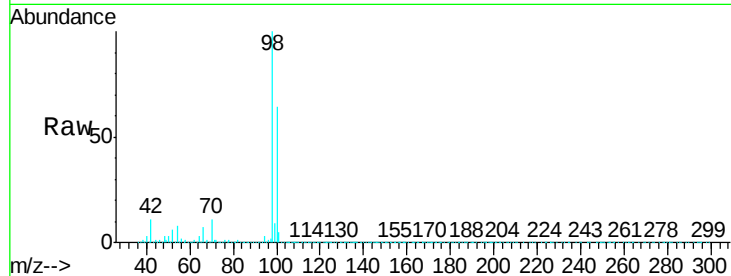

#62

4-Bromofluorobenzene

Concen: 45.714 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. -0.00 min

Lab File: VX013344.D

Acq: 07 Nov 2019 11:11




Tgt Ion: 95 Resp: 526388


Ion Ratio Lower Upper

95 100

174 89.1 0.0 179.8

176 86.8 0.0 173.0

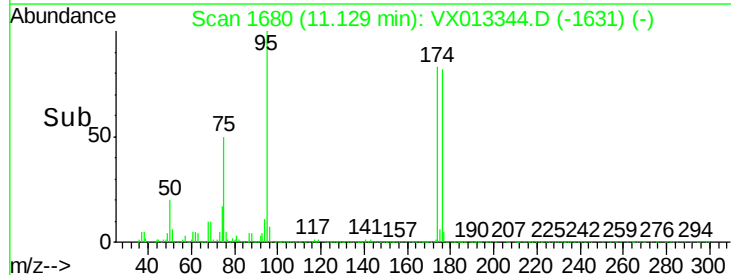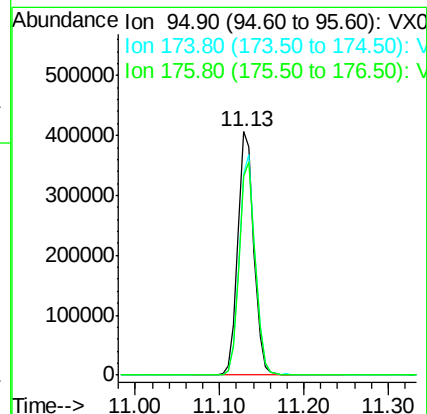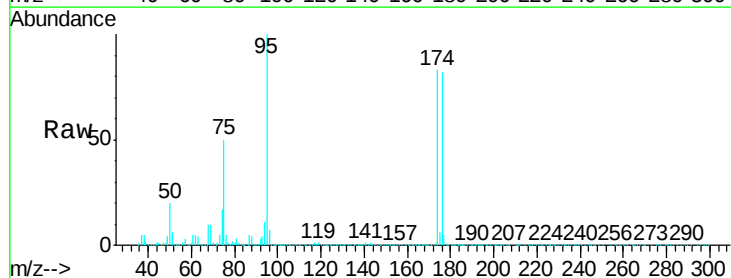


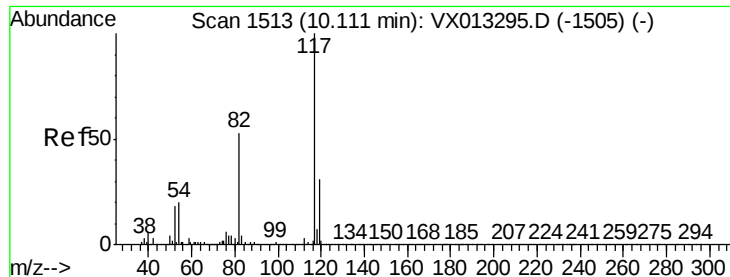




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1512
Delta R.T. -0.01 min
Lab File: VX013344.D
Acq: 07 Nov 2019 11:11

Instrument :
MSVOA_X
ClientSampleId :
VX1107WBL01

Tgt Ion:117 Resp: 1176792
Ion Ratio Lower Upper
117 100
82 55.4 42.6 64.0
119 32.0 24.8 37.2

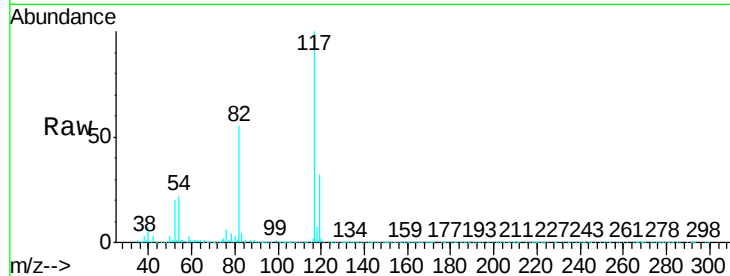


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

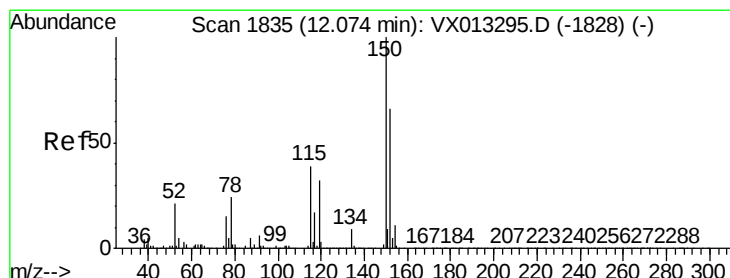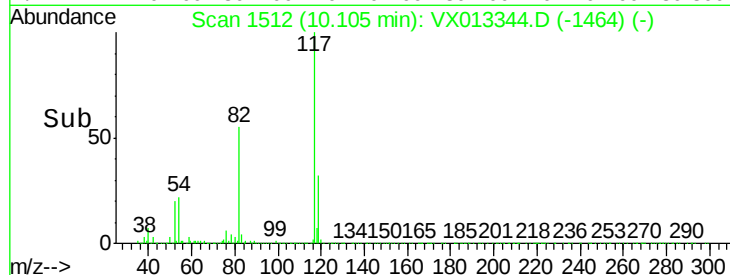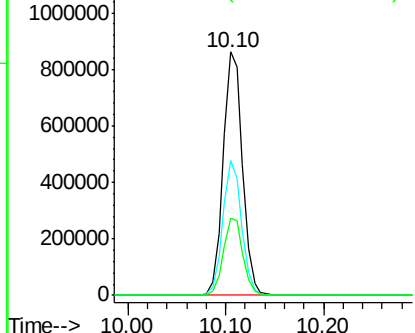

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.07 min Scan# 1835
Delta R.T. -0.00 min
Lab File: VX013344.D
Acq: 07 Nov 2019 11:11

Tgt Ion:152 Resp: 509794
Ion Ratio Lower Upper
152 100
115 55.7 39.5 118.3
150 157.6 0.0 344.4

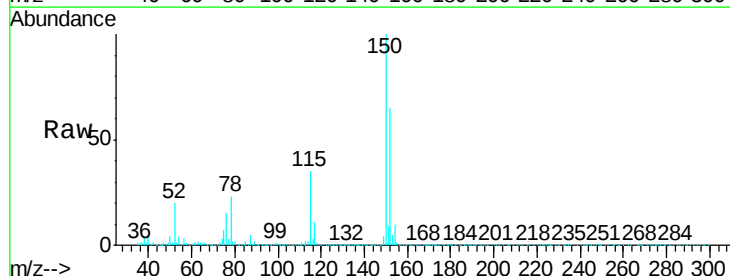

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

