


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX110719\
Data File : VX013342.D
Acq On : 07 Nov 2019 09:16
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
Title : SW846 8260
Last Update : Sat Nov 02 07:06:38 2019

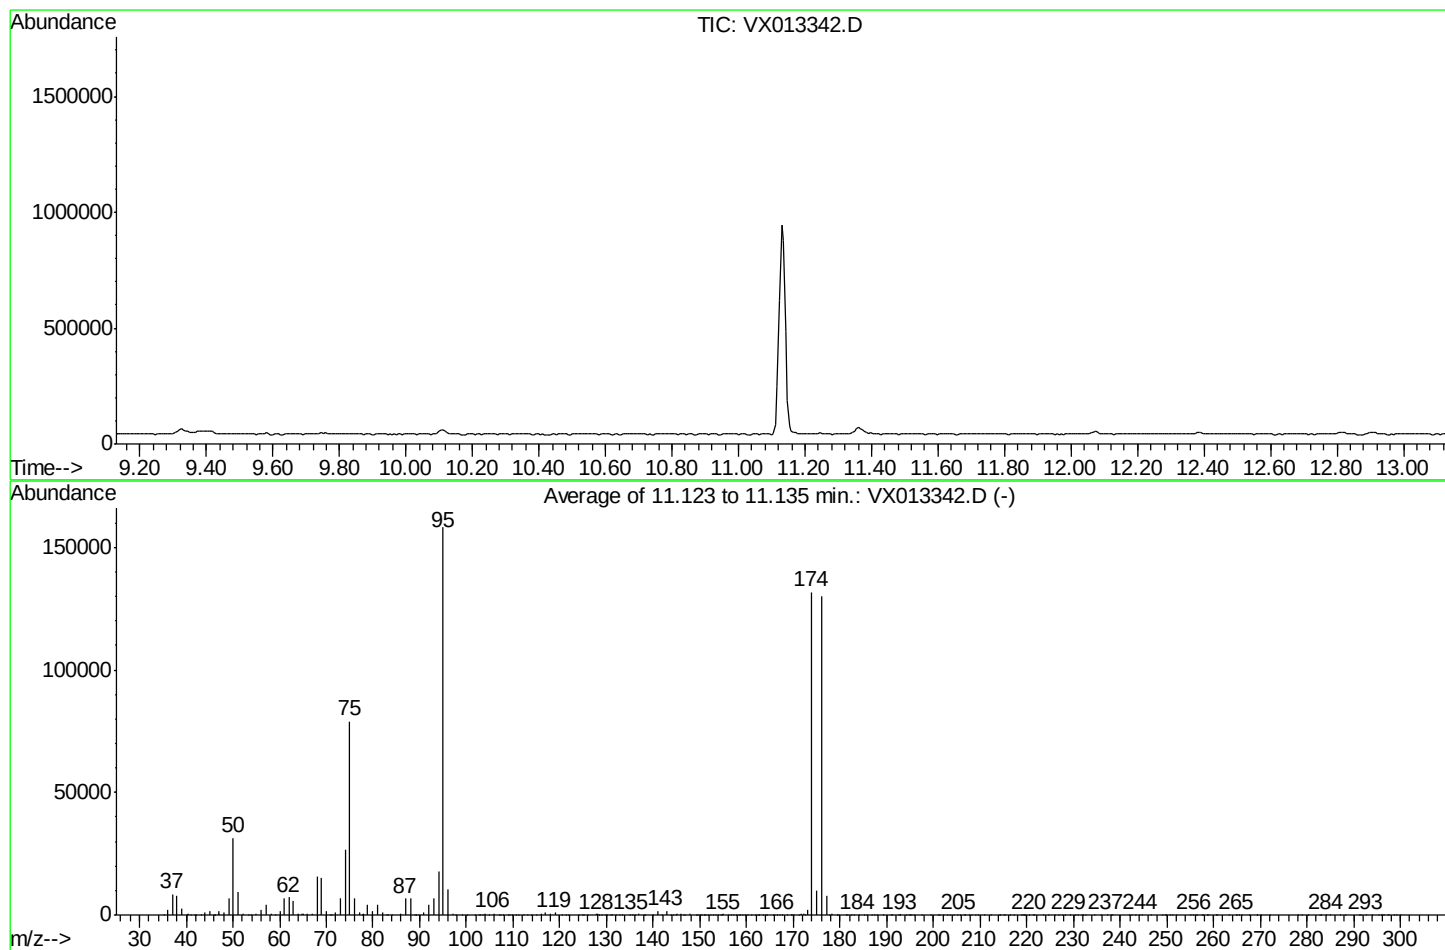

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1671

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	31508	PASS
75	95	30	60	49.9	78935	PASS
95	95	100	100	100.0	158225	PASS
96	95	5	9	6.8	10687	PASS
173	174	0.00	2	1.4	1883	PASS
174	95	50	100	83.3	131860	PASS
175	174	5	9	7.7	10105	PASS
176	174	95	101	98.6	130070	PASS
177	176	5	9	5.9	7676	PASS