

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX110720\
 Data File : VX019333.D
 Acq On : 06 Nov 2020 11:59
 Operator : JC/MD
 Sample : L4656-15
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-11-5-2020

Quant Time: Nov 07 01:40:06 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X102720W.M
 Quant Title : SW846 8260
 QLast Update : Tue Oct 27 13:55:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	301988	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	519265	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	478991	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	238740	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.03	65	204731	52.57	ug/l	0.00
Spiked Amount	50.000		Recovery	=	105.14%	
35) Dibromofluoromethane	5.46	113	161009	49.36	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.72%	
50) Toluene-d8	8.70	98	627095	51.00	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.00%	
62) 4-Bromofluorobenzene	11.12	95	243363	52.26	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.52%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX110720\
Data File : VX019333.D
Acq On : 06 Nov 2020 11:59
Operator : JC/MD
Sample : L4656-15
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampled :
TB-11-5-2020

Quant Time: Nov 07 01:40:06 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X102720W.M
Quant Title : SW846 8260
QLast Update : Tue Oct 27 13:55:07 2020
Response via : Initial Calibration

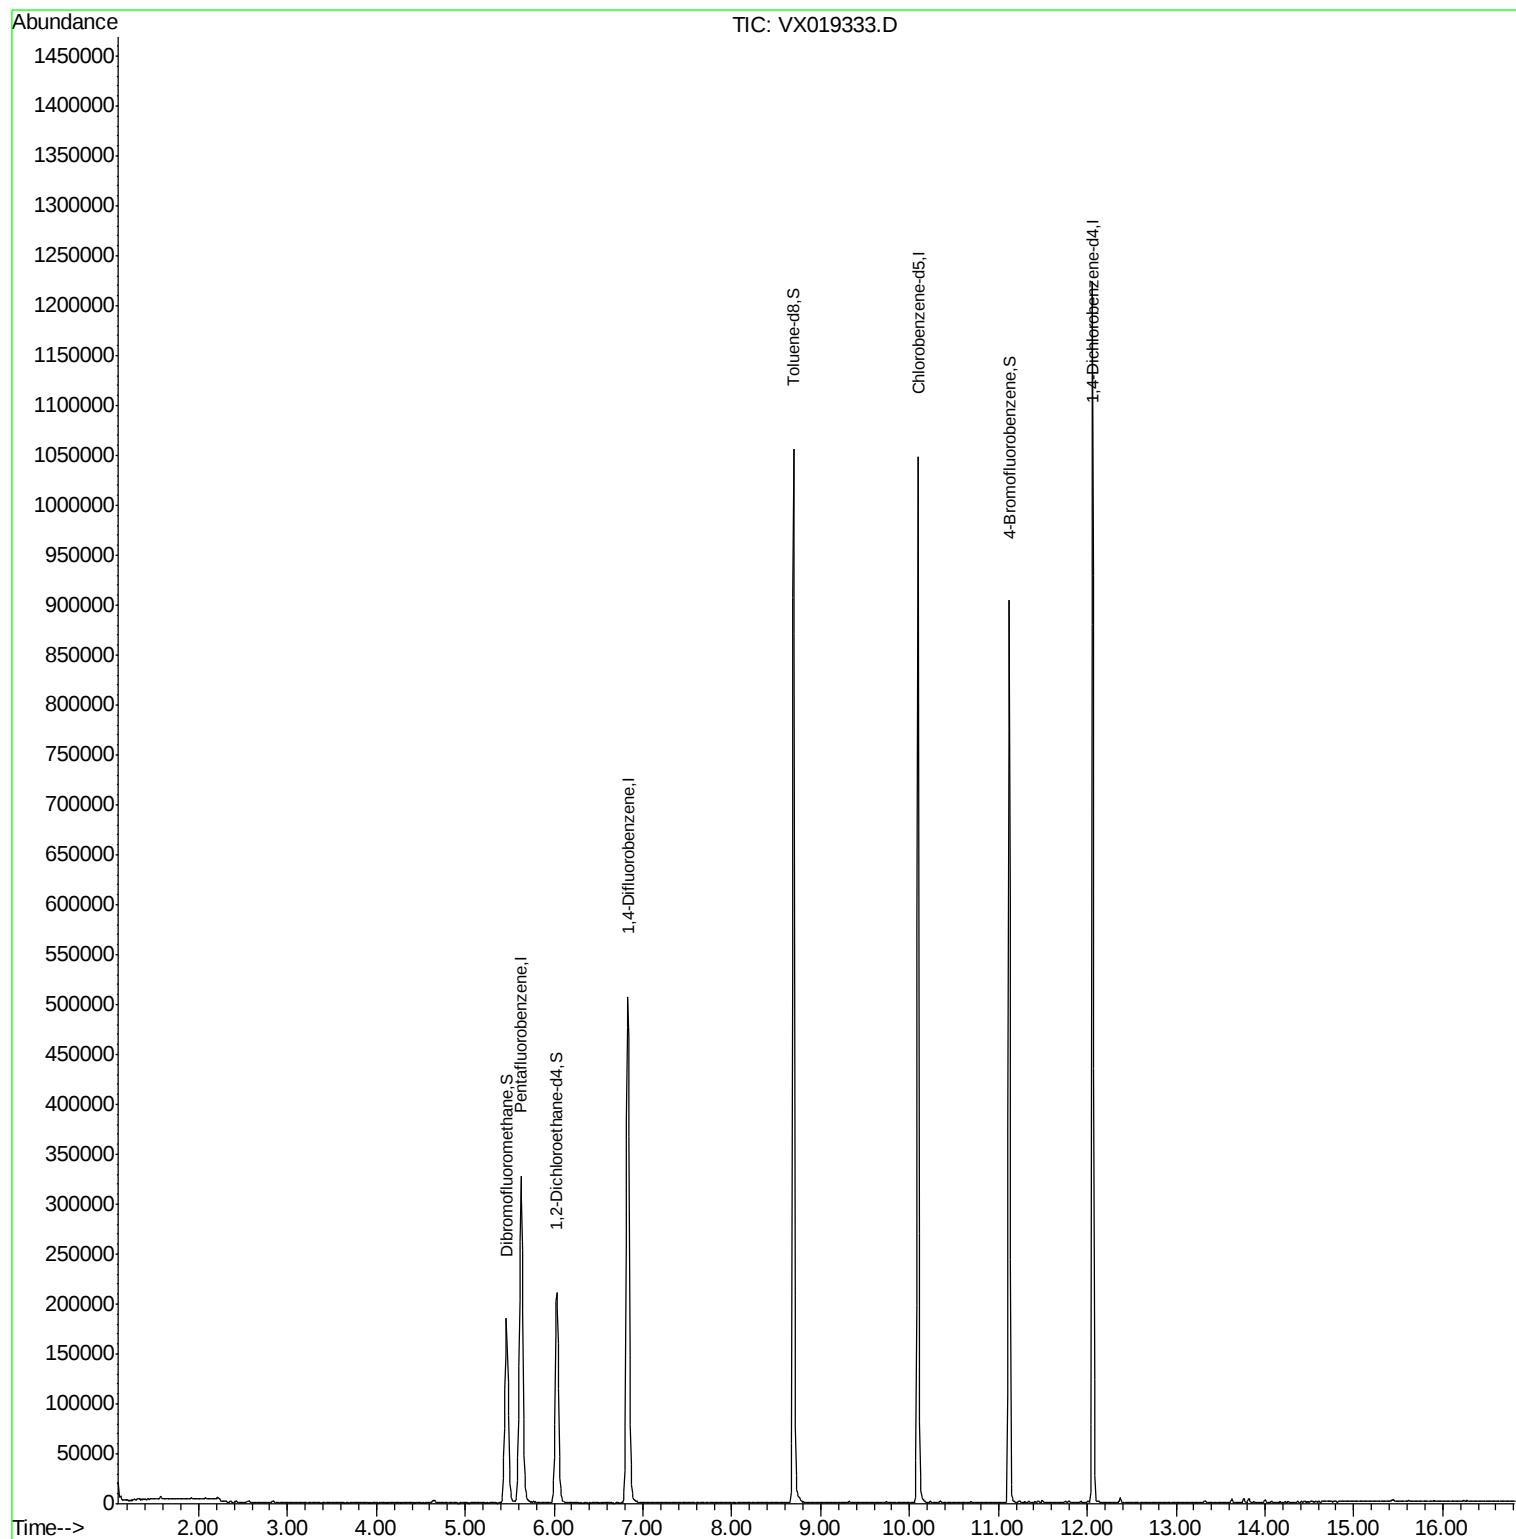

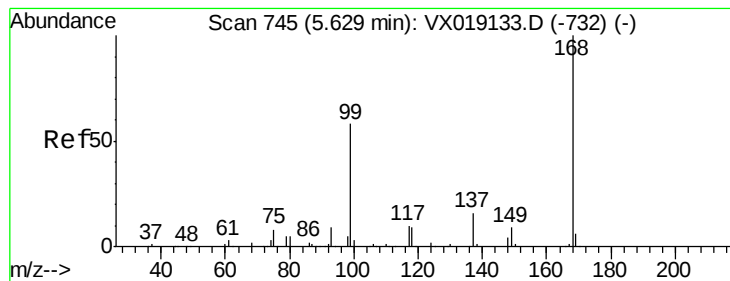

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. 0.00 min

Lab File: VX019333.D

Acq: 06 Nov 2020 11:59

Instrument :

MSVOA_X

ClientSampleId :


TB-11-5-2020

Tot Ion:168 Resp: 301988

Ion Ratio Lower Upper

168 100

99 60.0 46.6 69.8

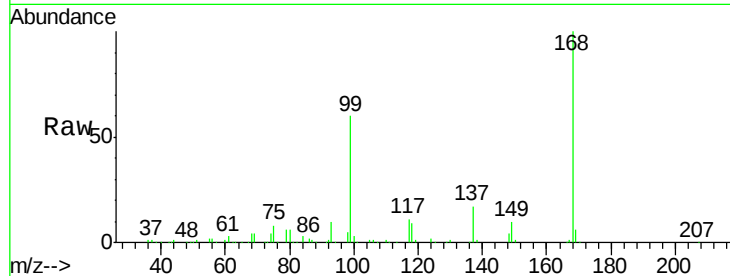

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.63

120000

100000

80000

60000



40000

20000

0

Time-->

5.50 5.60 5.70 5.80

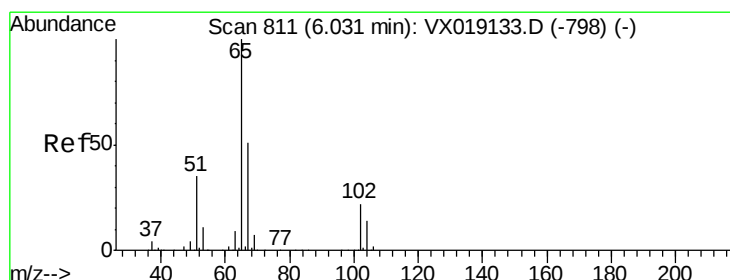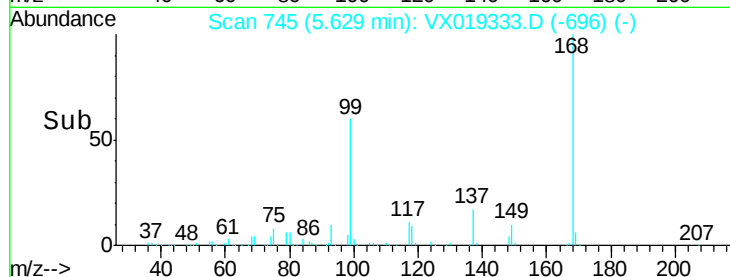

#33

1,2-Dichloroethane-d4

Concen: 52.569 ug/l

RT: 6.03 min Scan# 811

Delta R.T. 0.00 min

Lab File: VX019333.D


Acq: 06 Nov 2020 11:59

Tgt Ion: 65 Resp: 204731

Ion Ratio Lower Upper

65 100

67 51.2 0.0 103.0

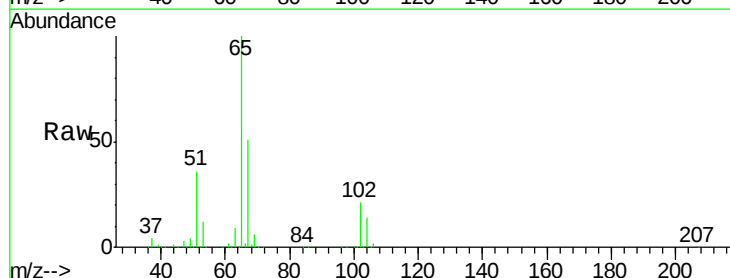

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.03

80000

60000


40000


20000

0

Time-->

5.90 6.00 6.10 6.20

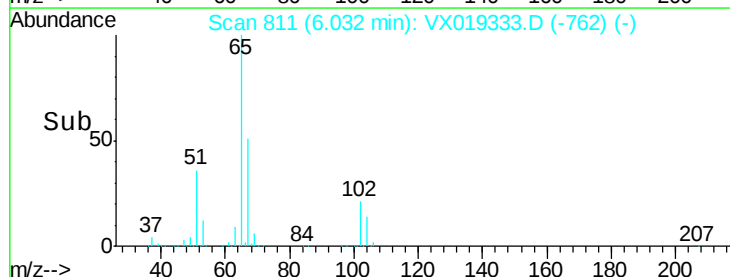

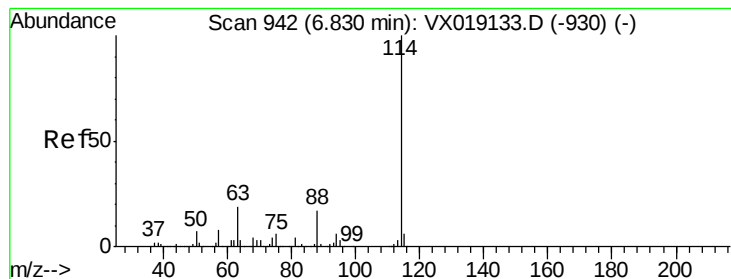

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. 0.00 min

Lab File: VX019333.D

Acq: 06 Nov 2020 11:59

Instrument :

MSVOA_X

ClientSampleId :

TB-11-5-2020


Tot Ion:114 Resp: 519265

Ion Ratio Lower Upper

114 100

63 20.7 0.0 38.8




88 16.5 0.0 34.2

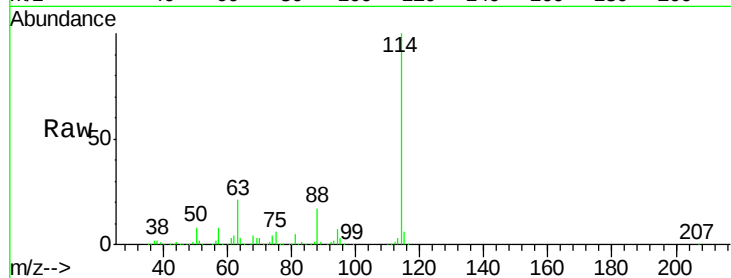

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

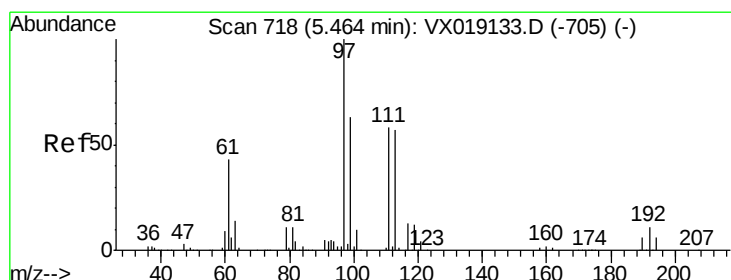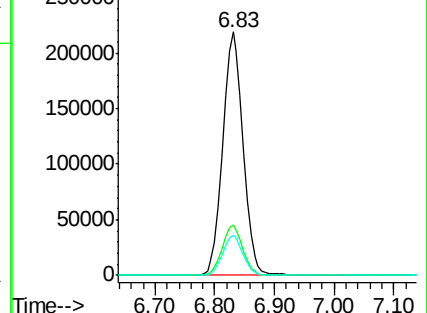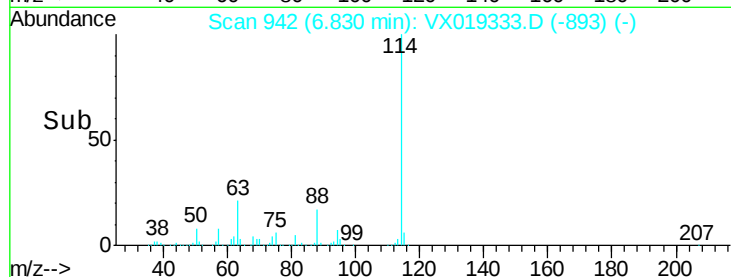

#35

Dibromofluoromethane

Concen: 49.364 ug/l

RT: 5.46 min Scan# 718

Delta R.T. 0.00 min

Lab File: VX019333.D

Acq: 06 Nov 2020 11:59


Tgt Ion:113 Resp: 161009

Ion Ratio Lower Upper

113 100

111 103.3 82.3 123.5



192 19.7 16.2 24.2

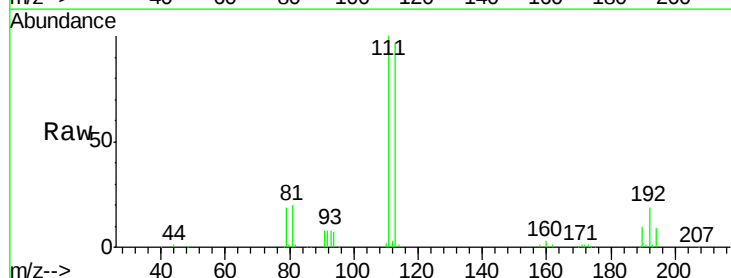


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



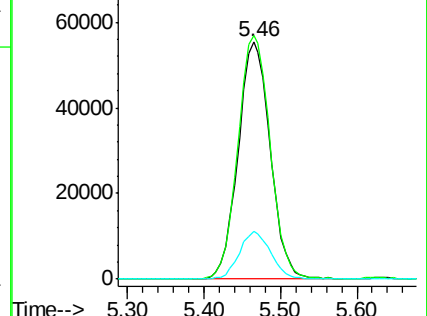
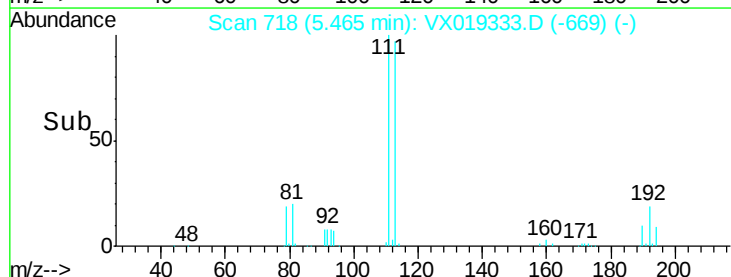


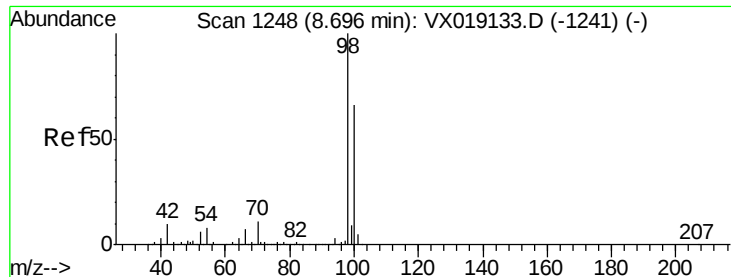

#50
Toluene-d8
Concen: 51.002 ug/l
RT: 8.70 min Scan# 1248
Delta R.T. 0.00 min
Lab File: VX019333.D
Acq: 06 Nov 2020 11:59




Instrument :
MSVOA_X
ClientSampleId :
TB-11-5-2020


Tot Ion: 98 Resp: 627095
Ion Ratio Lower Upper
98 100
100 65.7 53.0 79.6

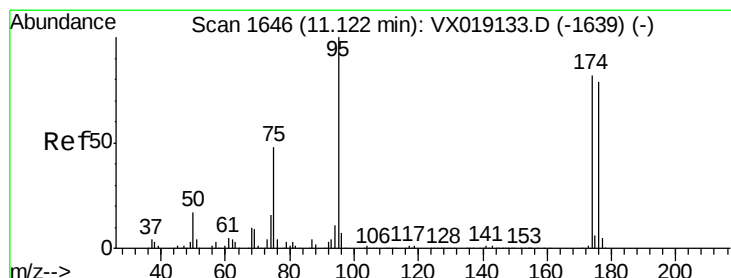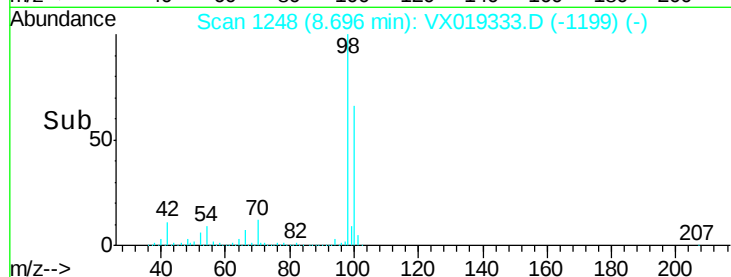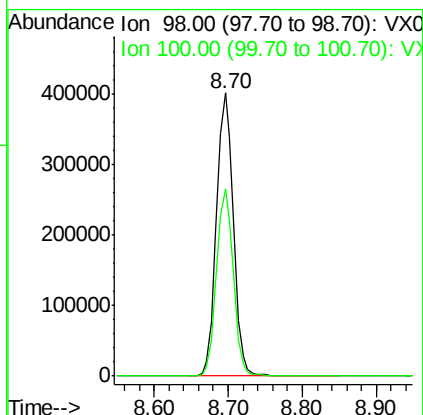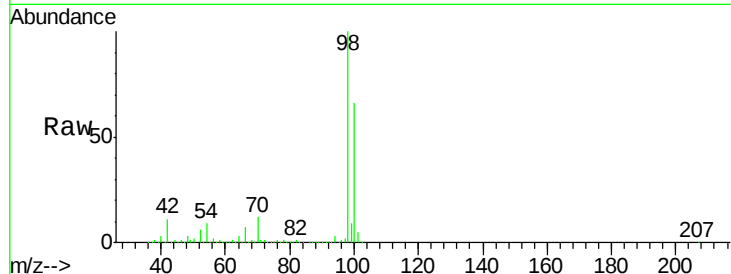

#62
4-Bromofluorobenzene
Concen: 52.265 ug/l
RT: 11.12 min Scan# 1646
Delta R.T. 0.00 min
Lab File: VX019333.D
Acq: 06 Nov 2020 11:59

Tgt Ion: 95 Resp: 243363
Ion Ratio Lower Upper
95 100
174 75.4 0.0 156.0
176 71.7 0.0 149.8


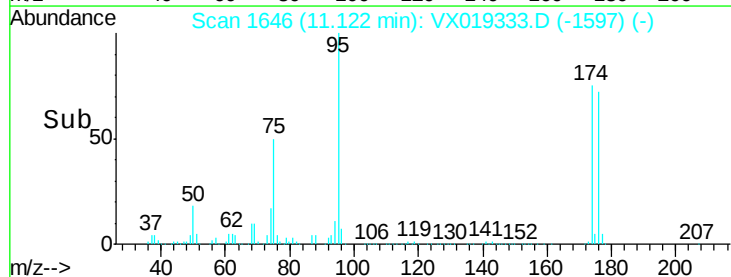
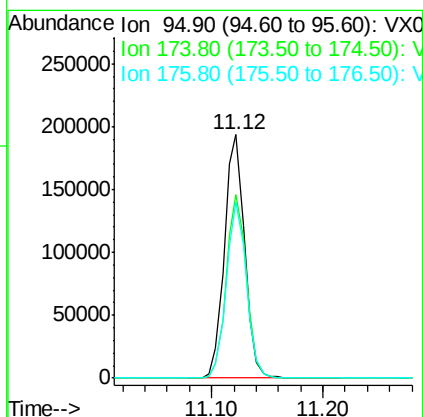
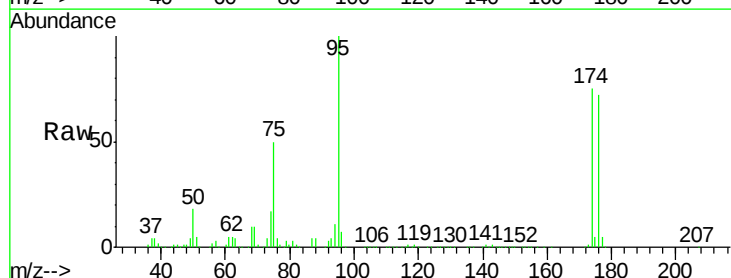


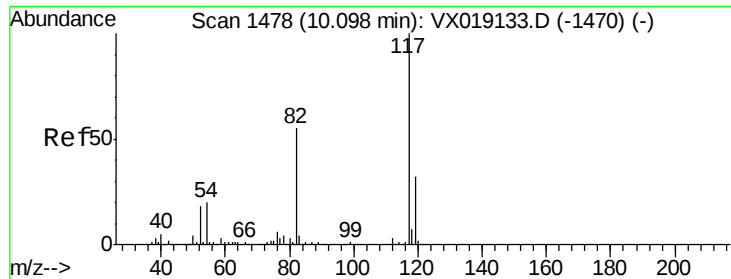

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. 0.00 min
Lab File: VX019333.D
Acq: 06 Nov 2020 11:59

Instrument :
MSVOA_X
ClientSampleId :
TB-11-5-2020

Tot Ion:117 Resp: 478991
Ion Ratio Lower Upper
117 100
82 56.0 43.6 65.4
119 32.8 25.5 38.3

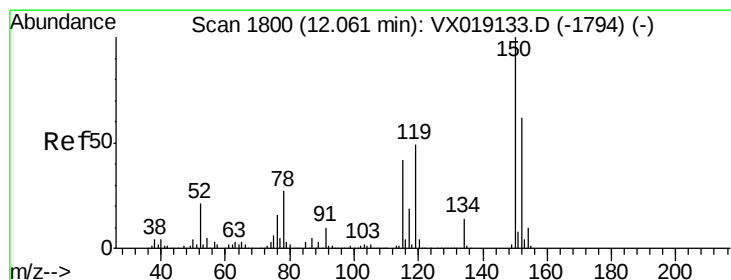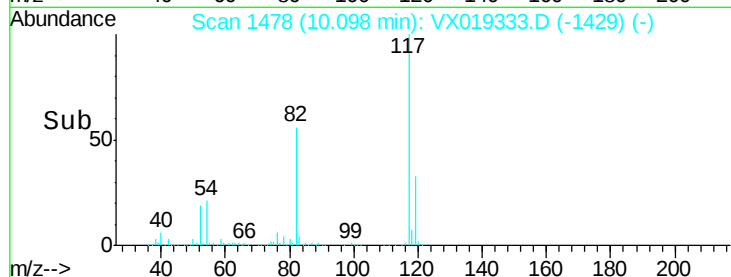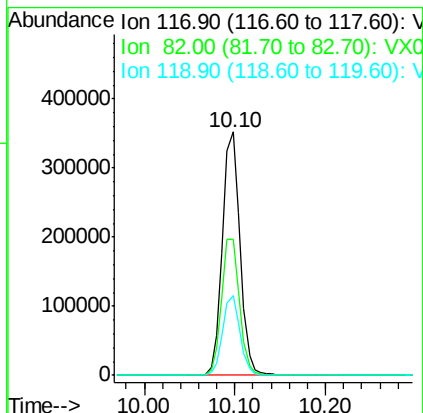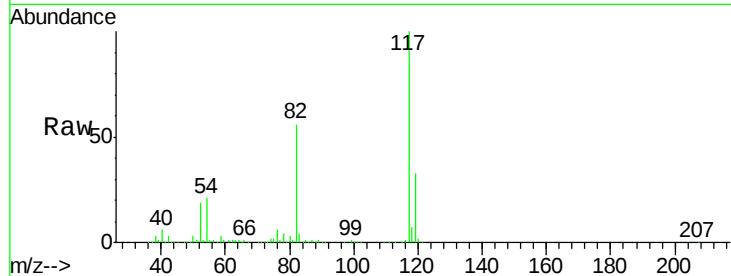

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1800
Delta R.T. 0.00 min
Lab File: VX019333.D
Acq: 06 Nov 2020 11:59

Tgt Ion:152 Resp: 238740
Ion Ratio Lower Upper
152 100
115 62.1 41.9 125.7
150 158.1 0.0 347.8

