

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110722\
 Data File : VX032620.D
 Acq On : 07 Nov 2022 12:31
 Operator : JC/MD
 Sample : N5486-04DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-23ADL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
 Title : SW846 8260

Signal : TIC: VX032620.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.605	73	85	90	rBV6	3729	10921	1.91%	0.314%
2	2.788	274	279	284	rBV3	3278	6060	1.06%	0.174%
3	3.111	323	332	347	rVB	148497	345044	60.47%	9.919%
4	3.757	431	438	449	rBV5	3358	9470	1.66%	0.272%
5	4.574	563	572	580	rBV2	2229	6715	1.18%	0.193%
6	5.385	694	705	721	rBV2	68078	202081	35.42%	5.809%
7	5.550	721	732	750	rVB	116047	330473	57.92%	9.500%
8	5.958	787	799	814	rBV2	74747	199817	35.02%	5.744%
9	6.763	919	931	947	rBV	180823	423897	74.29%	12.186%
10	8.653	1234	1241	1252	rBV	357156	570582	100.00%	16.403%
11	10.055	1465	1471	1482	rBV	370583	490171	85.91%	14.091%
12	11.079	1634	1639	1652	rBV	333574	424299	74.36%	12.198%
13	12.024	1789	1794	1805	rVB	360703	459037	80.45%	13.196%




Sum of corrected areas: 3478567

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110722\
Data File : VX032620.D
Acq On : 07 Nov 2022 12:31
Operator : JC/MD
Sample : N5486-04DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-23ADL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

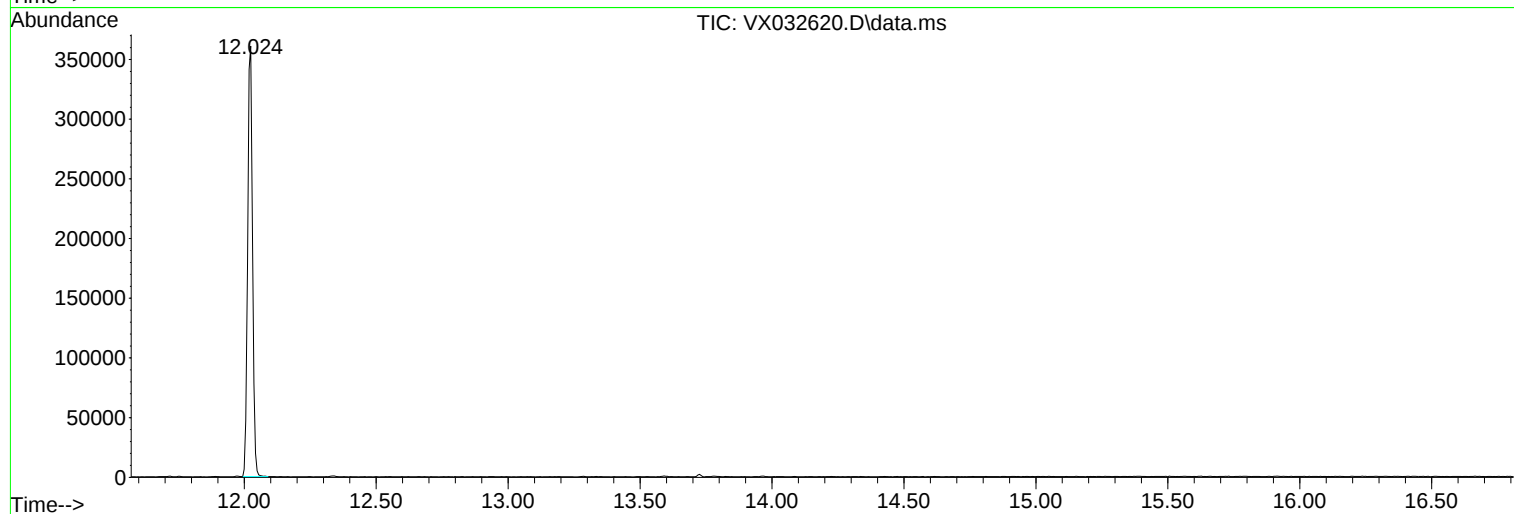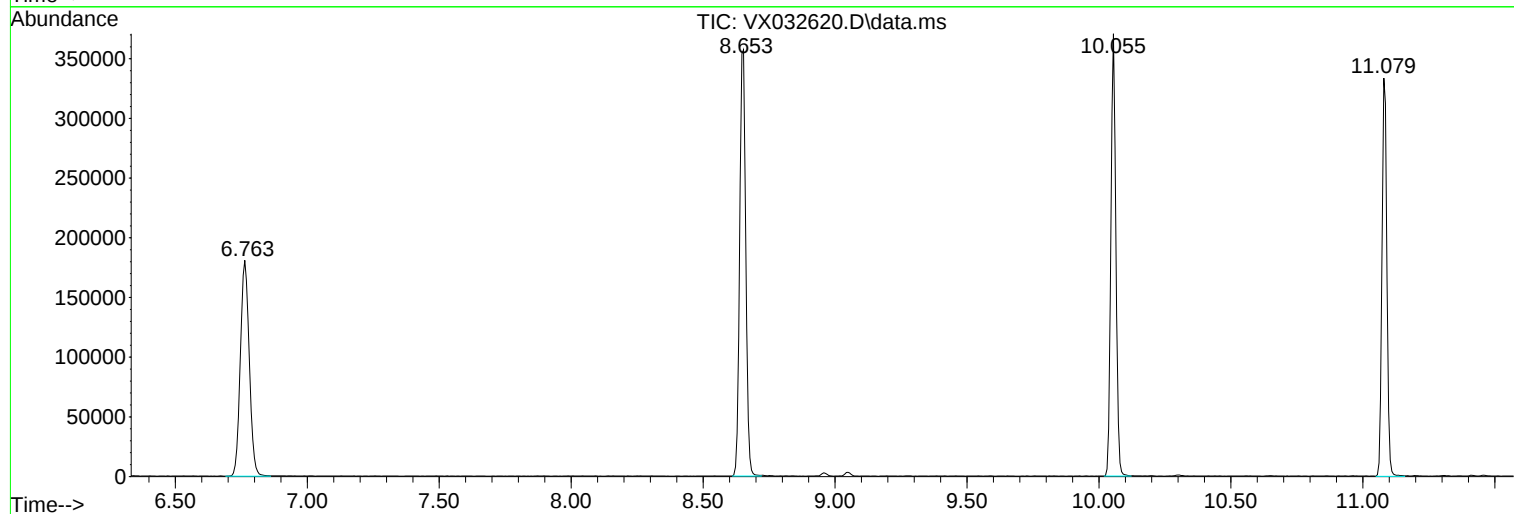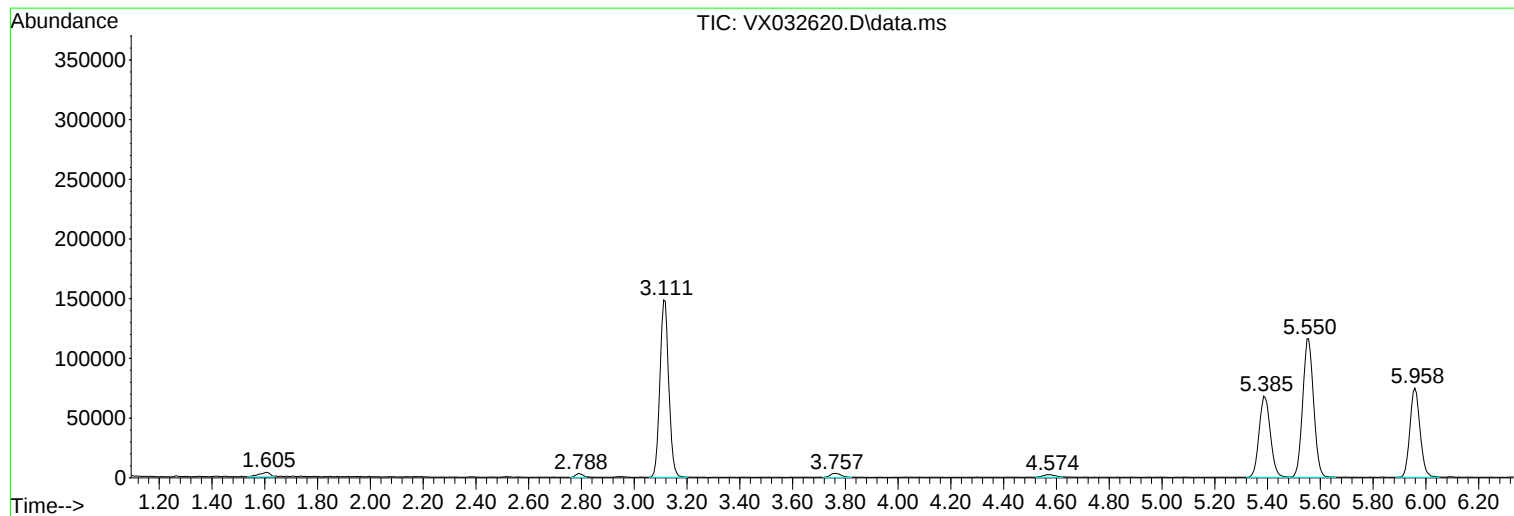

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110722\
Data File : VX032620.D
Acq On : 07 Nov 2022 12:31
Operator : JC/MD
Sample : N5486-04DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-23ADL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110722\
Data File : VX032620.D
Acq On : 07 Nov 2022 12:31
Operator : JC/MD
Sample : N5486-04DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-23ADL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------