

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110722\
 Data File : VX032638.D
 Acq On : 07 Nov 2022 19:31
 Operator : JC/MD
 Sample : N5482-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FLOOR-DRAIN-WATER

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
 Title : SW846 8260

Signal : TIC: VX032638.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.514	227	234	253	rVB	157298	260966	2.78%	1.962%
2	5.391	694	706	722	rBV	72841	212858	2.27%	1.601%
3	5.556	722	733	748	rVV	122011	344886	3.67%	2.593%
4	5.958	789	799	819	rBV	79986	212543	2.26%	1.598%
5	6.763	921	931	947	rBV	187753	445479	4.75%	3.350%
6	8.647	1234	1240	1249	rBV	379597	610766	6.51%	4.592%
7	10.055	1465	1471	1483	rBV	400386	528539	5.63%	3.974%
8	11.079	1634	1639	1646	rBV	383628	469865	5.01%	3.533%
9	12.024	1788	1794	1801	rBV	414943	512515	5.46%	3.854%
10	12.226	1821	1827	1850	rBV	7646153	9386604	100.00%	70.579%
11	13.774	2074	2081	2089	rBV	161137	202360	2.16%	1.522%
12	14.780	2241	2246	2257	rVB	89747	111965	1.19%	0.842%




Sum of corrected areas: 13299346

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110722\
Data File : VX032638.D
Acq On : 07 Nov 2022 19:31
Operator : JC/MD
Sample : N5482-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FLOOR-DRAIN-WATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

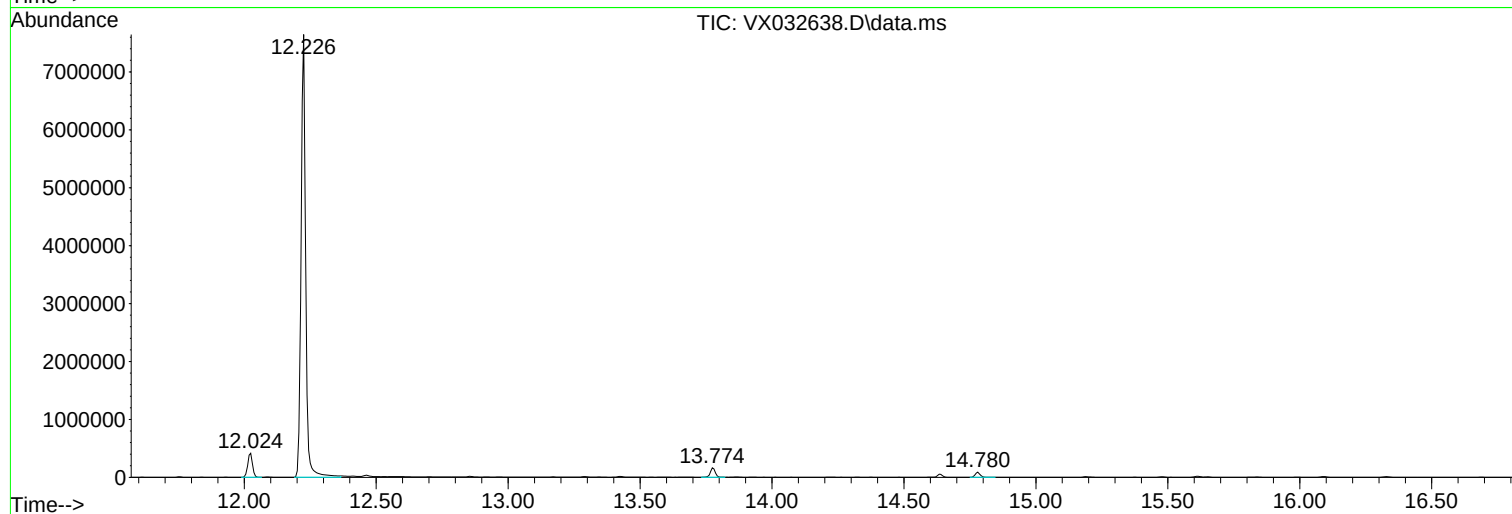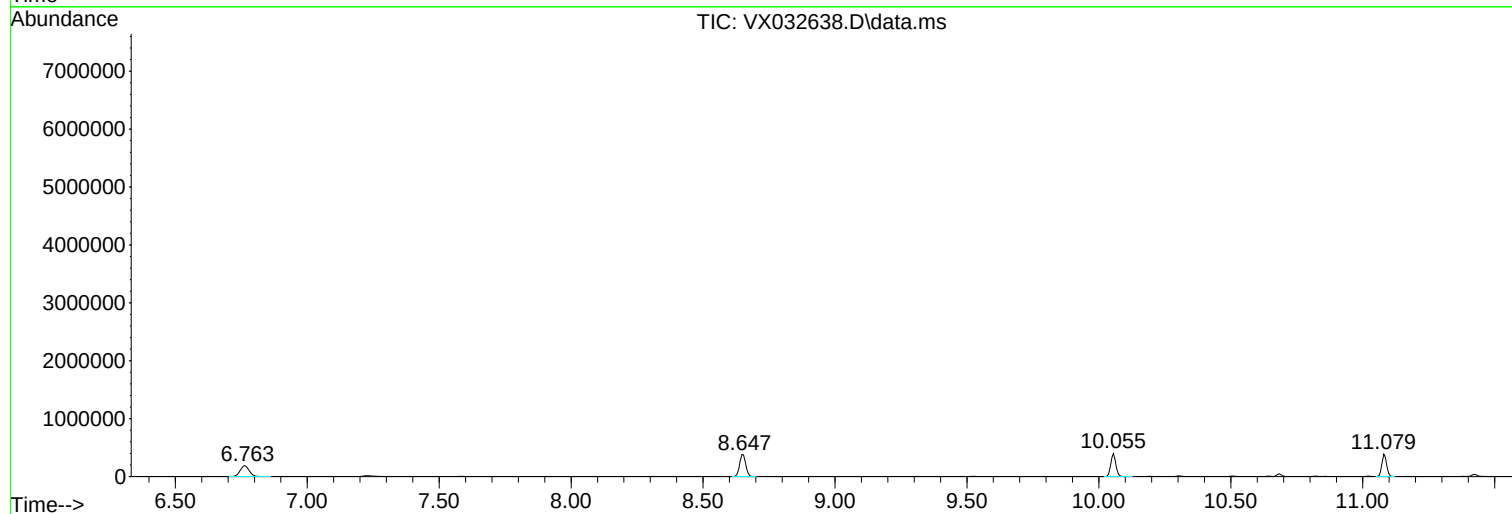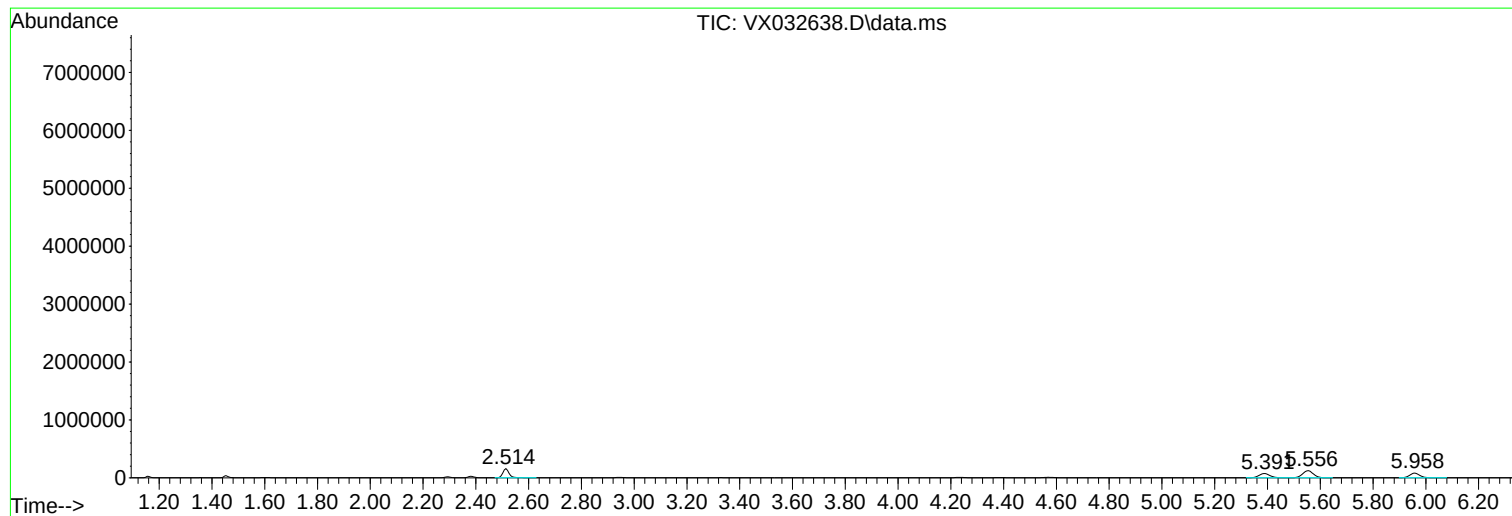

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110722\
Data File : VX032638.D
Acq On : 07 Nov 2022 19:31
Operator : JC/MD
Sample : N5482-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FLOOR-DRAIN-WATER










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Hexanol, 2-ethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.226	915.74 ug/l	9386600	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	90
2	Pentadecafluorooctanoic acid, 2-...			526	C16H17F15O2	1000406-80-9	53
3	Heptane, 1,1'-oxybis-			214	C14H30O	000629-64-1	50
4	2-Propyl-1-pentanol			130	C8H18O	058175-57-8	50
5	2-Ethyl-1-hexanol, methyl ether			144	C9H20O	1000365-10-2	47

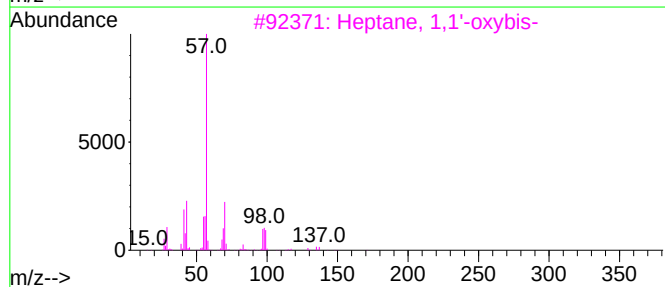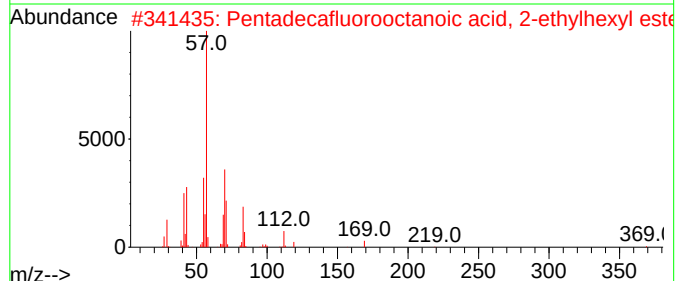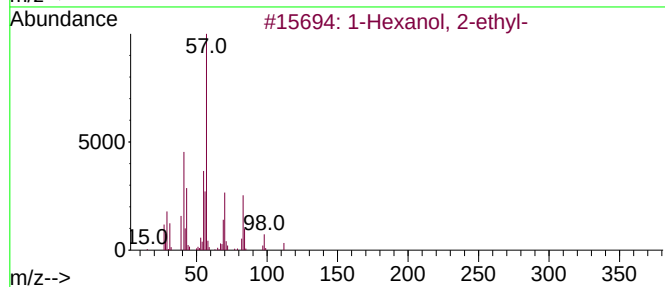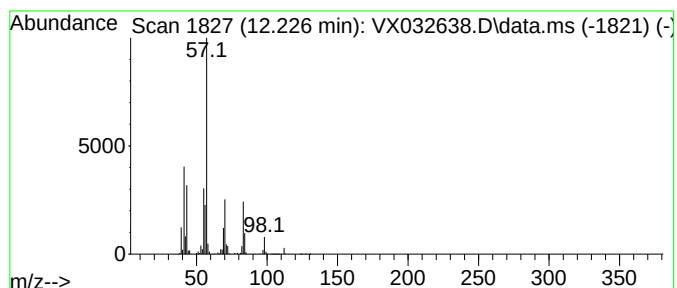

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110722\
Data File : VX032638.D
Acq On : 07 Nov 2022 19:31
Operator : JC/MD
Sample : N5482-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FLOOR-DRAIN-WATER










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Naphthalene, 2-methyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.780	10.92 ug/l	111965	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Naphthalene, 2-methyl-	142	C11H10	000091-57-6	96
2			Naphthalene, 1-methyl-	142	C11H10	000090-12-0	96
3			1,4-Methanonaphthalene, 1,4-dihy...	142	C11H10	004453-90-1	94
4			1H-Indene, 1-ethylidene-	142	C11H10	002471-83-2	91
5			Bicyclo[4.4.1]undeca-1,3,5,7,9-p...	142	C11H10	002443-46-1	91

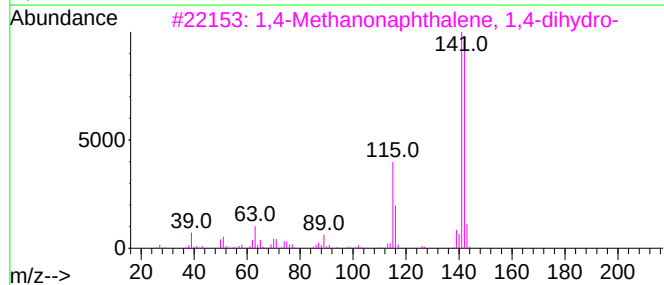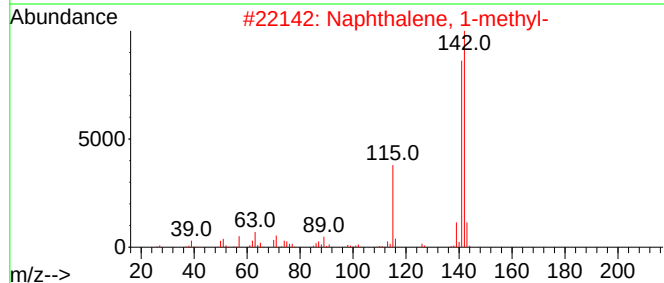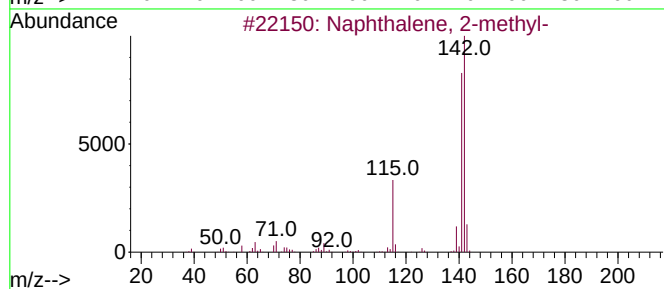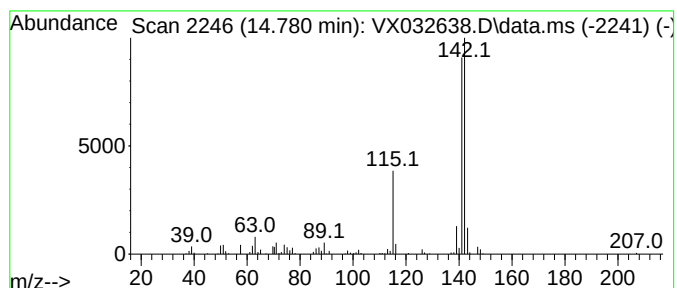

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110722\
Data File : VX032638.D
Acq On : 07 Nov 2022 19:31
Operator : JC/MD
Sample : N5482-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FLOOR-DRAIN-WATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Hexanol, 2-et...	12.226	915.7	ug/l	9386600	4	12.024	512515	50.0
Naphthalene, 2-...	14.780	10.9	ug/l	111965	4	12.024	512515	50.0