


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110723\
Data File : VX038629.D
Acq On : 07 Nov 2023 12:45
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110723W.M
Title : SW846 8260
Last Update : Wed Nov 08 03:19:07 2023

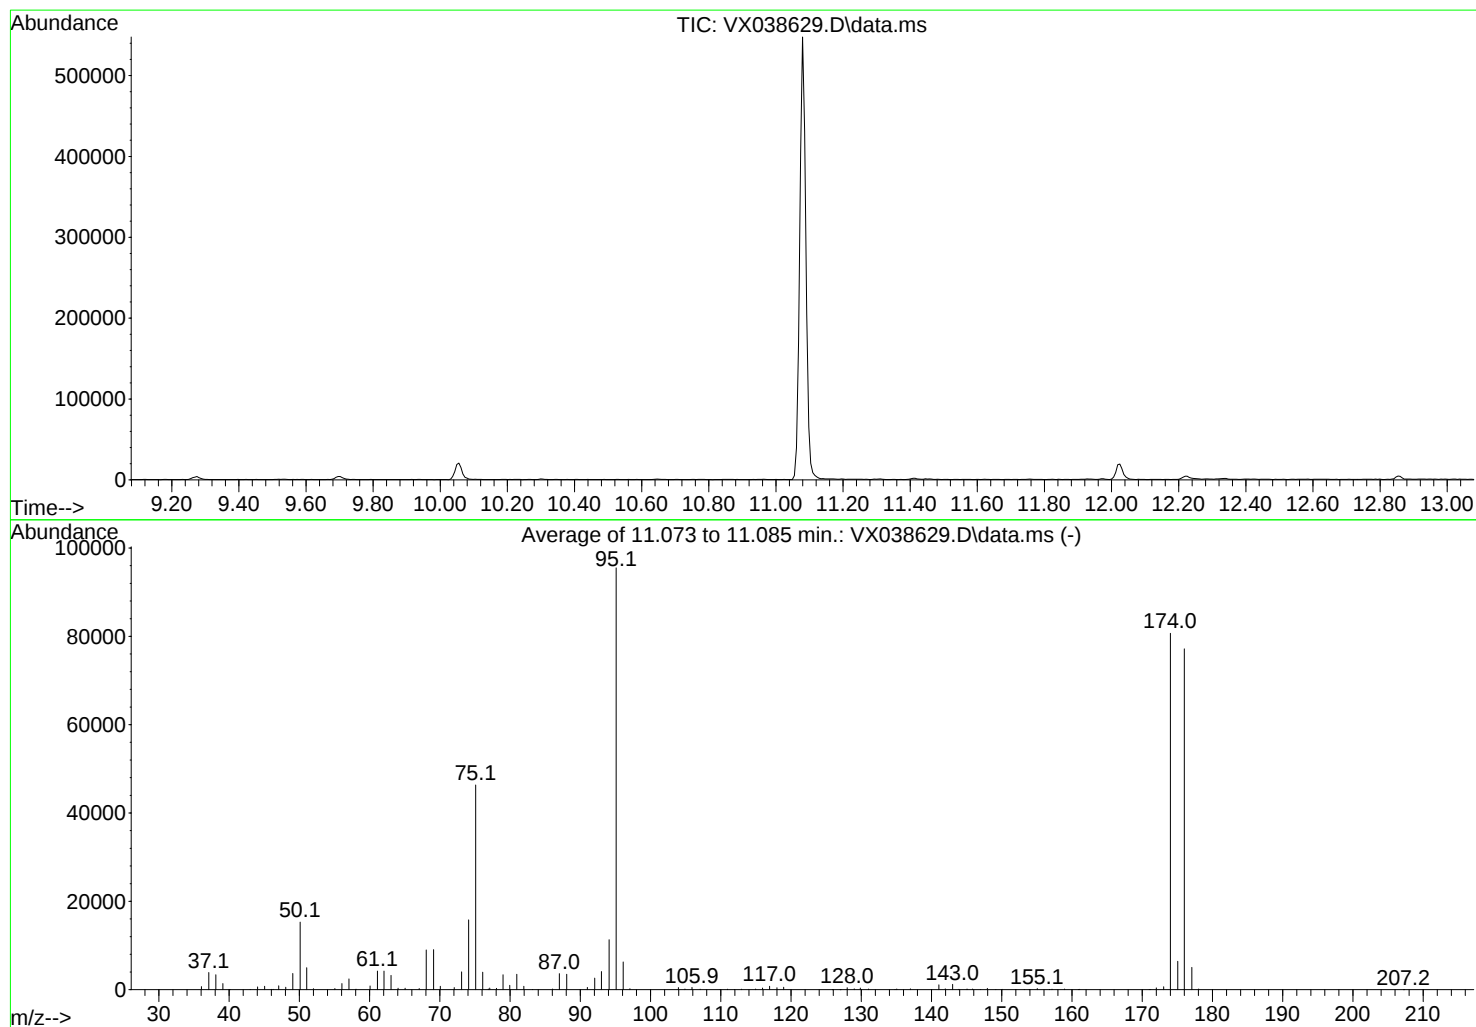

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.0	15283	PASS
75	95	30	60	48.5	46333	PASS
95	95	100	100	100.0	95517	PASS
96	95	5	9	6.6	6257	PASS
173	174	0.00	2	0.8	650	PASS
174	95	50	100	84.5	80699	PASS
175	174	5	9	8.0	6432	PASS
176	174	95	101	95.6	77165	PASS
177	176	5	9	6.5	5054	PASS