

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110724\
 Data File : VX043745.D
 Acq On : 07 Nov 2024 18:35
 Operator : JC/MD
 Sample : P4739-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 08 04:13:12 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102824W.M
 Quant Title : SW846 8260
 QLast Update : Mon Oct 28 13:41:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	83642	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	150865	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	132249	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	58071	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	48461	36.336	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	72.680%#		
35) Dibromofluoromethane	5.385	113	43920	42.932	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	85.860%		
50) Toluene-d8	8.647	98	172147	48.611	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	97.220%		
62) 4-Bromofluorobenzene	11.079	95	57659	43.940	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery =	87.880%		
Target Compounds						
					Qvalue	
5) Bromomethane	1.593	94	123	0.284	ug/l #	62
11) Tert butyl alcohol	3.056	59	163	0.655	ug/l #	100
13) Acrolein	2.246	56	126	0.647	ug/l	89
16) Acetone	2.404	43	9971	18.827	ug/l	94
17) Carbon Disulfide	2.489	76	392	0.209	ug/l #	75
18) Methyl Acetate	2.727	43	2103	1.359	ug/l	97
20) Methylene Chloride	2.782	84	2320	2.033	ug/l #	91
25) 2-Butanone	4.599	43	5207	6.740	ug/l	96
31) Cyclohexane	5.550	56	1551	1.101	ug/l #	1
36) 1,1-Dichloropropene	5.544	75	6253	5.155	ug/l #	46
38) Carbon Tetrachloride	5.550	117	8035	5.995	ug/l #	15
40) Benzene	6.038	78	7947	1.964	ug/l #	85
43) Isopropyl Acetate	6.348	43	46232	18.983	ug/l	97
48) Methyl methacrylate	7.806	41	38958	33.739	ug/l #	40
49) 1,4-Dioxane	7.799	88	44	1.855	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	34546	23.272	ug/l #	51
52) Toluene	8.726	92	768	0.313	ug/l	97
53) t-1,3-Dichloropropene	8.952	75	293	0.203	ug/l #	42
54) cis-1,3-Dichloropropene	8.555	75	18405	11.949	ug/l #	55
56) Ethyl methacrylate	9.244	69	511	0.308	ug/l #	1
57) 1,3-Dichloropropane	9.488	76	2129	1.253	ug/l #	42
59) 2-Hexanone	9.488	43	28163	24.980	ug/l #	57
73) Isopropylbenzene	10.963	105	1372	0.334	ug/l	92
74) N-amyl acetate	10.793	43	921	0.460	ug/l #	49
76) 1,2,3-Trichloropropane	11.079	75	27564	22.200	ug/l #	34
78) n-propylbenzene	11.305	91	977	0.218	ug/l	84
79) 2-Chlorotoluene	11.305	91	977	0.329	ug/l #	41
81) trans-1,4-Dichloro-2-b...	11.079	75	27564	61.072	ug/l #	7
82) 4-Chlorotoluene	11.305	91	977	0.293	ug/l #	46
83) tert-Butylbenzene	11.713	119	868	0.249	ug/l	86
85) sec-Butylbenzene	11.890	105	1398	0.342	ug/l	87
90) Hexachloroethane	12.646	117	1123	1.989	ug/l #	17
95) Naphthalene	13.780	128	941	0.208	ug/l #	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110724\
Data File : VX043745.D
Acq On : 07 Nov 2024 18:35
Operator : JC/MD
Sample : P4739-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Nov 08 04:13:12 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102824W.M
Quant Title : SW846 8260
QLast Update : Mon Oct 28 13:41:34 2024
Response via : Initial Calibration




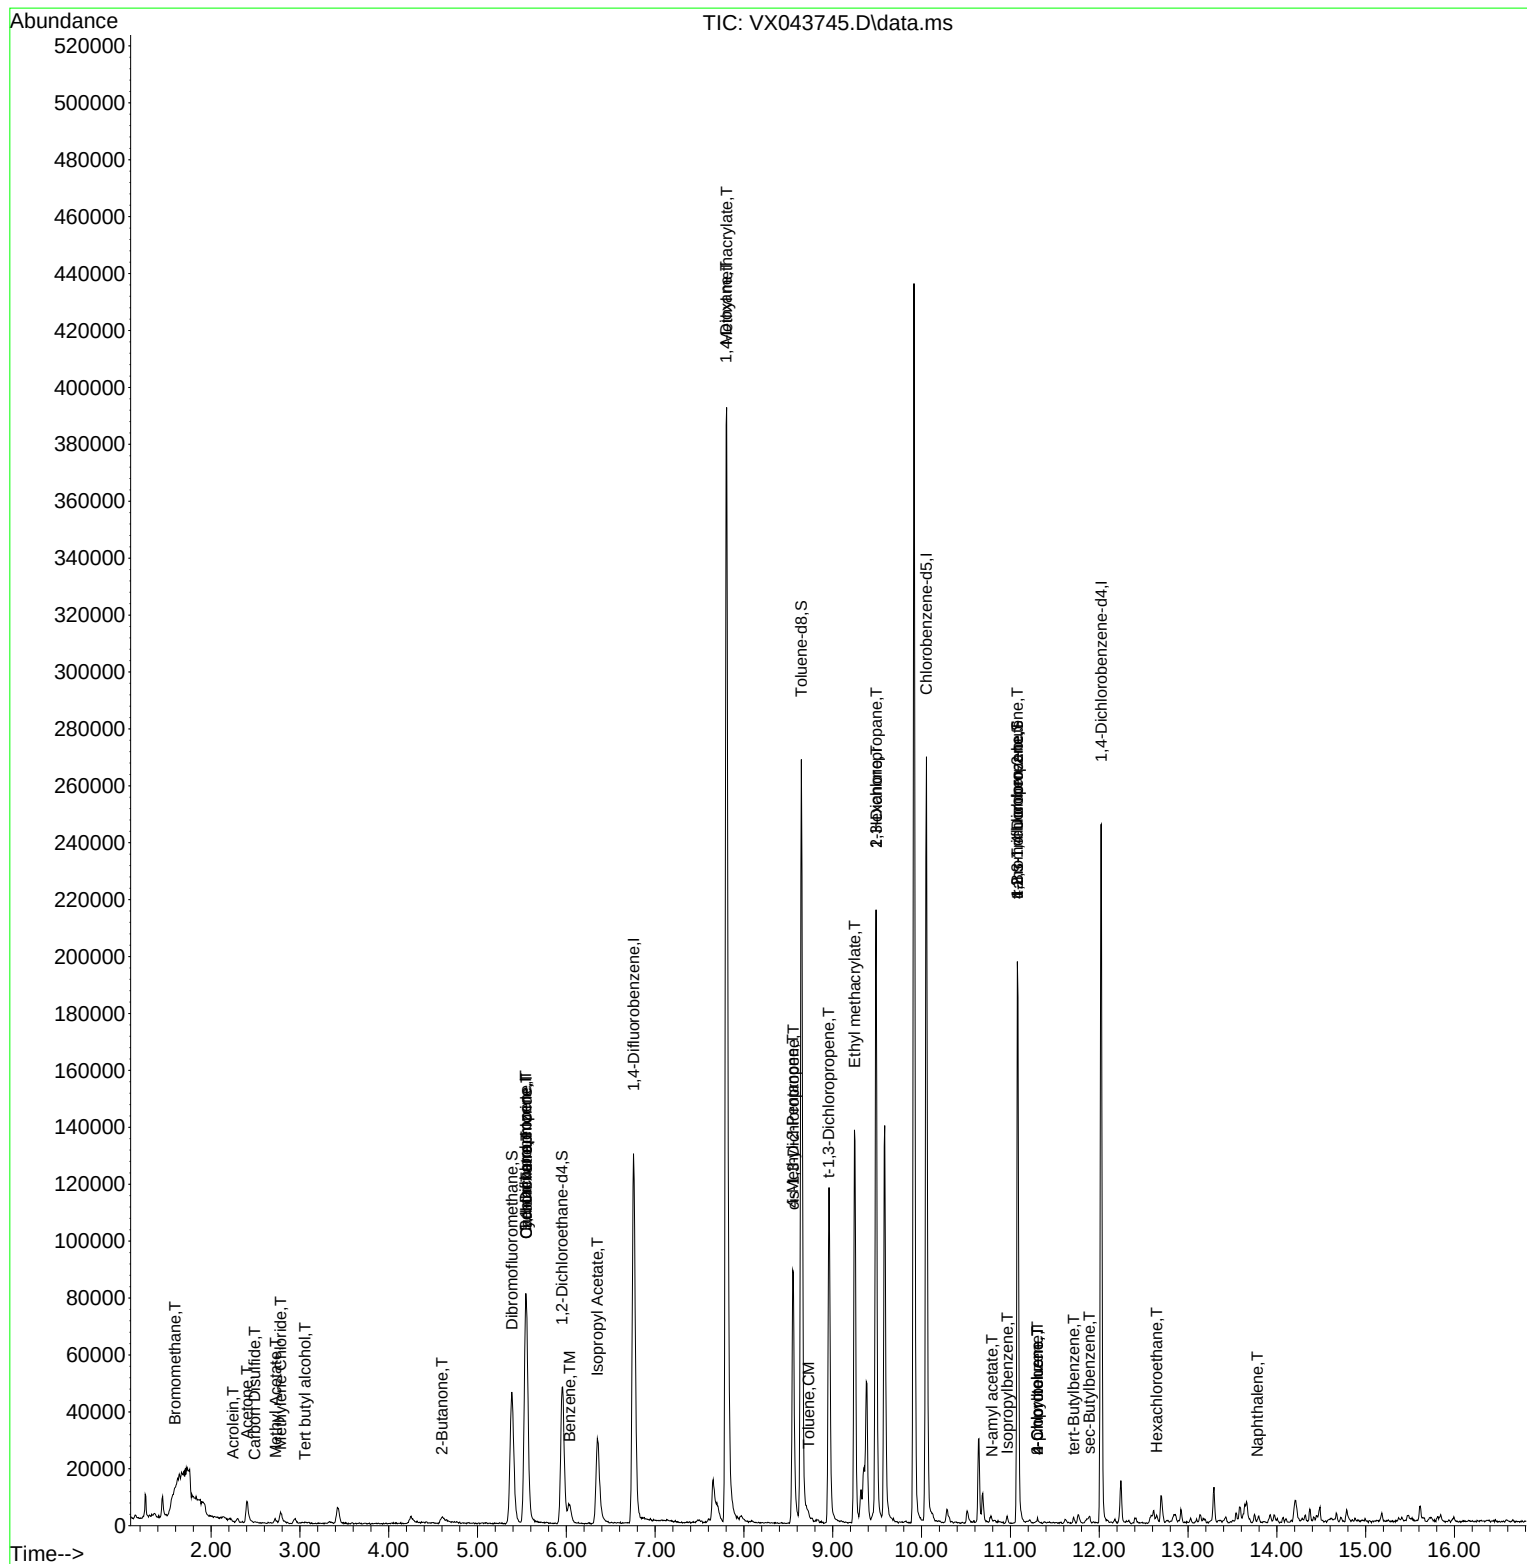




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX043745.D
Acq: 07 Nov 2024 18:35




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:168 Resp: 83642
Ion Ratio Lower Upper
168 100
99 57.6 52.6 78.8

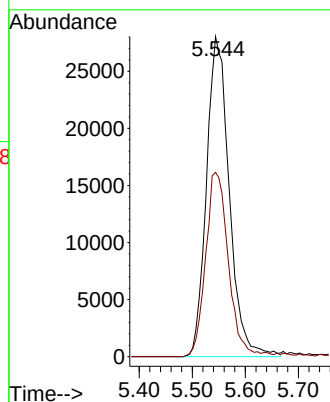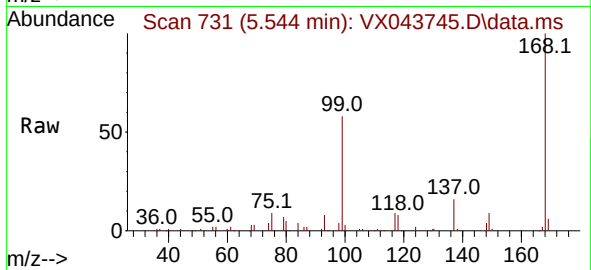

#5
Bromomethane
Concen: 0.284 ug/l
RT: 1.593 min Scan# 83
Delta R.T. 0.000 min
Lab File: VX043745.D
Acq: 07 Nov 2024 18:35


Tgt Ion: 94 Resp: 123
Ion Ratio Lower Upper
94 100
96 57.7 75.9 113.9#

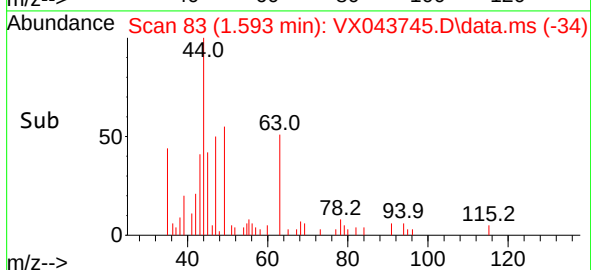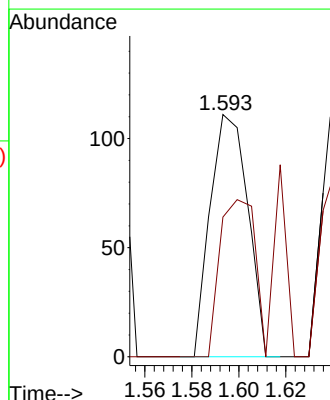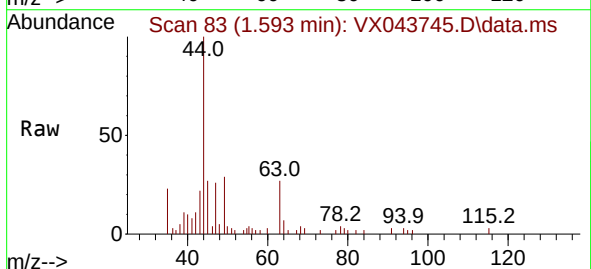






#11
Tert butyl alcohol
Concen: 0.655 ug/l
RT: 3.056 min Scan# 316
Delta R.T. 0.006 min
Lab File: VX043745.D
Acq: 07 Nov 2024 18:35

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 59 Resp: 163
Ion Ratio Lower Upper
59 100
57 19.6 0.0 0.0#



#13
Acrolein
Concen: 0.647 ug/l
RT: 2.246 min Scan# 190
Delta R.T. 0.006 min
Lab File: VX043745.D
Acq: 07 Nov 2024 18:35

Tgt Ion: 56 Resp: 126
Ion Ratio Lower Upper
56 100
55 77.8 55.3 82.9

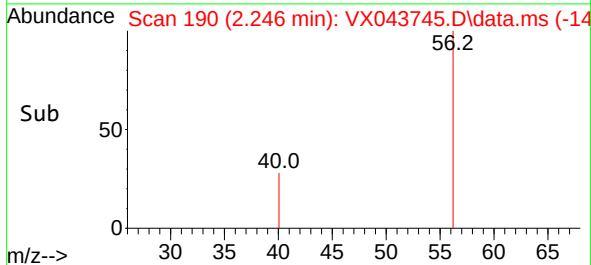



#16

Acetone

Concen: 18.827 ug/l

RT: 2.404 min Scan# 21

Delta R.T. 0.006 min

Lab File: VX043745.D

Acq: 07 Nov 2024 18:35

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 9971

Ion Ratio Lower Upper

43 100

58 34.6 25.1 37.7

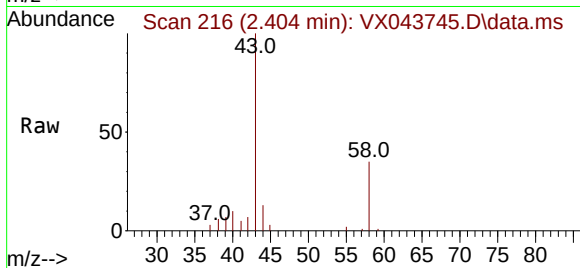

#17

Carbon Disulfide

Concen: 0.209 ug/l

RT: 2.489 min Scan# 230

Delta R.T. -0.006 min

Lab File: VX043745.D




Acq: 07 Nov 2024 18:35


Tgt Ion: 76 Resp: 392

Ion Ratio Lower Upper

76 100

78 0.0 7.1 10.7#


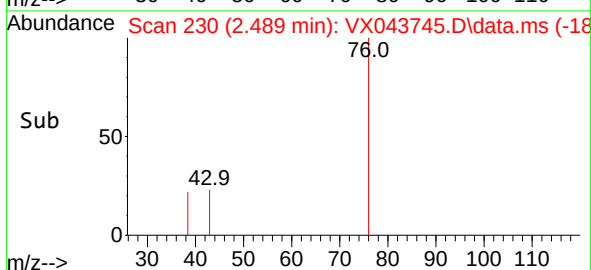

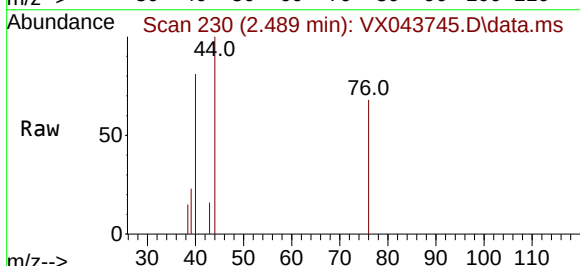




#18
Methyl Acetate
Concen: 1.359 ug/l
RT: 2.727 min Scan# 20
Delta R.T. 0.018 min
Lab File: VX043745.D
Acq: 07 Nov 2024 18:35




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 2103
Ion Ratio Lower Upper
43 100
74 22.3 19.1 28.7

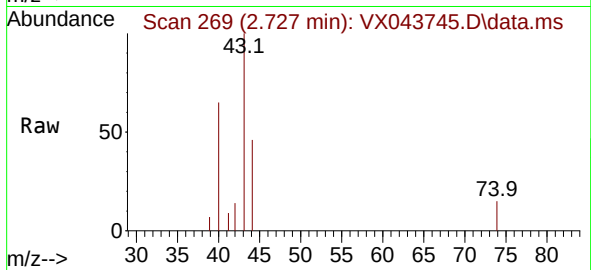

#20
Methylene Chloride
Concen: 2.033 ug/l
RT: 2.782 min Scan# 278
Delta R.T. 0.000 min
Lab File: VX043745.D
Acq: 07 Nov 2024 18:35

Tgt Ion: 84 Resp: 2320
Ion Ratio Lower Upper
84 100
49 118.4 97.0 145.6
51 44.0 29.8 44.8
86 52.0 53.1 79.7#





#25

2-Butanone

Concen: 6.740 ug/l

RT: 4.599 min Scan# 51

Delta R.T. 0.031 min

Lab File: VX043745.D

Acq: 07 Nov 2024 18:35

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 5207

Ion Ratio Lower Upper

43 100

72 28.4 21.1 31.7

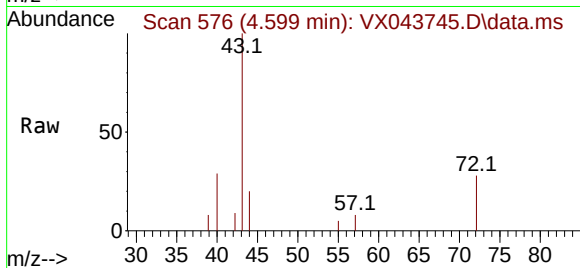

#31

Cyclohexane

Concen: 1.101 ug/l

RT: 5.550 min Scan# 732

Delta R.T. 0.092 min

Lab File: VX043745.D

Acq: 07 Nov 2024 18:35




Tgt Ion: 56 Resp: 1551


Ion Ratio Lower Upper

56 100

69 199.8 24.9 37.3#

84 149.5 73.3 109.9#

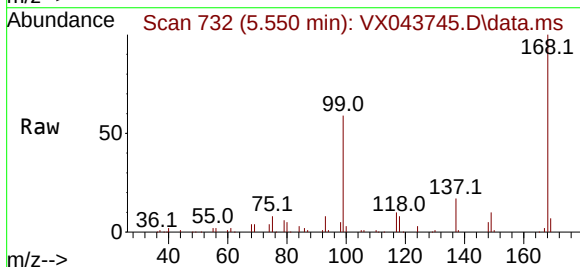

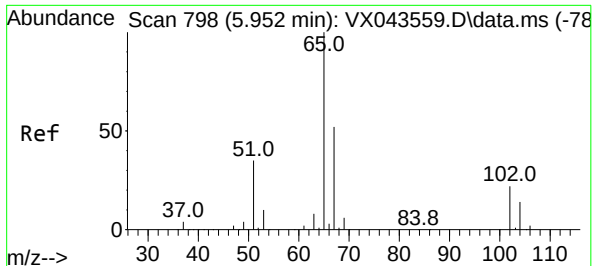

#33

1,2-Dichloroethane-d4

Concen: 36.336 ug/l

RT: 5.952 min Scan# 798

Delta R.T. 0.000 min

Lab File: VX043745.D

Acq: 07 Nov 2024 18:35

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 65 Resp: 48461

Ion Ratio Lower Upper

65 100

67 52.9 0.0 103.4

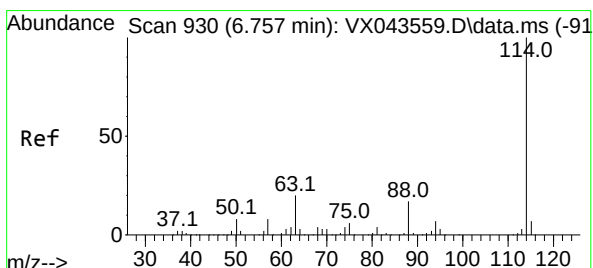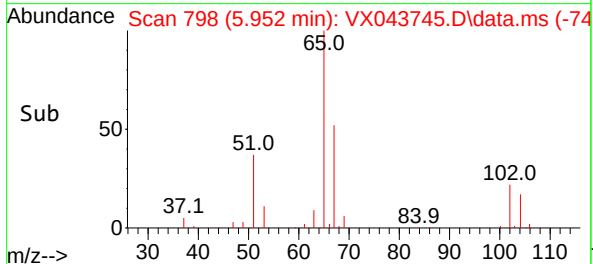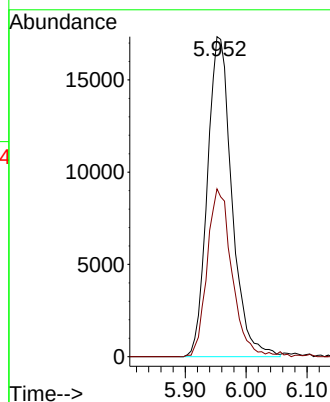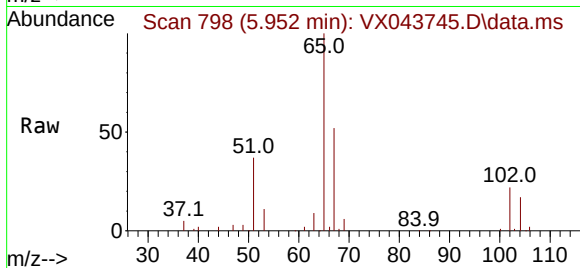

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. 0.000 min

Lab File: VX043745.D

Acq: 07 Nov 2024 18:35




Tgt Ion: 114 Resp: 150865


Ion Ratio Lower Upper

114 100

63 17.1 0.0 41.2


88 13.2 0.0 34.0

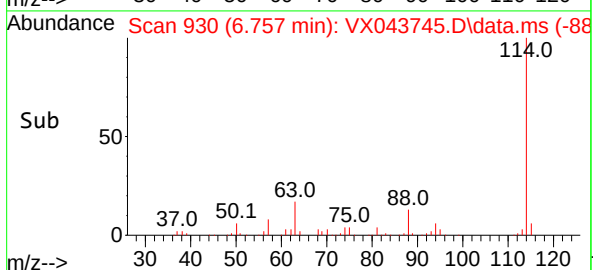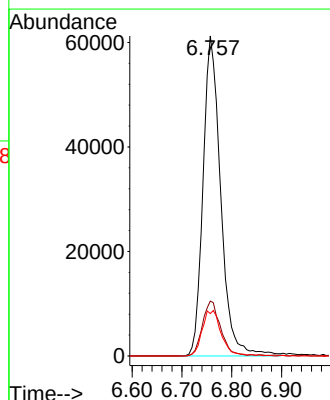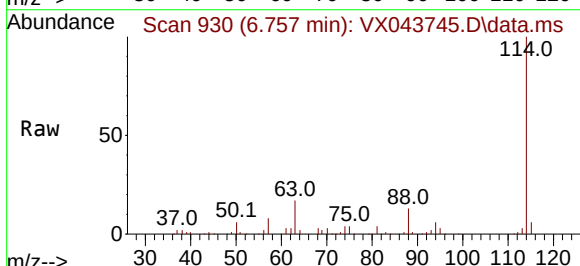



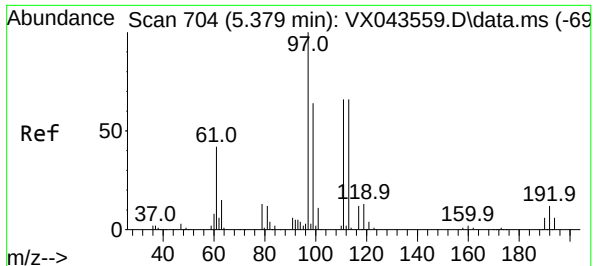


#35
Dibromofluoromethane
Concen: 42.932 ug/l
RT: 5.385 min Scan# 704
Delta R.T. 0.000 min
Lab File: VX043745.D
Acq: 07 Nov 2024 18:35

Instrument :
MSVOA_X
ClientSampleId :



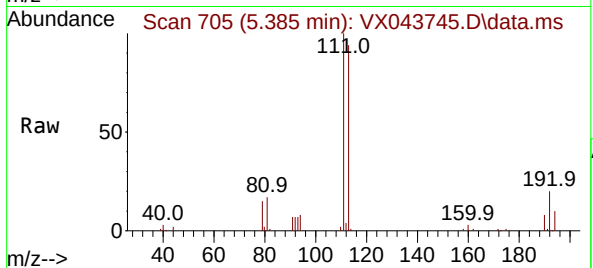



Tgt Ion:113 Resp: 43920
Ion Ratio Lower Upper
113 100
111 98.4 81.4 122.0
192 19.3 14.1 21.1

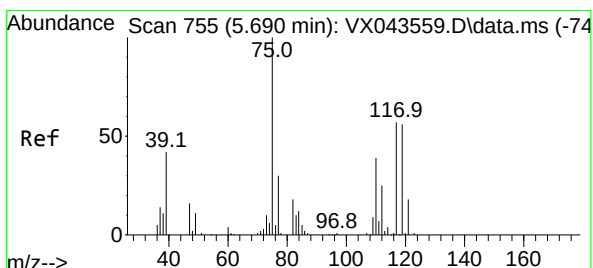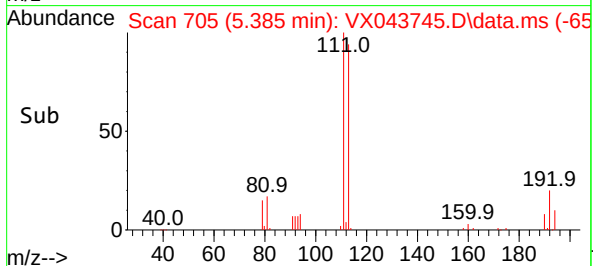

#36
1,1-Dichloropropene
Concen: 5.155 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.140 min
Lab File: VX043745.D
Acq: 07 Nov 2024 18:35


Tgt Ion: 75 Resp: 6253
Ion Ratio Lower Upper
75 100
110 5.4 17.9 53.7#
77 0.0 25.0 37.4#

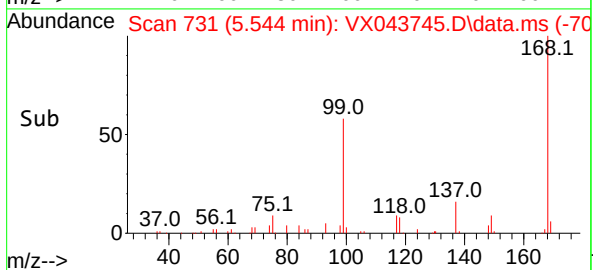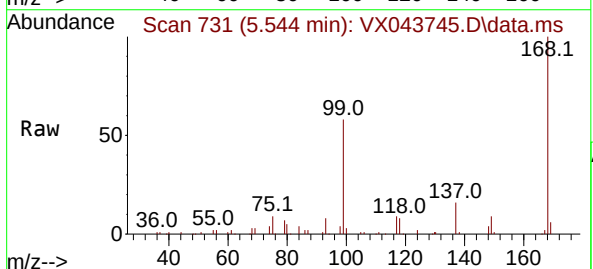






#38
Carbon Tetrachloride
Concen: 5.995 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.122 min
Lab File: VX043745.D
Acq: 07 Nov 2024 18:35

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:117 Resp: 8035
Ion Ratio Lower Upper
117 100
119 4.2 77.0 115.6#
121 0.0 24.7 37.1#



#40
Benzene
Concen: 1.964 ug/l
RT: 6.038 min Scan# 812
Delta R.T. 0.006 min
Lab File: VX043745.D
Acq: 07 Nov 2024 18:35

Tgt Ion: 78 Resp: 7947
Ion Ratio Lower Upper
78 100
77 30.4 18.4 27.6#









#43
Isopropyl Acetate
Concen: 18.983 ug/l
RT: 6.348 min Scan# 80
Delta R.T. 0.006 min
Lab File: VX043745.D
Acq: 07 Nov 2024 18:35




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 46232
Ion Ratio Lower Upper
43 100
61 21.3 16.2 24.4
87 15.9 11.0 16.6

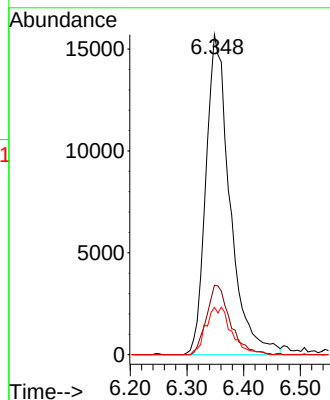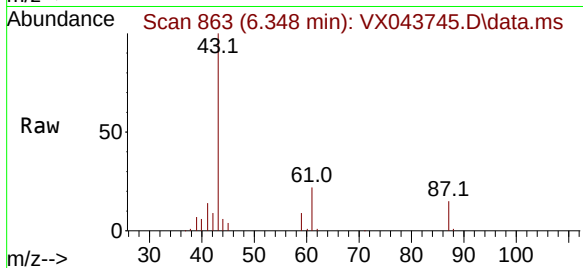

#48
Methyl methacrylate
Concen: 33.739 ug/l
RT: 7.806 min Scan# 1102
Delta R.T. 0.110 min
Lab File: VX043745.D
Acq: 07 Nov 2024 18:35

Tgt Ion: 41 Resp: 38958
Ion Ratio Lower Upper
41 100
69 0.1 67.7 101.5#
39 48.3 46.3 69.5



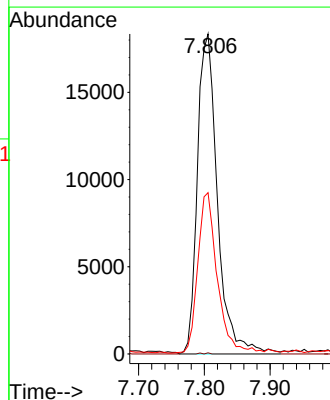
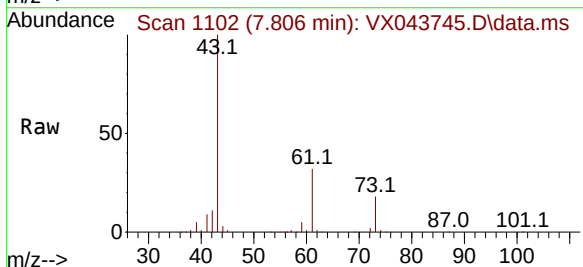




#49
 1,4-Dioxane
 Concen: 1.855 ug/l
 RT: 7.799 min Scan# 1101
 Delta R.T. 0.128 min
 Lab File: VX043745.D
 Acq: 07 Nov 2024 18:35




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion: 88 Resp: 44
 Ion Ratio Lower Upper
 88 100
 43 956904.5 25.3 37.9#
 58 5111.4 53.9 80.9#



#50
 Toluene-d8
 Concen: 48.611 ug/l
 RT: 8.647 min Scan# 1240
 Delta R.T. 0.000 min
 Lab File: VX043745.D
 Acq: 07 Nov 2024 18:35

Tgt Ion: 98 Resp: 172147
 Ion Ratio Lower Upper
 98 100
 100 66.4 53.4 80.2

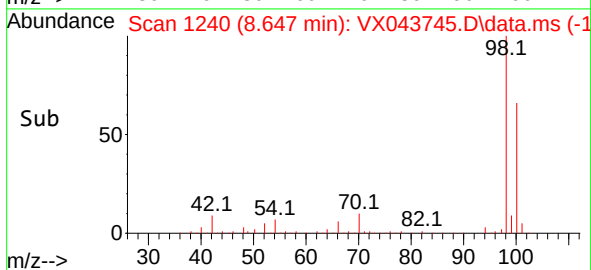

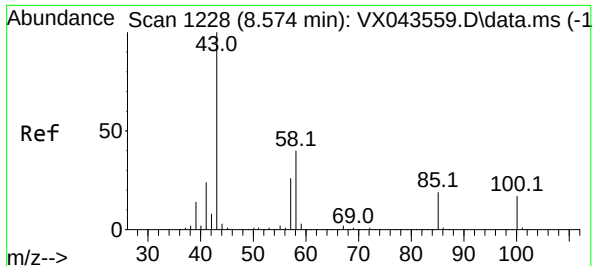

#51

4-Methyl-2-Pentanone

Concen: 23.272 ug/l

RT: 8.549 min Scan# 11

Delta R.T. -0.030 min

Lab File: VX043745.D

Acq: 07 Nov 2024 18:35

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 34546

Ion Ratio Lower Upper

43 100

58 9.3 31.7 47.5#

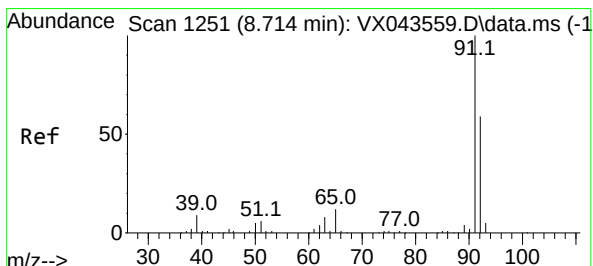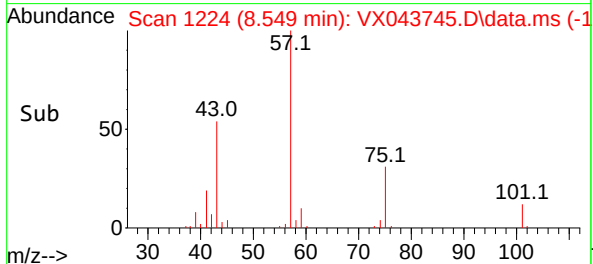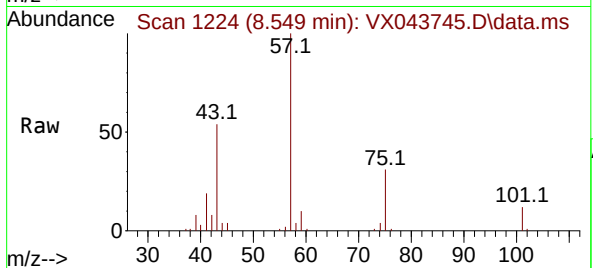

#52

Toluene

Concen: 0.313 ug/l

RT: 8.726 min Scan# 1253

Delta R.T. 0.012 min

Lab File: VX043745.D




Acq: 07 Nov 2024 18:35


Tgt Ion: 92 Resp: 768

Ion Ratio Lower Upper

92 100

91 164.8 135.7 203.5

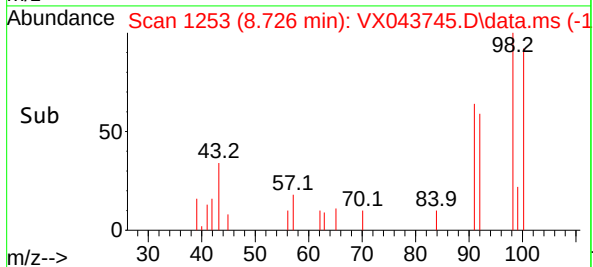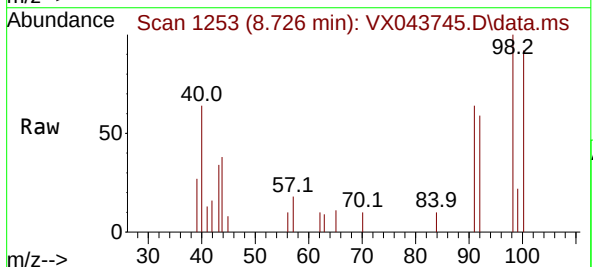



#53

t-1,3-Dichloropropene

Concen: 0.203 ug/l

RT: 8.952 min Scan# 11

Delta R.T. -0.024 min

Lab File: VX043745.D

Acq: 07 Nov 2024 18:35

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 75 Resp: 293

Ion Ratio Lower Upper

75 100

77 0.0 26.0 39.0#

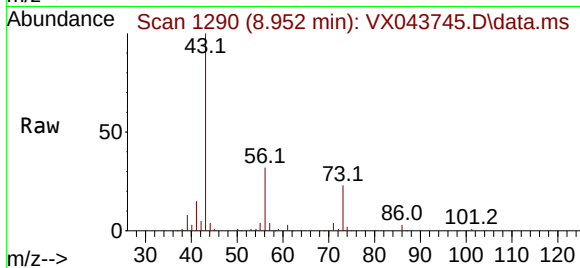

#54

cis-1,3-Dichloropropene

Concen: 11.949 ug/l

RT: 8.555 min Scan# 1225

Delta R.T. 0.189 min

Lab File: VX043745.D

Acq: 07 Nov 2024 18:35




Tgt Ion: 75 Resp: 18405


Ion Ratio Lower Upper

75 100

77 0.0 24.8 37.2#

39 22.6 37.7 56.5#




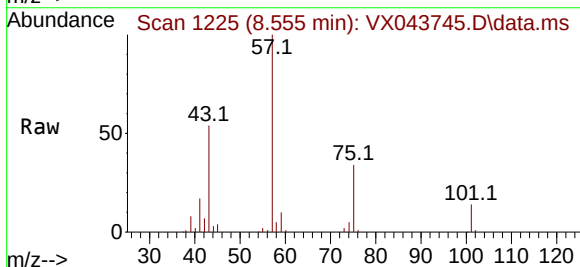




#56
Ethyl methacrylate
Concen: 0.308 ug/l
RT: 9.244 min Scan# 11
Delta R.T. 0.128 min
Lab File: VX043745.D
Acq: 07 Nov 2024 18:35




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 69 Resp: 511
Ion Ratio Lower Upper
69 100
41 4044.2 53.8 80.8#
39 1793.3 29.9 44.9#



#57
1,3-Dichloropropane
Concen: 1.253 ug/l
RT: 9.488 min Scan# 1378
Delta R.T. 0.183 min
Lab File: VX043745.D
Acq: 07 Nov 2024 18:35

Tgt Ion: 76 Resp: 2129
Ion Ratio Lower Upper
76 100
78 0.0 25.9 38.9#


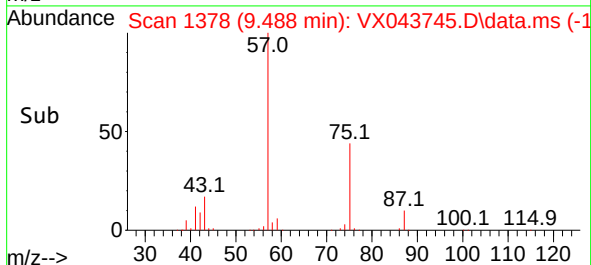
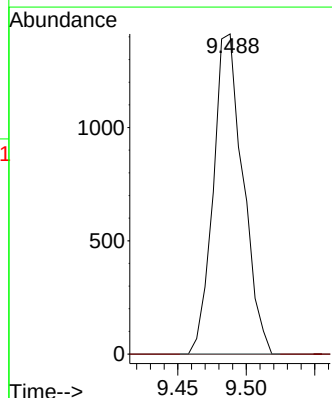





#59
2-Hexanone
Concen: 24.980 ug/l
RT: 9.488 min Scan# 11
Delta R.T. 0.055 min
Lab File: VX043745.D
Acq: 07 Nov 2024 18:35




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 28163
Ion Ratio Lower Upper
43 100
58 24.2 27.5 82.5#



#62
4-Bromofluorobenzene
Concen: 43.940 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX043745.D
Acq: 07 Nov 2024 18:35

Tgt Ion: 95 Resp: 57659
Ion Ratio Lower Upper
95 100
174 81.5 0.0 146.6
176 79.0 0.0 139.6

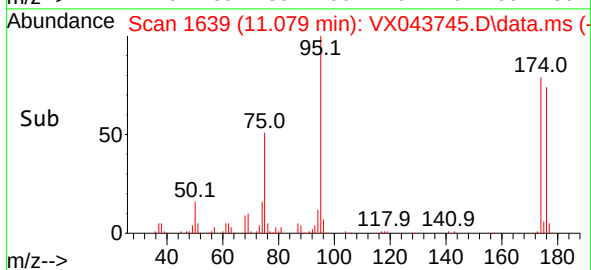



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX043745.D

Acq: 07 Nov 2024 18:35

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion:117 Resp: 132249

Ion Ratio Lower Upper

117 100

82 51.9 42.1 63.1

119 30.4 25.4 38.2

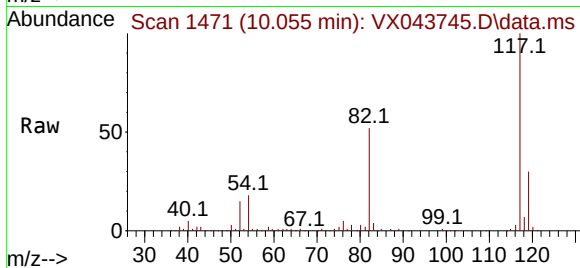

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.000 min

Lab File: VX043745.D

Acq: 07 Nov 2024 18:35




Tgt Ion:152 Resp: 58071


Ion Ratio Lower Upper

152 100

115 58.8 42.9 128.7

150 157.3 0.0 343.6

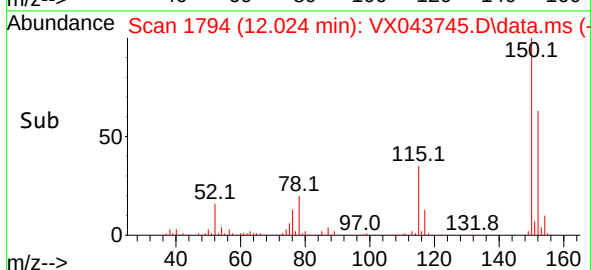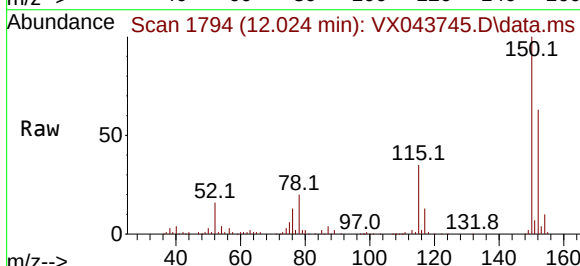



#73

Isopropylbenzene

Concen: 0.334 ug/l

RT: 10.963 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX043745.D

Acq: 07 Nov 2024 18:35

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 1372

Ion Ratio Lower Upper

105 100

120 30.4 13.2 39.6



#74

N-ethyl acetate

Concen: 0.460 ug/l

RT: 10.793 min Scan# 1592

Delta R.T. -0.049 min

Lab File: VX043745.D

Acq: 07 Nov 2024 18:35

Tgt Ion: 43 Resp: 921




Ion Ratio Lower Upper


43 100

70 0.0 34.6 52.0#

55 35.3 19.6 29.4#

61 0.0 20.2 30.2#

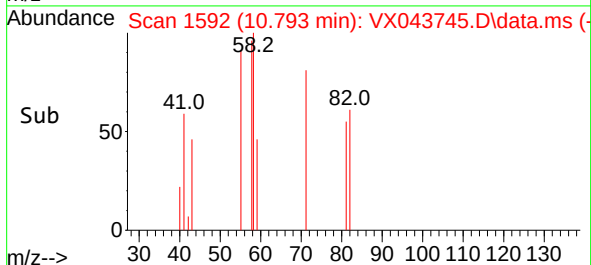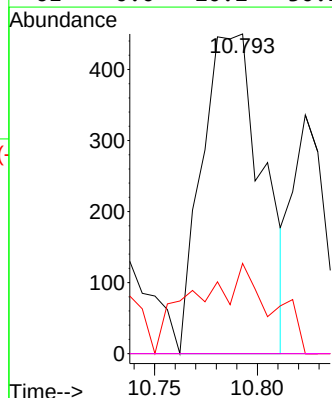



#76

1,2,3-Trichloropropane

Concen: 22.200 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.158 min

Lab File: VX043745.D

Acq: 07 Nov 2024 18:35

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 75 Resp: 27564

Ion Ratio Lower Upper

75 100

77 1.4 22.4 67.2#

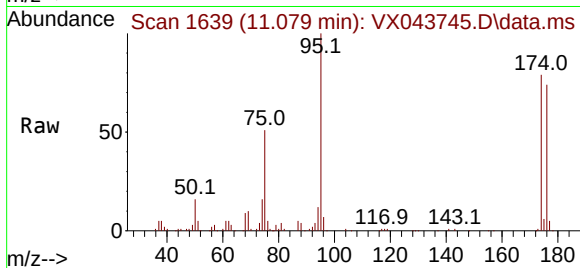

#78

n-propylbenzene

Concen: 0.218 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. 0.000 min

Lab File: VX043745.D




Acq: 07 Nov 2024 18:35


Tgt Ion: 91 Resp: 977

Ion Ratio Lower Upper

91 100

120 15.4 11.6 34.7

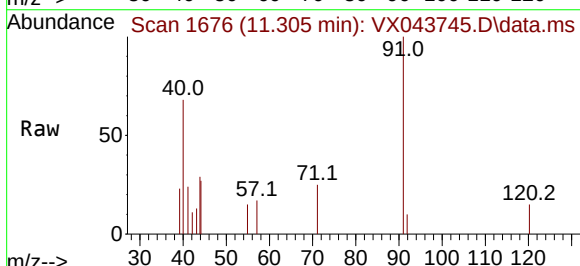



#79

2-Chlorotoluene

Concen: 0.329 ug/l

RT: 11.305 min Scan# 1686

Delta R.T. -0.061 min

Lab File: VX043745.D

Acq: 07 Nov 2024 18:35

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 977

Ion Ratio Lower Upper

91 100

126 0.0 16.7 50.0#

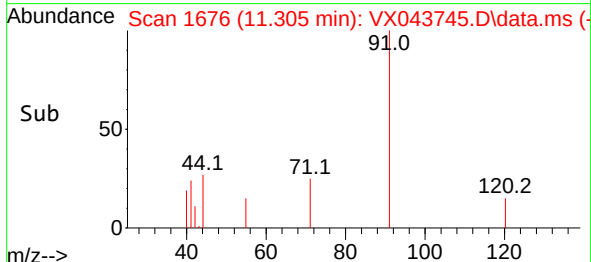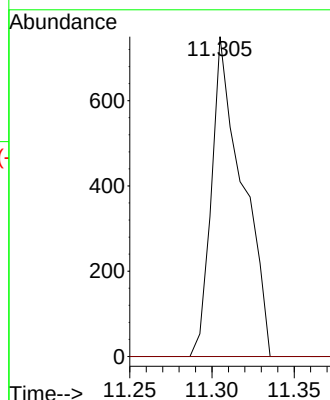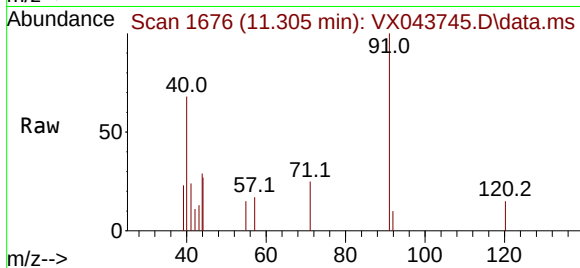

#81

trans-1,4-Dichloro-2-butene

Concen: 61.072 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX043745.D

Acq: 07 Nov 2024 18:35




Tgt Ion: 75 Resp: 27564


Ion Ratio Lower Upper

75 100

53 0.0 84.6 126.8#

89 0.1 38.6 58.0#


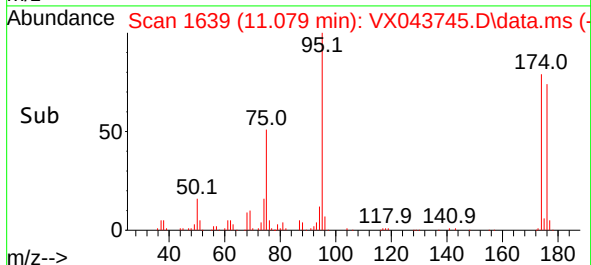
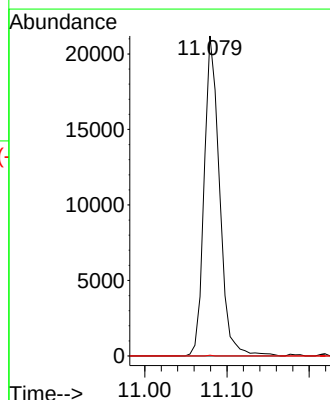
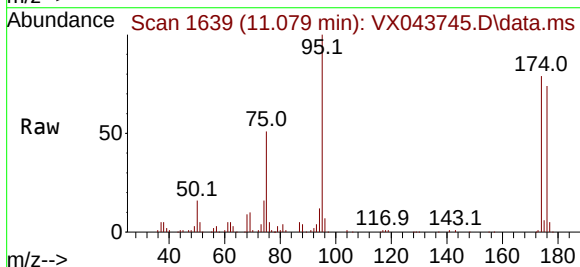




#82
4-Chlorotoluene
Concen: 0.293 ug/l
RT: 11.305 min Scan# 1700
Delta R.T. -0.146 min
Lab File: VX043745.D
Acq: 07 Nov 2024 18:35




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 977
Ion Ratio Lower Upper
91 100
126 0.0 14.2 42.8#



#83
tert-Butylbenzene
Concen: 0.249 ug/l
RT: 11.713 min Scan# 1743
Delta R.T. 0.000 min
Lab File: VX043745.D
Acq: 07 Nov 2024 18:35

Tgt Ion: 119 Resp: 868
Ion Ratio Lower Upper
119 100
91 73.7 29.5 88.5
134 23.7 11.8 35.3


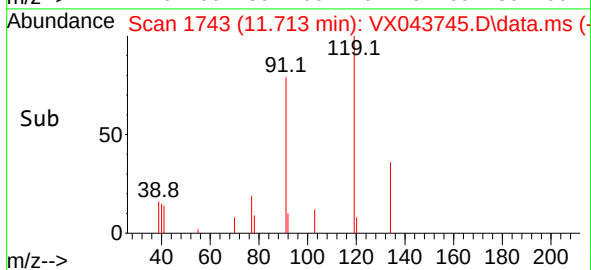






#85
 sec-Butylbenzene
 Concen: 0.342 ug/l
 RT: 11.890 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX043745.D
 Acq: 07 Nov 2024 18:35




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion:105 Resp: 1398
 Ion Ratio Lower Upper
 105 100
 134 25.8 9.8 29.5

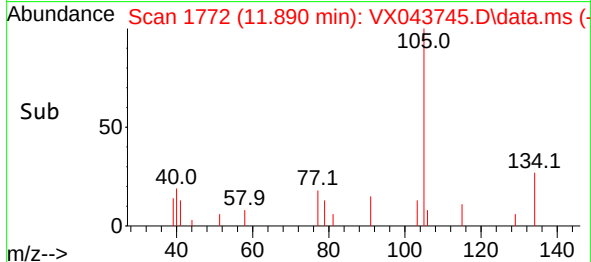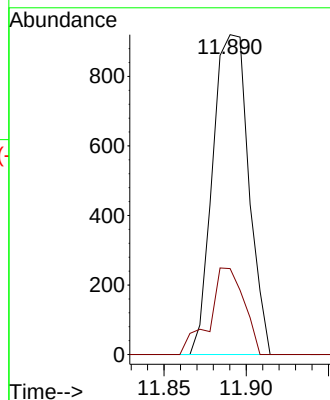

#90
 Hexachloroethane
 Concen: 1.989 ug/l
 RT: 12.646 min Scan# 1896
 Delta R.T. 0.110 min
 Lab File: VX043745.D
 Acq: 07 Nov 2024 18:35


Tgt Ion:117 Resp: 1123
 Ion Ratio Lower Upper
 117 100
 201 0.0 32.9 98.7#

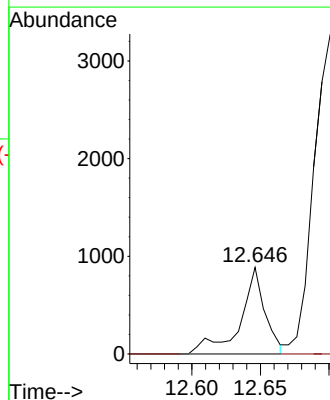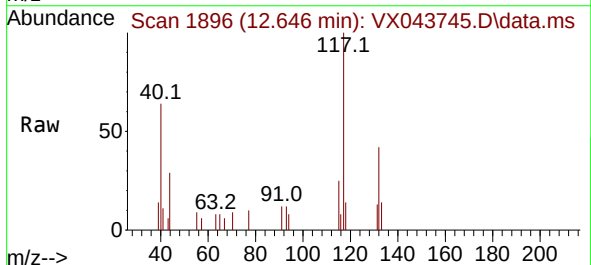



#95
Naphthalene
Concen: 0.208 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX043745.D
Acq: 07 Nov 2024 18:35

Instrument :
MSVOA_X
ClientSampleId :

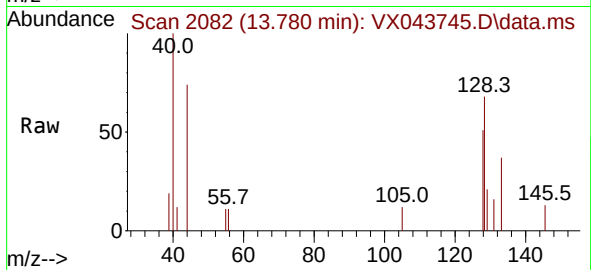

Tgt Ion:	128	Resp:	941
Ion	Ratio	Lower	Upper
128	100		
127	0.0	10.2	15.4#
129	9.2	8.7	13.1

