

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110724\
 Data File : VX043728.D
 Acq On : 07 Nov 2024 11:53
 Operator : JC/MD
 Sample : VX1107WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1107WBL01

Quant Time: Nov 08 04:04:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102824W.M
 Quant Title : SW846 8260
 QLast Update : Mon Oct 28 13:41:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	93207	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	162976	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	144247	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	66166	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	56688	38.143	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	76.280%
35) Dibromofluoromethane	5.385	113	50670	45.850	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	91.700%
50) Toluene-d8	8.647	98	186832	48.838	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	97.680%
62) 4-Bromofluorobenzene	11.079	95	66258	46.741	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	93.480%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110724\
Data File : VX043728.D
Acq On : 07 Nov 2024 11:53
Operator : JC/MD
Sample : VX1107WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1107WBL01


Quant Time: Nov 08 04:04:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102824W.M
Quant Title : SW846 8260
QLast Update : Mon Oct 28 13:41:34 2024
Response via : Initial Calibration

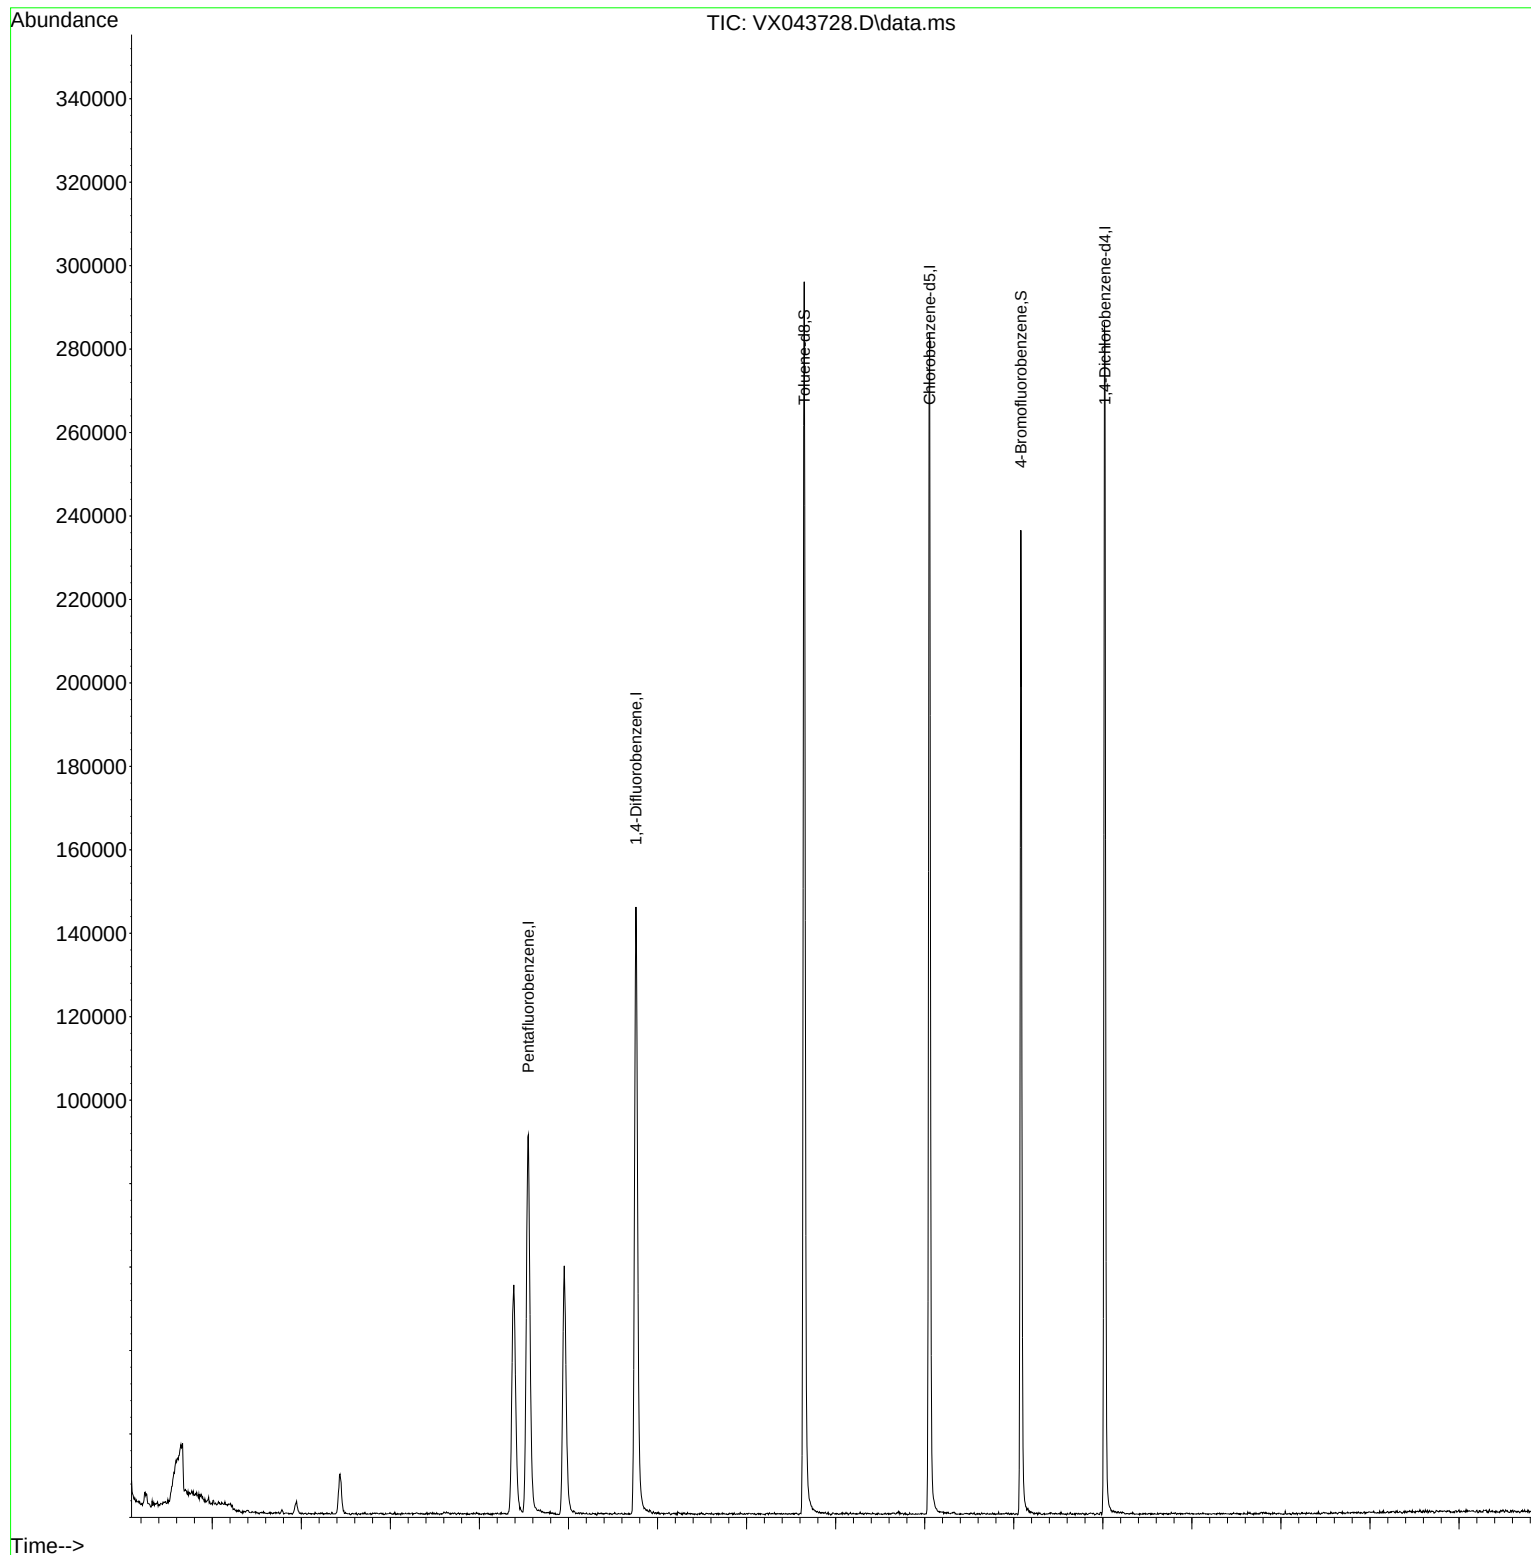



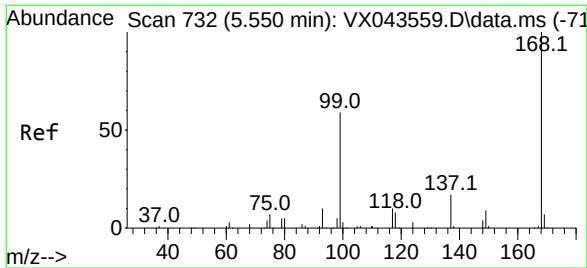


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.000 min
Lab File: VX043728.D
Acq: 07 Nov 2024 11:53

Instrument :
MSVOA_X
ClientSampleId :
VX1107WBL01



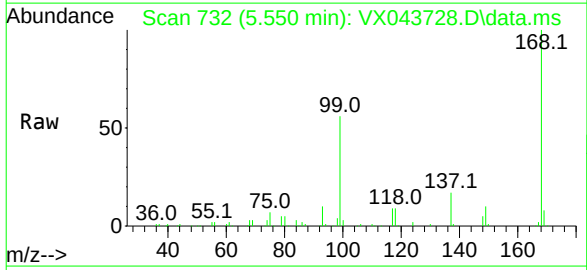



Tgt Ion:168 Resp: 93207
Ion Ratio Lower Upper
168 100
99 56.2 52.6 78.8

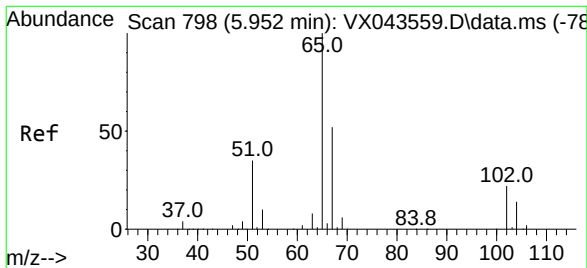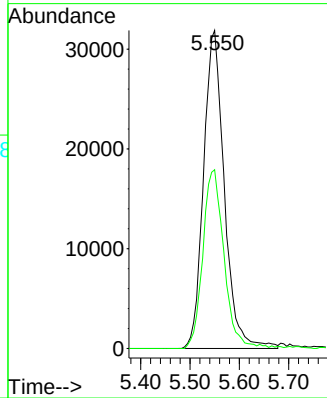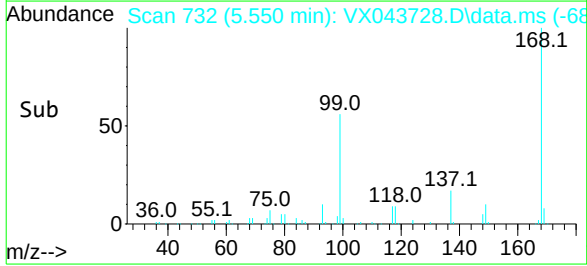

#33
1,2-Dichloroethane-d4
Concen: 38.143 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX043728.D
Acq: 07 Nov 2024 11:53

Tgt Ion: 65 Resp: 56688
Ion Ratio Lower Upper
65 100
67 52.6 0.0 103.4


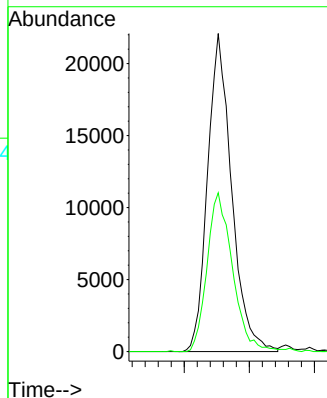
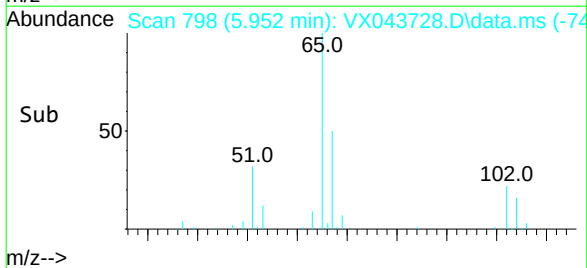
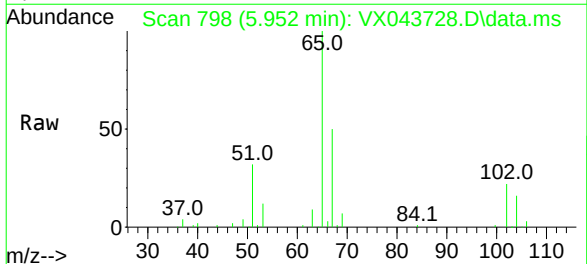


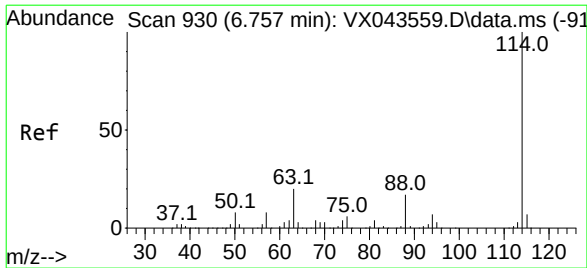

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 930
Delta R.T. 0.000 min
Lab File: VX043728.D
Acq: 07 Nov 2024 11:53




Instrument :
MSVOA_X
ClientSampleId :
VX1107WBL01


Tgt Ion:	114	Resp:	162976
Ion	Ratio	Lower	Upper
114	100		
63	18.4	0.0	41.2
88	14.7	0.0	34.0

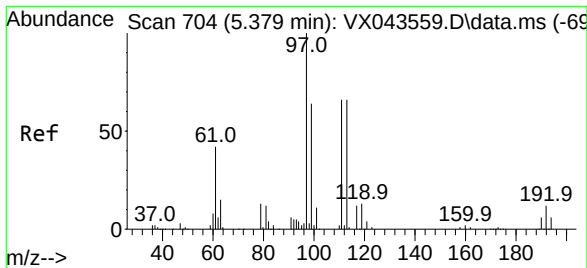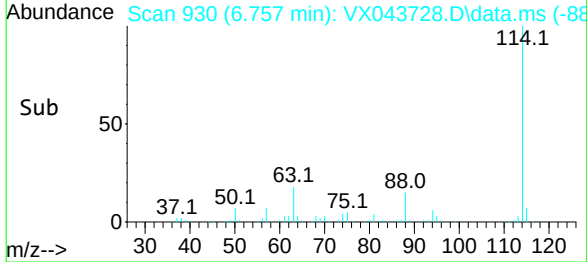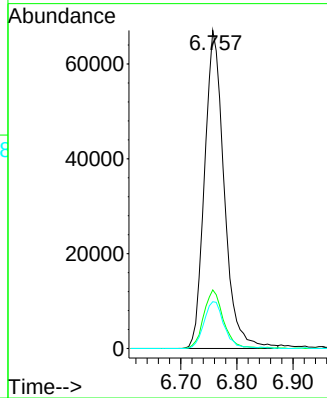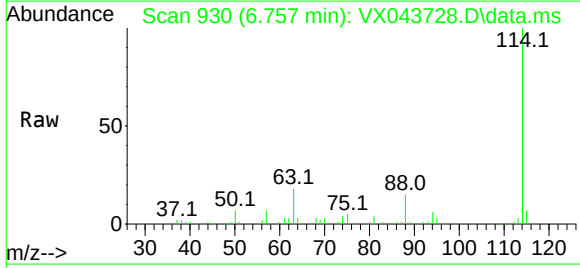

#35
Dibromofluoromethane
Concen: 45.850 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX043728.D
Acq: 07 Nov 2024 11:53

Tgt Ion:	113	Resp:	50670
Ion	Ratio	Lower	Upper
113	100		
111	101.8	81.4	122.0
192	20.0	14.1	21.1

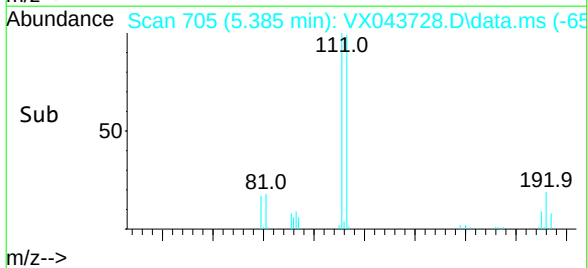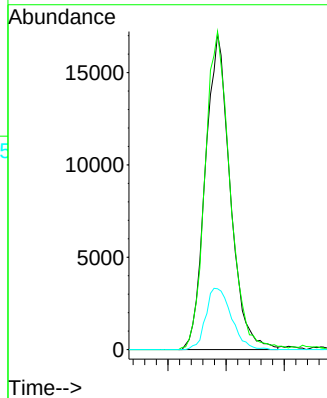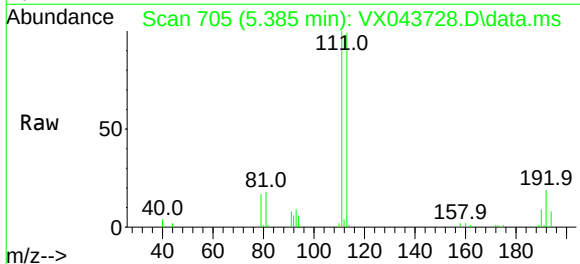

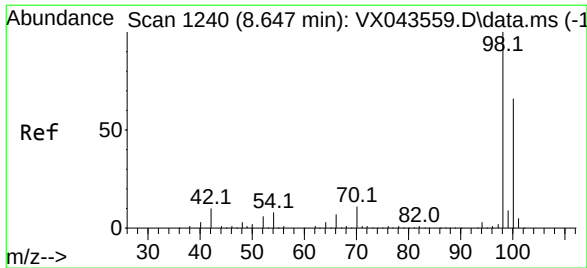

#50

Toluene-d8

Concen: 48.838 ug/l

RT: 8.647 min Scan# 12

Delta R.T. 0.000 min

Lab File: VX043728.D

Acq: 07 Nov 2024 11:53

Instrument :

MSVOA_X

ClientSampleId :





VX1107WBL01

Tgt Ion: 98 Resp: 186832

Ion Ratio Lower Upper

98 100

100 67.7 53.4 80.2

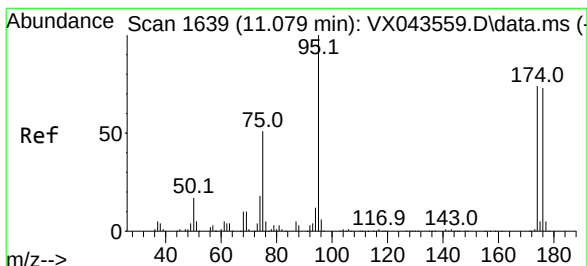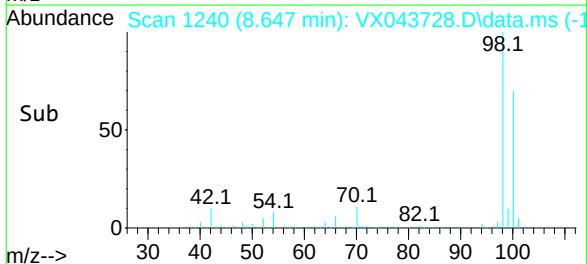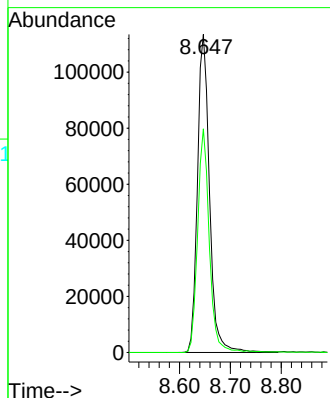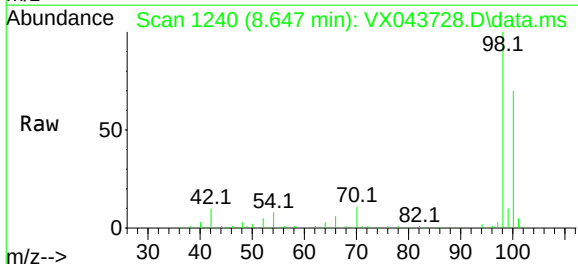

#62

4-Bromofluorobenzene

Concen: 46.741 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX043728.D

Acq: 07 Nov 2024 11:53




Tgt Ion: 95 Resp: 66258


Ion Ratio Lower Upper

95 100

174 81.8 0.0 146.6

176 78.4 0.0 139.6


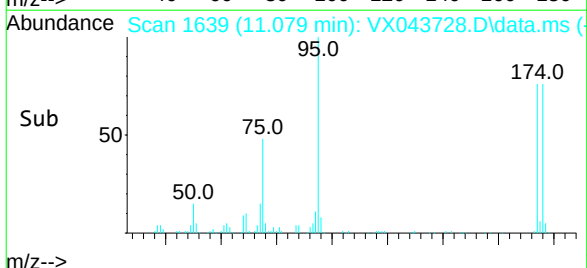
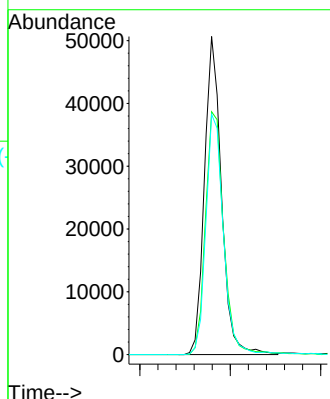
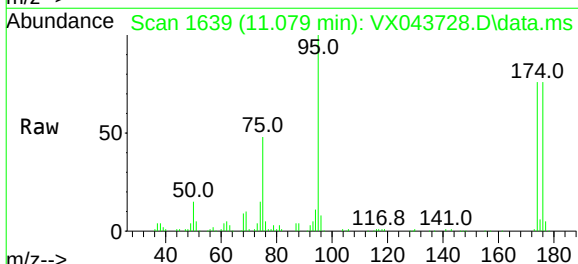


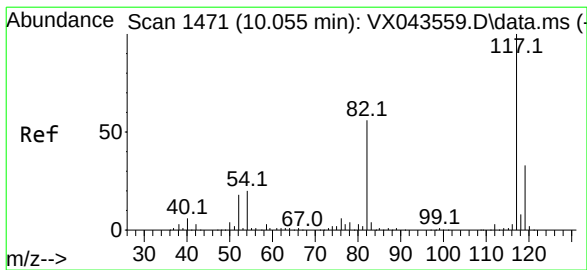

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX043728.D
Acq: 07 Nov 2024 11:53

Instrument :
MSVOA_X
ClientSampleId :
VX1107WBL01

Tgt Ion:117 Resp: 144247
Ion Ratio Lower Upper
117 100
82 52.0 42.1 63.1
119 33.8 25.4 38.2

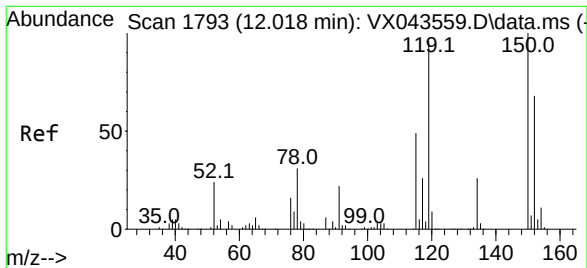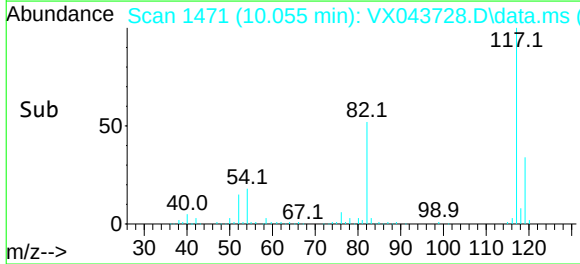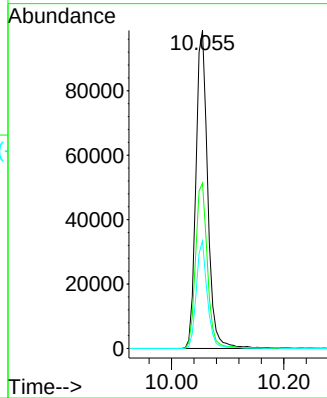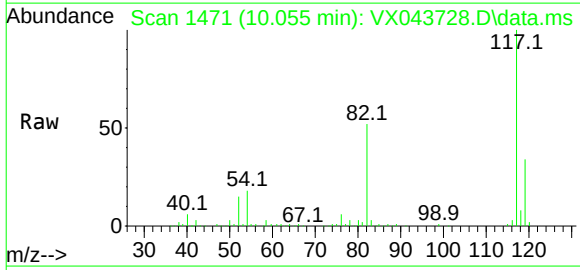

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX043728.D
Acq: 07 Nov 2024 11:53

Tgt Ion:152 Resp: 66166
Ion Ratio Lower Upper
152 100
115 59.2 42.9 128.7
150 156.8 0.0 343.6

