
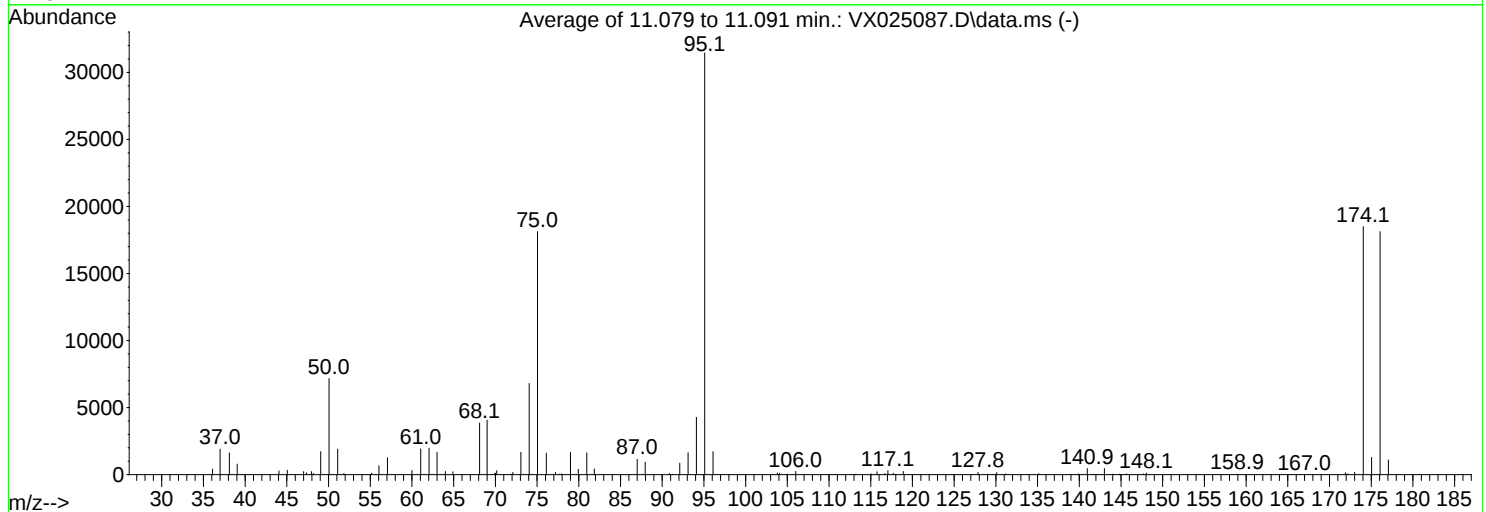


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110821\
 Data File : VX025087.D
 Acq On : 08 Nov 2021 08:43
 Operator : JC/MD
 Sample : BFB611
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB611

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110821WMA.M
 Title : VOC Analysis
 Last Update : Wed Nov 10 02:50:07 2021

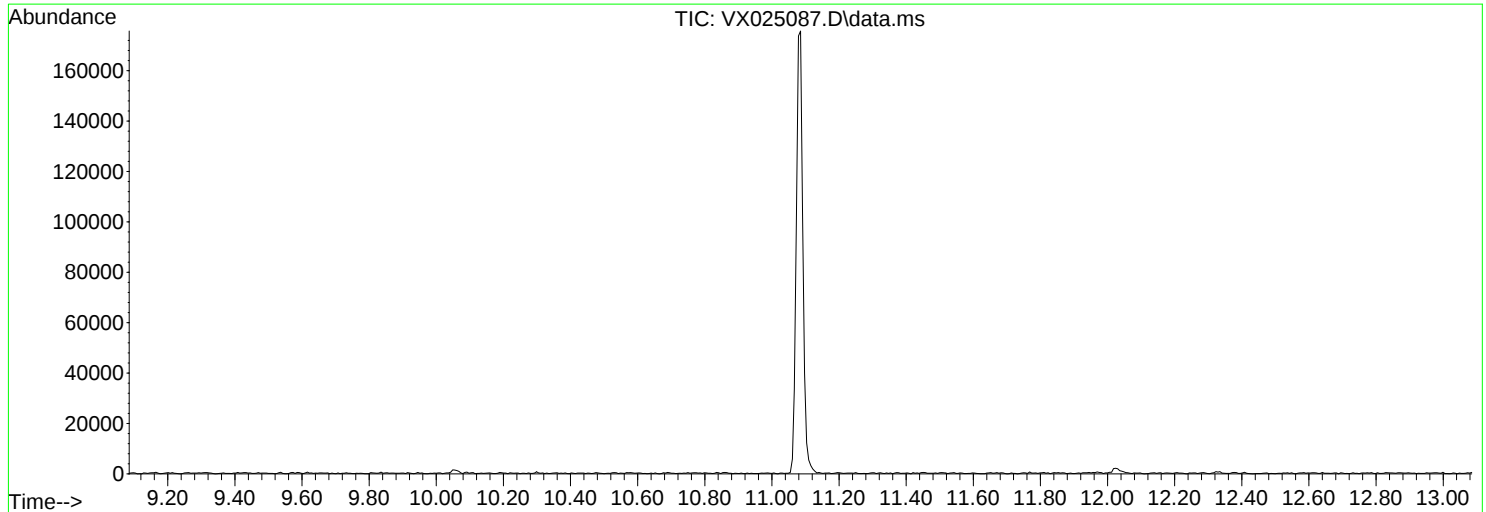

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.8	7170	PASS
75	95	30	80	57.6	18128	PASS
95	95	100	100	100.0	31456	PASS
96	95	5	9	5.5	1724	PASS
173	174	0.00	2	0.9	175	PASS
174	95	50	120	58.8	18493	PASS
175	174	5	9	7.0	1288	PASS
176	174	95	101	98.0	18122	PASS
177	176	5	9	6.1	1104	PASS

m/z	Abundance
40.00	130.0
41.90	62.0
44.10	93.0

Instrument :
MSVOA_X
ClientSampleId :
BFB611

m/z	Abundance
36.20	536.0
37.00	2257.0
38.10	2159.0
39.10	923.0
44.00	448.0
45.10	504.0
47.00	299.0
47.40	201.0
48.20	234.0
49.10	2503.0
50.00	9247.0
51.10	2457.0
51.90	117.0
55.20	64.0
56.10	654.0
57.00	1672.0
60.10	260.0
61.10	2767.0
62.10	2003.0
63.00	2312.0
64.00	560.0
64.90	229.0
68.10	4487.0
69.00	4791.0
69.90	241.0
70.20	231.0
72.10	279.0
73.10	2085.0
74.00	7790.0
75.10	22840.0
76.10	1739.0
77.20	250.0
77.70	120.0
79.00	2183.0
79.90	471.0
80.90	1761.0
81.80	535.0
87.00	1247.0
88.00	941.0
90.90	52.0
92.10	1100.0
93.10	1413.0
94.10	5349.0
95.10	36544.0
96.10	1937.0
103.80	368.0
105.00	70.0
106.00	253.0
115.00	69.0
115.90	327.0
117.10	410.0
117.70	191.0
119.00	283.0
127.80	254.0
129.00	148.0
130.10	100.0
135.10	136.0
139.90	181.0
141.00	556.0
141.70	99.0
142.90	509.0
144.00	87.0
145.70	87.0
147.70	93.0
148.00	157.0
171.90	133.0
173.00	126.0
174.00	17872.0
175.00	1292.0
176.10	18128.0
177.00	1061.0

Instrument :
MSVOA_X
ClientSampleId :
BFB611

m/z	Abundance
36.00	433.0
37.00	1960.0
38.10	1771.0
39.00	931.0
44.10	378.0
45.10	209.0
47.00	389.0
47.90	468.0
49.10	1843.0
50.10	7799.0
51.10	2173.0
51.80	100.0
54.70	57.0
55.10	119.0
56.00	940.0
57.10	1358.0
60.00	463.0
61.00	1930.0
62.10	2455.0
63.00	1831.0
63.90	119.0
65.00	245.0
68.10	4651.0
69.00	5061.0
70.10	659.0
71.80	152.0
73.10	1711.0
74.10	7976.0
75.00	19968.0
76.10	1462.0
77.20	245.0
77.90	107.0
79.00	1782.0
80.00	385.0
81.00	2096.0
81.90	460.0
87.00	1528.0
88.00	1068.0
90.90	118.0
92.10	867.0
93.10	2504.0
94.10	4531.0
95.10	37064.0
96.10	1626.0
104.00	200.0
105.00	78.0
106.00	222.0
113.20	56.0
115.10	109.0
115.70	197.0
116.70	268.0
117.10	239.0
117.70	142.0
118.80	240.0
127.90	168.0
130.10	286.0
131.20	100.0
135.20	96.0
140.90	442.0
143.00	444.0
144.10	70.0
144.80	114.0
145.60	85.0
147.70	76.0
148.00	74.0
158.90	58.0
161.00	55.0
167.00	63.0
171.90	291.0
173.00	186.0
174.00	23240.0
175.00	1472.0
176.00	21176.0
177.10	1516.0

Instrument :
MSVOA_X
ClientSampleId :
BFB611

m/z	Abundance
36.00	274.0
37.00	1462.0
38.10	948.0
39.00	495.0
40.20	97.0
44.00	290.0
45.00	304.0
47.30	195.0
48.00	216.0
48.90	796.0
50.10	4465.0
51.10	1064.0
51.90	73.0
55.20	128.0
56.00	411.0
57.00	752.0
59.90	212.0
61.00	1064.0
61.90	1498.0
62.90	835.0
63.90	51.0
64.80	156.0
68.00	2442.0
69.00	2373.0
70.00	307.0
72.10	227.0
72.90	1198.0
74.10	4651.0
75.10	11577.0
76.10	1624.0
77.90	61.0
79.00	1058.0
79.90	334.0
80.90	1021.0
81.90	304.0
83.00	63.0
87.10	660.0
87.90	770.0
90.70	98.0
91.20	63.0
92.00	604.0
93.00	995.0
94.00	2952.0
95.10	20760.0
96.10	1608.0
104.10	120.0
106.00	232.0
113.20	67.0
115.60	132.0
117.00	254.0
118.00	77.0
118.90	186.0
127.90	88.0
129.60	56.0
130.00	97.0
131.20	67.0
140.90	373.0
143.10	391.0
148.10	79.0
159.00	55.0
172.20	173.0
173.00	214.0
174.10	14367.0
175.10	1099.0
176.00	15061.0
177.00	735.0

Instrument :
MSVOA_X
ClientSampleId :
BFB611