

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110822\
 Data File : VX032649.D
 Acq On : 08 Nov 2022 13:20
 Operator : JC/MD
 Sample : N5497-02 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 09 04:37:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 27 08:28:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	108427	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	177876	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	160819	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	78971	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	74330	49.337	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	98.680%
35) Dibromofluoromethane	5.385	113	58058	45.758	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	91.520%
50) Toluene-d8	8.647	98	215614	48.871	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	97.740%
62) 4-Bromofluorobenzene	11.079	95	86030	49.919	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	99.840%
Target Compounds						
					Qvalue	
5) Bromomethane	1.624	94	230	0.247	ug/l #	53
10) Methyl Iodide	2.453	142	42	1.947	ug/l #	37
16) Acetone	2.386	43	151	0.276	ug/l #	45
19) Methyl tert-butyl Ether	3.111	73	1233	0.323	ug/l #	43
20) Methylene Chloride	2.788	84	438	0.349	ug/l #	87
31) Cyclohexane	5.464	56	785	0.430	ug/l #	83
36) 1,1-Dichloropropene	5.550	75	8466	4.792	ug/l #	49
38) Carbon Tetrachloride	5.550	117	11396	5.815	ug/l #	15
39) Methylcyclohexane	7.373	83	794	0.380	ug/l #	93
40) Benzene	6.044	78	9203	1.841	ug/l #	88
51) 4-Methyl-2-Pentanone	8.653	43	991	0.557	ug/l #	1
52) Toluene	8.720	92	6418	1.967	ug/l	93
67) Ethyl Benzene	10.195	91	146001	22.664	ug/l	99
68) m/p-Xylenes	10.299	106	224142	89.604	ug/l	100
69) o-Xylene	10.640	106	104537	42.982	ug/l	98
70) Styrene	10.640	104	5369	1.328	ug/l #	1
73) Isopropylbenzene	10.963	105	7497	1.198	ug/l	100
76) 1,2,3-Trichloropropane	11.079	75	46941	26.718	ug/l #	35
78) n-propylbenzene	11.305	91	19711	2.734	ug/l	98
79) 2-Chlorotoluene	11.378	91	18528	4.291	ug/l #	41
80) 1,3,5-Trimethylbenzene	11.451	105	43820	8.193	ug/l	98
81) trans-1,4-Dichloro-2-b...	11.079	75	46941	85.017	ug/l #	6
82) 4-Chlorotoluene	11.451	91	5206	1.030	ug/l #	45
83) tert-Butylbenzene	11.750	119	20966	3.927	ug/l #	51
84) 1,2,4-Trimethylbenzene	11.750	105	177187	33.309	ug/l	100
85) sec-Butylbenzene	11.750	105	177187	27.578	ug/l #	57
86) p-Isopropyltoluene	11.969	119	1669	0.306	ug/l #	75
89) n-Butylbenzene	12.323	91	2827	0.596	ug/l #	9
90) Hexachloroethane	12.616	117	1199	1.346	ug/l #	12
95) Naphthalene	13.774	128	63285	10.208	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110822\
Data File : VX032649.D
Acq On : 08 Nov 2022 13:20
Operator : JC/MD
Sample : N5497-02 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Nov 09 04:37:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 27 08:28:06 2022
Response via : Initial Calibration

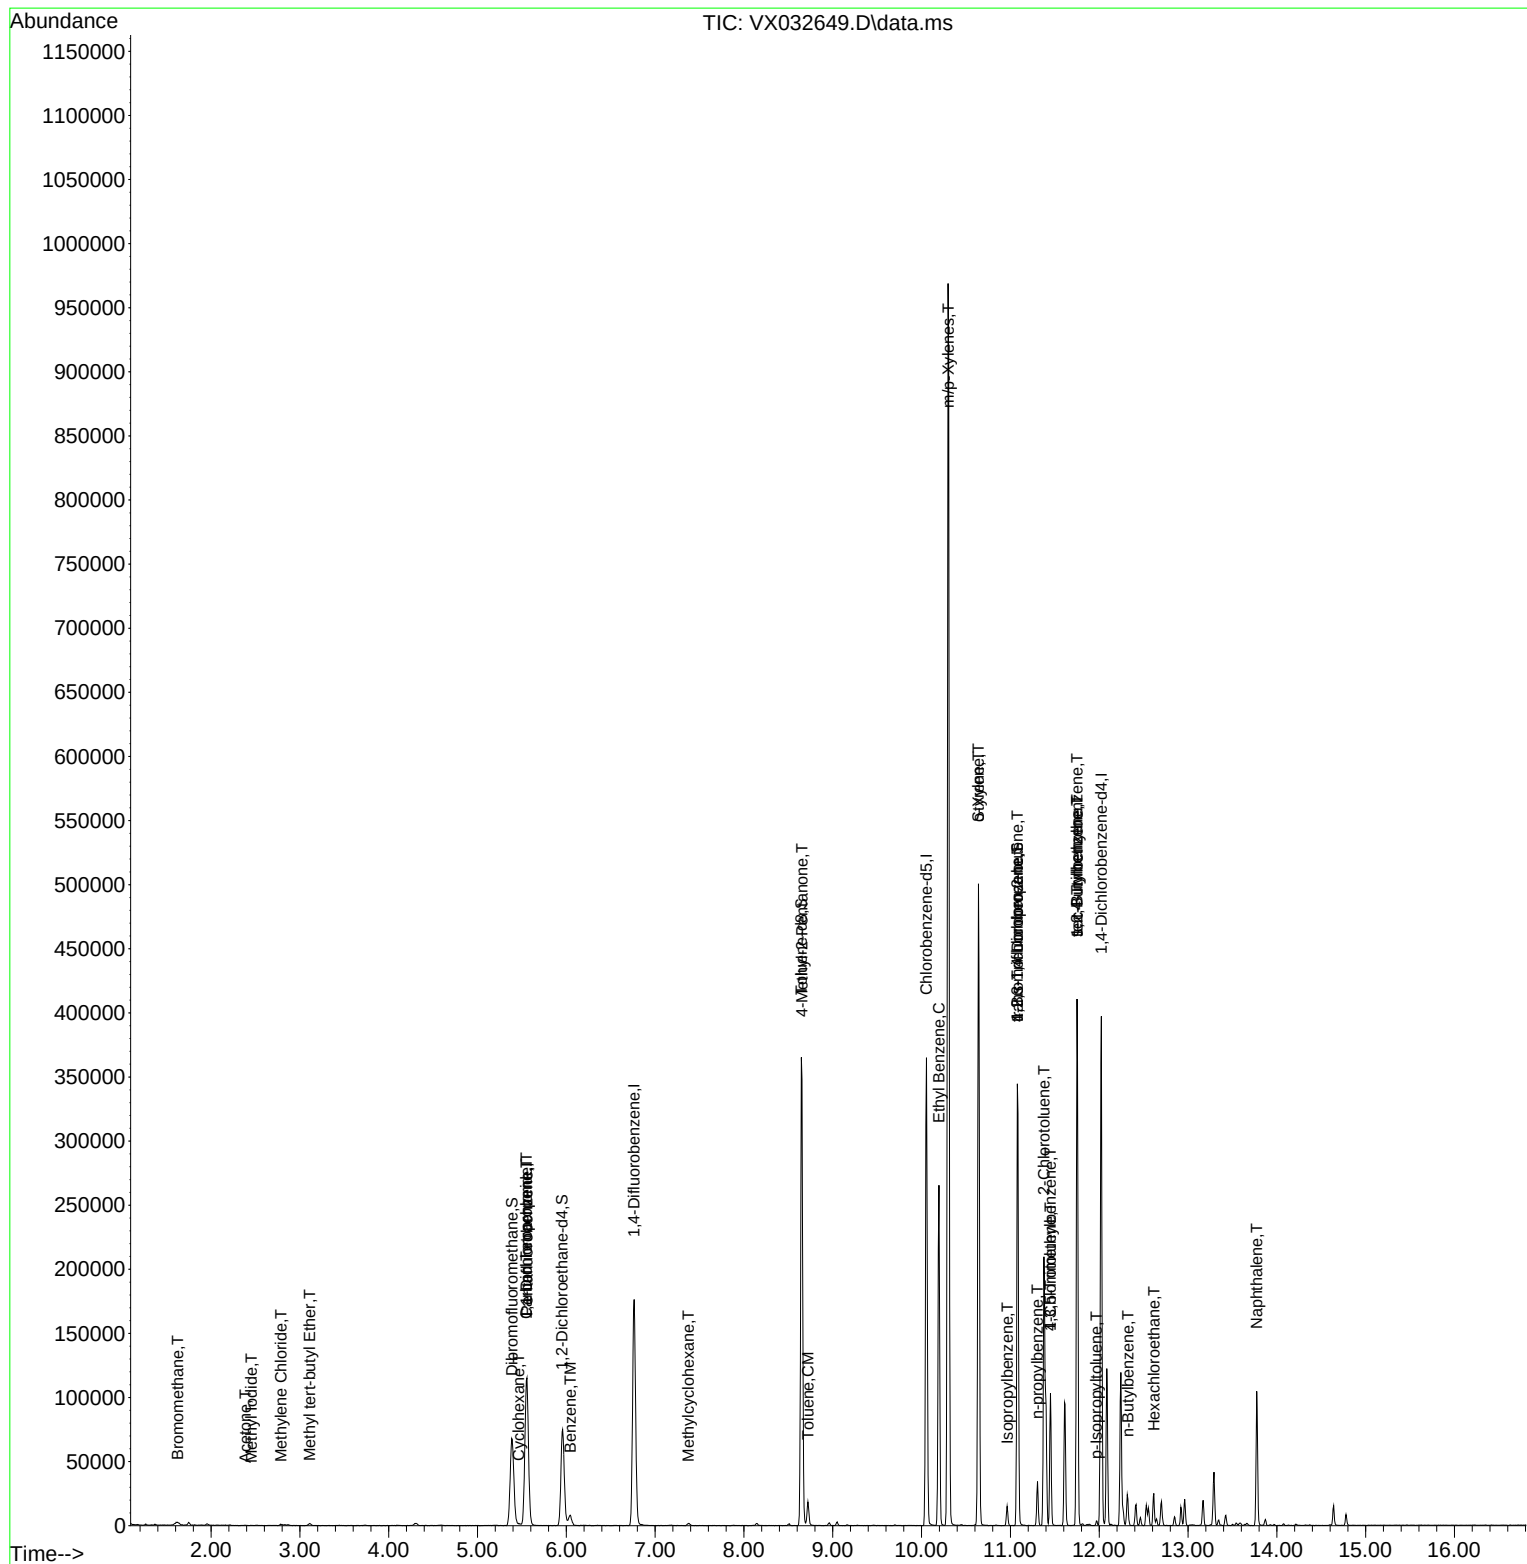






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20

Instrument :
MSVOA_X
ClientSampleId :



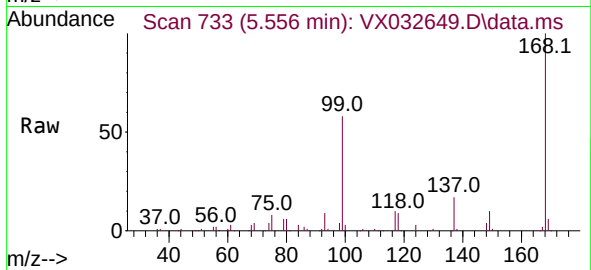



Tgt Ion:168 Resp: 108427
Ion Ratio Lower Upper
168 100
99 58.2 46.1 69.1



#5
Bromomethane
Concen: 0.247 ug/l
RT: 1.624 min Scan# 88
Delta R.T. 0.018 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20


Tgt Ion: 94 Resp: 230
Ion Ratio Lower Upper
94 100
96 51.3 77.6 116.4#

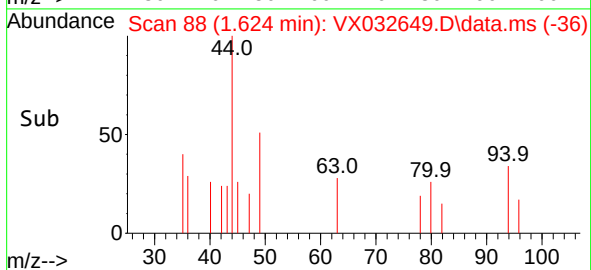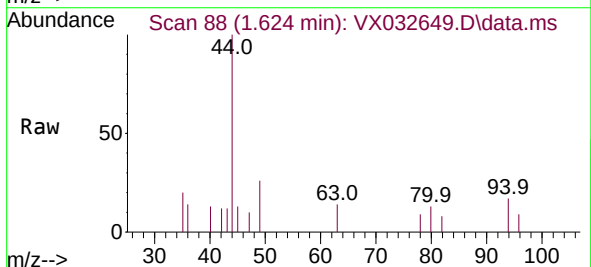



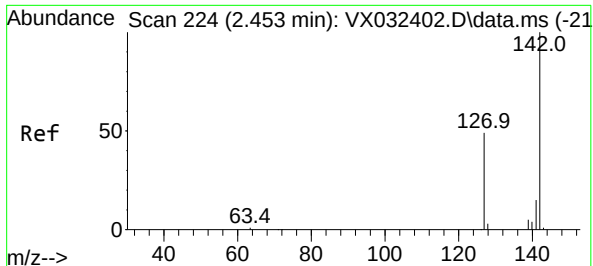


#10
Methyl Iodide
Concen: 1.947 ug/l
RT: 2.453 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20

Instrument :
MSVOA_X
ClientSampleId :



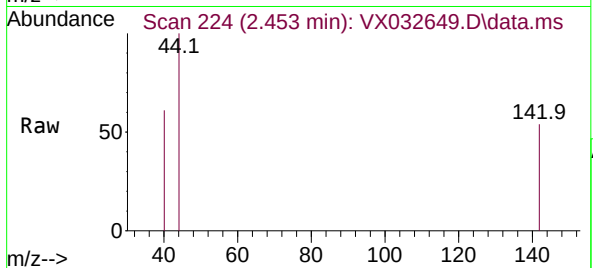



Tgt Ion:142 Resp: 42
Ion Ratio Lower Upper
142 100
127 0.0 38.6 57.8#
141 0.0 11.4 17.2#

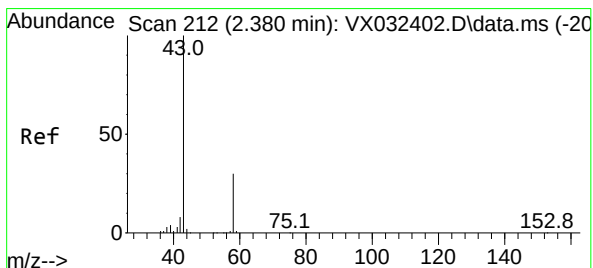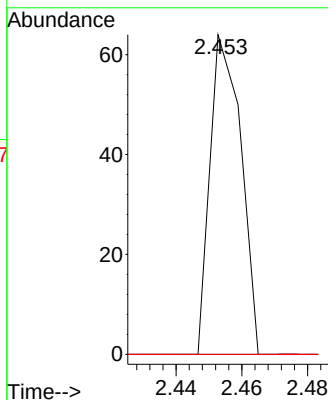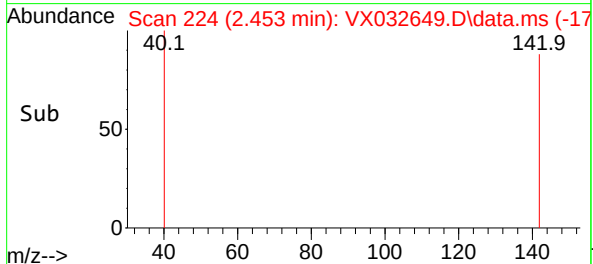

#16
Acetone
Concen: 0.276 ug/l
RT: 2.386 min Scan# 213
Delta R.T. 0.006 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20

Tgt Ion: 43 Resp: 151
Ion Ratio Lower Upper
43 100
58 0.0 23.8 35.8#


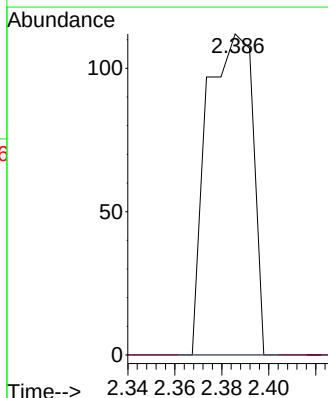
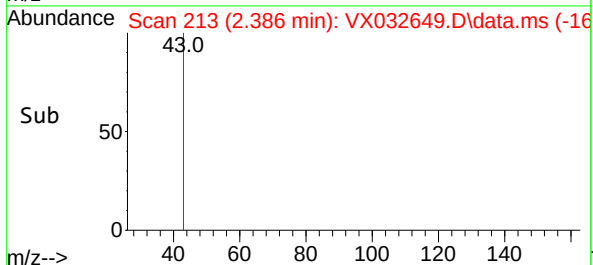
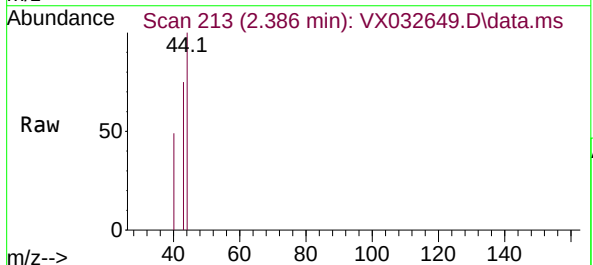




#19
Methyl tert-butyl Ether
Concen: 0.323 ug/l
RT: 3.111 min Scan# 311
Delta R.T. 0.000 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 73 Resp: 1233
Ion Ratio Lower Upper
73 100
57 47.2 16.6 25.0#

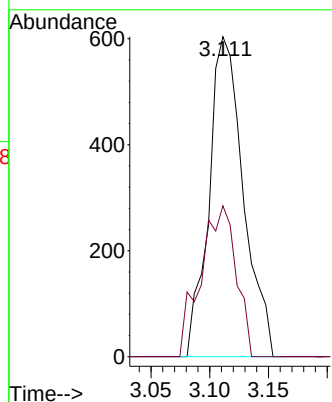

#20
Methylene Chloride
Concen: 0.349 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.000 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20


Tgt Ion: 84 Resp: 438
Ion Ratio Lower Upper
84 100
49 130.3 101.0 151.6
51 32.8 31.1 46.7
86 38.5 52.3 78.5#

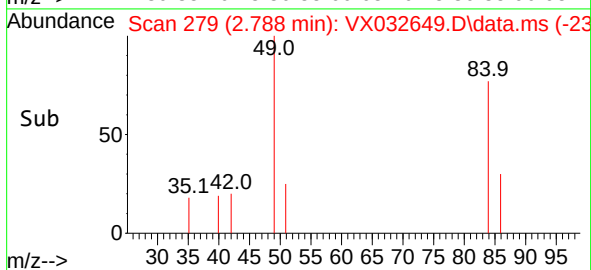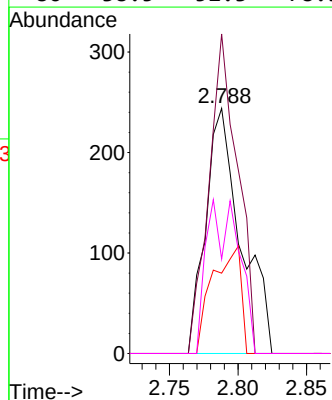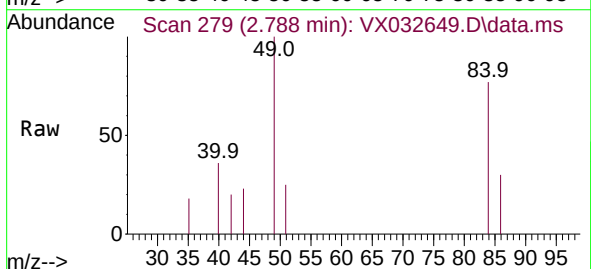






#31
Cyclohexane
Concen: 0.430 ug/l
RT: 5.464 min Scan# 718
Delta R.T. -0.006 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 56 Resp: 785
Ion Ratio Lower Upper
56 100
69 0.0 24.1 36.1#
84 80.8 66.9 100.3



#33
1,2-Dichloroethane-d4
Concen: 49.337 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20

Tgt Ion: 65 Resp: 74330
Ion Ratio Lower Upper
65 100
67 51.8 0.0 101.8


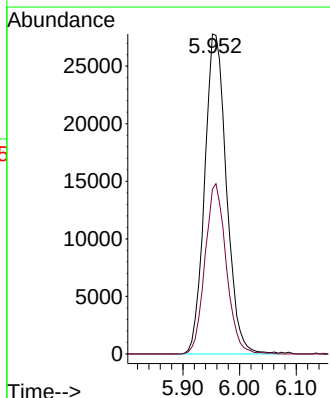
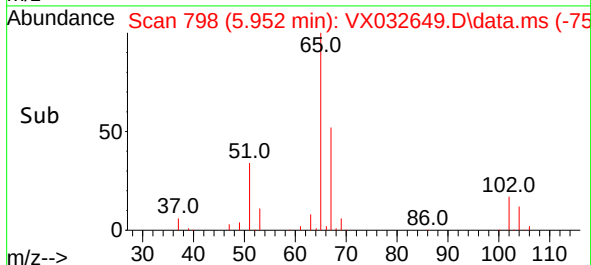
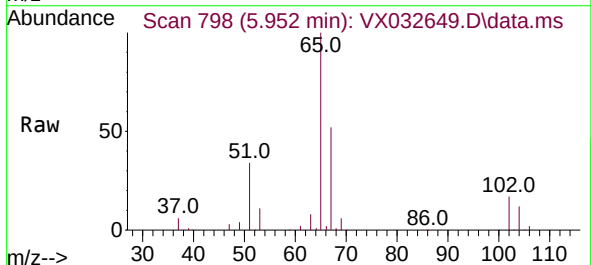




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:114 Resp: 177876
Ion Ratio Lower Upper
114 100
63 20.0 0.0 41.6
88 16.1 0.0 33.4



#35
Dibromofluoromethane
Concen: 45.758 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20

Tgt Ion:113 Resp: 58058
Ion Ratio Lower Upper
113 100
111 103.1 82.4 123.6
192 19.6 15.4 23.2


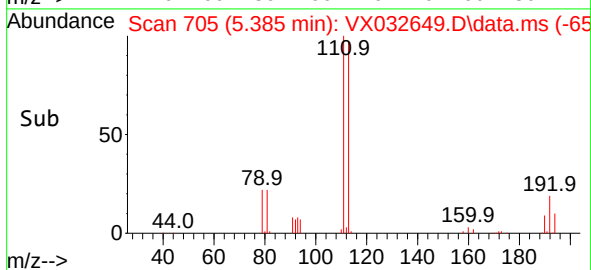

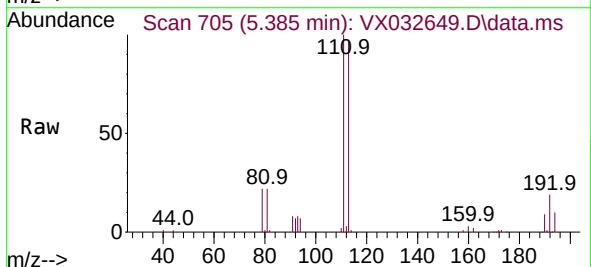


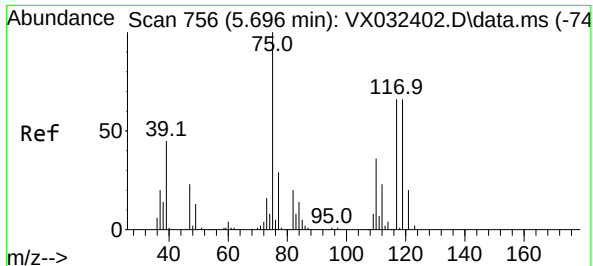

#36
 1,1-Dichloropropene
 Concen: 4.792 ug/l
 RT: 5.550 min Scan# 712
 Delta R.T. -0.146 min
 Lab File: VX032649.D
 Acq: 08 Nov 2022 13:20




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion: 75 Resp: 8466
 Ion Ratio Lower Upper
 75 100
 110 9.0 18.4 55.2#
 77 0.0 24.5 36.7#

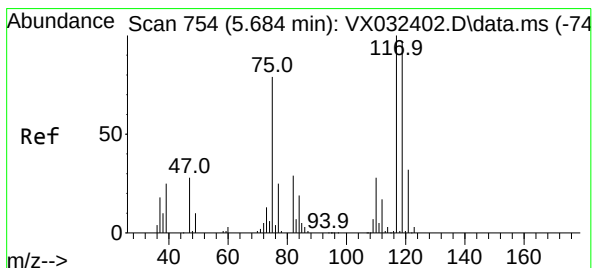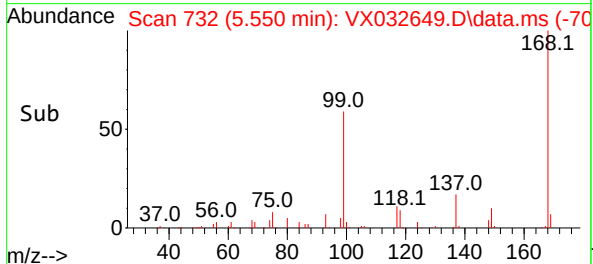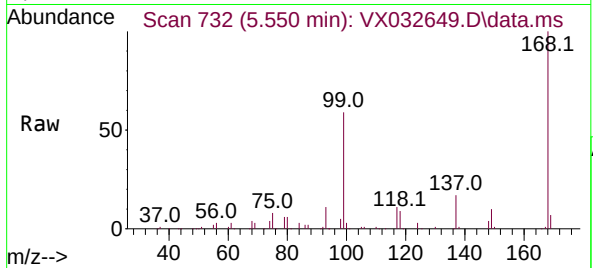

#38
 Carbon Tetrachloride
 Concen: 5.815 ug/l
 RT: 5.550 min Scan# 732
 Delta R.T. -0.134 min
 Lab File: VX032649.D
 Acq: 08 Nov 2022 13:20

Tgt Ion: 117 Resp: 11396
 Ion Ratio Lower Upper
 117 100
 119 4.2 77.2 115.8#
 121 0.0 25.8 38.6#

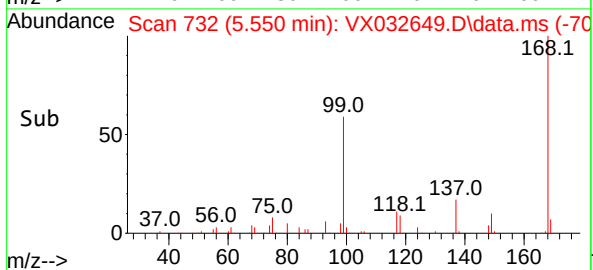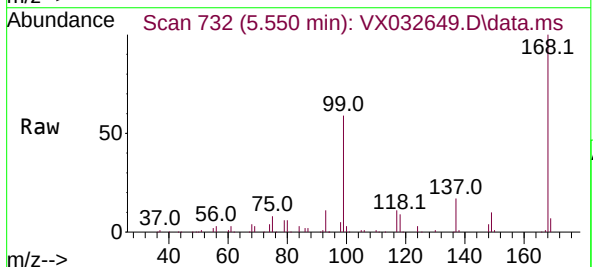



#39

Methylcyclohexane

Concen: 0.380 ug/l

RT: 7.373 min Scan# 1031

Delta R.T. -0.012 min

Lab File: VX032649.D

Acq: 08 Nov 2022 13:20

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 83 Resp: 794

Ion Ratio Lower Upper

83 100

55 71.0 58.4 87.6

98 36.7 37.2 55.8#

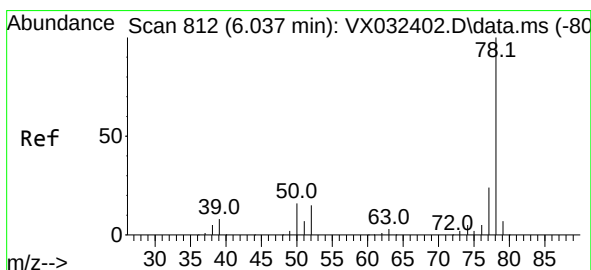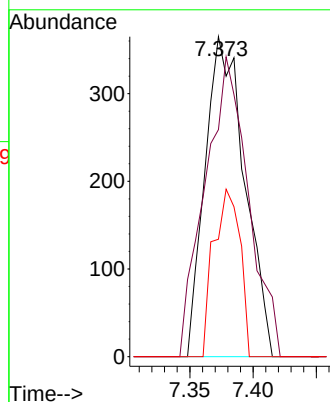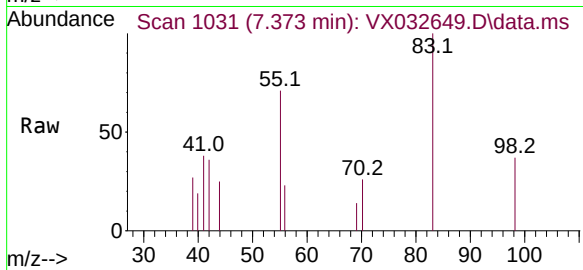

#40

Benzene

Concen: 1.841 ug/l

RT: 6.044 min Scan# 813

Delta R.T. 0.006 min

Lab File: VX032649.D




Acq: 08 Nov 2022 13:20


Tgt Ion: 78 Resp: 9203

Ion Ratio Lower Upper

78 100

77 29.6 19.0 28.4#

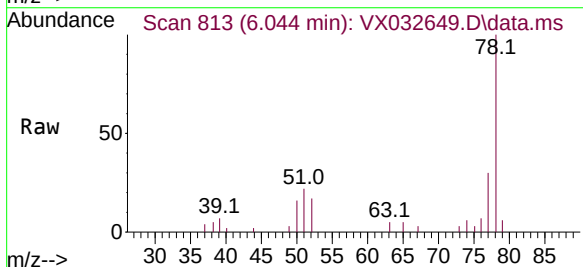

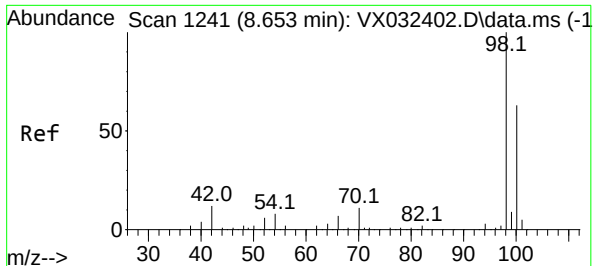

#50

Toluene-d8

Concen: 48.871 ug/l

RT: 8.647 min Scan# 11

Delta R.T. -0.006 min

Lab File: VX032649.D

Acq: 08 Nov 2022 13:20

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 98 Resp: 215614

Ion Ratio Lower Upper

98 100

100 63.7 50.9 76.3

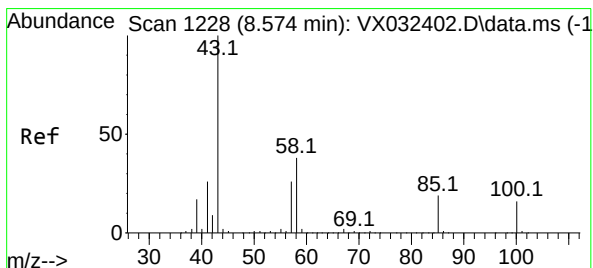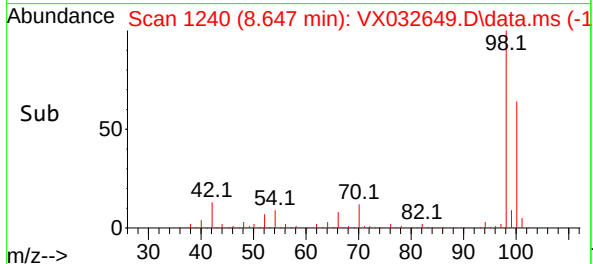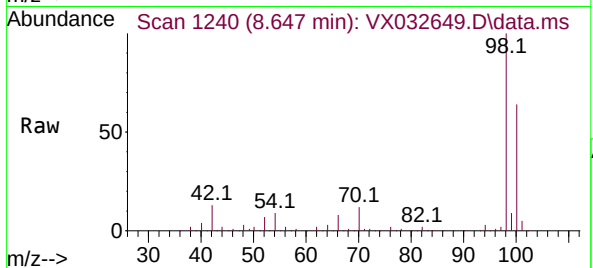

#51

4-Methyl-2-Pentanone

Concen: 0.557 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. 0.079 min

Lab File: VX032649.D




Acq: 08 Nov 2022 13:20


Tgt Ion: 43 Resp: 991

Ion Ratio Lower Upper

43 100

58 188.0 30.9 46.3#


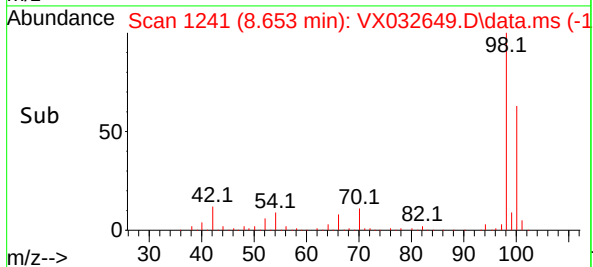

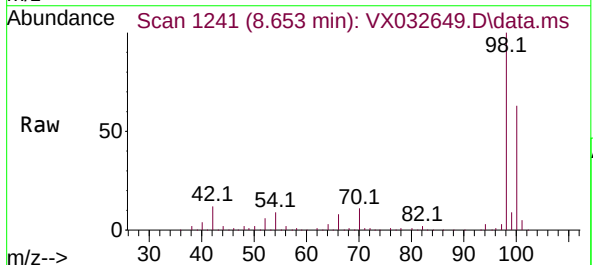




#52
Toluene
Concen: 1.967 ug/l
RT: 8.720 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 92 Resp: 6418
Ion Ratio Lower Upper
92 100
91 183.0 138.3 207.5



#62
4-Bromofluorobenzene
Concen: 49.919 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20

Tgt Ion: 95 Resp: 86030
Ion Ratio Lower Upper
95 100
174 84.0 0.0 164.0
176 81.5 0.0 154.4


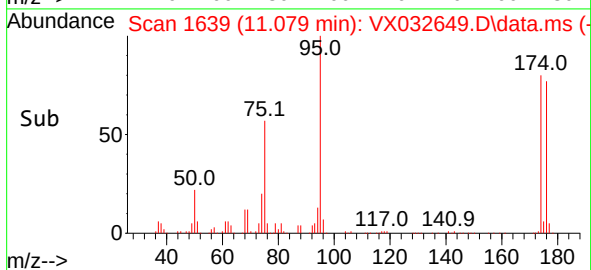

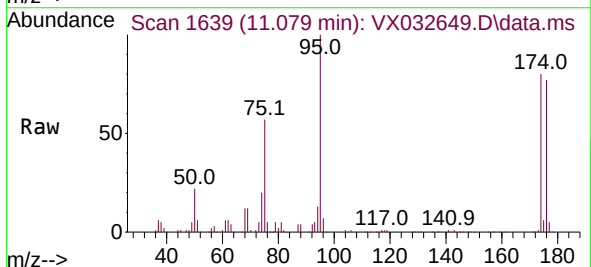




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:117 Resp: 160819
Ion Ratio Lower Upper
117 100
82 54.5 44.3 66.5
119 32.2 25.7 38.5

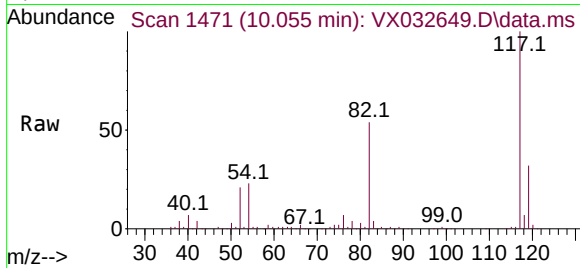

#67
Ethyl Benzene
Concen: 22.664 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20

Tgt Ion: 91 Resp: 146001
Ion Ratio Lower Upper
91 100
106 31.9 25.0 37.6



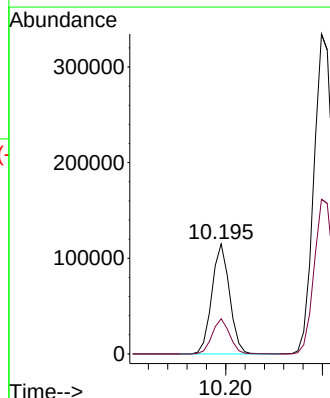
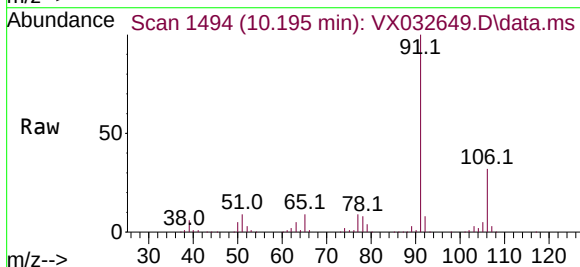




#68
m/p-Xylenes
Concen: 89.604 ug/l
RT: 10.299 min Scan# 1512
Delta R.T. -0.006 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 224142
Ion Ratio Lower Upper
106 100
91 205.7 164.5 246.7

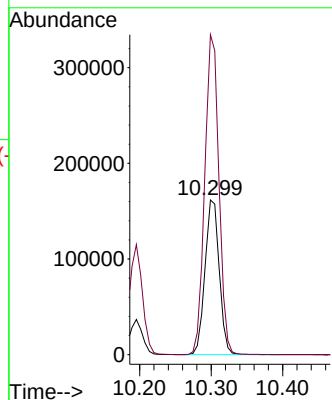

#69
o-Xylene
Concen: 42.982 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. 0.000 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20

Tgt Ion:106 Resp: 104537
Ion Ratio Lower Upper
106 100
91 215.8 109.2 327.6



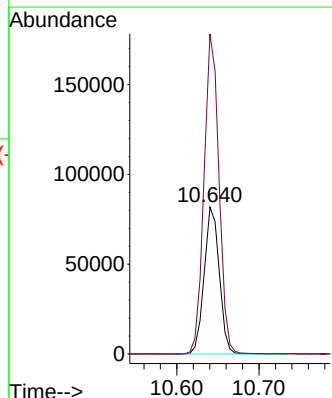
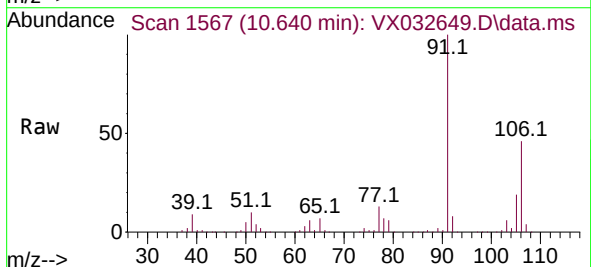




#70
Styrene
Concen: 1.328 ug/l
RT: 10.640 min Scan# 11
Delta R.T. -0.018 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:104 Resp: 5369
Ion Ratio Lower Upper
104 100
78 306.5 41.8 62.8#
103 269.4 44.5 66.7#

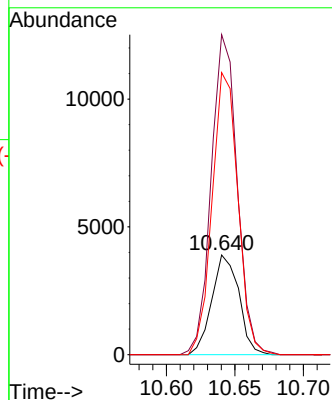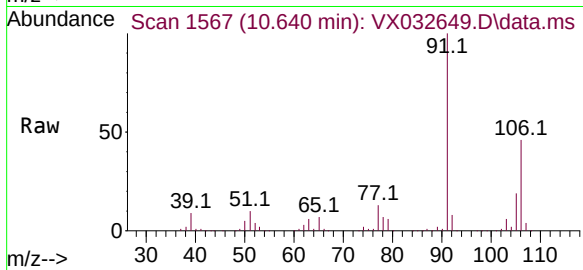

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20

Tgt Ion:152 Resp: 78971
Ion Ratio Lower Upper
152 100
115 60.8 44.0 132.0
150 158.3 0.0 351.8

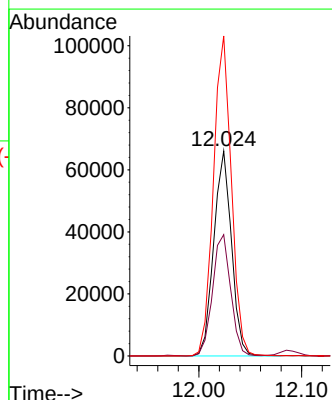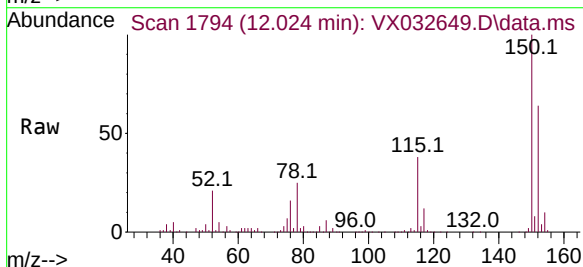



#73

Isopropylbenzene

Concen: 1.198 ug/l

RT: 10.963 min Scan# 1620

Delta R.T. 0.000 min

Lab File: VX032649.D

Acq: 08 Nov 2022 13:20

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 7497

Ion Ratio Lower Upper

105 100

120 26.2 13.1 39.3

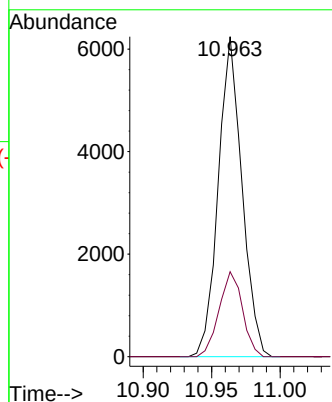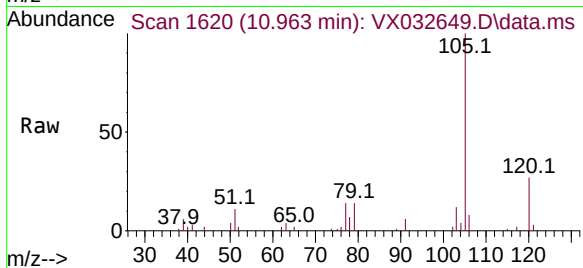

#76

1,2,3-Trichloropropane

Concen: 26.718 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.165 min

Lab File: VX032649.D




Acq: 08 Nov 2022 13:20


Tgt Ion: 75 Resp: 46941

Ion Ratio Lower Upper

75 100

77 0.0 20.0 60.0#


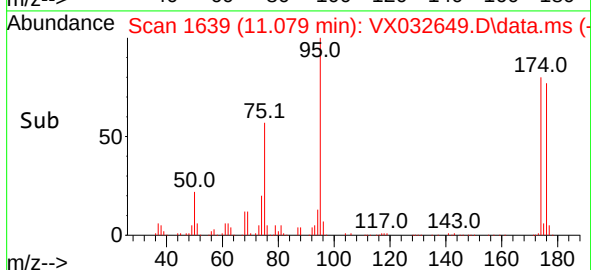
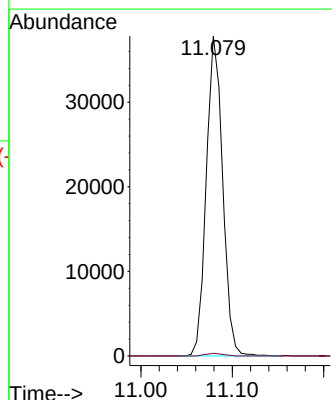
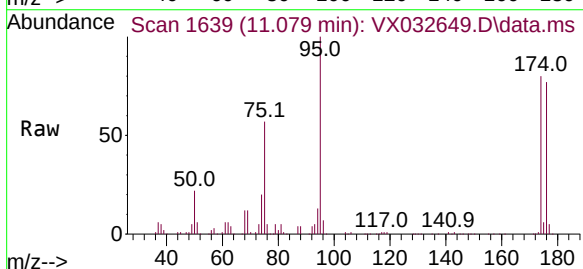


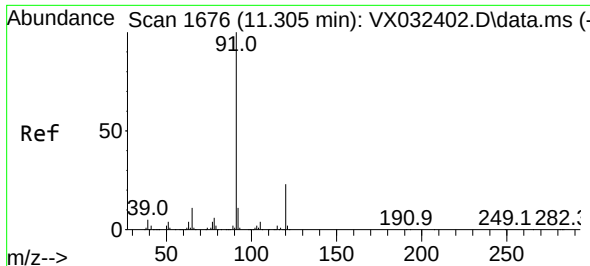

#78
n-propylbenzene
Concen: 2.734 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.000 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 19711
Ion Ratio Lower Upper
91 100
120 22.4 11.6 34.8

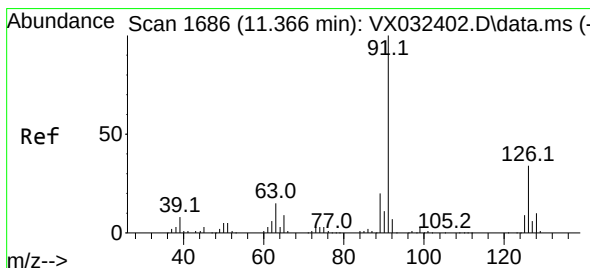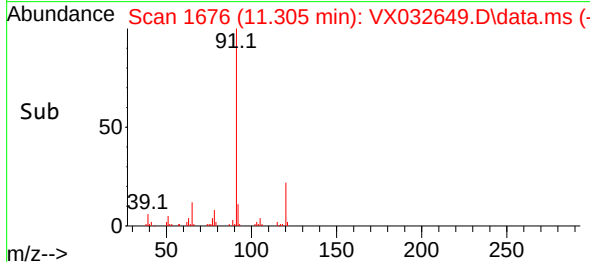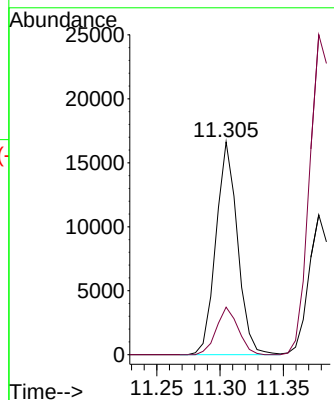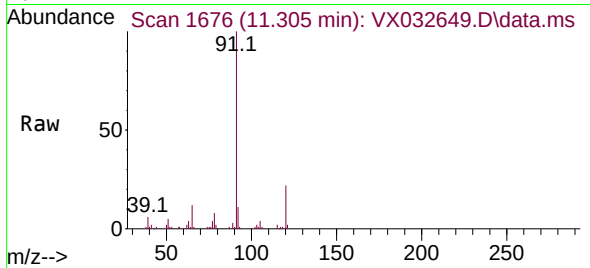

#79
2-Chlorotoluene
Concen: 4.291 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.012 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20

Tgt Ion: 91 Resp: 18528
Ion Ratio Lower Upper
91 100
126 0.0 17.1 51.2#


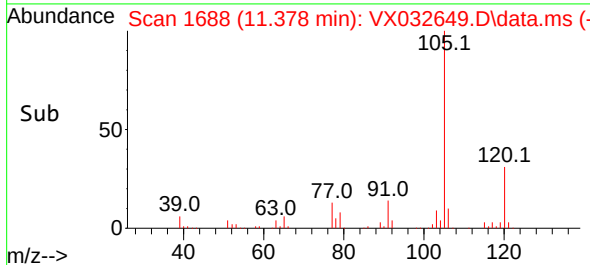
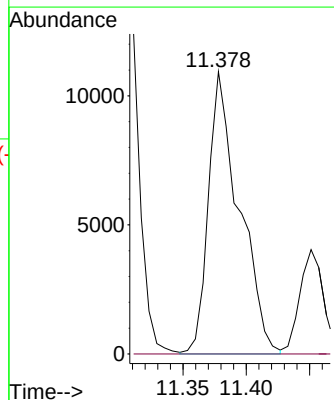
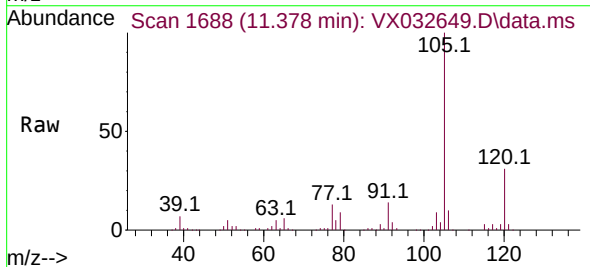




#80
1,3,5-Trimethylbenzene
Concen: 8.193 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:105 Resp: 43820
Ion Ratio Lower Upper
105 100
120 46.0 23.6 71.0

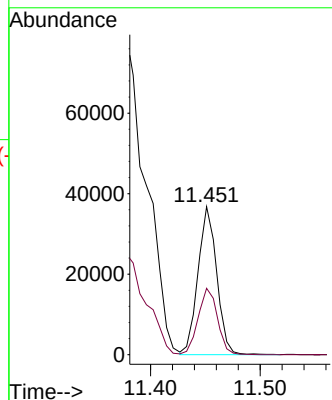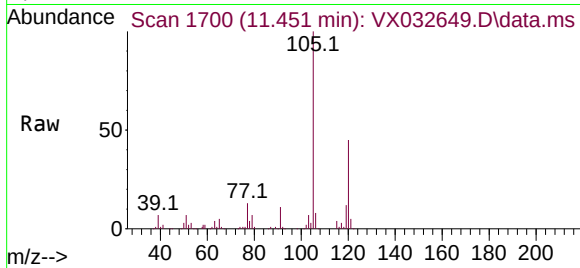

#81
trans-1,4-Dichloro-2-butene
Concen: 85.017 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20

Tgt Ion: 75 Resp: 46941
Ion Ratio Lower Upper
75 100
53 0.0 86.9 130.3#
89 0.0 38.3 57.5#

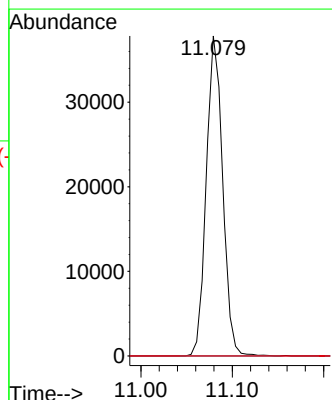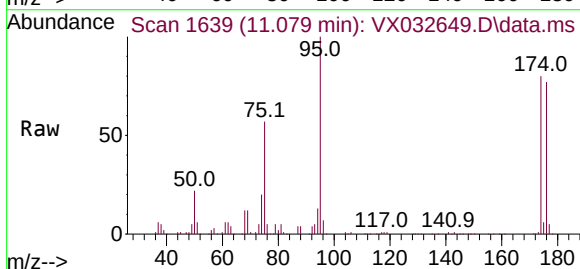



#82

4-Chlorotoluene

Concen: 1.030 ug/l

RT: 11.451 min Scan# 11

Delta R.T. -0.006 min

Lab File: VX032649.D

Acq: 08 Nov 2022 13:20

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 5206

Ion Ratio Lower Upper

91 100

126 0.0 14.8 44.4#

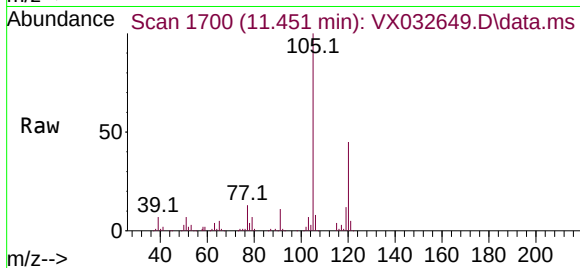

#83

tert-Butylbenzene

Concen: 3.927 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. 0.037 min

Lab File: VX032649.D

Acq: 08 Nov 2022 13:20




Tgt Ion: 119 Resp: 20966


Ion Ratio Lower Upper

119 100

91 95.8 29.4 88.2#

134 0.0 11.0 33.0#


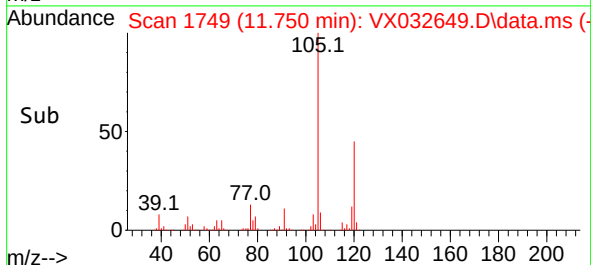
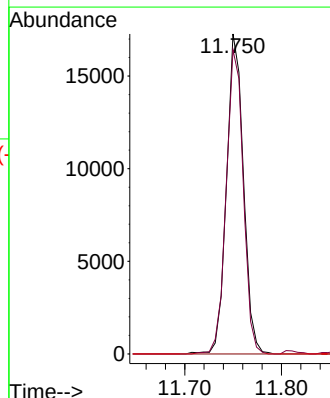
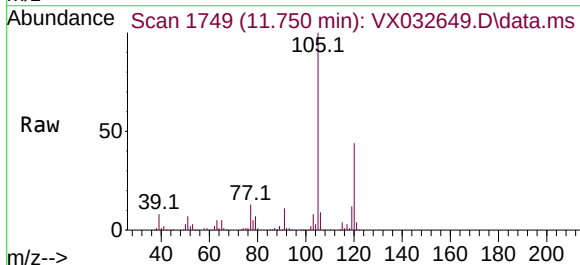




#84
 1,2,4-Trimethylbenzene
 Concen: 33.309 ug/l
 RT: 11.750 min Scan# 1749
 Delta R.T. 0.000 min
 Lab File: VX032649.D
 Acq: 08 Nov 2022 13:20




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion:105 Resp: 177187
 Ion Ratio Lower Upper
 105 100
 120 43.7 21.9 65.5

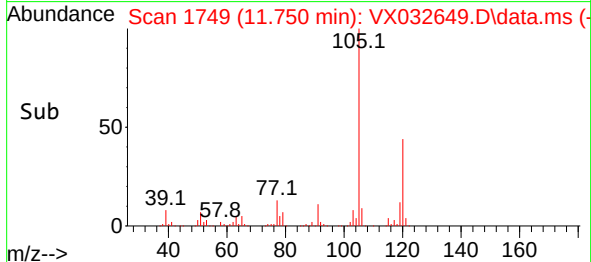

#85
 sec-Butylbenzene
 Concen: 27.578 ug/l
 RT: 11.750 min Scan# 1749
 Delta R.T. -0.140 min
 Lab File: VX032649.D
 Acq: 08 Nov 2022 13:20

Tgt Ion:105 Resp: 177187
 Ion Ratio Lower Upper
 105 100
 134 0.0 9.9 29.7#


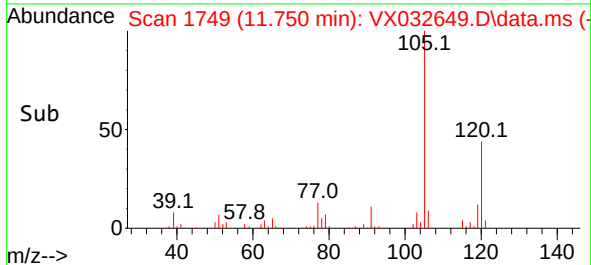

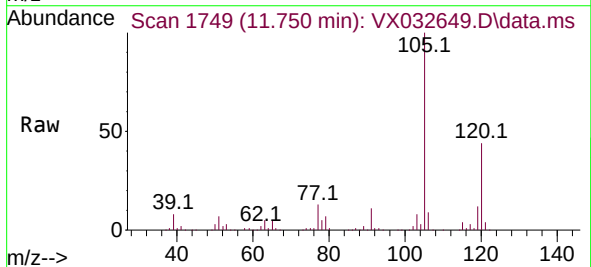




#86
p-Isopropyltoluene
Concen: 0.306 ug/l
RT: 11.969 min Scan# 11
Delta R.T. -0.043 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:119 Resp: 1669
Ion Ratio Lower Upper
119 100
134 26.7 12.9 38.7
91 0.0 12.5 37.5#

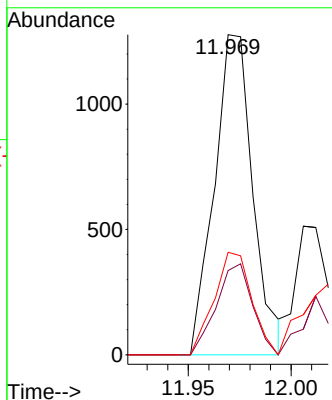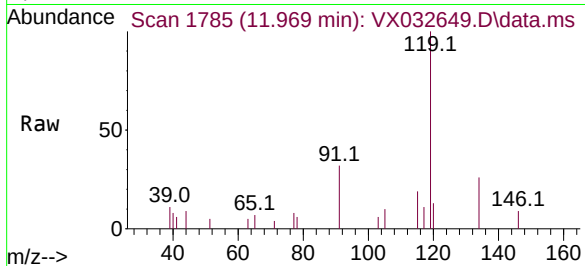

#89
n-Butylbenzene
Concen: 0.596 ug/l
RT: 12.323 min Scan# 1843
Delta R.T. -0.012 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20

Tgt Ion: 91 Resp: 2827
Ion Ratio Lower Upper
91 100
92 25.3 26.2 78.6#
134 126.9 12.9 38.6#


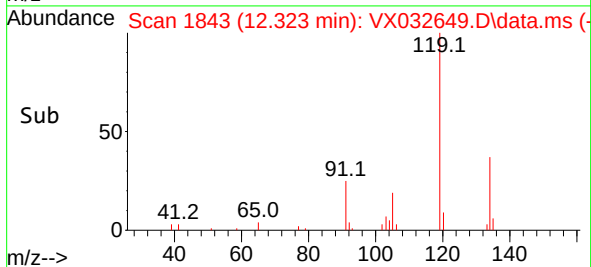
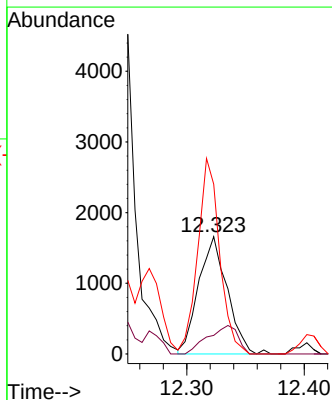
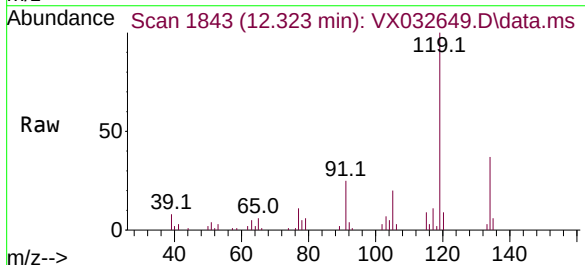




#90
Hexachloroethane
Concen: 1.346 ug/l
RT: 12.616 min Scan# 1879
Delta R.T. 0.073 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion:117 Resp: 1199
Ion Ratio Lower Upper
117 100
201 0.0 37.6 112.9#

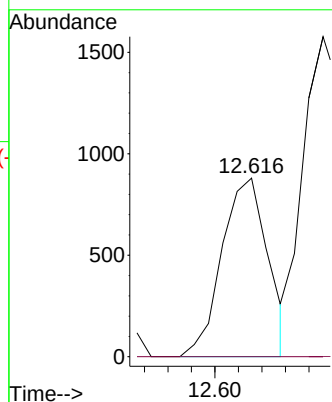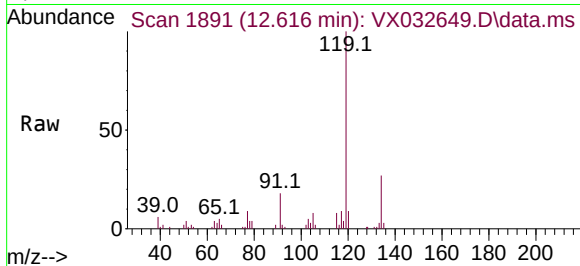

#95
Naphthalene
Concen: 10.208 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.006 min
Lab File: VX032649.D
Acq: 08 Nov 2022 13:20

Tgt Ion:128 Resp: 63285
Ion Ratio Lower Upper
128 100
127 12.6 10.2 15.4
129 11.1 8.9 13.3

