

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110822\
 Data File : VX032665.D
 Acq On : 08 Nov 2022 19:32
 Operator : JC/MD
 Sample : N5514-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-17IR

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
 Title : SW846 8260

Signal : TIC: VX032665.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.782	269	278	287	rBV4	3948	9244	1.54%	0.222%
2	2.953	298	306	321	rVB2	4008	14497	2.41%	0.348%
3	3.111	321	332	350	rBV	251834	573019	95.39%	13.747%
4	3.764	428	439	453	rBV2	29817	80666	13.43%	1.935%
5	4.562	560	570	586	rBV2	8864	31952	5.32%	0.767%
6	5.385	692	705	720	rBV	69224	202487	33.71%	4.858%
7	5.550	720	732	746	rVB	118204	336372	56.00%	8.070%
8	5.958	789	799	809	rBV2	79500	210982	35.12%	5.062%
9	6.086	809	820	832	rVV	44404	123802	20.61%	2.970%
10	6.251	834	847	853	rVV3	5810	18745	3.12%	0.450%
11	6.763	918	931	945	rBV	187073	439854	73.22%	10.552%
12	7.982	1125	1131	1138	rBV2	3857	7276	1.21%	0.175%
13	8.110	1144	1152	1158	rBV2	4555	8936	1.49%	0.214%
14	8.647	1234	1240	1249	rBV	380226	600713	100.00%	14.411%
15	8.958	1284	1291	1298	rBV	30397	45139	7.51%	1.083%
16	9.049	1300	1306	1315	rVB	36317	53477	8.90%	1.283%
17	10.055	1465	1471	1487	rVB	390489	513726	85.52%	12.325%
18	11.079	1634	1639	1650	rBV	336024	432814	72.05%	10.383%
19	12.024	1788	1794	1802	rBV	371919	464623	77.35%	11.147%




Sum of corrected areas: 4168324

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110822\
Data File : VX032665.D
Acq On : 08 Nov 2022 19:32
Operator : JC/MD
Sample : N5514-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-17IR

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

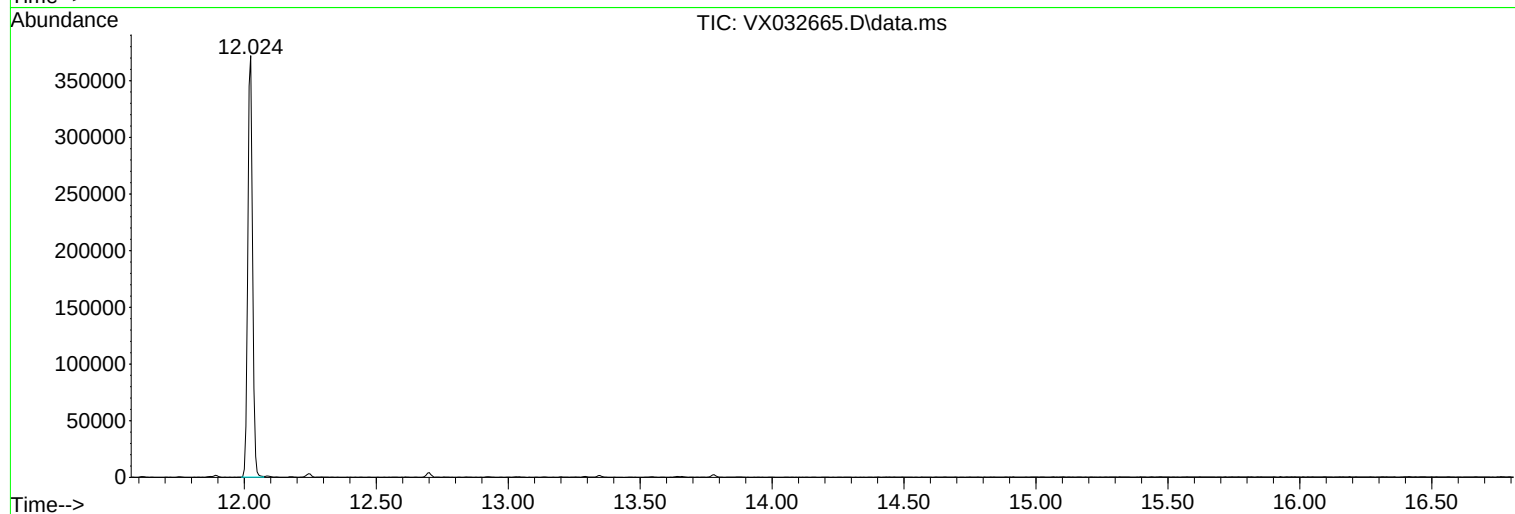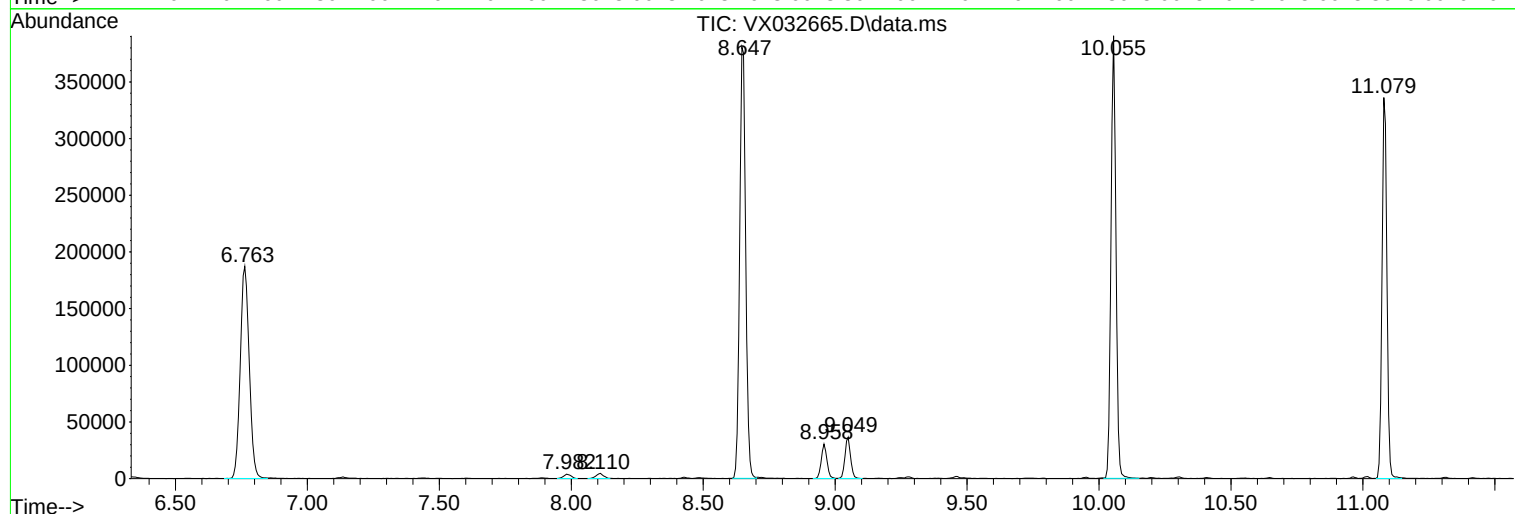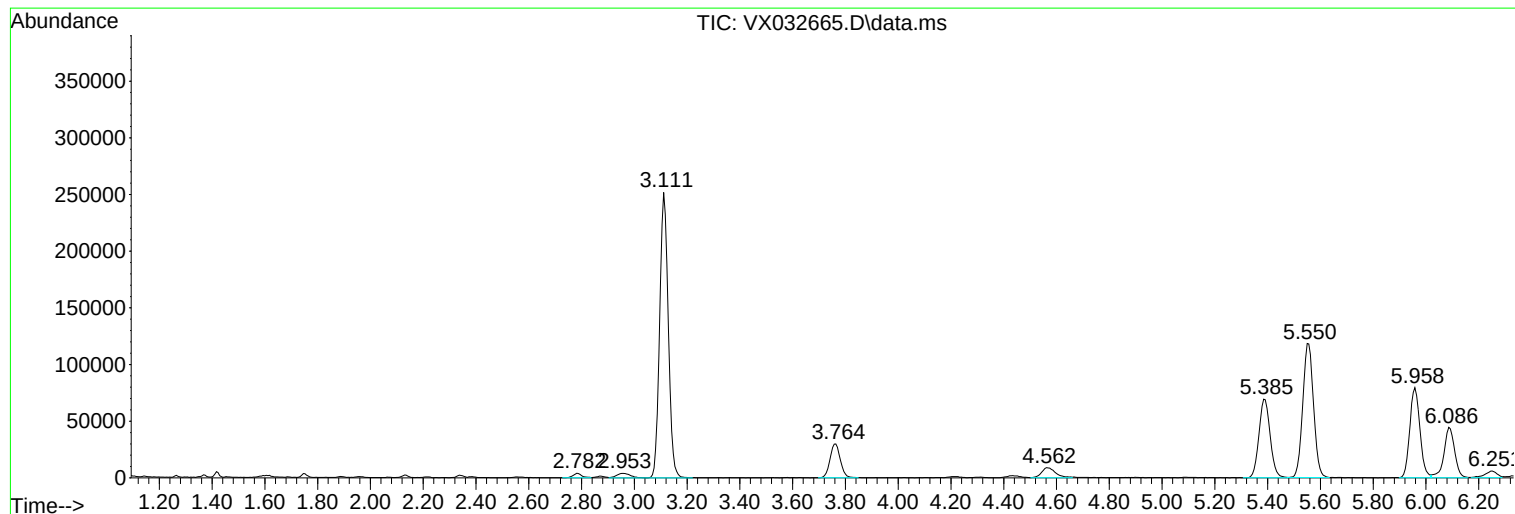

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110822\
Data File : VX032665.D
Acq On : 08 Nov 2022 19:32
Operator : JC/MD
Sample : N5514-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-17IR










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Di-sec-Butyl ether Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.049	5.20 ug/l	53477	Chlorobenzene-d5	10.055

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Di-sec-Butyl ether	130	C8H18O	006863-58-7	83
2			3-Pentanol, 3-ethyl-2-methyl-	130	C8H18O	000597-05-7	64
3			Butane, 1-(1-methylpropoxy)-	130	C8H18O	000999-65-5	53
4			DL-Lactamide, butyl ether	145	C7H15NO2	1000452-56-5	50
5			2-t-Butyl-5-methyl[1,3]dioxolan-...	158	C8H14O3	130930-47-1	38

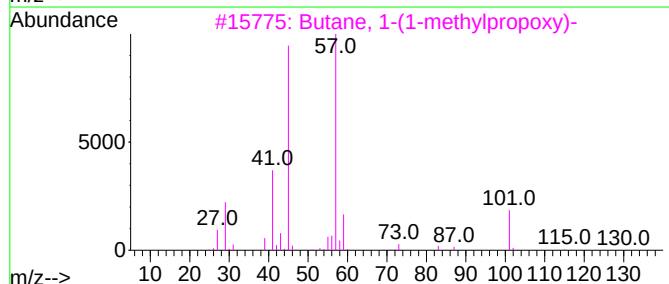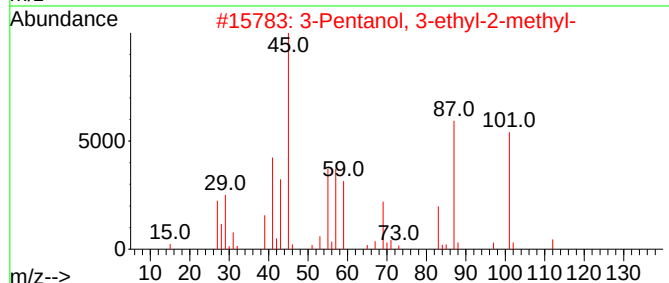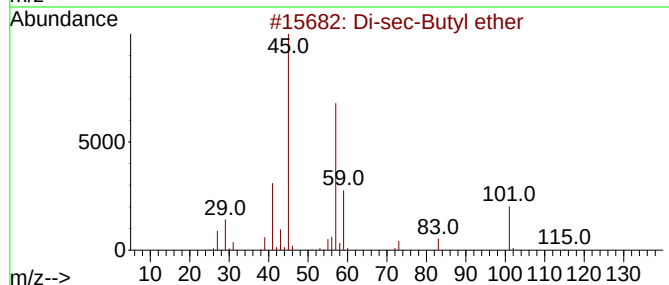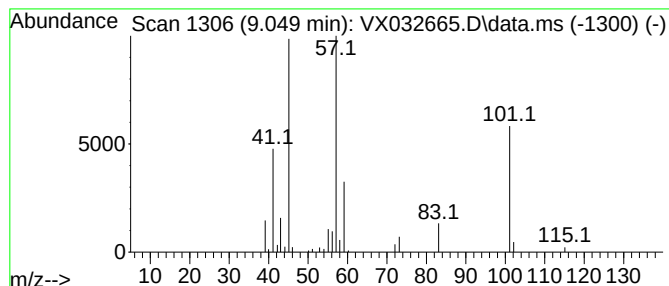

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110822\
Data File : VX032665.D
Acq On : 08 Nov 2022 19:32
Operator : JC/MD
Sample : N5514-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-17IR

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Di-sec-Butyl ether	9.049	5.2	ug/l	53477	3	10.055	513726	50.0