

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110823\
 Data File : VX038661.D
 Acq On : 08 Nov 2023 17:13
 Operator : JC/MD
 Sample : 05223-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FSND-B-3-20231031

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110723W.M

Title : SW846 8260

Signal : TIC: VX038661.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	21	29	39	rBV4	6843	22082	1.54%	0.284%
2	2.526	229	236	248	rBV	8135	17094	1.19%	0.220%
3	5.385	694	705	721	rBV	162254	469460	32.73%	6.031%
4	5.550	721	732	753	rVB	255333	735314	51.26%	9.446%
5	5.958	789	799	816	rBV	150475	409291	28.53%	5.258%
6	6.763	921	931	948	rBV	390525	946538	65.99%	12.159%
7	8.647	1233	1240	1265	rBV	796231	1302360	90.80%	16.730%
8	9.275	1337	1343	1356	rBV	98763	148198	10.33%	1.904%
9	10.055	1465	1471	1492	rBV	915955	1253156	87.37%	16.098%
10	11.079	1634	1639	1653	rBV	812009	1046590	72.96%	13.445%
11	12.018	1788	1793	1817	rBV	1100047	1434380	100.00%	18.426%




Sum of corrected areas: 7784463

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110823\
Data File : VX038661.D
Acq On : 08 Nov 2023 17:13
Operator : JC/MD
Sample : 05223-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-B-3-20231031

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

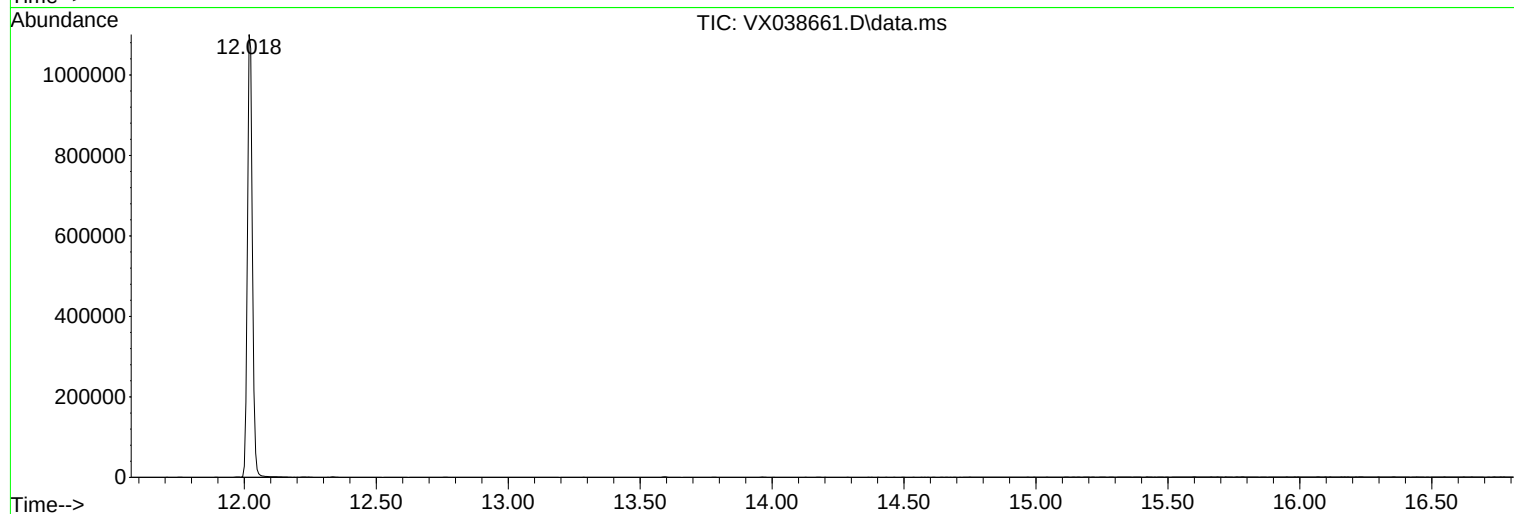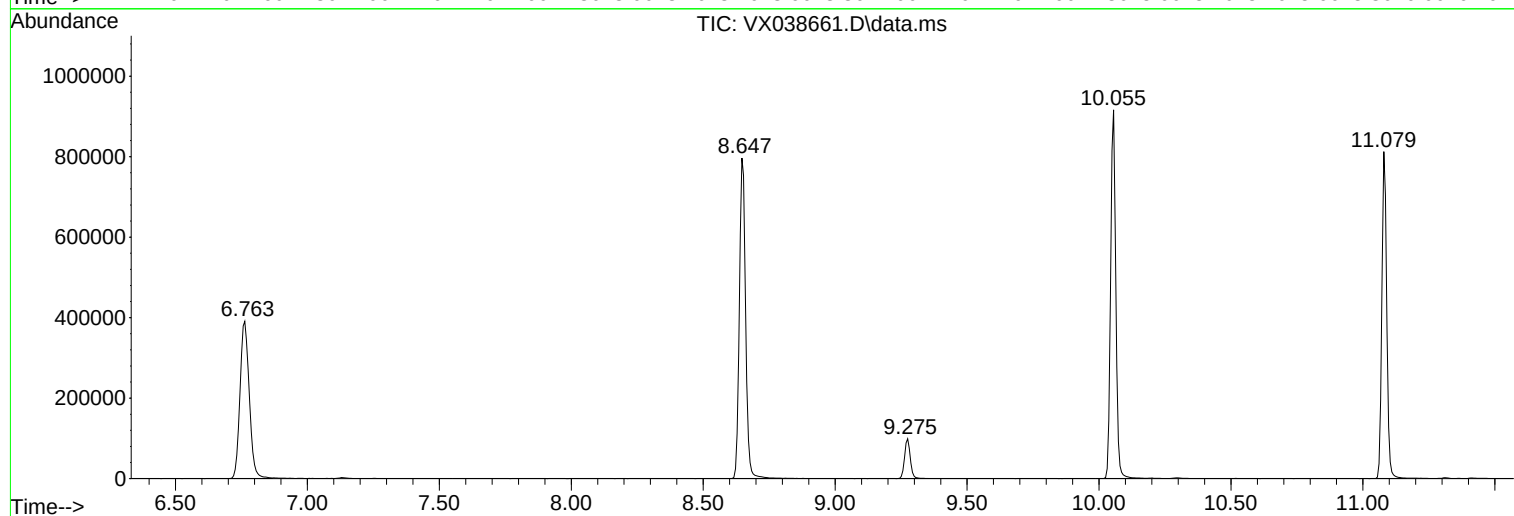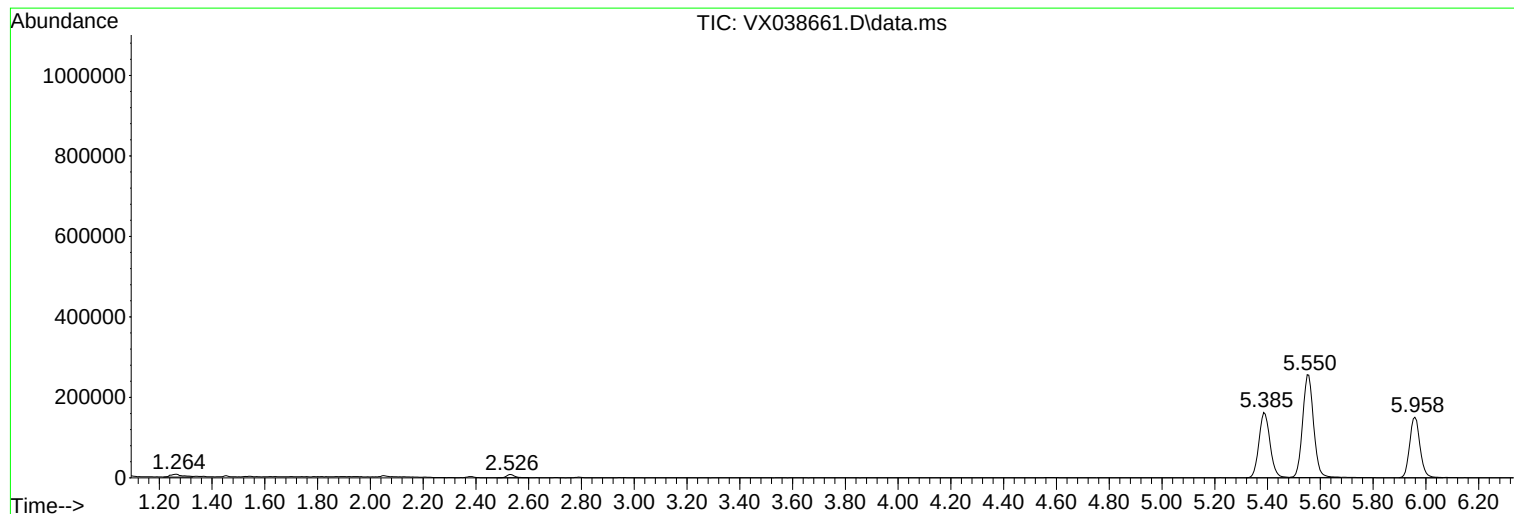

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110823\
Data File : VX038661.D
Acq On : 08 Nov 2023 17:13
Operator : JC/MD
Sample : 05223-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-B-3-20231031

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110823\
Data File : VX038661.D
Acq On : 08 Nov 2023 17:13
Operator : JC/MD
Sample : 05223-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-B-3-20231031

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------