

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
 Data File : VX043751.D
 Acq On : 08 Nov 2024 10:04
 Operator : JC/MD
 Sample : VX1108MBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 08 23:56:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 08 23:56:14 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	187534	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.049	117	171724	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	77294	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	52367	52.416	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	104.840%	
7) Chloroethane-d5	1.648	69	35336	82.284	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	164.560%#	
11) 1,1-Dichloroethene-d2	2.300	65	22949	49.759	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	99.520%	
21) 2-Butanone-d5	4.458	46	77030	117.758	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	117.760%	
24) Chloroform-d	5.050	84	114942	53.369	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	106.740%	
26) 1,2-Dichloroethane-d4	5.946	65	72029	52.645	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	105.280%	
32) Benzene-d6	5.964	84	236440	53.255	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	106.520%	
36) 1,2-Dichloropropane-d6	7.299	67	73913	54.720	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	109.440%	
41) Toluene-d8	8.646	98	210446	52.179	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	104.360%	
43) trans-1,3-Dichloroprop...	8.951	79	30922	47.869	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	95.740%	
47) 2-Hexanone-d5	9.384	63	57139	106.890	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	106.890%	
56) 1,1,2,2-Tetrachloroeth...	11.189	84	94589	54.579	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	109.160%	
66) 1,2-Dichlorobenzene-d4	12.317	152	78298	58.466	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	116.940%	
Target Compounds						
37) 1,2-Dichloropropane	7.299	63	7952	6.099	ug/L	Qvalue # 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043751.D
Acq On : 08 Nov 2024 10:04
Operator : JC/MD
Sample : VX1108MBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Nov 08 23:56:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 08 23:56:14 2024
Response via : Initial Calibration

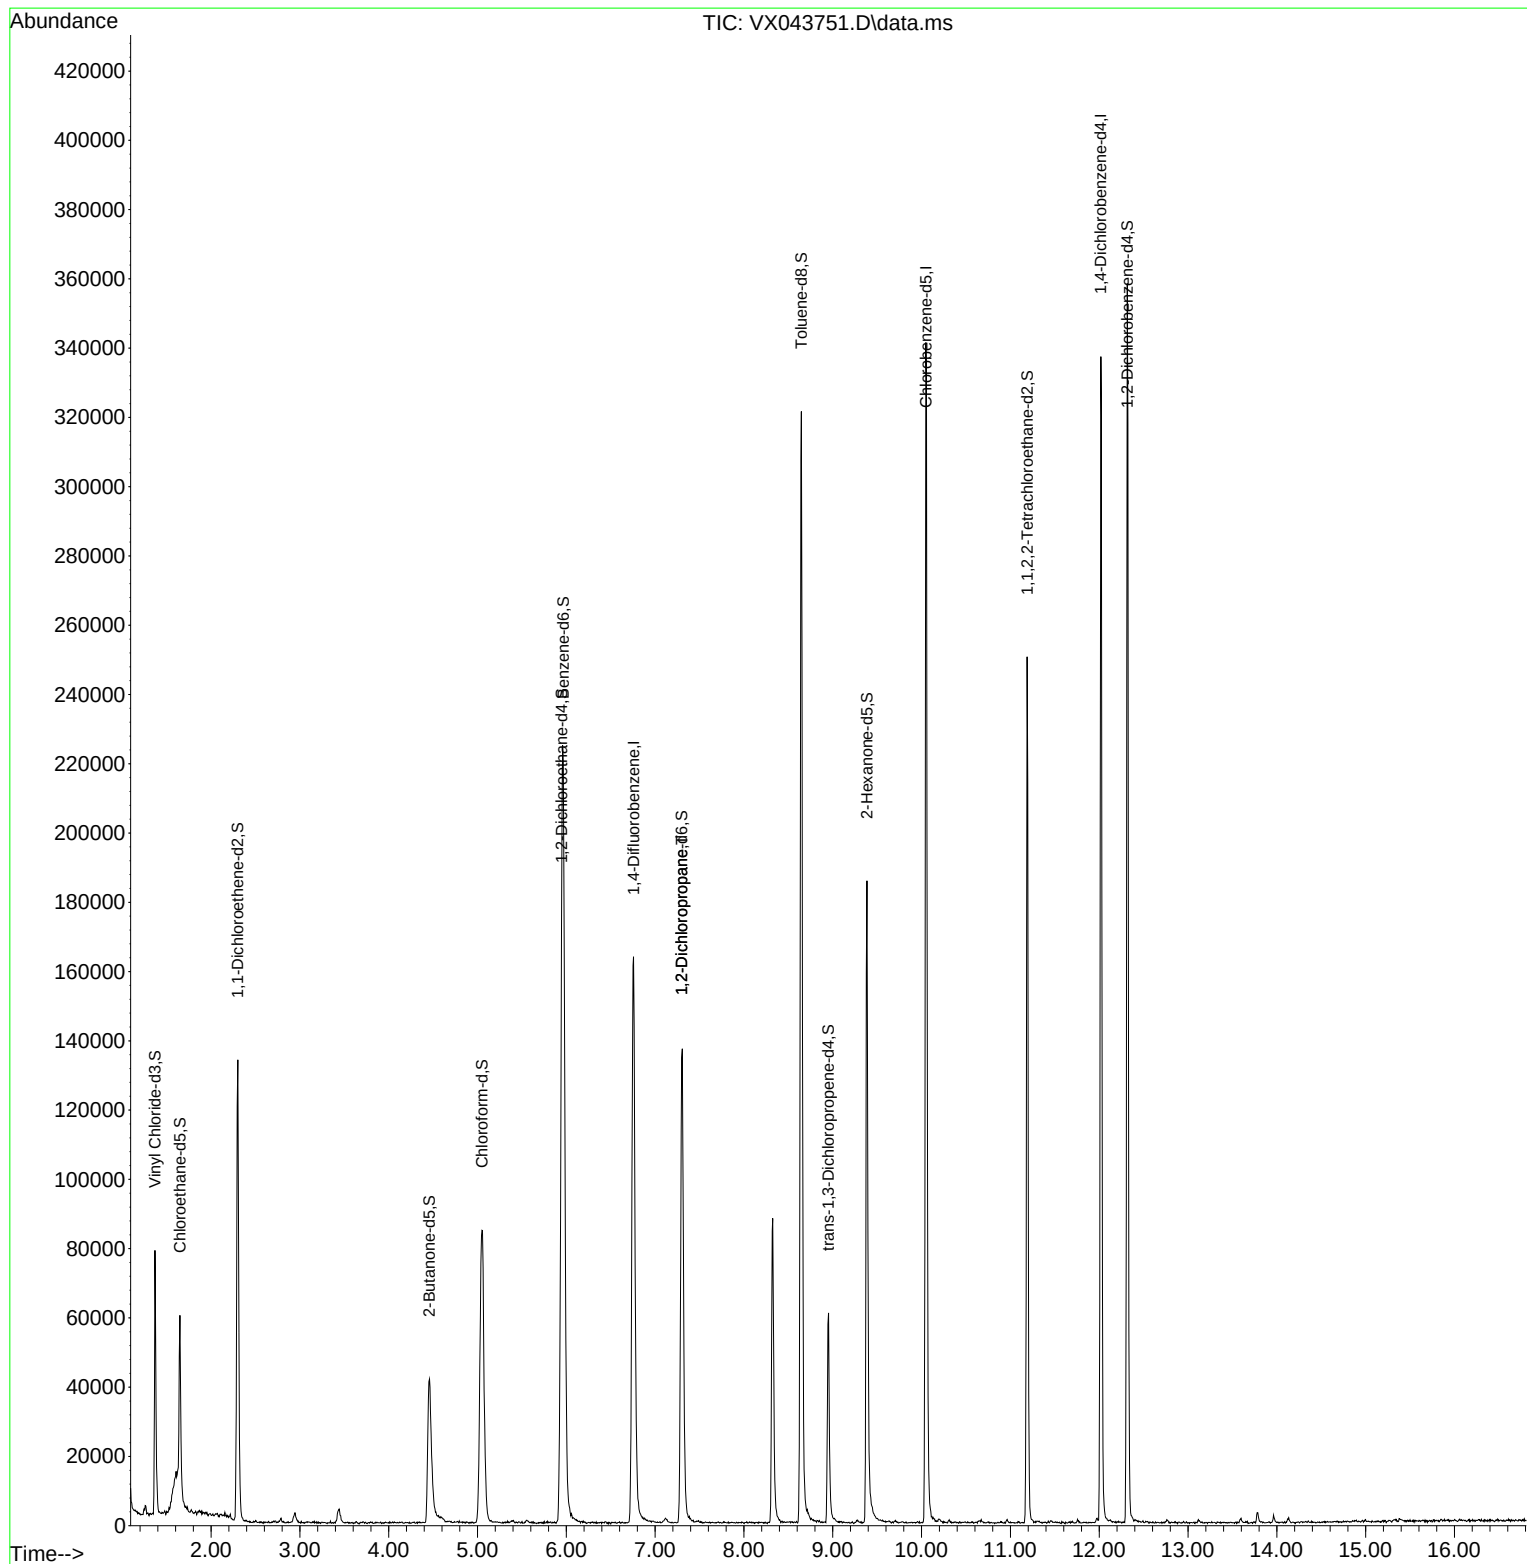

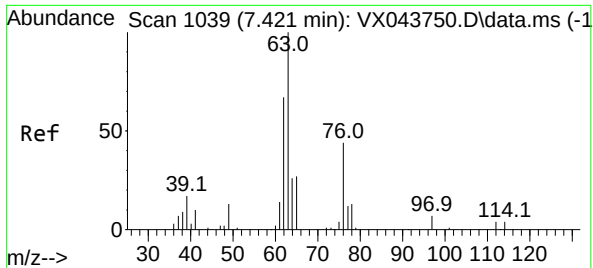

#37
 1,2-Dichloropropane
 Concen: 6.099 ug/L
 RT: 7.299 min Scan# 10
 Delta R.T. -0.122 min
 Lab File: VX043751.D
 Acq: 08 Nov 2024 10:04

Instrument :
 MSVOA_X
 ClientSampleId :

Tgt Ion: 63 Resp: 7952
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.8 5.8#

