

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
 Data File : VX043752.D
 Acq On : 08 Nov 2024 10:27
 Operator : JC/MD
 Sample : VX1108WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 08 23:56:59 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 08 23:56:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	199496	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.049	117	187146	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	80853	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	43676	41.096	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.200%
7) Chloroethane-d5	1.648	69	26042	57.006	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	114.020%
11) 1,1-Dichloroethene-d2	2.300	65	19326	39.391	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.780%
21) 2-Butanone-d5	4.464	46	63307	90.976	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	90.980%
24) Chloroform-d	5.056	84	97797	42.685	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.380%
26) 1,2-Dichloroethane-d4	5.952	65	60172	41.342	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.680%
32) Benzene-d6	5.970	84	202869	41.928	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.860%
36) 1,2-Dichloropropane-d6	7.305	67	62153	42.222	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	84.440%
41) Toluene-d8	8.647	98	181587	41.314	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.620%
43) trans-1,3-Dichloroprop...	8.951	79	24580	34.916	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.840%
47) 2-Hexanone-d5	9.384	63	49730	85.364	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.360%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	78676	41.656	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.320%
66) 1,2-Dichlorobenzene-d4	12.317	152	65105	46.475	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.940%
Target Compounds						
61) 1,2,3-Trichloropropane	12.018	75	8627	5.497	ug/L	Qvalue # 61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043752.D
Acq On : 08 Nov 2024 10:27
Operator : JC/MD
Sample : VX1108WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Nov 08 23:56:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 08 23:56:14 2024
Response via : Initial Calibration

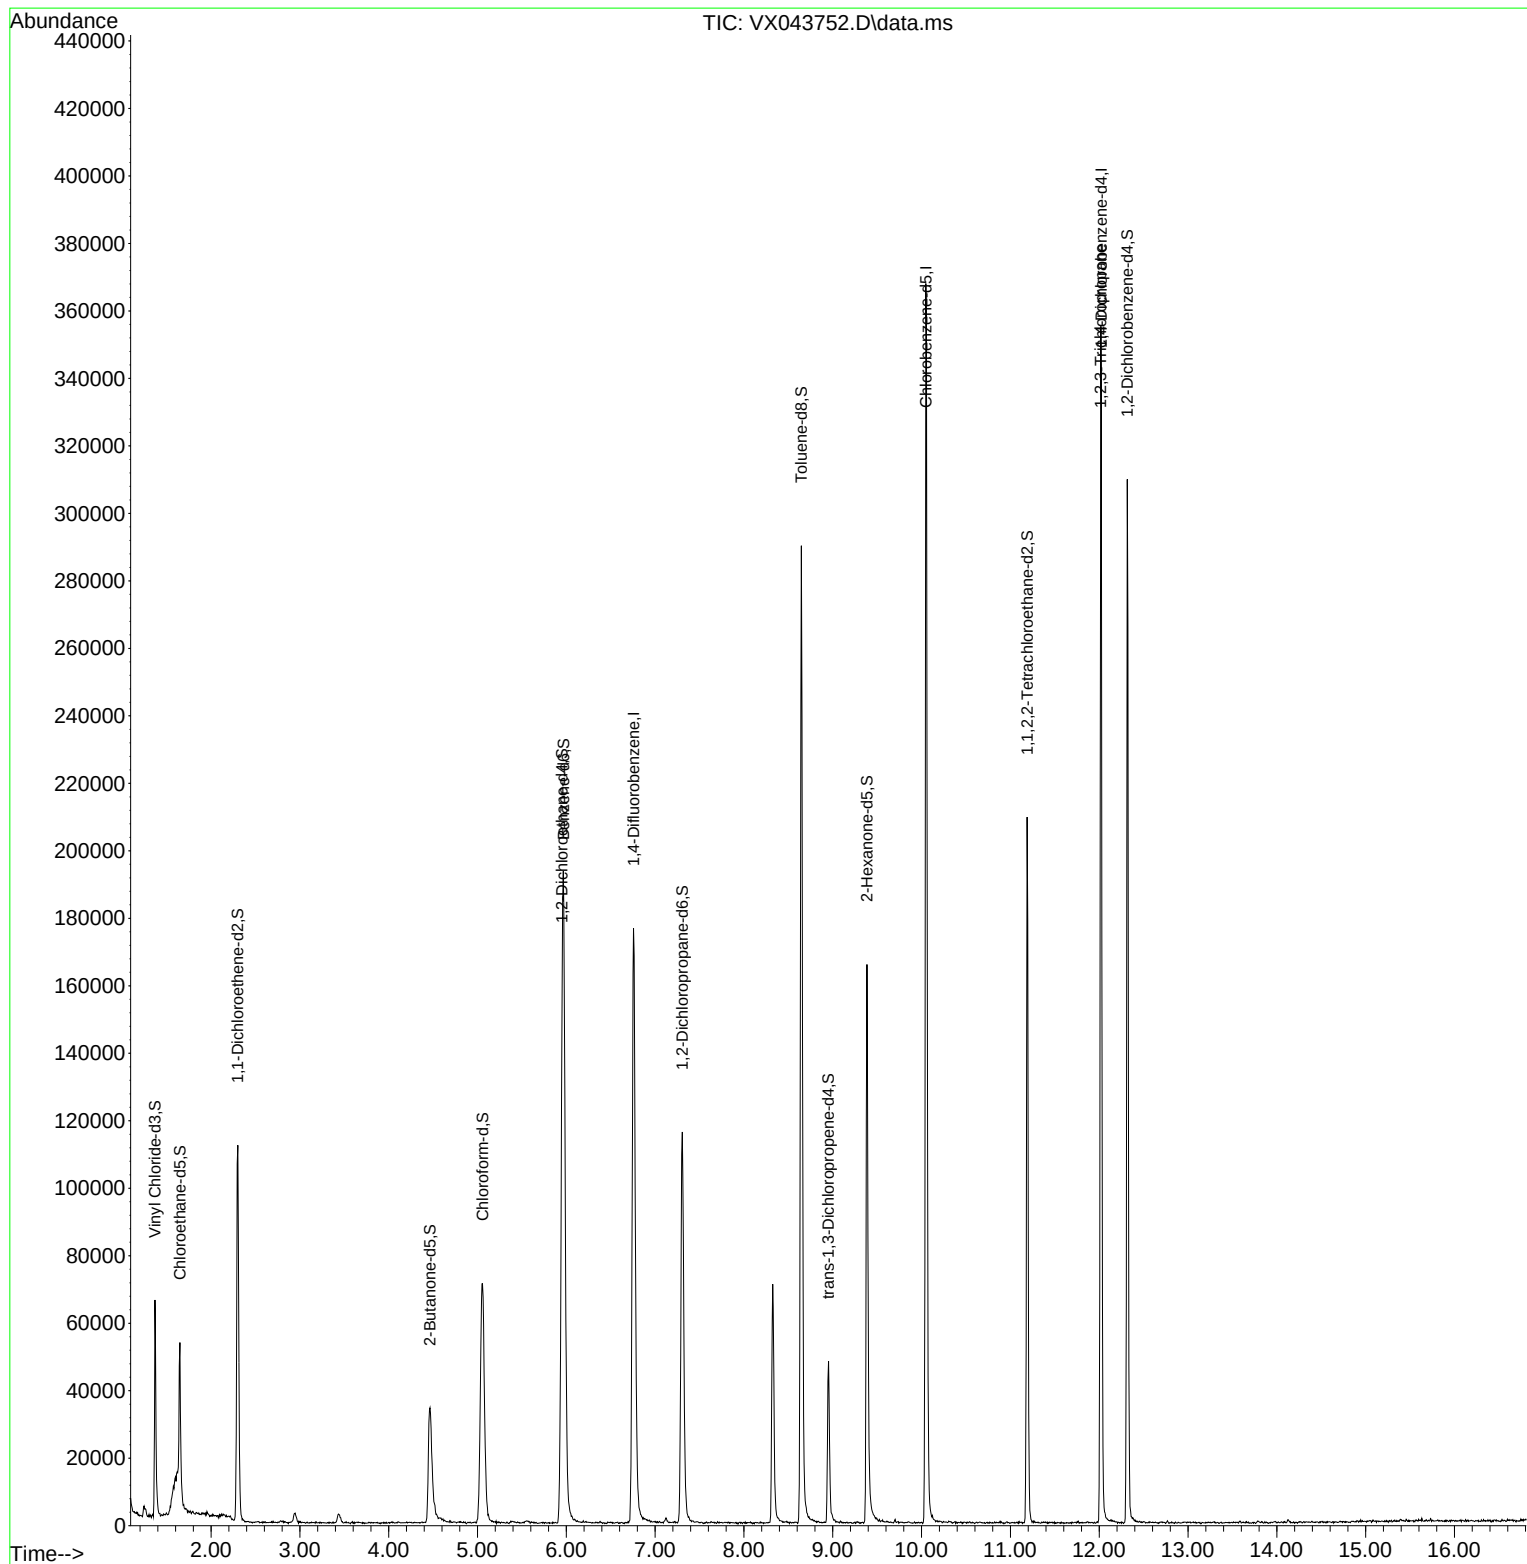

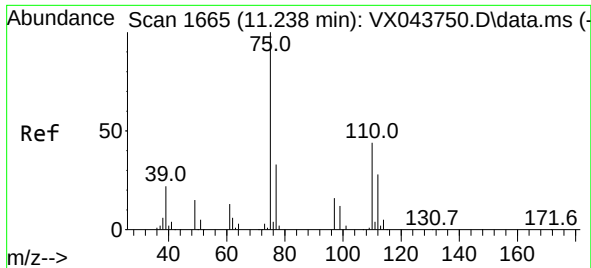

#61

1,2,3-Trichloropropane

Concen: 5.497 ug/L

RT: 12.018 min Scan# 11

Delta R.T. 0.780 min


Lab File: VX043752.D

Acq: 08 Nov 2024 10:27

Instrument :

MSVOA_X

ClientSampleId :

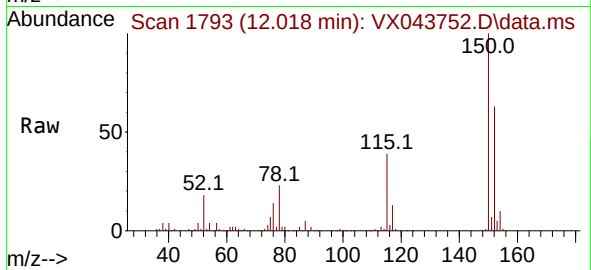

Tgt Ion: 75 Resp: 8627

Ion Ratio Lower Upper

75 100

77 36.4 25.4 38.0

110 3.2 33.6 50.4#

