

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
 Data File : VX043759.D
 Acq On : 08 Nov 2024 13:17
 Operator : JC/MD
 Sample : P4742-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 08 23:58:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 08 23:56:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	207258	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	190359	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	81241	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	56435	51.112	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	102.220%
7) Chloroethane-d5	1.648	69	37533	79.083	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	158.160%#
11) 1,1-Dichloroethene-d2	2.300	65	23744	46.583	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.160%
21) 2-Butanone-d5	4.465	46	71112	98.365	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	98.370%
24) Chloroform-d	5.056	84	119502	50.205	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.420%
26) 1,2-Dichloroethane-d4	5.958	65	72357	47.852	ug/L	0.01
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.700%
32) Benzene-d6	5.970	84	255095	51.832	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.660%
36) 1,2-Dichloropropane-d6	7.306	67	74537	49.780	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.560%
41) Toluene-d8	8.647	98	224850	50.293	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.580%
43) trans-1,3-Dichloroprop...	8.952	79	30046	41.960	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.920%
47) 2-Hexanone-d5	9.384	63	52637	88.829	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	88.830%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	92292	48.040	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.080%
66) 1,2-Dichlorobenzene-d4	12.323	152	76499	54.347	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	108.700%
Target Compounds						Qvalue
13) Acetone	2.386	43	2423	3.604	ug/L	89
61) 1,2,3-Trichloropropane	12.018	75	8829	5.599	ug/L #	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043759.D
Acq On : 08 Nov 2024 13:17
Operator : JC/MD
Sample : P4742-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Nov 08 23:58:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 08 23:56:14 2024
Response via : Initial Calibration

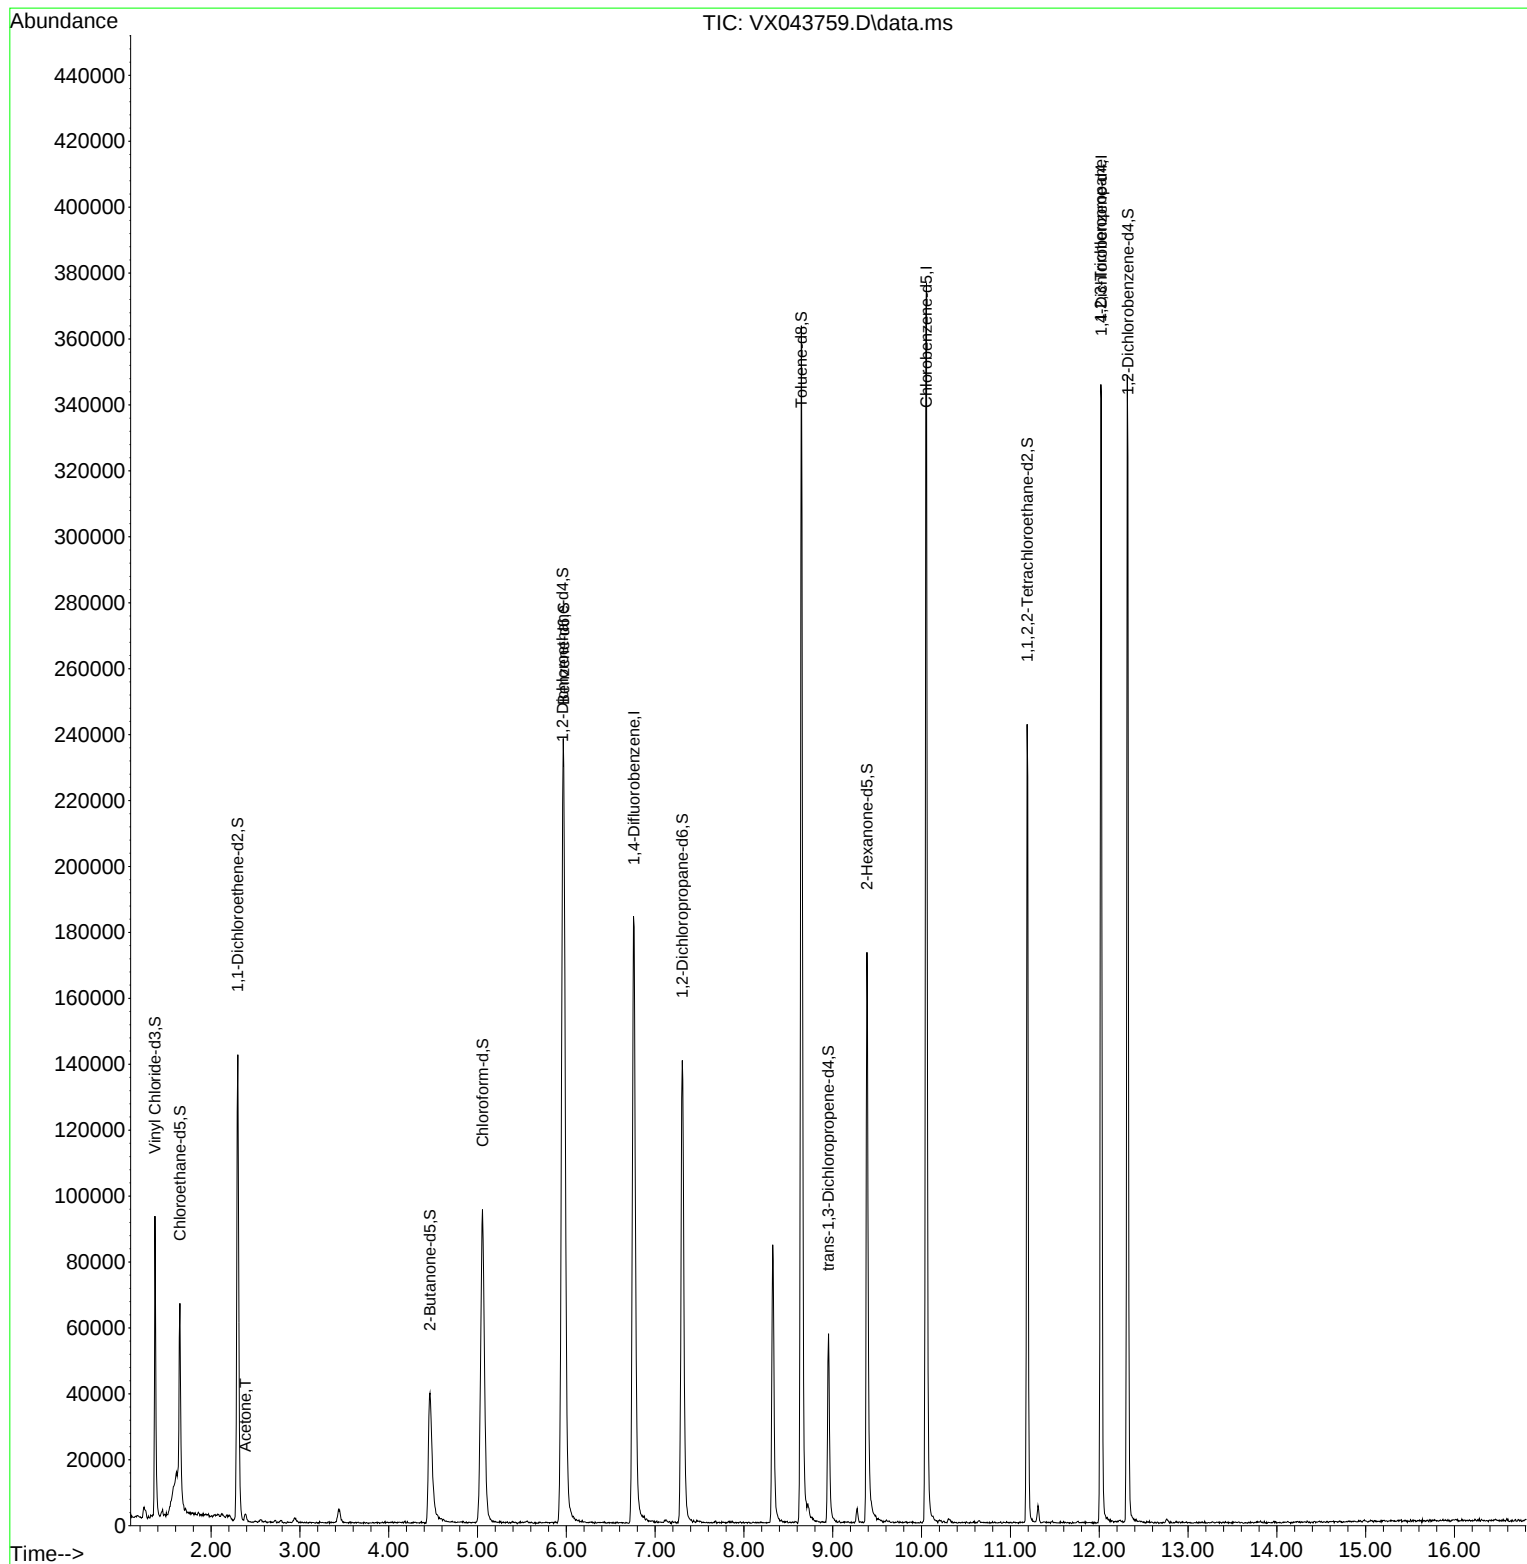



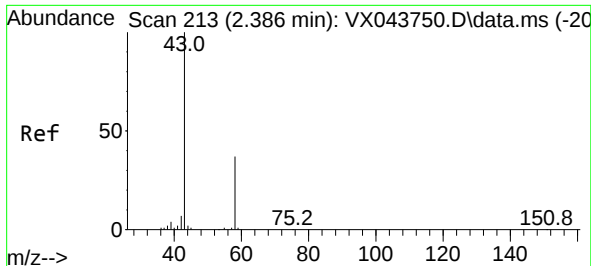


#13
Acetone
Concen: 3.604 ug/L
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX043759.D
Acq: 08 Nov 2024 13:17

Instrument :
MSVOA_X
ClientSampleId :

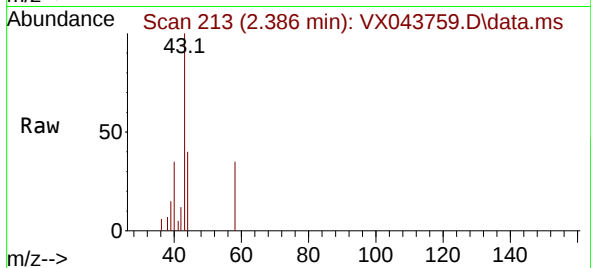

Tgt Ion: 43 Resp: 2423
Ion Ratio Lower Upper
43 100
58 38.0 0.0 63.6

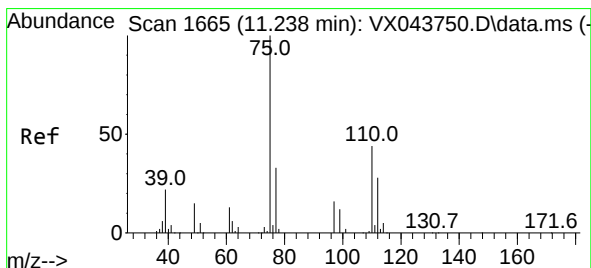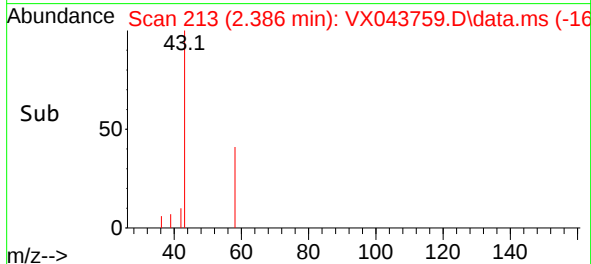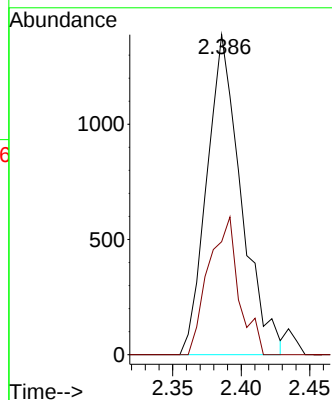

#61
1,2,3-Trichloropropane
Concen: 5.599 ug/L
RT: 12.018 min Scan# 1793
Delta R.T. 0.780 min
Lab File: VX043759.D
Acq: 08 Nov 2024 13:17

Tgt Ion: 75 Resp: 8829
Ion Ratio Lower Upper
75 100
77 34.5 25.4 38.0
110 3.4 33.6 50.4#

