

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
 Data File : VX043760.D
 Acq On : 08 Nov 2024 13:40
 Operator : JC/MD
 Sample : P4742-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 08 23:58:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 08 23:56:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	193985	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	179376	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	77884	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	54809	53.036	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	106.080%
7) Chloroethane-d5	1.648	69	28910	65.082	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	130.160%#
11) 1,1-Dichloroethene-d2	2.294	65	22617	47.409	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.820%
21) 2-Butanone-d5	4.464	46	64969	96.017	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.020%
24) Chloroform-d	5.056	84	115099	51.664	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.320%
26) 1,2-Dichloroethane-d4	5.952	65	68593	48.466	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.940%
32) Benzene-d6	5.970	84	244755	52.776	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.560%
36) 1,2-Dichloropropane-d6	7.305	67	73283	51.940	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	103.880%
41) Toluene-d8	8.646	98	213803	50.750	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.500%
43) trans-1,3-Dichloroprop...	8.951	79	27300	40.459	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.920%
47) 2-Hexanone-d5	9.384	63	50378	90.222	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.220%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	89583	49.485	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.980%
66) 1,2-Dichlorobenzene-d4	12.323	152	79060	58.588	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	117.180%
Target Compounds						Qvalue
13) Acetone	2.385	43	2272	3.610	ug/L	87
61) 1,2,3-Trichloropropane	12.018	75	8307	5.495	ug/L #	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043760.D
Acq On : 08 Nov 2024 13:40
Operator : JC/MD
Sample : P4742-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Nov 08 23:58:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 08 23:56:14 2024
Response via : Initial Calibration

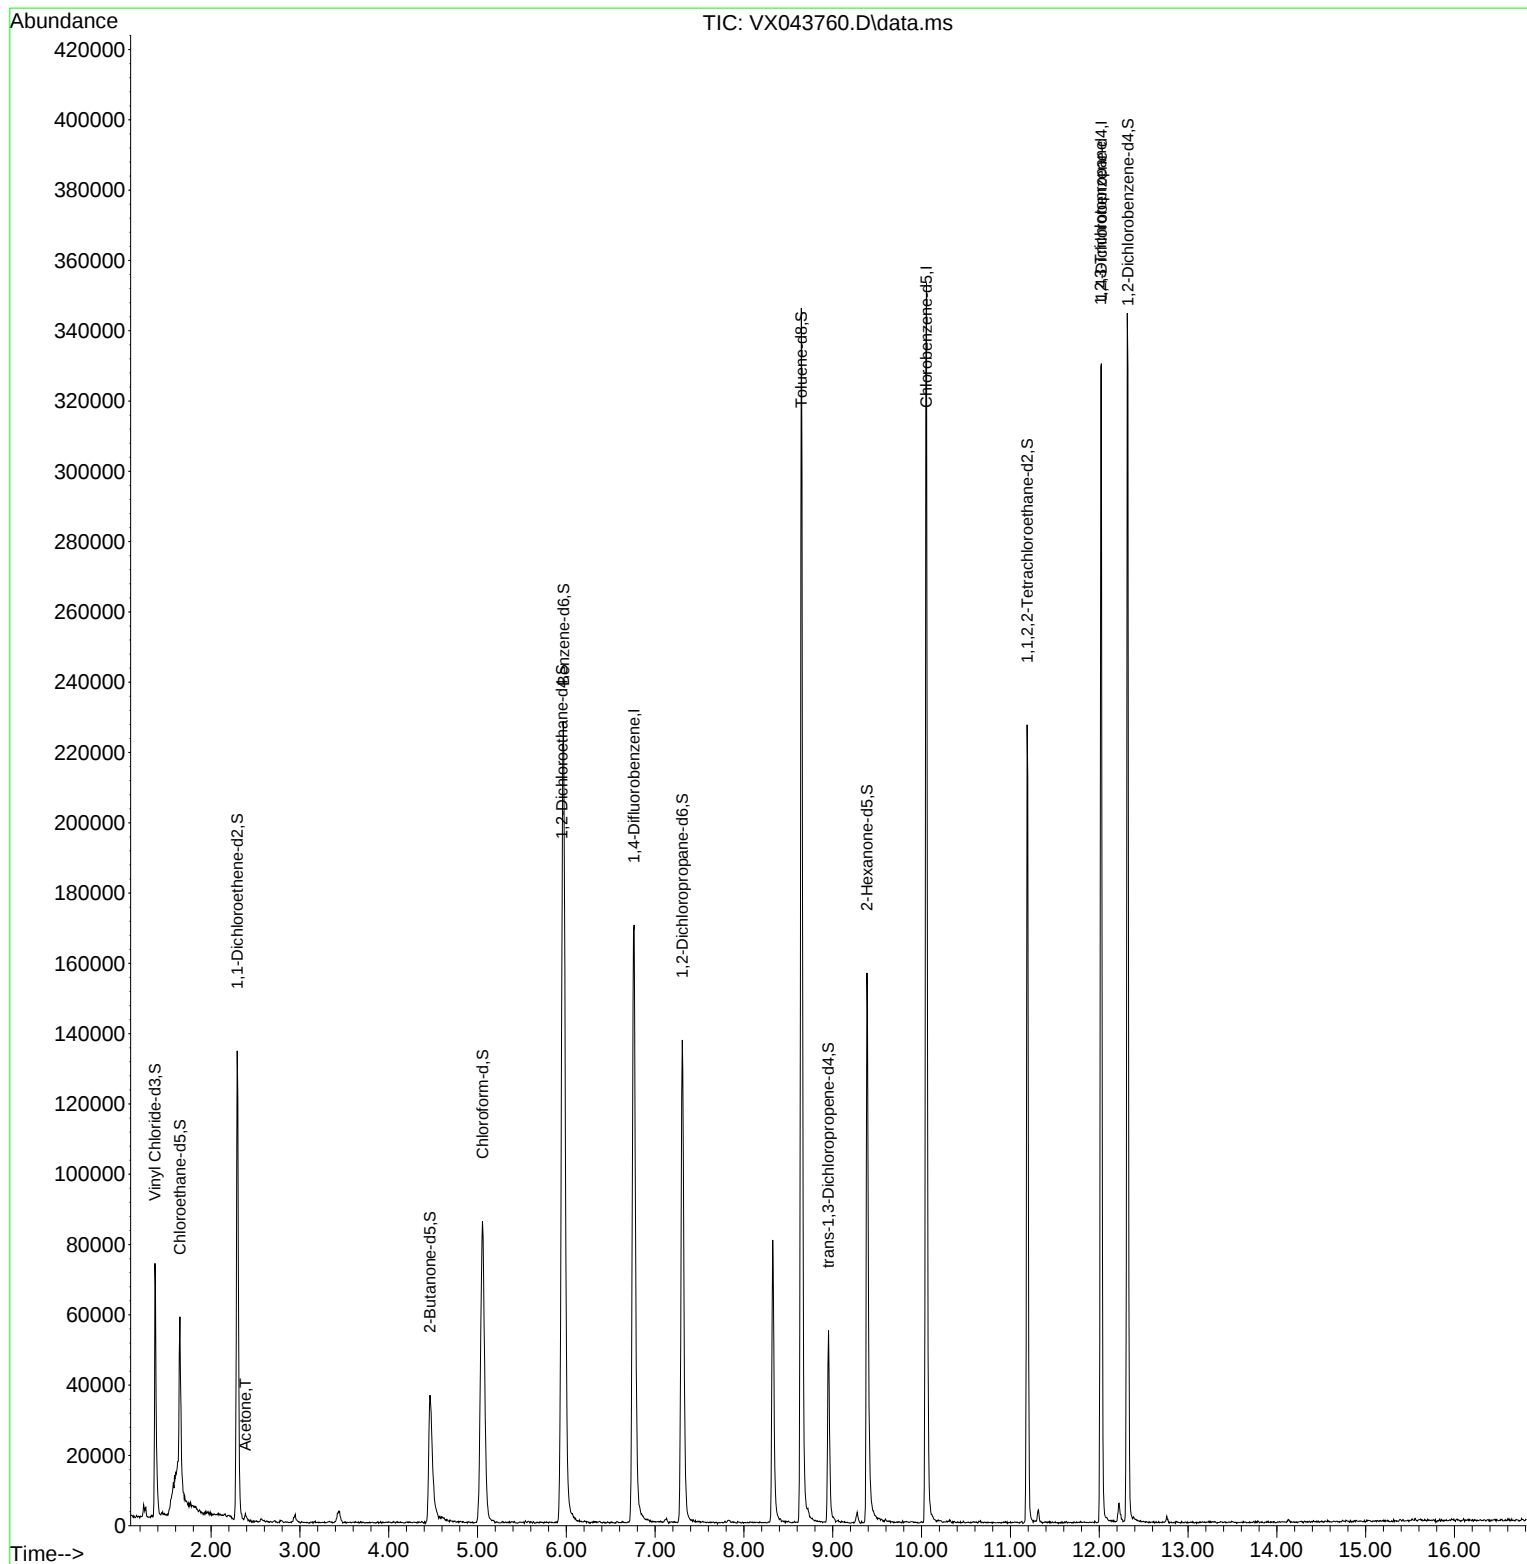



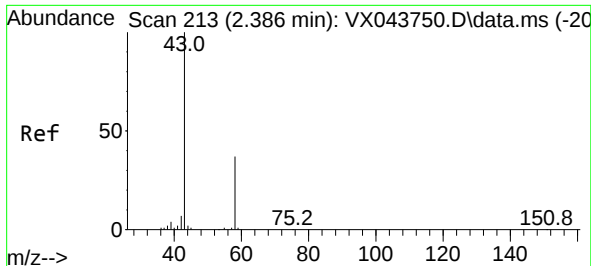


#13
Acetone
Concen: 3.610 ug/L
RT: 2.385 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX043760.D
Acq: 08 Nov 2024 13:40

Instrument :
MSVOA_X
ClientSampleId :

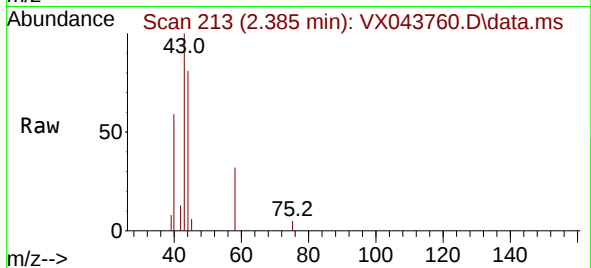

Tgt Ion: 43 Resp: 2272
Ion Ratio Lower Upper
43 100
58 24.7 0.0 63.6

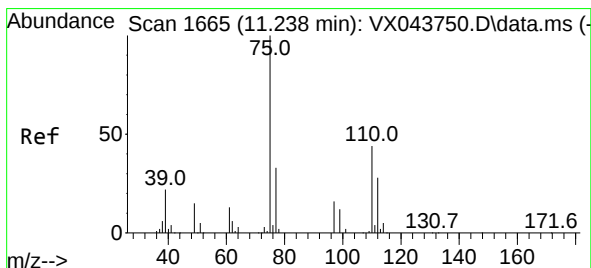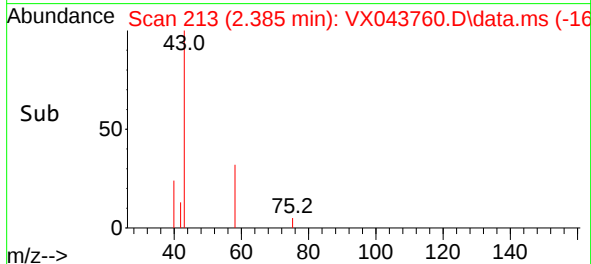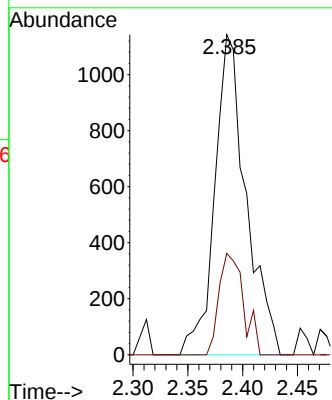

#61
1,2,3-Trichloropropane
Concen: 5.495 ug/L
RT: 12.018 min Scan# 1793
Delta R.T. 0.780 min
Lab File: VX043760.D
Acq: 08 Nov 2024 13:40

Tgt Ion: 75 Resp: 8307
Ion Ratio Lower Upper
75 100
77 33.2 25.4 38.0
110 1.7 33.6 50.4#

