

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
 Data File : VX043757.D
 Acq On : 08 Nov 2024 12:30
 Operator : JC/MD
 Sample : P4742-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1H12

Quant Time: Nov 08 23:58:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 08 23:56:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	164439	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	150512	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	65427	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	48154	54.969	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 109.940%			
7) Chloroethane-d5	1.648	69	24073	63.930	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 127.860%			
11) 1,1-Dichloroethene-d2	2.294	65	20574	50.875	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 101.740%			
21) 2-Butanone-d5	4.471	46	60154	104.875	ug/L	0.01
Spiked Amount 100.000	Range 40 - 130		Recovery = 104.870%			
24) Chloroform-d	5.056	84	100851	53.403	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 106.800%			
26) 1,2-Dichloroethane-d4	5.952	65	62195	51.842	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 103.680%			
32) Benzene-d6	5.970	84	215664	55.421	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 110.840%			
36) 1,2-Dichloropropane-d6	7.305	67	63757	53.854	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 107.700%			
41) Toluene-d8	8.647	98	188683	53.377	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 106.760%			
43) trans-1,3-Dichloroprop...	8.951	79	24649	43.536	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 87.080%			
47) 2-Hexanone-d5	9.390	63	46167	98.536	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 98.540%			
56) 1,1,2,2-Tetrachloroeth...	11.189	84	79521	52.351	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 104.700%			
66) 1,2-Dichlorobenzene-d4	12.323	152	69584	61.383	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 122.760%#			
Target Compounds						Qvalue
13) Acetone	2.386	43	5045	9.457	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043757.D
Acq On : 08 Nov 2024 12:30
Operator : JC/MD
Sample : P4742-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1H12

Quant Time: Nov 08 23:58:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 08 23:56:14 2024
Response via : Initial Calibration

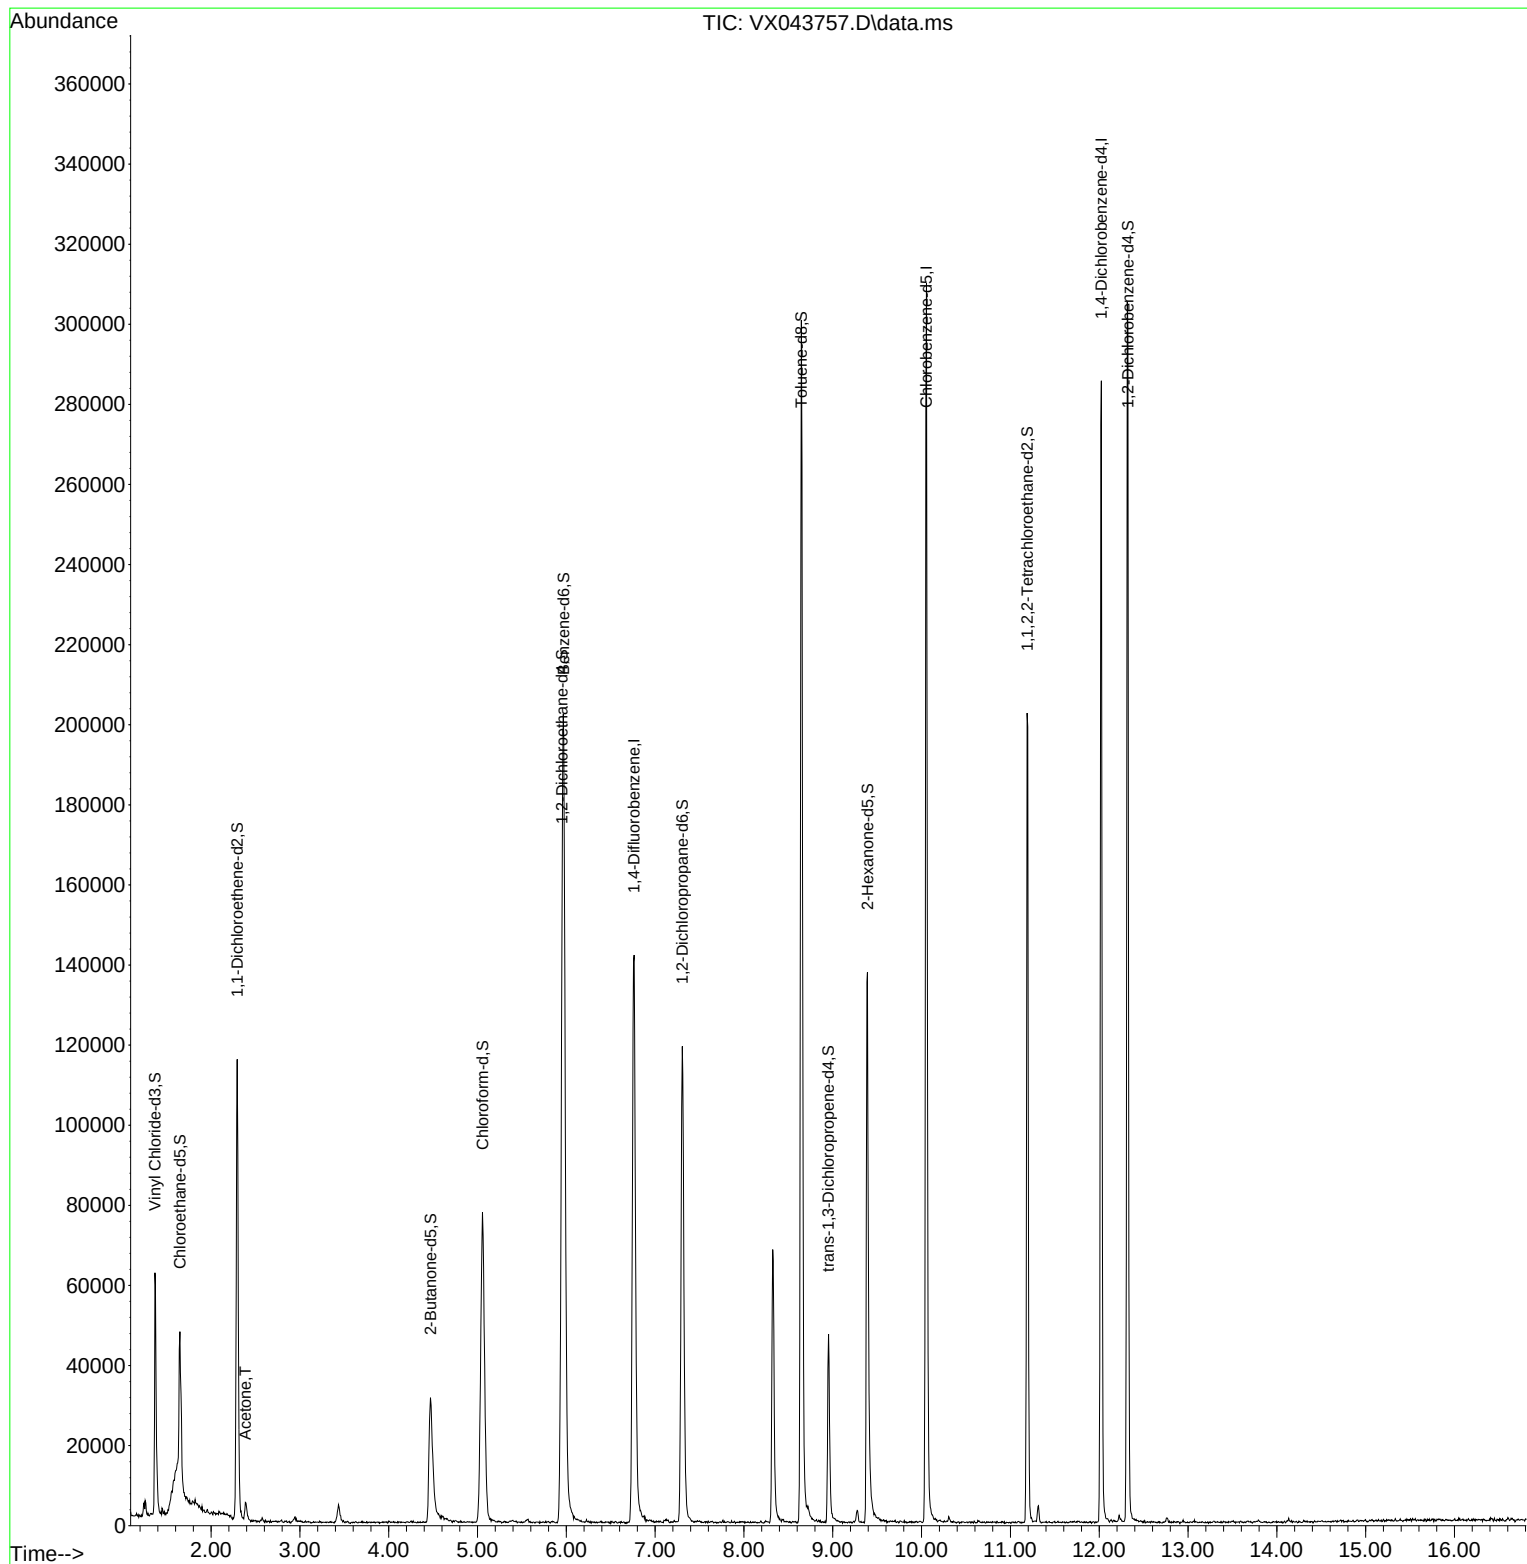

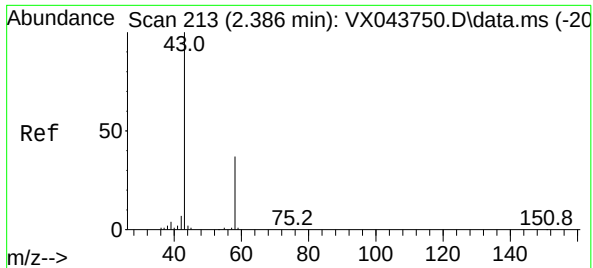

#13
 Acetone
 Concen: 9.457 ug/L
 RT: 2.386 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VX043757.D
 Acq: 08 Nov 2024 12:30

Instrument :
 MSVOA_X
 ClientSampleId :
 E1H12

Tgt Ion: 43 Resp: 5045
 Ion Ratio Lower Upper
 43 100
 58 33.7 0.0 63.6

