

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
 Data File : VX043760.D
 Acq On : 08 Nov 2024 13:40
 Operator : JC/MD
 Sample : P4742-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1H24

Quant Time: Nov 08 23:58:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 08 23:56:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	193985	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	179376	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	77884	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	54809	53.036	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 106.080%			
7) Chloroethane-d5	1.648	69	28910	65.082	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 130.160%#			
11) 1,1-Dichloroethene-d2	2.294	65	22617	47.409	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 94.820%			
21) 2-Butanone-d5	4.464	46	64969	96.017	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 96.020%			
24) Chloroform-d	5.056	84	115099	51.664	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 103.320%			
26) 1,2-Dichloroethane-d4	5.952	65	68593	48.466	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 96.940%			
32) Benzene-d6	5.970	84	244755	52.776	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 105.560%			
36) 1,2-Dichloropropane-d6	7.305	67	73283	51.940	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 103.880%			
41) Toluene-d8	8.646	98	213803	50.750	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 101.500%			
43) trans-1,3-Dichloroprop...	8.951	79	27300	40.459	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 80.920%			
47) 2-Hexanone-d5	9.384	63	50378	90.222	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 90.220%			
56) 1,1,2,2-Tetrachloroeth...	11.189	84	89583	49.485	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 98.980%			
66) 1,2-Dichlorobenzene-d4	12.323	152	79060	58.588	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 117.180%			
Target Compounds					Qvalue	
13) Acetone	2.385	43	2272	3.610	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043760.D
Acq On : 08 Nov 2024 13:40
Operator : JC/MD
Sample : P4742-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1H24

Quant Time: Nov 08 23:58:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 08 23:56:14 2024
Response via : Initial Calibration

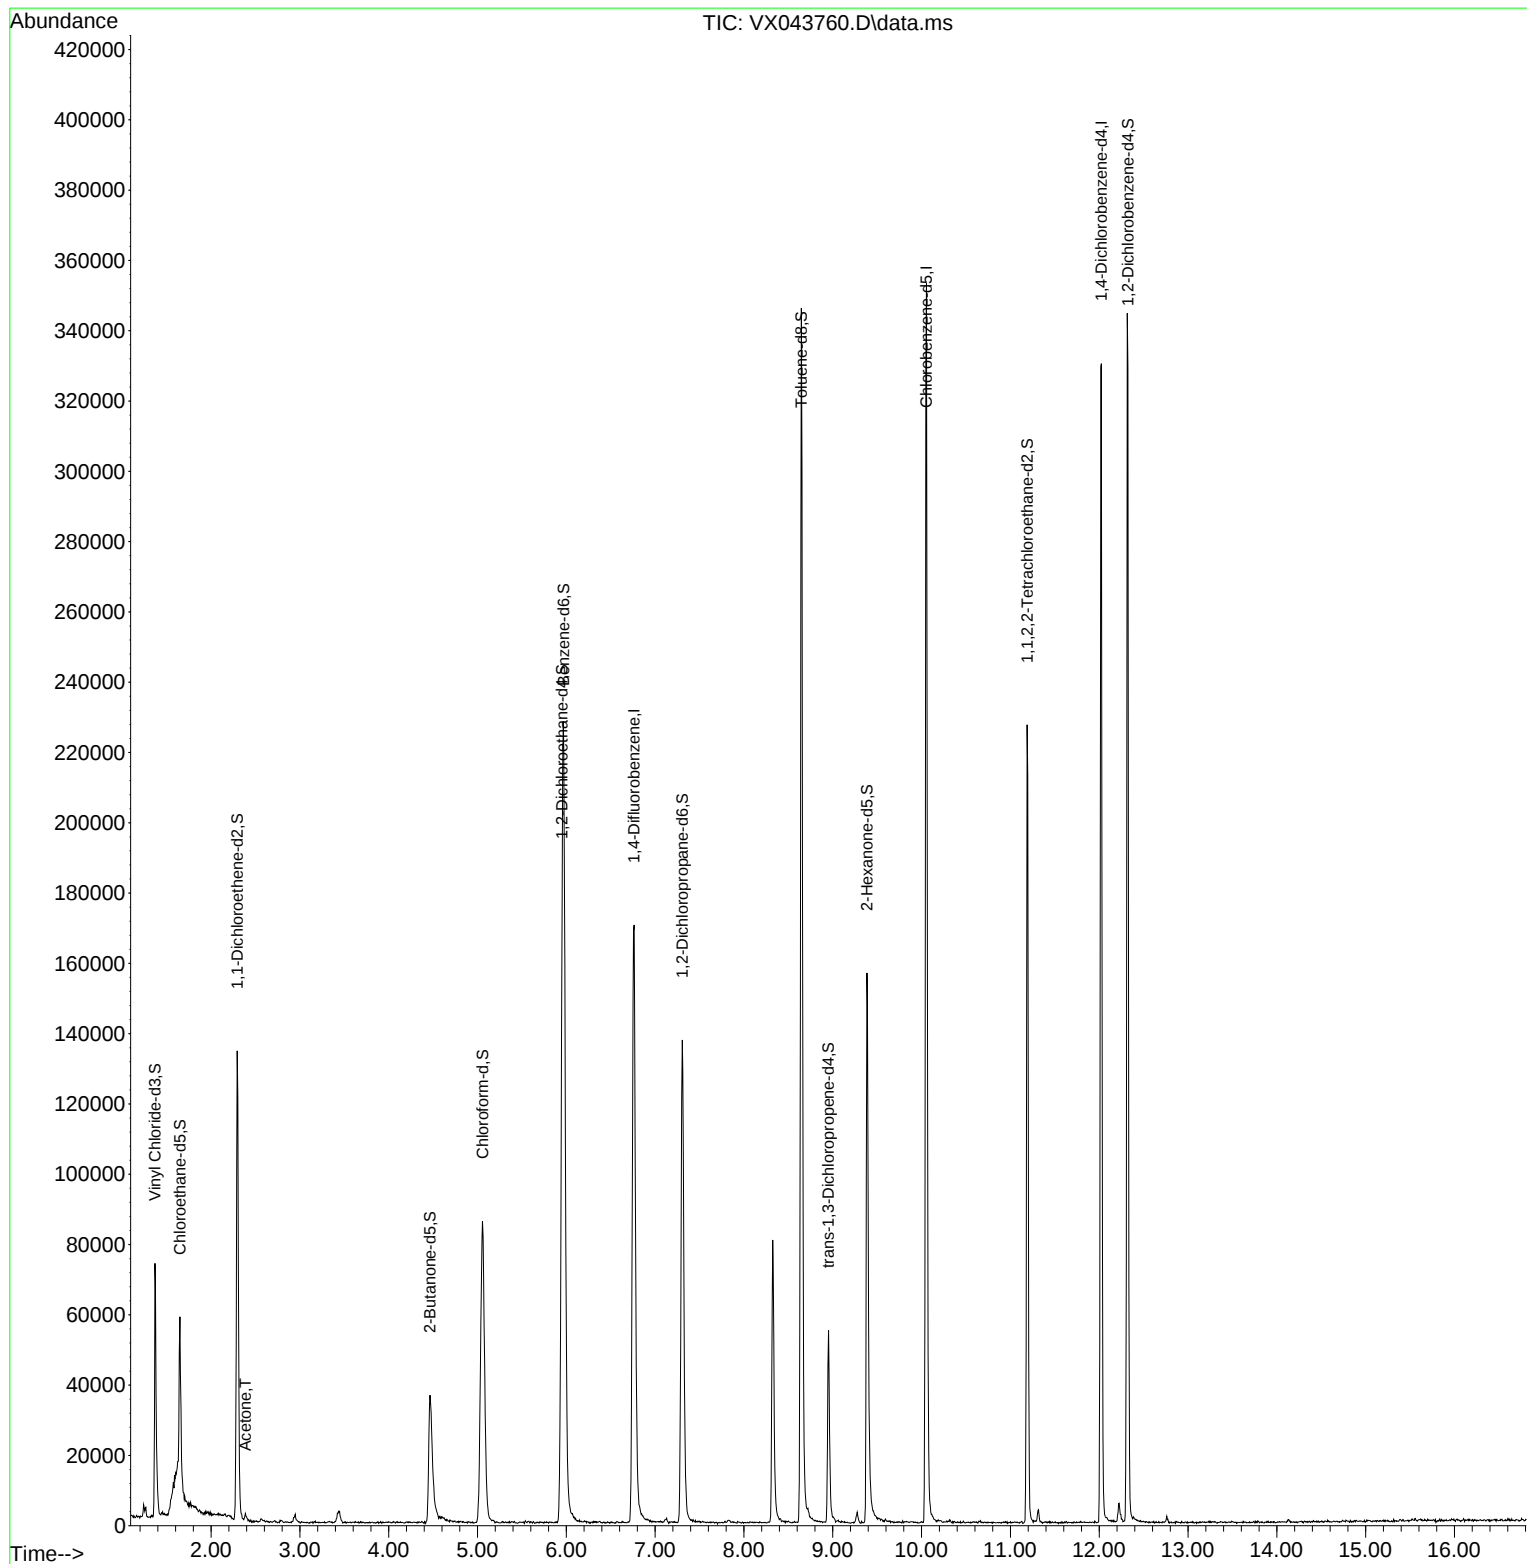

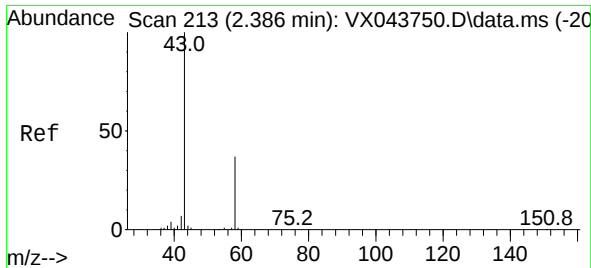

#13

Acetone

Concen: 3.610 ug/L

RT: 2.385 min Scan# 21

Delta R.T. -0.000 min

Lab File: VX043760.D


Acq: 08 Nov 2024 13:40

Instrument :

MSVOA_X

ClientSampleId :

E1H24

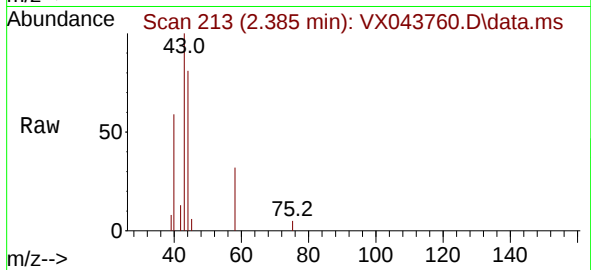

Tgt Ion: 43 Resp: 2272

Ion Ratio Lower Upper

43 100

58 24.7 0.0 63.6

