

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
 Data File : VX043752.D
 Acq On : 08 Nov 2024 10:27
 Operator : JC/MD
 Sample : VX1108WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK720

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043752.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	27	rBV2	3199	3527	0.61%	0.077%
2	1.367	43	46	54	rBV	64207	72046	12.42%	1.579%
3	1.648	89	92	102	rVB	49393	63875	11.01%	1.400%
4	2.300	193	199	214	rVB	111663	179961	31.03%	3.944%
5	2.593	245	247	248	rBV2	400	299	0.05%	0.007%
6	2.946	300	305	311	rVB2	3013	6590	1.14%	0.144%
7	2.989	311	312	313	rBV	574	284	0.05%	0.006%
8	3.373	373	375	376	rBV	414	262	0.05%	0.006%
9	3.434	380	385	395	rVB3	2655	6679	1.15%	0.146%
10	3.581	407	409	410	rBV	450	378	0.07%	0.008%
11	3.648	415	420	421	rBV2	358	632	0.11%	0.014%
12	3.709	429	430	433	rVB	349	255	0.04%	0.006%
13	3.922	462	465	468	rBV2	343	543	0.09%	0.012%
14	4.105	493	495	500	rBV3	409	485	0.08%	0.011%
15	4.464	546	554	569	rBV	33968	104890	18.09%	2.298%
16	4.891	621	624	626	rBV2	443	582	0.10%	0.013%
17	5.056	639	651	668	rBV2	71010	229961	39.65%	5.039%
18	5.208	675	676	677	rVB	745	272	0.05%	0.006%
19	5.233	677	680	681	rBV2	584	622	0.11%	0.014%
20	5.269	684	686	689	rBV2	354	387	0.07%	0.008%
21	5.330	694	696	700	rVB2	449	399	0.07%	0.009%
22	5.373	700	703	704	rBV2	675	647	0.11%	0.014%
23	5.605	739	741	742	rBV2	475	365	0.06%	0.008%
24	5.659	748	750	752	rVB	352	256	0.04%	0.006%
25	5.763	765	767	770	rBV2	290	291	0.05%	0.006%
26	5.964	789	800	820	rBV2	193235	579929	100.00%	12.708%
27	6.190	835	837	840	rBV2	502	338	0.06%	0.007%
28	6.379	866	868	870	rBV2	451	347	0.06%	0.008%
29	6.464	880	882	885	rBV	435	534	0.09%	0.012%
30	6.665	913	915	916	rBV2	348	307	0.05%	0.007%
31	6.757	922	930	949	rVV	175927	437016	75.36%	9.576%
32	7.049	976	978	981	rVB3	442	367	0.06%	0.008%
33	7.123	985	990	995	rBV5	1547	2741	0.47%	0.060%
34	7.220	1004	1006	1007	rVB2	431	275	0.05%	0.006%
35	7.305	1011	1020	1035	rBV	115896	264482	45.61%	5.796%
36	7.580	1059	1065	1067	rBV	504	823	0.14%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
 Data File : VX043752.D
 Acq On : 08 Nov 2024 10:27
 Operator : JC/MD
 Sample : VX1108WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK720

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

37	7.629	1071	1073	1076	rBV2	410	362	0.06%	0.008%
38	7.702	1083	1085	1087	rBV	491	364	0.06%	0.008%
39	7.927	1120	1122	1123	rVB	363	259	0.04%	0.006%
40	7.952	1123	1126	1128	rBV3	551	789	0.14%	0.017%
41	7.994	1131	1133	1135	rVV2	353	369	0.06%	0.008%
42	8.013	1135	1136	1139	rVB2	456	276	0.05%	0.006%
43	8.135	1153	1156	1157	rBV2	403	503	0.09%	0.011%
44	8.324	1181	1187	1200	rBV	70638	126051	21.74%	2.762%
45	8.519	1218	1219	1222	rBV2	435	437	0.08%	0.010%
46	8.647	1234	1240	1253	rBV	289449	465234	80.22%	10.195%
47	8.951	1285	1290	1300	rBV	47761	76950	13.27%	1.686%
48	9.086	1310	1312	1317	rVB3	585	693	0.12%	0.015%
49	9.250	1337	1339	1340	rVB	460	257	0.04%	0.006%
50	9.275	1340	1343	1345	rBV2	562	637	0.11%	0.014%
51	9.384	1356	1361	1382	rBV	165320	251324	43.34%	5.507%
52	9.701	1410	1413	1415	rBV	1084	942	0.16%	0.021%
53	9.756	1420	1422	1423	rBV2	331	293	0.05%	0.006%
54	10.049	1465	1470	1481	rBV	367213	536022	92.43%	11.746%
55	10.244	1500	1502	1506	rBV2	429	558	0.10%	0.012%
56	10.305	1510	1512	1519	rVV3	640	1179	0.20%	0.026%
57	10.378	1519	1524	1525	rVB3	534	689	0.12%	0.015%
58	10.512	1545	1546	1549	rBV	360	306	0.05%	0.007%
59	10.616	1560	1563	1565	rBV3	424	526	0.09%	0.012%
60	10.738	1580	1583	1586	rBV2	410	480	0.08%	0.011%
61	10.884	1605	1607	1608	rBV	511	270	0.05%	0.006%
62	10.963	1617	1620	1621	rVV2	502	550	0.09%	0.012%
63	11.018	1625	1629	1630	rBV2	308	397	0.07%	0.009%
64	11.189	1652	1657	1666	rBV	209079	268022	46.22%	5.873%
65	11.256	1666	1668	1669	rVB	457	303	0.05%	0.007%
66	11.354	1682	1684	1686	rBV	337	251	0.04%	0.006%
67	11.372	1686	1687	1690	rVV2	403	405	0.07%	0.009%
68	11.591	1721	1723	1725	rVB2	323	288	0.05%	0.006%
69	11.695	1739	1740	1742	rBV2	440	322	0.06%	0.007%
70	11.762	1748	1751	1753	rVB3	648	598	0.10%	0.013%
71	11.975	1784	1786	1788	rBV2	402	353	0.06%	0.008%
72	12.018	1788	1793	1810	rVV	354542	465258	80.23%	10.195%
73	12.219	1824	1826	1828	rBV2	309	293	0.05%	0.006%
74	12.256	1831	1832	1835	rVB2	469	316	0.05%	0.007%
75	12.317	1837	1842	1851	rBV	309050	385419	66.46%	8.446%
76	12.768	1913	1916	1919	rVB2	816	888	0.15%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043752.D
Acq On : 08 Nov 2024 10:27
Operator : JC/MD
Sample : VX1108WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK720

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs : 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Title : VOC Analysis

77	12.798	1919	1921	1923	rBV	266	270	0.05%	0.006%
78	12.817	1923	1924	1927	rVV2	453	335	0.06%	0.007%
79	12.859	1929	1931	1934	rBV	381	336	0.06%	0.007%
80	12.890	1934	1936	1940	rVB2	291	294	0.05%	0.006%
81	13.000	1952	1954	1955	rBV	347	281	0.05%	0.006%
82	13.158	1978	1980	1986	rBV2	467	956	0.16%	0.021%
83	13.201	1986	1987	1989	rVV2	347	258	0.04%	0.006%
84	13.225	1989	1991	1995	rVV2	322	455	0.08%	0.010%
85	13.378	2011	2016	2017	rBV3	346	468	0.08%	0.010%
86	13.591	2047	2051	2053	rBV2	574	762	0.13%	0.017%
87	13.786	2079	2083	2088	rBV3	718	1421	0.25%	0.031%
88	14.091	2130	2133	2135	rBV2	430	481	0.08%	0.011%
89	14.127	2136	2139	2142	rVV	941	1267	0.22%	0.028%
90	14.188	2147	2149	2151	rVB2	416	282	0.05%	0.006%
91	14.219	2151	2154	2156	rVB4	335	377	0.07%	0.008%
92	14.249	2156	2159	2160	rBV2	462	477	0.08%	0.010%
93	14.566	2209	2211	2212	rBV	484	327	0.06%	0.007%
94	15.456	2355	2357	2361	rVB3	700	589	0.10%	0.013%
95	15.731	2400	2402	2404	rVB3	872	682	0.12%	0.015%
96	15.914	2431	2432	2435	rBV2	524	441	0.08%	0.010%
97	16.304	2495	2496	2498	rBV	548	346	0.06%	0.008%
98	16.432	2515	2517	2518	rBV	491	338	0.06%	0.007%
99	16.596	2542	2544	2545	rBV2	698	429	0.07%	0.009%
100	16.700	2560	2561	2564	rBV2	475	488	0.08%	0.011%

Sum of corrected areas: 4563440




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043752.D
Acq On : 08 Nov 2024 10:27
Operator : JC/MD
Sample : VX1108WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK720

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

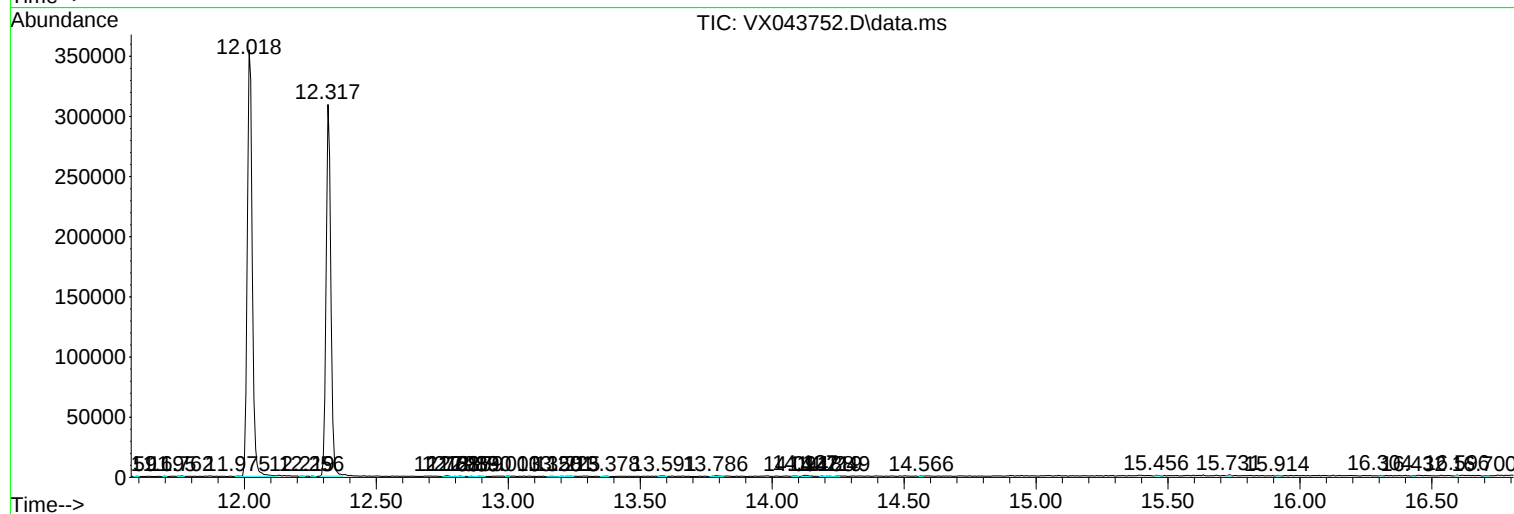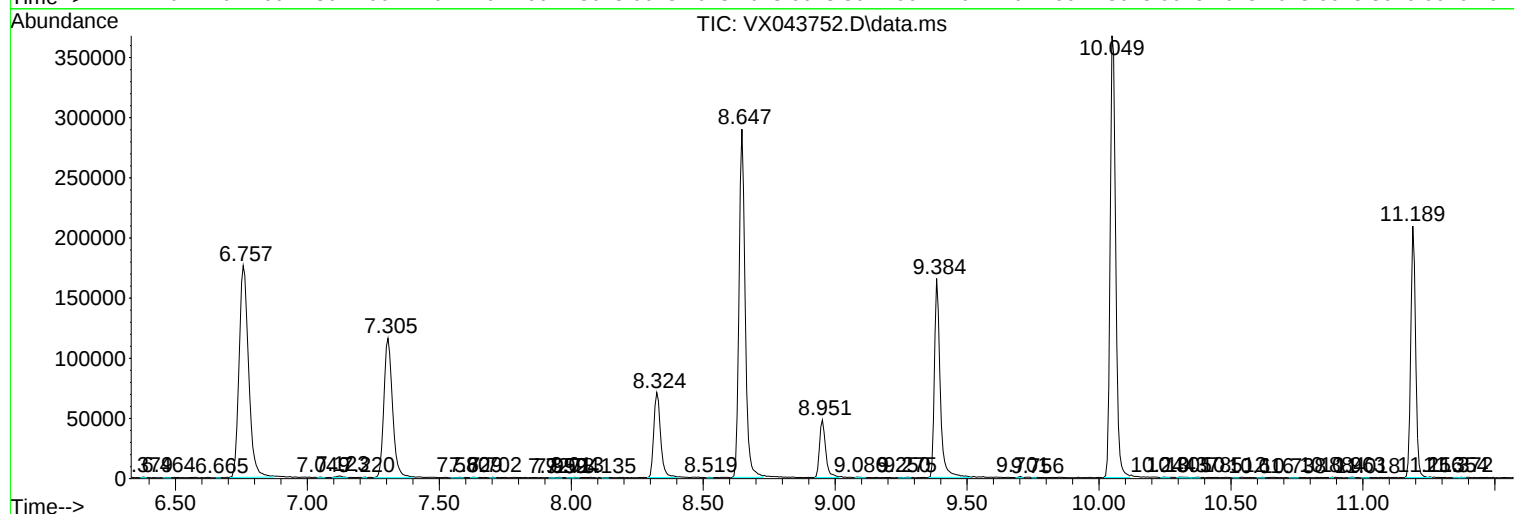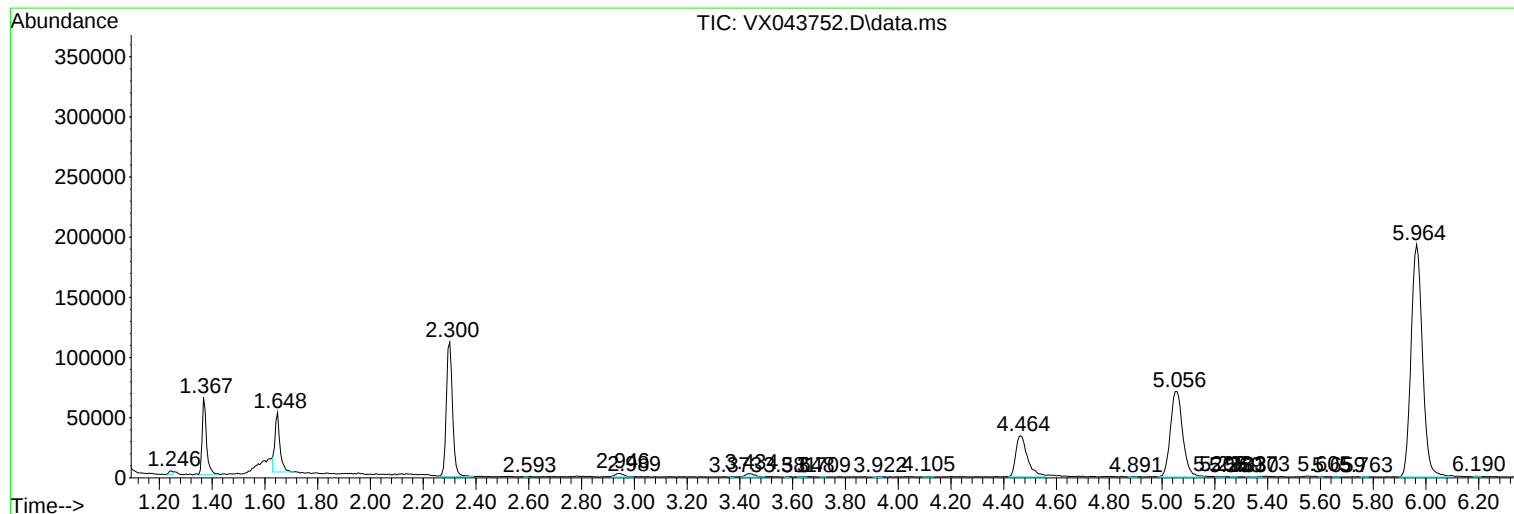

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043752.D
Acq On : 08 Nov 2024 10:27
Operator : JC/MD
Sample : VX1108WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK720

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043752.D
Acq On : 08 Nov 2024 10:27
Operator : JC/MD
Sample : VX1108WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK720

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------