

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
 Data File : VX043754.D
 Acq On : 08 Nov 2024 11:21
 Operator : JC/MD
 Sample : P4621-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043754.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	27	rBV2	3155	3881	0.63%	0.082%
2	1.374	43	47	55	rBV	59835	83295	13.52%	1.753%
3	1.648	89	92	102	rVB	39695	77448	12.57%	1.630%
4	2.294	192	198	209	rVB	121103	187698	30.46%	3.951%
5	2.508	231	233	235	rBV	437	422	0.07%	0.009%
6	2.544	238	239	241	rBV	394	335	0.05%	0.007%
7	2.715	265	267	270	rBV3	521	450	0.07%	0.009%
8	2.776	275	277	279	rBV2	601	647	0.10%	0.014%
9	2.849	283	289	298	rBV2	11888	24270	3.94%	0.511%
10	2.941	298	304	309	rBV4	1781	3074	0.50%	0.065%
11	2.983	309	311	314	rBV	425	318	0.05%	0.007%
12	3.319	364	366	367	rBV	487	313	0.05%	0.007%
13	3.380	374	376	379	rBV2	281	408	0.07%	0.009%
14	3.428	379	384	396	rVB5	4991	12060	1.96%	0.254%
15	3.575	407	408	413	rVV2	525	438	0.07%	0.009%
16	3.623	414	416	418	rVV2	590	491	0.08%	0.010%
17	3.666	421	423	426	rVV2	401	562	0.09%	0.012%
18	3.697	426	428	430	rVB	790	457	0.07%	0.010%
19	3.800	444	445	447	rBV	423	359	0.06%	0.008%
20	3.837	449	451	454	rVB2	351	331	0.05%	0.007%
21	4.239	511	517	518	rBB2	462	515	0.08%	0.011%
22	4.276	518	523	531	rBV2	315	930	0.15%	0.020%
23	4.355	534	536	539	rBV3	397	480	0.08%	0.010%
24	4.471	547	555	570	rBV	31903	100299	16.27%	2.111%
25	4.818	611	612	615	rVB2	499	330	0.05%	0.007%
26	4.849	615	617	621	rBV	397	488	0.08%	0.010%
27	4.916	626	628	629	rBV	563	373	0.06%	0.008%
28	5.056	639	651	664	rBV2	81968	252355	40.95%	5.312%
29	5.312	691	693	695	rVB	685	576	0.09%	0.012%
30	5.330	695	696	698	rBV2	542	449	0.07%	0.009%
31	5.495	720	723	724	rBV	251	303	0.05%	0.006%
32	5.544	728	731	732	rBV3	741	904	0.15%	0.019%
33	5.684	752	754	755	rBV2	429	283	0.05%	0.006%
34	5.800	771	773	776	rVB2	332	340	0.06%	0.007%
35	5.964	789	800	815	rBV3	208710	616289	100.00%	12.973%
36	6.349	861	863	865	rBV	656	457	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
 Data File : VX043754.D
 Acq On : 08 Nov 2024 11:21
 Operator : JC/MD
 Sample : P4621-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	6.385	865	869	871	rVV2	528	602	0.10%	0.013%
38	6.452	878	880	883	rBV2	532	642	0.10%	0.014%
39	6.507	887	889	892	rVV2	500	534	0.09%	0.011%
40	6.641	910	911	914	rVB2	444	419	0.07%	0.009%
41	6.757	922	930	944	rBV	167704	416032	67.51%	8.757%
42	7.153	993	995	1000	rVB3	623	634	0.10%	0.013%
43	7.306	1012	1020	1034	rVV	125571	283178	45.95%	5.961%
44	7.482	1047	1049	1055	rVB3	799	1139	0.18%	0.024%
45	7.714	1085	1087	1088	rBV2	392	324	0.05%	0.007%
46	7.873	1112	1113	1114	rBV	652	341	0.06%	0.007%
47	8.037	1137	1140	1142	rBV2	463	598	0.10%	0.013%
48	8.226	1168	1171	1173	rBV2	401	518	0.08%	0.011%
49	8.324	1181	1187	1199	rBV	76906	132432	21.49%	2.788%
50	8.586	1229	1230	1233	rBV2	824	505	0.08%	0.011%
51	8.647	1234	1240	1249	rBV	317099	508244	82.47%	10.698%
52	8.872	1276	1277	1280	rBV2	407	358	0.06%	0.008%
53	8.952	1285	1290	1301	rBV	49198	79696	12.93%	1.678%
54	9.275	1338	1343	1349	rBV2	2261	3857	0.63%	0.081%
55	9.391	1356	1362	1376	rBV	142570	244730	39.71%	5.152%
56	9.683	1408	1410	1412	rBV2	538	311	0.05%	0.007%
57	9.769	1421	1424	1425	rBV3	427	376	0.06%	0.008%
58	9.884	1442	1443	1448	rVV	268	322	0.05%	0.007%
59	10.055	1465	1471	1485	rBV	339199	496981	80.64%	10.461%
60	10.244	1500	1502	1504	rBV3	909	830	0.13%	0.017%
61	10.518	1545	1547	1549	rVB2	416	278	0.05%	0.006%
62	10.653	1565	1569	1580	rVB2	6918	11722	1.90%	0.247%
63	10.964	1615	1620	1622	rBV2	506	813	0.13%	0.017%
64	11.018	1627	1629	1633	rBV2	296	448	0.07%	0.009%
65	11.189	1652	1657	1667	rVB	219779	283240	45.96%	5.962%
66	11.311	1674	1677	1683	rVB3	2461	3165	0.51%	0.067%
67	11.421	1691	1695	1697	rBV2	232	339	0.06%	0.007%
68	11.445	1697	1699	1701	rBV2	318	369	0.06%	0.008%
69	11.604	1723	1725	1727	rVB	442	323	0.05%	0.007%
70	11.689	1737	1739	1744	rVB2	512	586	0.10%	0.012%
71	11.750	1748	1749	1755	rVB3	579	771	0.13%	0.016%
72	11.829	1761	1762	1764	rBV2	364	280	0.05%	0.006%
73	12.018	1788	1793	1804	rBV	338572	450673	73.13%	9.487%
74	12.195	1820	1822	1823	rBV2	614	538	0.09%	0.011%
75	12.226	1823	1827	1837	rVV2	4682	8655	1.40%	0.182%
76	12.317	1837	1842	1850	rBV	330644	430066	69.78%	9.053%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
 Data File : VX043754.D
 Acq On : 08 Nov 2024 11:21
 Operator : JC/MD
 Sample : P4621-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

77	12.652	1896	1897	1900	rVB	477	386	0.06%	0.008%
78	12.732	1905	1910	1911	rBV2	366	360	0.06%	0.008%
79	12.768	1911	1916	1917	rBV3	549	826	0.13%	0.017%
80	12.988	1950	1952	1954	rVB2	456	361	0.06%	0.008%
81	13.219	1988	1990	1994	rBV2	332	443	0.07%	0.009%
82	13.286	1998	2001	2002	rBV	372	340	0.06%	0.007%
83	13.494	2032	2035	2038	rBV2	492	831	0.13%	0.017%
84	13.750	2073	2077	2079	rBV	427	581	0.09%	0.012%
85	13.975	2112	2114	2115	rBV	457	329	0.05%	0.007%
86	14.122	2135	2138	2139	rBV2	1098	1027	0.17%	0.022%
87	14.189	2147	2149	2153	rBV3	391	532	0.09%	0.011%
88	14.317	2168	2170	2173	rBV2	477	384	0.06%	0.008%
89	14.384	2178	2181	2185	rVB4	300	406	0.07%	0.009%
90	14.475	2195	2196	2200	rBV2	318	441	0.07%	0.009%
91	14.573	2210	2212	2214	rBV2	419	377	0.06%	0.008%
92	14.652	2223	2225	2227	rBV2	492	560	0.09%	0.012%
93	14.701	2231	2233	2235	rVB2	510	447	0.07%	0.009%
94	14.743	2238	2240	2241	rVV2	526	447	0.07%	0.009%
95	15.152	2305	2307	2308	rBV	609	418	0.07%	0.009%
96	15.365	2339	2342	2344	rBV2	631	767	0.12%	0.016%
97	16.018	2447	2449	2451	rBV2	844	523	0.08%	0.011%
98	16.036	2451	2452	2453	rBV	490	282	0.05%	0.006%
99	16.322	2497	2499	2502	rBV3	583	522	0.08%	0.011%
100	16.676	2555	2557	2560	rBV3	679	546	0.09%	0.011%




Sum of corrected areas: 4750633

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043754.D
Acq On : 08 Nov 2024 11:21
Operator : JC/MD
Sample : P4621-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

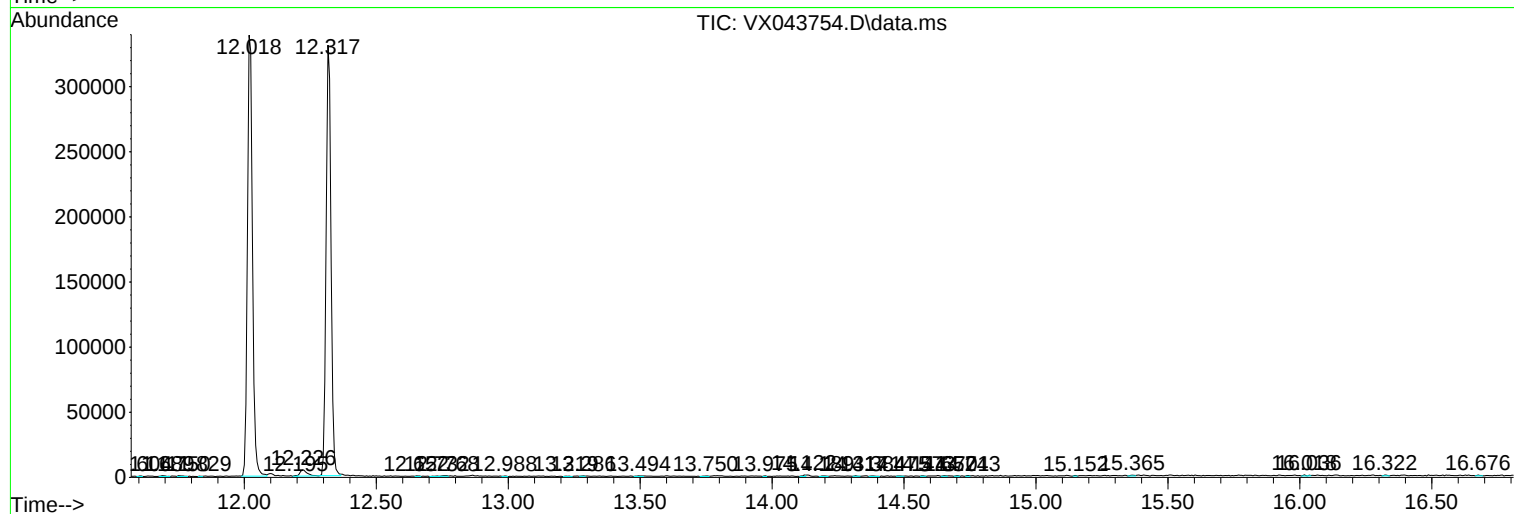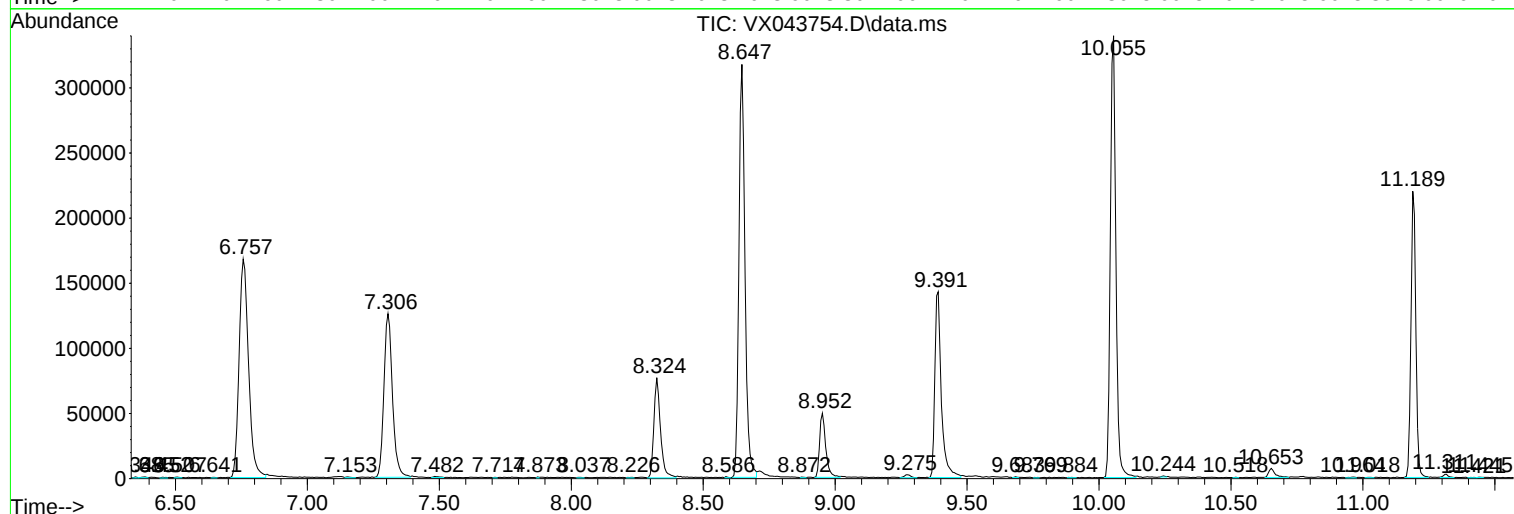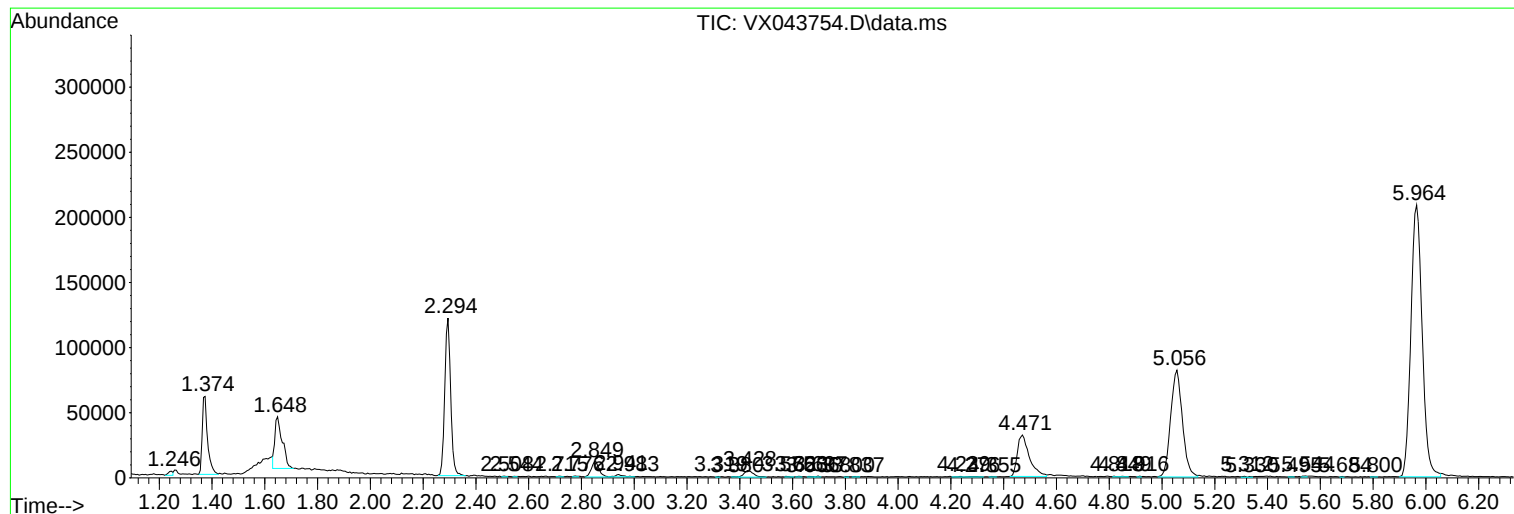

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043754.D
Acq On : 08 Nov 2024 11:21
Operator : JC/MD
Sample : P4621-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043754.D
Acq On : 08 Nov 2024 11:21
Operator : JC/MD
Sample : P4621-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------