

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
 Data File : VX043755.D
 Acq On : 08 Nov 2024 11:44
 Operator : JC/MD
 Sample : VIBLK676
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK676

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043755.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	27	rBV	3843	4296	0.86%	0.107%
2	1.368	43	46	57	rVB	43307	64320	12.81%	1.608%
3	1.648	89	92	102	rVB2	29747	72498	14.44%	1.813%
4	2.288	192	197	208	rVB	92802	147505	29.39%	3.689%
5	2.672	259	260	263	rBV	396	336	0.07%	0.008%
6	2.758	273	274	275	rBV	545	302	0.06%	0.008%
7	2.782	275	278	281	rVB3	748	818	0.16%	0.020%
8	3.026	316	318	320	rVB2	362	312	0.06%	0.008%
9	3.294	359	362	363	rBV2	394	373	0.07%	0.009%
10	3.434	378	385	392	rVB3	5338	11848	2.36%	0.296%
11	3.538	400	402	405	rVB3	414	416	0.08%	0.010%
12	3.605	411	413	415	rBV2	486	450	0.09%	0.011%
13	3.660	419	422	423	rBV	544	347	0.07%	0.009%
14	3.751	433	437	439	rBV	391	386	0.08%	0.010%
15	4.087	488	492	495	rBV2	489	912	0.18%	0.023%
16	4.404	543	544	546	rBV	396	289	0.06%	0.007%
17	4.471	548	555	574	rBV	23878	81081	16.15%	2.028%
18	4.879	620	622	625	rBV2	438	423	0.08%	0.011%
19	5.050	639	650	669	rBV2	62674	198664	39.58%	4.968%
20	5.227	677	679	681	rBV2	334	415	0.08%	0.010%
21	5.294	688	690	691	rBV	397	383	0.08%	0.010%
22	5.544	729	731	732	rBV	530	458	0.09%	0.011%
23	5.781	768	770	773	rBV2	320	305	0.06%	0.008%
24	5.824	775	777	779	rBV	373	330	0.07%	0.008%
25	5.885	785	787	788	rBV	309	294	0.06%	0.007%
26	5.964	790	800	818	rVV2	166670	501944	100.00%	12.552%
27	6.361	862	865	867	rBV2	372	381	0.08%	0.010%
28	6.385	867	869	873	rVB2	413	450	0.09%	0.011%
29	6.464	881	882	886	rVB2	423	363	0.07%	0.009%
30	6.544	892	895	899	rBV2	411	654	0.13%	0.016%
31	6.690	918	919	922	rBV3	483	480	0.10%	0.012%
32	6.757	922	930	943	rBV	159901	402185	80.13%	10.057%
33	7.306	1010	1020	1031	rBV2	99431	224407	44.71%	5.612%
34	7.476	1045	1048	1049	rBV2	320	271	0.05%	0.007%
35	7.604	1065	1069	1071	rBV2	258	455	0.09%	0.011%
36	7.623	1071	1072	1075	rVV2	349	322	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
 Data File : VX043755.D
 Acq On : 08 Nov 2024 11:44
 Operator : JC/MD
 Sample : VIBLK676
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK676

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	7.745	1089	1092	1093	rBV	475	350	0.07%	0.009%
38	7.885	1113	1115	1119	rBV3	272	323	0.06%	0.008%
39	7.964	1125	1128	1130	rBV2	280	383	0.08%	0.010%
40	8.123	1152	1154	1156	rBV	384	285	0.06%	0.007%
41	8.324	1181	1187	1201	rVV	56946	102133	20.35%	2.554%
42	8.555	1223	1225	1229	rVB2	372	267	0.05%	0.007%
43	8.647	1234	1240	1253	rBV	249139	404376	80.56%	10.112%
44	8.866	1274	1276	1279	rBV2	445	505	0.10%	0.013%
45	8.952	1285	1290	1303	rVV	37774	63245	12.60%	1.582%
46	9.086	1309	1312	1316	rBV2	375	486	0.10%	0.012%
47	9.122	1316	1318	1321	rVB	478	491	0.10%	0.012%
48	9.226	1331	1335	1338	rBV2	330	647	0.13%	0.016%
49	9.281	1341	1344	1347	rBV2	634	635	0.13%	0.016%
50	9.391	1357	1362	1380	rBV	117581	203378	40.52%	5.086%
51	9.799	1427	1429	1432	rBV2	464	425	0.08%	0.011%
52	9.830	1432	1434	1435	rVB	552	328	0.07%	0.008%
53	9.933	1450	1451	1453	rBV2	408	361	0.07%	0.009%
54	10.055	1465	1471	1483	rBV	342432	486540	96.93%	12.167%
55	10.268	1505	1506	1509	rBV2	401	315	0.06%	0.008%
56	10.390	1525	1526	1529	rBV3	314	295	0.06%	0.007%
57	10.488	1541	1542	1544	rBV	464	309	0.06%	0.008%
58	10.537	1548	1550	1551	rBV	463	409	0.08%	0.010%
59	10.781	1587	1590	1593	rBV	509	656	0.13%	0.016%
60	10.903	1608	1610	1613	rVB	406	355	0.07%	0.009%
61	10.951	1613	1618	1619	rBV2	448	592	0.12%	0.015%
62	10.970	1619	1621	1624	rVV	456	306	0.06%	0.008%
63	11.006	1624	1627	1631	rVB2	384	474	0.09%	0.012%
64	11.043	1631	1633	1634	rBV	464	284	0.06%	0.007%
65	11.110	1642	1644	1647	rVB2	426	519	0.10%	0.013%
66	11.189	1652	1657	1665	rBV	166471	222060	44.24%	5.553%
67	11.274	1670	1671	1674	rVB	611	309	0.06%	0.008%
68	11.341	1680	1682	1684	rBV2	280	319	0.06%	0.008%
69	11.445	1698	1699	1701	rBV	371	289	0.06%	0.007%
70	11.463	1701	1702	1704	rVB2	380	270	0.05%	0.007%
71	11.634	1728	1730	1733	rBV2	329	461	0.09%	0.012%
72	11.750	1747	1749	1753	rVB2	355	358	0.07%	0.009%
73	11.890	1770	1772	1775	rVB3	368	327	0.07%	0.008%
74	11.927	1777	1778	1780	rBV	381	263	0.05%	0.007%
75	12.018	1788	1793	1803	rBV	327977	428794	85.43%	10.723%
76	12.317	1837	1842	1857	rBV	264123	346247	68.98%	8.658%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
 Data File : VX043755.D
 Acq On : 08 Nov 2024 11:44
 Operator : JC/MD
 Sample : VIBLK676
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK676

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	12.841	1925	1928	1929	rBV2	300	323	0.06%	0.008%
78	13.116	1972	1973	1975	rBB	513	284	0.06%	0.007%
79	13.189	1983	1985	1987	rVB	451	295	0.06%	0.007%
80	13.244	1992	1994	1997	rVB3	383	285	0.06%	0.007%
81	13.292	2001	2002	2005	rBV2	511	518	0.10%	0.013%
82	13.335	2008	2009	2013	rBV	367	292	0.06%	0.007%
83	13.548	2040	2044	2045	rBV2	347	484	0.10%	0.012%
84	13.591	2049	2051	2052	rVB	416	263	0.05%	0.007%
85	13.664	2061	2063	2066	rVB2	346	265	0.05%	0.007%
86	13.713	2069	2071	2073	rBV2	406	290	0.06%	0.007%
87	13.750	2075	2077	2080	rBV2	375	407	0.08%	0.010%
88	13.786	2082	2083	2085	rBV2	398	345	0.07%	0.009%
89	13.859	2093	2095	2098	rVB2	561	453	0.09%	0.011%
90	13.932	2105	2107	2109	rBV2	403	380	0.08%	0.010%
91	14.128	2136	2139	2142	rBV2	572	808	0.16%	0.020%
92	14.420	2185	2187	2189	rVB2	452	316	0.06%	0.008%
93	14.627	2219	2221	2222	rBV	511	355	0.07%	0.009%
94	14.731	2236	2238	2239	rBV2	422	271	0.05%	0.007%
95	14.792	2244	2248	2250	rBV3	578	899	0.18%	0.022%
96	14.908	2265	2267	2272	rBV3	382	426	0.08%	0.011%
97	14.944	2272	2273	2275	rBV2	587	406	0.08%	0.010%
98	15.670	2391	2392	2394	rBV	566	471	0.09%	0.012%
99	15.828	2416	2418	2422	rBV2	489	703	0.14%	0.018%
100	16.036	2450	2452	2455	rVB3	664	421	0.08%	0.011%


Sum of corrected areas: 3999002

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043755.D
Acq On : 08 Nov 2024 11:44
Operator : JC/MD
Sample : VIBLK676
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK676

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

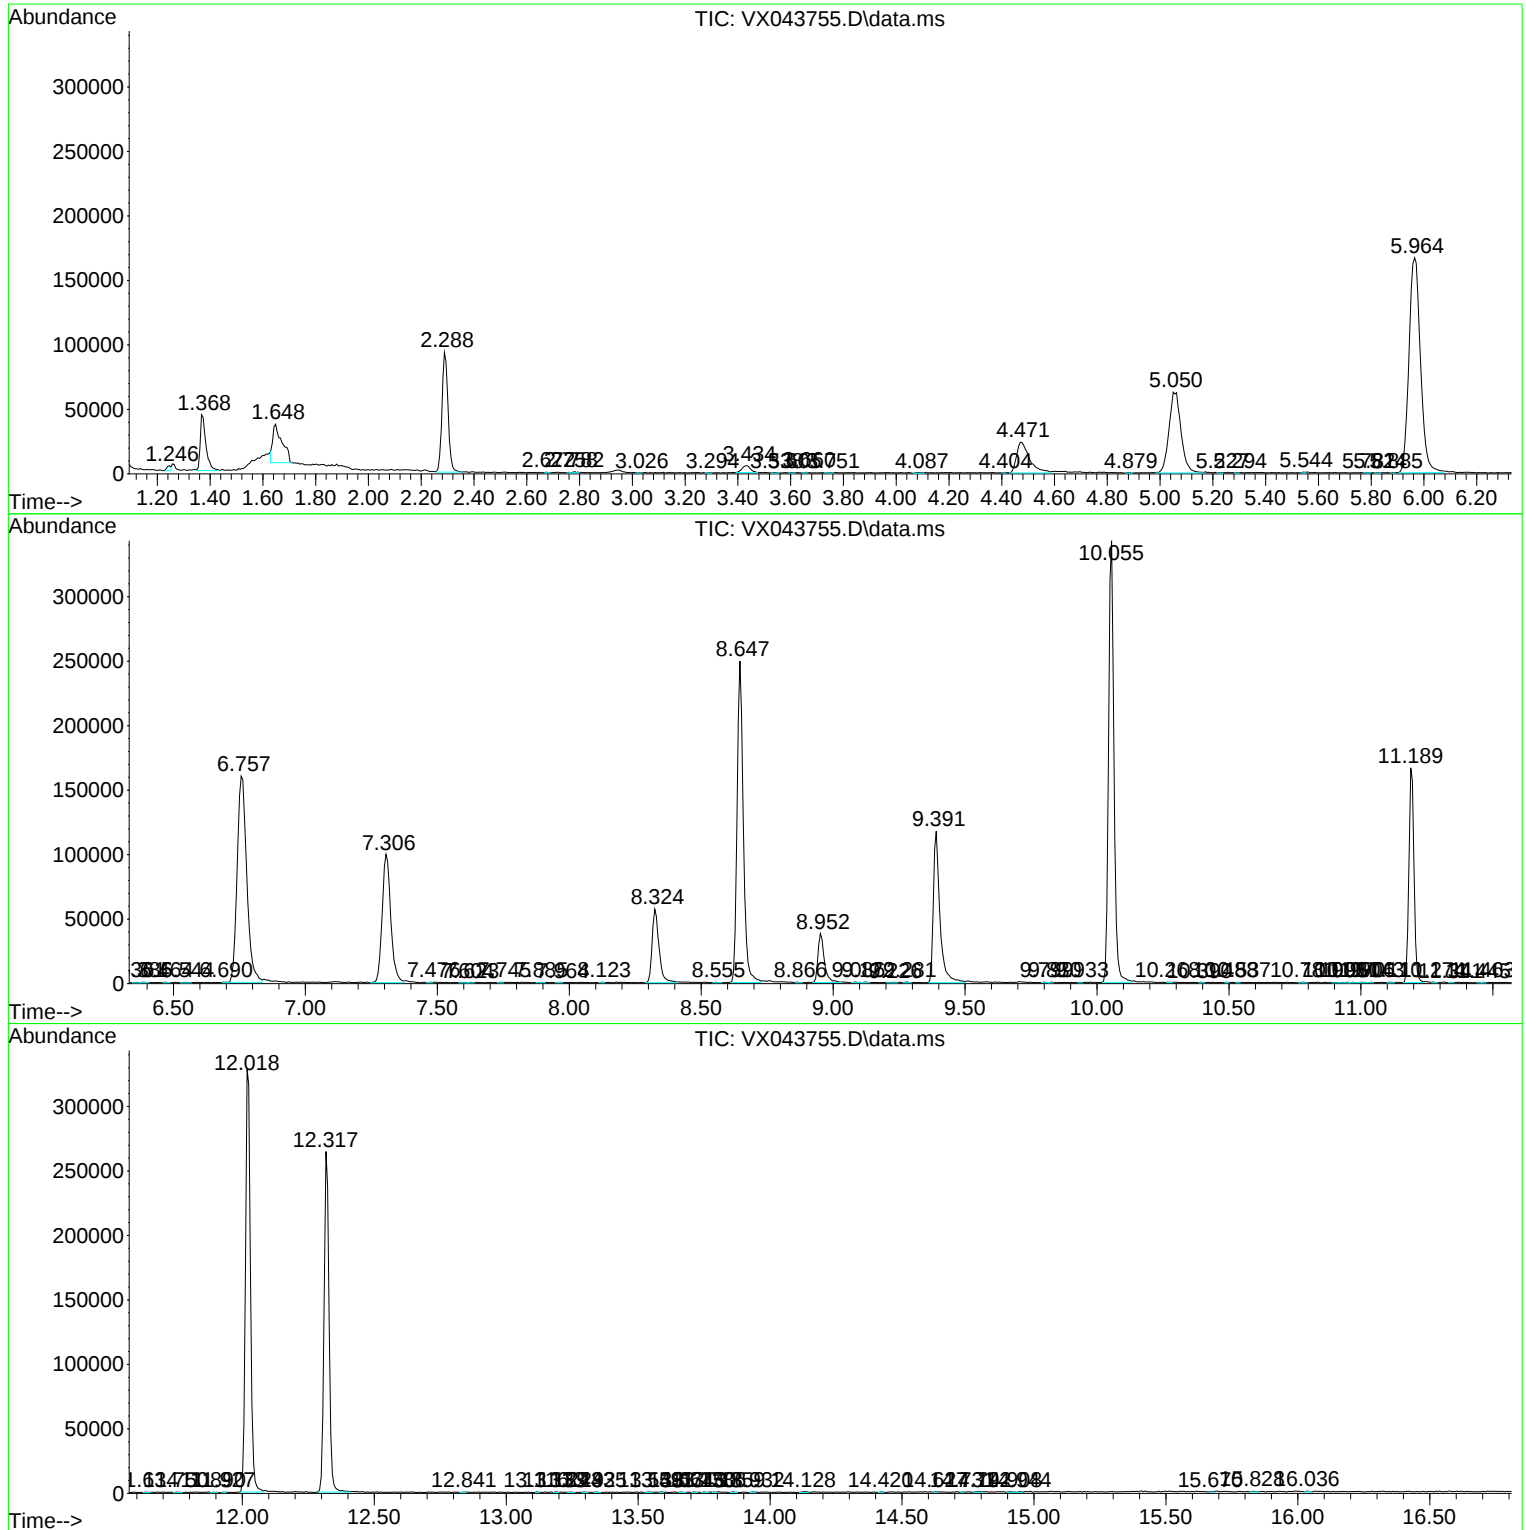

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043755.D
Acq On : 08 Nov 2024 11:44
Operator : JC/MD
Sample : VIBLK676
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK676

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043755.D
Acq On : 08 Nov 2024 11:44
Operator : JC/MD
Sample : VIBLK676
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK676

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------