

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043757.D
Acq On : 08 Nov 2024 12:30
Operator : JC/MD
Sample : P4742-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1H12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M

Title : VOC Analysis

Signal : TIC: VX043757.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	27	rBV2	3183	3228	0.54%	0.074%
2	1.368	43	46	56	rVB	60120	77305	12.83%	1.761%
3	1.648	89	92	103	rVB	41802	71730	11.90%	1.634%
4	2.294	192	198	210	rVB	114736	178776	29.66%	4.073%
5	2.386	210	213	223	rVB2	4899	9597	1.59%	0.219%
6	2.459	223	225	227	rBV	469	341	0.06%	0.008%
7	2.575	239	244	248	rVB3	1171	1666	0.28%	0.038%
8	2.611	248	250	251	rBV	600	383	0.06%	0.009%
9	2.642	253	255	258	rVB2	375	395	0.07%	0.009%
10	2.831	284	286	288	rBV2	368	363	0.06%	0.008%
11	2.946	297	305	309	rBV4	1609	3518	0.58%	0.080%
12	3.434	377	385	393	rBV3	4564	10389	1.72%	0.237%
13	3.538	400	402	405	rVB	498	456	0.08%	0.010%
14	3.587	407	410	411	rBV2	319	345	0.06%	0.008%
15	3.879	453	458	461	rVB3	406	797	0.13%	0.018%
16	3.922	461	465	466	rBV2	335	467	0.08%	0.011%
17	4.001	476	478	481	rBV2	539	619	0.10%	0.014%
18	4.111	495	496	500	rBV2	316	425	0.07%	0.010%
19	4.251	517	519	522	rVV2	455	393	0.07%	0.009%
20	4.471	547	555	569	rBV	31120	96706	16.04%	2.203%
21	4.727	595	597	599	rBV	473	405	0.07%	0.009%
22	5.056	640	651	665	rBV2	77286	234057	38.83%	5.333%
23	5.367	698	702	703	rBV	429	544	0.09%	0.012%
24	5.568	729	735	737	rVV3	804	1432	0.24%	0.033%
25	5.666	748	751	752	rBV2	303	399	0.07%	0.009%
26	5.800	769	773	776	rVB3	423	603	0.10%	0.014%
27	5.842	776	780	781	rBV	461	577	0.10%	0.013%
28	5.964	789	800	819	rBV2	201944	602733	100.00%	13.732%
29	6.226	841	843	846	rVV3	631	510	0.08%	0.012%
30	6.513	888	890	892	rBV2	575	614	0.10%	0.014%
31	6.617	906	907	910	rBV	406	326	0.05%	0.007%
32	6.763	921	931	946	rVV	141672	358781	59.53%	8.174%
33	7.056	977	979	983	rVB2	414	369	0.06%	0.008%
34	7.098	985	986	987	rBV	582	392	0.07%	0.009%
35	7.214	1003	1005	1008	rVV3	517	522	0.09%	0.012%
36	7.305	1012	1020	1037	rVV	118733	268291	44.51%	6.112%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043757.D
Acq On : 08 Nov 2024 12:30
Operator : JC/MD
Sample : P4742-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1H12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Title : VOC Analysis

37	7.458	1042	1045	1046	rBV	311	330	0.05%	0.008%
38	7.726	1086	1089	1090	rBV2	309	358	0.06%	0.008%
39	7.763	1093	1095	1097	rVV	625	361	0.06%	0.008%
40	7.891	1115	1116	1118	rVB2	551	358	0.06%	0.008%
41	7.921	1118	1121	1122	rBV3	344	346	0.06%	0.008%
42	8.189	1163	1165	1168	rVB	502	394	0.07%	0.009%
43	8.244	1170	1174	1175	rBV	582	549	0.09%	0.013%
44	8.324	1181	1187	1199	rBV	68292	124959	20.73%	2.847%
45	8.549	1221	1224	1227	rBV3	422	618	0.10%	0.014%
46	8.647	1234	1240	1251	rBV	300124	493038	81.80%	11.233%
47	8.952	1285	1290	1299	rBV	47043	75182	12.47%	1.713%
48	9.122	1316	1318	1321	rBV2	384	503	0.08%	0.011%
49	9.238	1334	1337	1338	rBV2	415	386	0.06%	0.009%
50	9.275	1338	1343	1348	rBV2	2928	4504	0.75%	0.103%
51	9.390	1356	1362	1374	rBV	137483	232695	38.61%	5.301%
52	9.622	1398	1400	1402	rBV2	446	475	0.08%	0.011%
53	9.646	1402	1404	1407	rVV3	381	476	0.08%	0.011%
54	9.756	1420	1422	1428	rBV2	502	919	0.15%	0.021%
55	10.055	1465	1471	1485	rBV	309150	435716	72.29%	9.927%
56	10.305	1510	1512	1520	rVB5	1424	1774	0.29%	0.040%
57	10.415	1526	1530	1532	rVB2	425	571	0.09%	0.013%
58	10.537	1548	1550	1553	rVB2	305	363	0.06%	0.008%
59	10.591	1558	1559	1562	rBV2	496	355	0.06%	0.008%
60	10.634	1564	1566	1567	rBV	571	359	0.06%	0.008%
61	10.707	1575	1578	1580	rVB	352	337	0.06%	0.008%
62	10.848	1600	1601	1603	rBV	522	338	0.06%	0.008%
63	10.957	1616	1619	1621	rBV2	325	416	0.07%	0.009%
64	11.018	1627	1629	1631	rBV2	411	455	0.08%	0.010%
65	11.091	1638	1641	1644	rVB2	363	510	0.08%	0.012%
66	11.189	1652	1657	1667	rBV	202063	270701	44.91%	6.167%
67	11.317	1674	1678	1683	rVB3	4325	6164	1.02%	0.140%
68	11.439	1694	1698	1700	rBV3	350	411	0.07%	0.009%
69	11.488	1703	1706	1707	rBV2	338	398	0.07%	0.009%
70	11.939	1776	1780	1782	rBV3	413	645	0.11%	0.015%
71	12.024	1788	1794	1804	rBV	284947	376338	62.44%	8.574%
72	12.225	1824	1827	1836	rVB5	1559	2135	0.35%	0.049%
73	12.317	1837	1842	1852	rVV	304268	411245	68.23%	9.369%
74	12.542	1876	1879	1880	rBV2	379	362	0.06%	0.008%
75	12.591	1885	1887	1889	rBV2	410	339	0.06%	0.008%
76	12.762	1913	1915	1919	rVV3	1254	1750	0.29%	0.040%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
 Data File : VX043757.D
 Acq On : 08 Nov 2024 12:30
 Operator : JC/MD
 Sample : P4742-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1H12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

77	12.920	1939	1941	1942	rBV	421	404	0.07%	0.009%
78	12.945	1943	1945	1946	rVV	600	363	0.06%	0.008%
79	13.024	1956	1958	1962	rBV3	248	337	0.06%	0.008%
80	13.292	1999	2002	2005	rVB2	370	443	0.07%	0.010%
81	13.591	2049	2051	2054	rBV3	453	513	0.09%	0.012%
82	13.676	2061	2065	2066	rBV2	453	600	0.10%	0.014%
83	13.957	2107	2111	2113	rBV2	378	476	0.08%	0.011%
84	14.048	2124	2126	2129	rVB2	406	404	0.07%	0.009%
85	14.085	2129	2132	2134	rBV	519	505	0.08%	0.012%
86	14.115	2134	2137	2138	rBV2	555	522	0.09%	0.012%
87	14.134	2138	2140	2144	rVV2	1012	920	0.15%	0.021%
88	14.182	2147	2148	2152	rBV2	425	463	0.08%	0.011%
89	14.304	2165	2168	2171	rBV3	561	671	0.11%	0.015%
90	14.426	2185	2188	2190	rBV3	560	657	0.11%	0.015%
91	14.633	2218	2222	2223	rBV2	406	391	0.06%	0.009%
92	15.200	2312	2315	2317	rBV3	605	505	0.08%	0.012%
93	15.237	2320	2321	2323	rBV2	481	332	0.06%	0.008%
94	15.530	2367	2369	2370	rBV2	665	455	0.08%	0.010%
95	15.670	2389	2392	2394	rVB4	641	682	0.11%	0.016%
96	15.694	2394	2396	2399	rBV2	605	694	0.12%	0.016%
97	15.780	2408	2410	2412	rBV2	604	525	0.09%	0.012%
98	15.804	2412	2414	2415	rBV	551	404	0.07%	0.009%
99	16.450	2518	2520	2521	rBV2	778	503	0.08%	0.011%
100	16.706	2558	2562	2563	rBV3	599	876	0.15%	0.020%




Sum of corrected areas: 4389232

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043757.D
Acq On : 08 Nov 2024 12:30
Operator : JC/MD
Sample : P4742-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1H12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

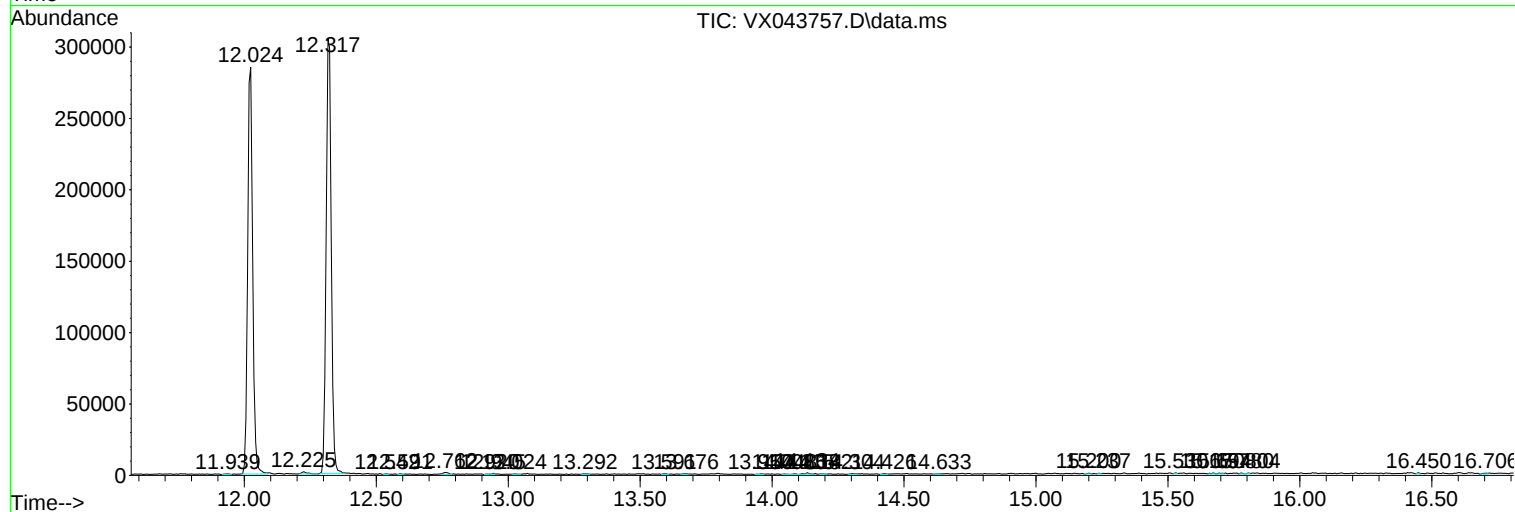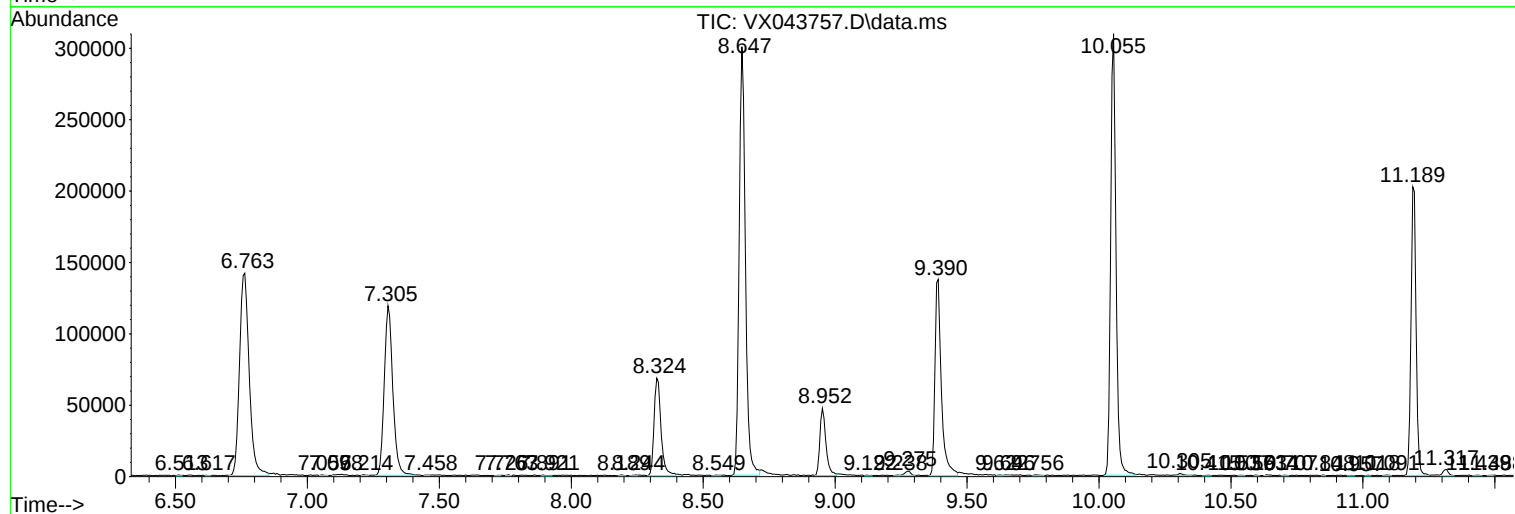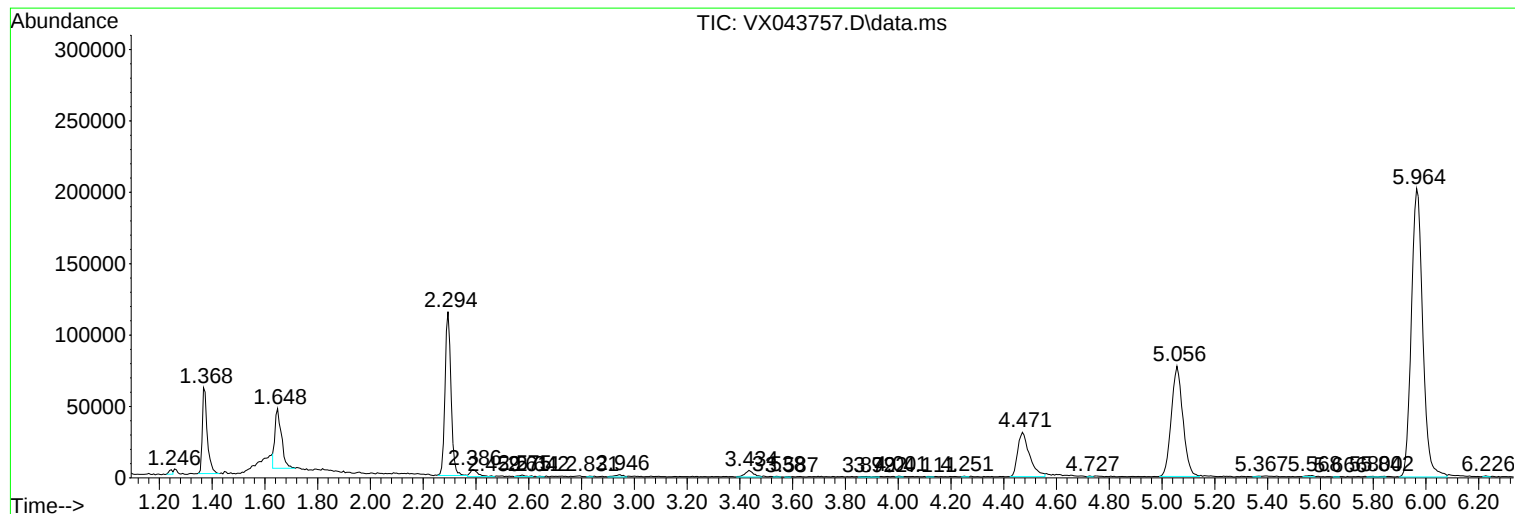

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043757.D
Acq On : 08 Nov 2024 12:30
Operator : JC/MD
Sample : P4742-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1H12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043757.D
Acq On : 08 Nov 2024 12:30
Operator : JC/MD
Sample : P4742-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1H12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------