

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
 Data File : VX043764.D
 Acq On : 08 Nov 2024 15:12
 Operator : JC/MD
 Sample : P4742-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1H14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043764.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	17	rVB	7686	7587	1.07%	0.142%
2	1.239	22	25	27	rBV2	3877	4513	0.64%	0.085%
3	1.368	43	46	56	rVB	93159	93730	13.20%	1.758%
4	1.648	89	92	102	rVB	58641	82685	11.65%	1.550%
5	2.300	193	199	210	rBV	140507	217145	30.59%	4.072%
6	2.489	228	230	232	rBV2	571	576	0.08%	0.011%
7	2.690	262	263	264	rBV	599	354	0.05%	0.007%
8	2.946	301	305	308	rVB4	842	1269	0.18%	0.024%
9	3.117	331	333	336	rVB2	391	367	0.05%	0.007%
10	3.434	380	385	390	rBV4	2859	6315	0.89%	0.118%
11	3.507	395	397	400	rVB2	328	350	0.05%	0.007%
12	3.556	403	405	407	rBV2	495	403	0.06%	0.008%
13	3.611	407	414	419	rBV2	1373	3081	0.43%	0.058%
14	3.879	455	458	459	rBV3	320	333	0.05%	0.006%
15	4.038	482	484	486	rVB2	486	398	0.06%	0.007%
16	4.074	486	490	492	rBV2	352	560	0.08%	0.011%
17	4.202	507	511	513	rBV2	641	754	0.11%	0.014%
18	4.294	523	526	530	rVV2	423	535	0.08%	0.010%
19	4.397	542	543	545	rBV	442	351	0.05%	0.007%
20	4.458	545	553	572	rVV	40886	121451	17.11%	2.277%
21	5.050	639	650	670	rBV	89869	288687	40.66%	5.413%
22	5.385	695	705	715	rVB5	8981	26769	3.77%	0.502%
23	5.464	715	718	721	rVB4	471	590	0.08%	0.011%
24	5.519	725	727	732	rVB	566	444	0.06%	0.008%
25	5.556	732	733	735	rBV	694	424	0.06%	0.008%
26	5.659	747	750	751	rBV2	310	358	0.05%	0.007%
27	5.781	769	770	775	rVB2	630	667	0.09%	0.013%
28	5.964	787	800	820	rBV2	232255	709935	100.00%	13.312%
29	6.300	853	855	856	rVB2	654	389	0.05%	0.007%
30	6.379	865	868	870	rVB2	563	648	0.09%	0.012%
31	6.696	917	920	922	rBV3	461	415	0.06%	0.008%
32	6.757	922	930	947	rBV	190715	476807	67.16%	8.941%
33	7.049	976	978	979	rVB2	696	400	0.06%	0.008%
34	7.086	981	984	985	rBV2	452	409	0.06%	0.008%
35	7.110	986	988	990	rVV3	601	424	0.06%	0.008%
36	7.190	999	1001	1005	rVB4	339	469	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043764.D
Acq On : 08 Nov 2024 15:12
Operator : JC/MD
Sample : P4742-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1H14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Title : VOC Analysis

37	7.220	1005	1006	1010	rVB2	438	436	0.06%	0.008%
38	7.305	1010	1020	1038	rBV	141590	324465	45.70%	6.084%
39	7.562	1060	1062	1065	rVB2	358	386	0.05%	0.007%
40	7.879	1112	1114	1117	rVB2	574	414	0.06%	0.008%
41	7.952	1121	1126	1127	rBV2	334	419	0.06%	0.008%
42	7.994	1131	1133	1137	rBV2	433	454	0.06%	0.009%
43	8.061	1143	1144	1147	rVB	507	422	0.06%	0.008%
44	8.086	1147	1148	1153	rBV2	456	504	0.07%	0.009%
45	8.177	1161	1163	1167	rVB3	465	531	0.07%	0.010%
46	8.214	1167	1169	1173	rBV	312	506	0.07%	0.009%
47	8.324	1181	1187	1199	rBV	84778	147057	20.71%	2.757%
48	8.647	1233	1240	1250	rBV	353415	570731	80.39%	10.702%
49	8.952	1284	1290	1300	rBV	59052	93189	13.13%	1.747%
50	9.122	1316	1318	1321	rVB2	614	435	0.06%	0.008%
51	9.183	1326	1328	1330	rBV2	458	390	0.05%	0.007%
52	9.269	1338	1342	1346	rBV3	1946	3017	0.42%	0.057%
53	9.384	1356	1361	1377	rBV	173452	272893	38.44%	5.117%
54	9.665	1403	1407	1408	rBV3	435	622	0.09%	0.012%
55	9.787	1425	1427	1430	rBV2	441	449	0.06%	0.008%
56	9.872	1437	1441	1442	rBV2	283	406	0.06%	0.008%
57	9.915	1446	1448	1450	rBV2	618	490	0.07%	0.009%
58	10.055	1465	1471	1484	rVV	388989	570874	80.41%	10.704%
59	10.195	1492	1494	1497	rVB4	689	703	0.10%	0.013%
60	10.299	1509	1511	1518	rVV3	703	1173	0.17%	0.022%
61	10.433	1531	1533	1535	rVB	629	463	0.07%	0.009%
62	10.646	1565	1568	1574	rVB3	751	1187	0.17%	0.022%
63	10.695	1574	1576	1579	rBV2	263	406	0.06%	0.008%
64	10.793	1591	1592	1595	rBV	404	400	0.06%	0.008%
65	10.908	1609	1611	1613	rBV	425	459	0.06%	0.009%
66	11.043	1630	1633	1634	rBV3	338	374	0.05%	0.007%
67	11.097	1641	1642	1644	rVB	644	377	0.05%	0.007%
68	11.152	1644	1651	1652	rBV2	546	981	0.14%	0.018%
69	11.189	1652	1657	1667	rVV	250516	320085	45.09%	6.002%
70	11.274	1669	1671	1672	rVV	603	403	0.06%	0.008%
71	11.311	1674	1677	1683	rVB3	2273	3051	0.43%	0.057%
72	11.408	1689	1693	1696	rVB2	312	448	0.06%	0.008%
73	11.555	1713	1717	1719	rVB3	453	559	0.08%	0.010%
74	11.579	1719	1721	1726	rBV	399	611	0.09%	0.011%
75	11.671	1733	1736	1738	rBV2	384	348	0.05%	0.007%
76	11.817	1759	1760	1763	rBV	406	391	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
 Data File : VX043764.D
 Acq On : 08 Nov 2024 15:12
 Operator : JC/MD
 Sample : P4742-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1H14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

77	11.969	1784	1785	1788	rBV2	376	406	0.06%	0.008%
78	12.018	1788	1793	1804	rBV	368561	481532	67.83%	9.029%
79	12.225	1824	1827	1829	rBV2	1461	1491	0.21%	0.028%
80	12.317	1837	1842	1854	rBV	357636	466756	65.75%	8.752%
81	12.634	1893	1894	1897	rVV2	500	423	0.06%	0.008%
82	13.079	1966	1967	1970	rBV2	405	356	0.05%	0.007%
83	13.195	1983	1986	1988	rBV	533	556	0.08%	0.010%
84	13.213	1988	1989	1995	rVV3	347	520	0.07%	0.010%
85	13.353	2007	2012	2015	rBV2	451	690	0.10%	0.013%
86	13.499	2035	2036	2042	rVB4	481	531	0.07%	0.010%
87	13.682	2063	2066	2067	rVV2	499	472	0.07%	0.009%
88	14.121	2135	2138	2139	rBV2	532	589	0.08%	0.011%
89	14.188	2147	2149	2152	rVB3	530	485	0.07%	0.009%
90	14.225	2152	2155	2157	rBV2	307	386	0.05%	0.007%
91	14.249	2157	2159	2161	rBV2	446	371	0.05%	0.007%
92	14.310	2168	2169	2172	rBV2	577	523	0.07%	0.010%
93	14.353	2172	2176	2178	rBV2	256	352	0.05%	0.007%
94	14.518	2199	2203	2204	rBV4	682	853	0.12%	0.016%
95	14.786	2245	2247	2248	rBV2	519	442	0.06%	0.008%
96	14.993	2279	2281	2283	rBV3	474	351	0.05%	0.007%
97	15.298	2329	2331	2335	rBV3	432	596	0.08%	0.011%
98	15.688	2391	2395	2398	rBV4	536	1057	0.15%	0.020%
99	16.176	2474	2475	2477	rBV	796	697	0.10%	0.013%
100	16.694	2558	2560	2563	rVB2	688	542	0.08%	0.010%




Sum of corrected areas: 5333078

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043764.D
Acq On : 08 Nov 2024 15:12
Operator : JC/MD
Sample : P4742-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1H14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

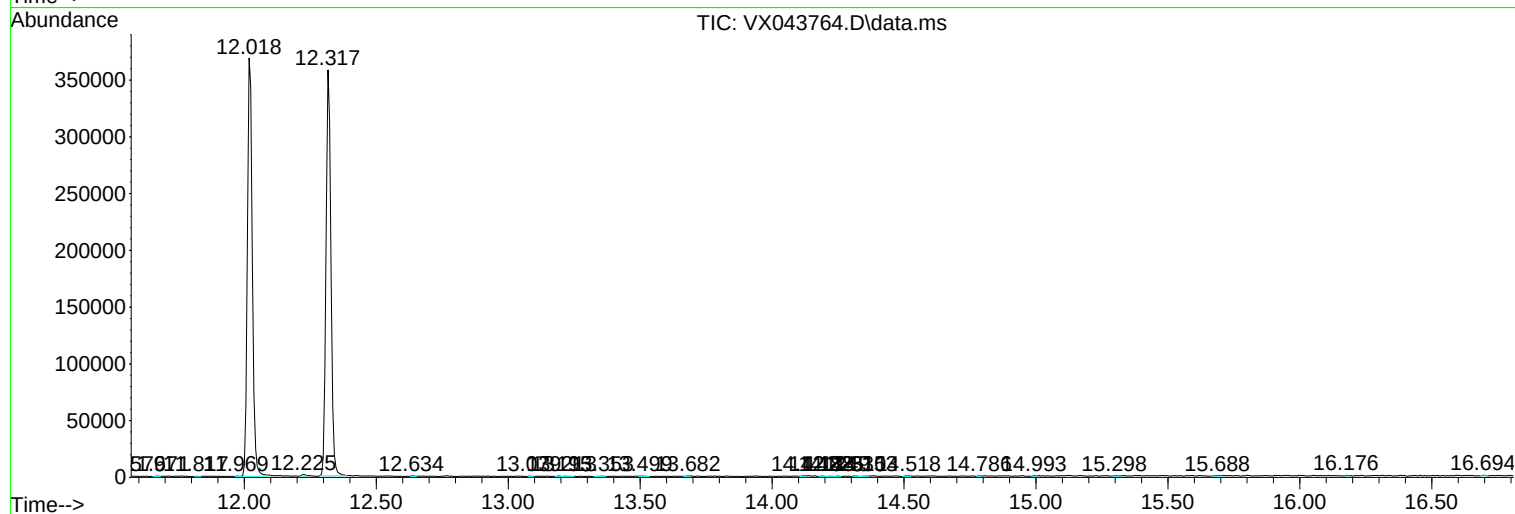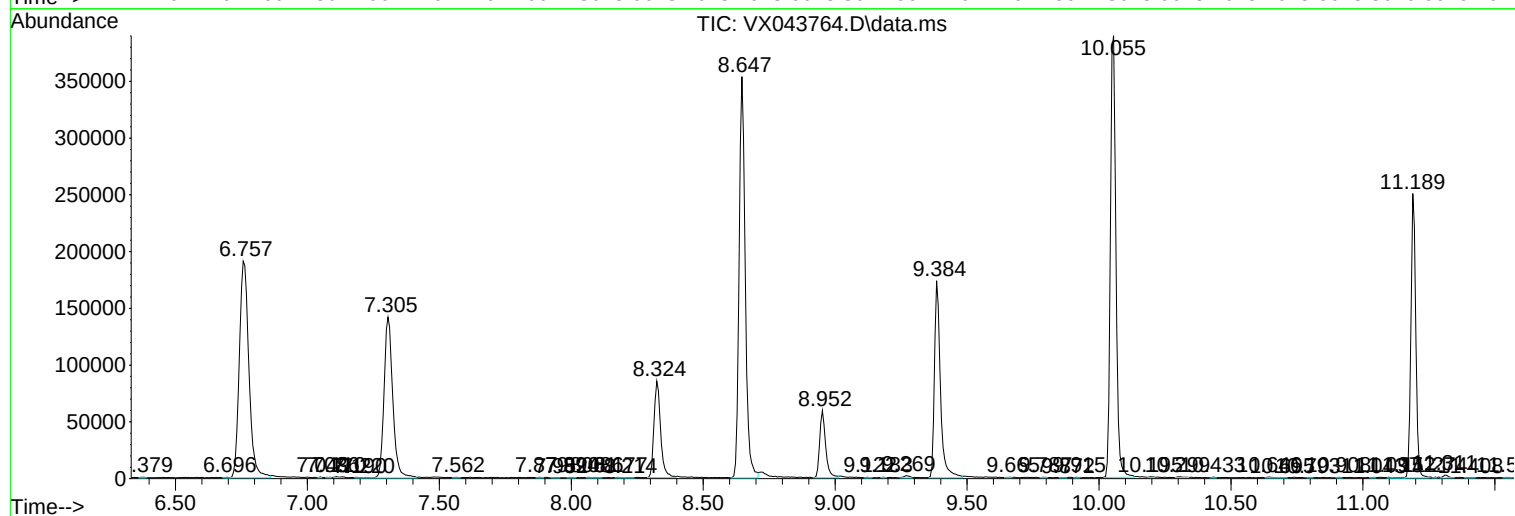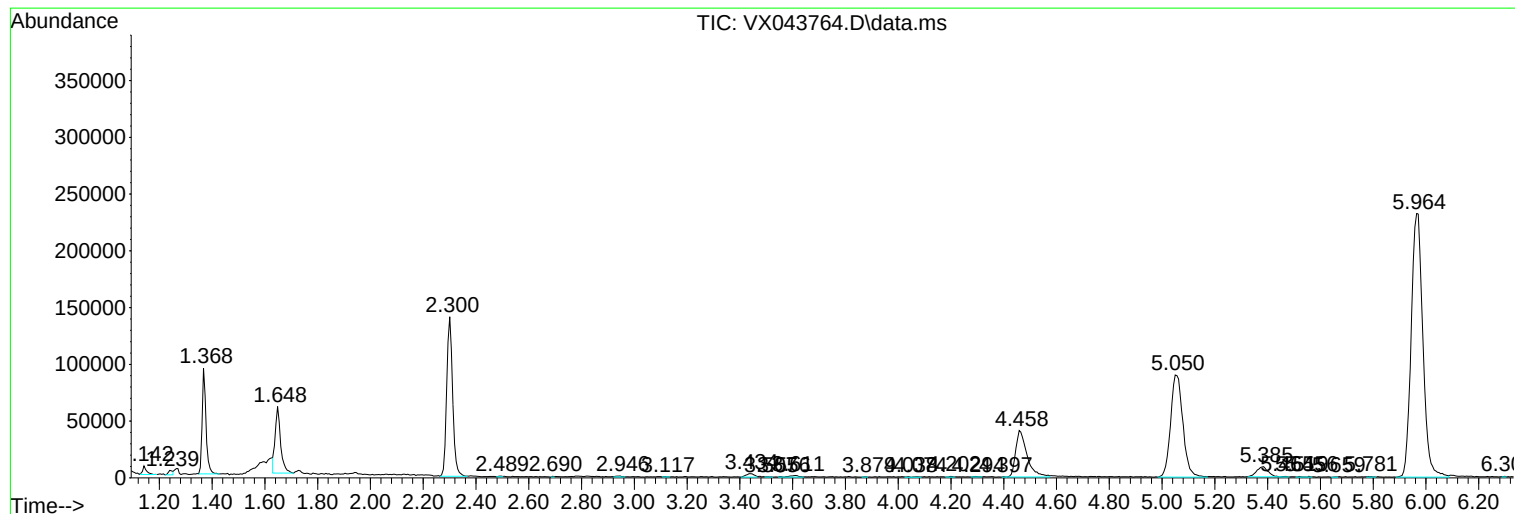

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043764.D
Acq On : 08 Nov 2024 15:12
Operator : JC/MD
Sample : P4742-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1H14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043764.D
Acq On : 08 Nov 2024 15:12
Operator : JC/MD
Sample : P4742-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1H14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------