

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043771.D
Acq On : 08 Nov 2024 17:54
Operator : JC/MD
Sample : P4742-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1H23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M

Title : VOC Analysis

Signal : TIC: VX043771.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	32	rVB4	7274	11197	0.98%	0.126%
2	1.368	42	46	57	rBV	125010	153180	13.39%	1.729%
3	1.642	88	91	102	rVB	76254	107390	9.39%	1.212%
4	2.294	192	198	210	rVB	242363	377077	32.96%	4.256%
5	2.501	230	232	235	rVB3	586	505	0.04%	0.006%
6	2.550	237	240	241	rBV3	999	943	0.08%	0.011%
7	2.660	256	258	259	rBV2	530	373	0.03%	0.004%
8	2.703	263	265	266	rBV	630	472	0.04%	0.005%
9	2.782	275	278	283	rBV4	1060	1490	0.13%	0.017%
10	2.934	298	303	311	rBV2	3208	6997	0.61%	0.079%
11	3.361	371	373	374	rBV2	443	361	0.03%	0.004%
12	3.392	376	378	379	rVV	541	440	0.04%	0.005%
13	3.434	379	385	394	rVV5	5916	14128	1.23%	0.159%
14	3.495	394	395	399	rVB	371	381	0.03%	0.004%
15	3.599	407	412	413	rBV	760	1033	0.09%	0.012%
16	3.782	439	442	444	rBV2	281	440	0.04%	0.005%
17	3.831	448	450	453	rBV2	277	408	0.04%	0.005%
18	3.946	467	469	471	rVB	505	362	0.03%	0.004%
19	3.965	471	472	475	rBV2	480	398	0.03%	0.004%
20	4.056	485	487	491	rVB2	490	588	0.05%	0.007%
21	4.087	491	492	495	rBV2	360	356	0.03%	0.004%
22	4.148	499	502	505	rVB2	425	606	0.05%	0.007%
23	4.251	517	519	522	rBV2	460	461	0.04%	0.005%
24	4.282	522	524	528	rVB2	508	568	0.05%	0.006%
25	4.465	545	554	571	rBV	68399	224918	19.66%	2.539%
26	4.751	599	601	603	rBV2	501	572	0.05%	0.006%
27	4.812	607	611	612	rVB3	459	558	0.05%	0.006%
28	5.056	638	651	666	rBV	149032	451020	39.42%	5.090%
29	5.330	694	696	697	rVV	874	715	0.06%	0.008%
30	5.379	697	704	711	rVV2	5601	16134	1.41%	0.182%
31	5.727	758	761	765	rBV2	496	438	0.04%	0.005%
32	5.964	788	800	817	rBV2	386123	1144165	100.00%	12.914%
33	6.251	845	847	848	rBV	361	319	0.03%	0.004%
34	6.391	868	870	872	rVB2	311	314	0.03%	0.004%
35	6.440	875	878	880	rBV2	520	549	0.05%	0.006%
36	6.623	905	908	909	rBV2	396	360	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
 Data File : VX043771.D
 Acq On : 08 Nov 2024 17:54
 Operator : JC/MD
 Sample : P4742-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1H23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	6.635	909	910	912	rVB2	603	378	0.03%	0.004%
38	6.757	921	930	945	rBV	331445	808141	70.63%	9.121%
39	7.123	982	990	1004	rBV2	45979	109136	9.54%	1.232%
40	7.306	1011	1020	1037	rBV	221207	507328	44.34%	5.726%
41	7.775	1096	1097	1100	rVB2	424	332	0.03%	0.004%
42	7.805	1100	1102	1104	rBV3	456	450	0.04%	0.005%
43	7.946	1123	1125	1127	rBV2	452	347	0.03%	0.004%
44	8.049	1140	1142	1144	rVV2	415	397	0.03%	0.004%
45	8.074	1144	1146	1148	rVV	392	321	0.03%	0.004%
46	8.092	1148	1149	1153	rVB2	510	497	0.04%	0.006%
47	8.183	1160	1164	1168	rBV2	292	685	0.06%	0.008%
48	8.324	1181	1187	1197	rBV	144402	241370	21.10%	2.724%
49	8.647	1234	1240	1260	rBV	589440	939122	82.08%	10.599%
50	8.952	1285	1290	1300	rBV	93890	151788	13.27%	1.713%
51	9.134	1318	1320	1323	rBV3	438	527	0.05%	0.006%
52	9.214	1330	1333	1335	rVB3	434	408	0.04%	0.005%
53	9.275	1339	1343	1347	rVB3	2904	4702	0.41%	0.053%
54	9.384	1356	1361	1382	rBV	312018	487306	42.59%	5.500%
55	9.829	1429	1434	1436	rBV2	630	667	0.06%	0.008%
56	9.854	1436	1438	1440	rBV2	462	393	0.03%	0.004%
57	9.970	1454	1457	1460	rBV3	328	555	0.05%	0.006%
58	10.055	1465	1471	1488	rVV	644119	934841	81.71%	10.551%
59	10.518	1545	1547	1550	rVB2	345	463	0.04%	0.005%
60	10.622	1562	1564	1567	rVB	363	327	0.03%	0.004%
61	10.659	1569	1570	1572	rVV	502	309	0.03%	0.003%
62	10.707	1575	1578	1579	rBV2	358	342	0.03%	0.004%
63	10.762	1584	1587	1588	rVB2	475	415	0.04%	0.005%
64	10.823	1594	1597	1598	rBV2	451	512	0.04%	0.006%
65	10.860	1600	1603	1607	rBV2	503	845	0.07%	0.010%
66	11.189	1652	1657	1667	rVV	442256	550446	48.11%	6.213%
67	11.311	1673	1677	1682	rVB6	2920	4217	0.37%	0.048%
68	11.384	1688	1689	1694	rVB3	449	429	0.04%	0.005%
69	11.536	1712	1714	1718	rBV3	440	471	0.04%	0.005%
70	11.878	1768	1770	1774	rBV2	487	505	0.04%	0.006%
71	12.018	1788	1793	1806	rVV	618736	810984	70.88%	9.153%
72	12.317	1837	1842	1854	rBV	592811	763740	66.75%	8.620%
73	12.555	1879	1881	1886	rBV2	571	1078	0.09%	0.012%
74	12.750	1910	1913	1919	rVB2	836	1628	0.14%	0.018%
75	12.896	1935	1937	1939	rVB	434	402	0.04%	0.005%
76	13.018	1956	1957	1960	rVB	654	364	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
 Data File : VX043771.D
 Acq On : 08 Nov 2024 17:54
 Operator : JC/MD
 Sample : P4742-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1H23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

77	13.079	1965	1967	1971	rBV2	377	487	0.04%	0.005%
78	13.140	1974	1977	1978	rBV2	356	320	0.03%	0.004%
79	13.402	2018	2020	2023	rVV3	471	519	0.05%	0.006%
80	13.493	2033	2035	2038	rVB	373	409	0.04%	0.005%
81	13.536	2040	2042	2045	rBV3	452	457	0.04%	0.005%
82	13.573	2045	2048	2050	rBV2	312	431	0.04%	0.005%
83	13.713	2068	2071	2072	rBV2	475	411	0.04%	0.005%
84	13.731	2072	2074	2082	rBV2	325	759	0.07%	0.009%
85	13.835	2087	2091	2092	rBV2	484	516	0.05%	0.006%
86	13.890	2098	2100	2103	rBV3	318	407	0.04%	0.005%
87	13.938	2106	2108	2110	rVV3	478	479	0.04%	0.005%
88	13.963	2110	2112	2114	rVV2	462	471	0.04%	0.005%
89	13.999	2116	2118	2120	rVB	465	376	0.03%	0.004%
90	14.079	2129	2131	2133	rBV3	410	398	0.03%	0.004%
91	14.127	2135	2139	2141	rBV4	778	945	0.08%	0.011%
92	14.213	2152	2153	2158	rVB3	379	359	0.03%	0.004%
93	14.603	2216	2217	2220	rBV2	344	317	0.03%	0.004%
94	14.749	2239	2241	2244	rVB4	445	444	0.04%	0.005%
95	14.774	2244	2245	2249	rBV2	577	468	0.04%	0.005%
96	14.871	2257	2261	2262	rBV3	493	525	0.05%	0.006%
97	15.024	2284	2286	2288	rBV2	514	453	0.04%	0.005%
98	16.145	2468	2470	2471	rBV2	647	469	0.04%	0.005%
99	16.249	2485	2487	2492	rBV4	621	1115	0.10%	0.013%
100	16.493	2523	2527	2530	rBV4	727	1249	0.11%	0.014%




Sum of corrected areas: 8860168

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043771.D
Acq On : 08 Nov 2024 17:54
Operator : JC/MD
Sample : P4742-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1H23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

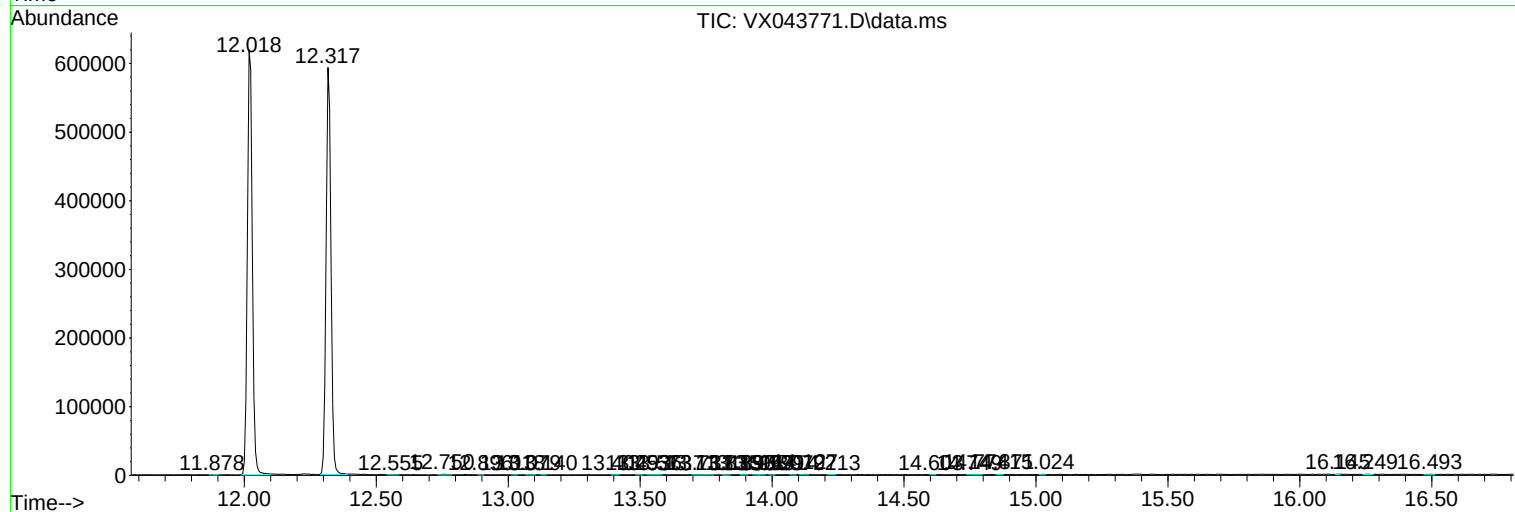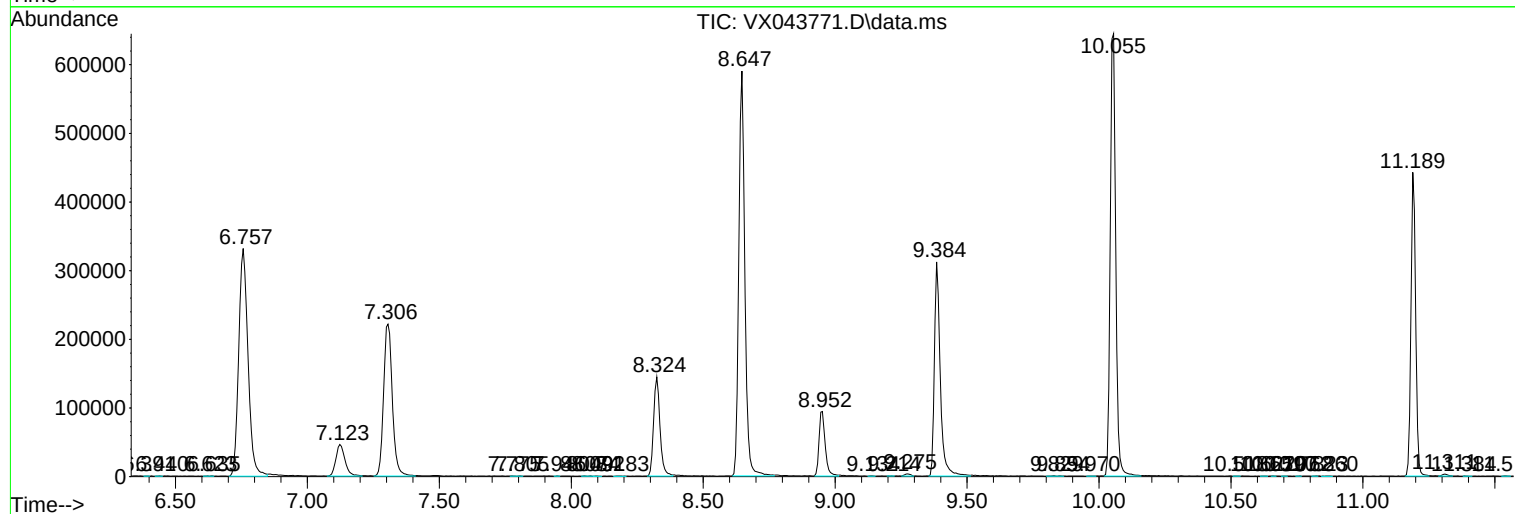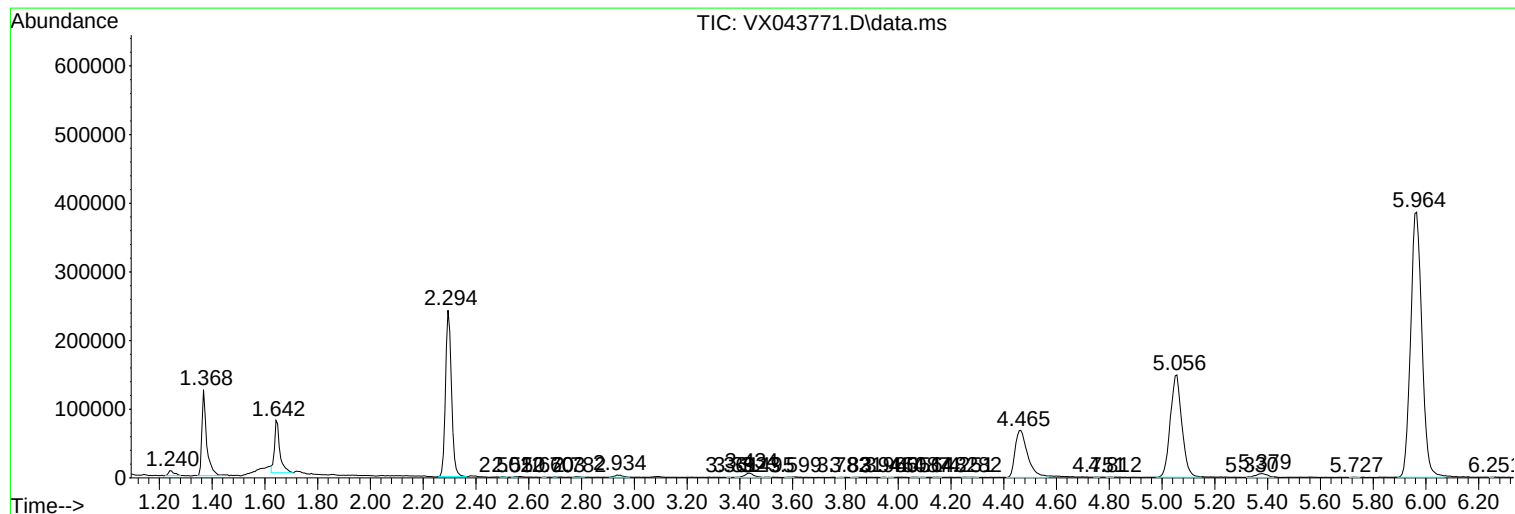

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043771.D
Acq On : 08 Nov 2024 17:54
Operator : JC/MD
Sample : P4742-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1H23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043771.D
Acq On : 08 Nov 2024 17:54
Operator : JC/MD
Sample : P4742-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1H23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------