
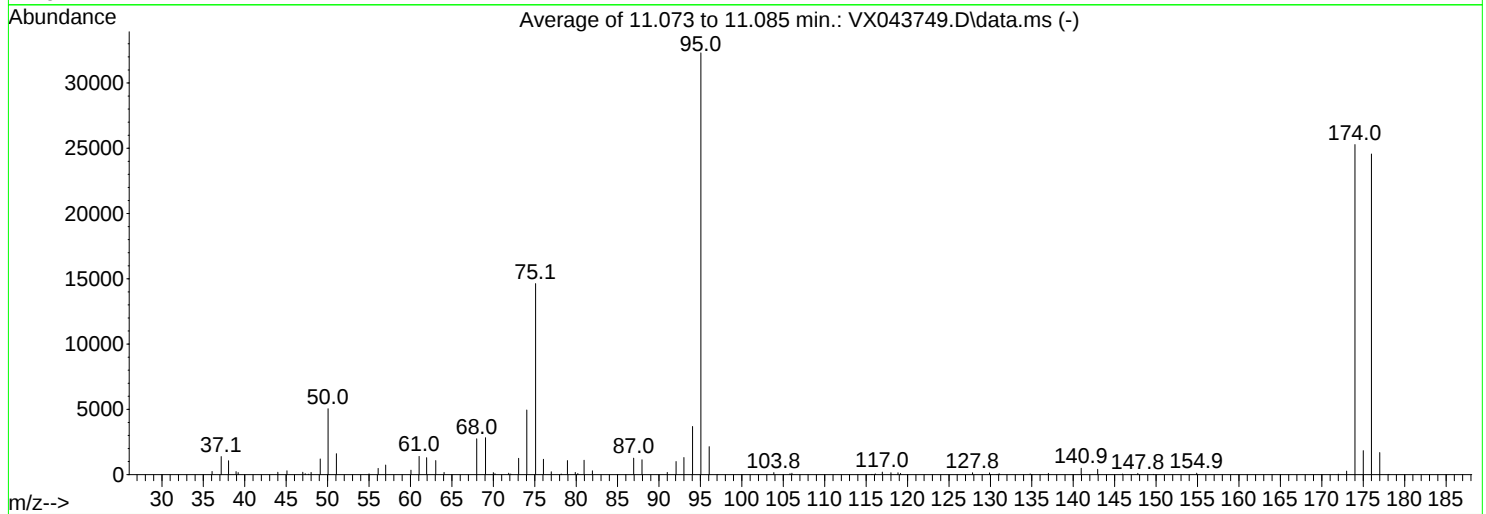


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110824\
Data File : VX043749.D
Acq On : 08 Nov 2024 08:17
Operator : JC/MD
Sample : BFB695
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB695

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Title : VOC Analysis
Last Update : Fri Nov 08 23:56:14 2024

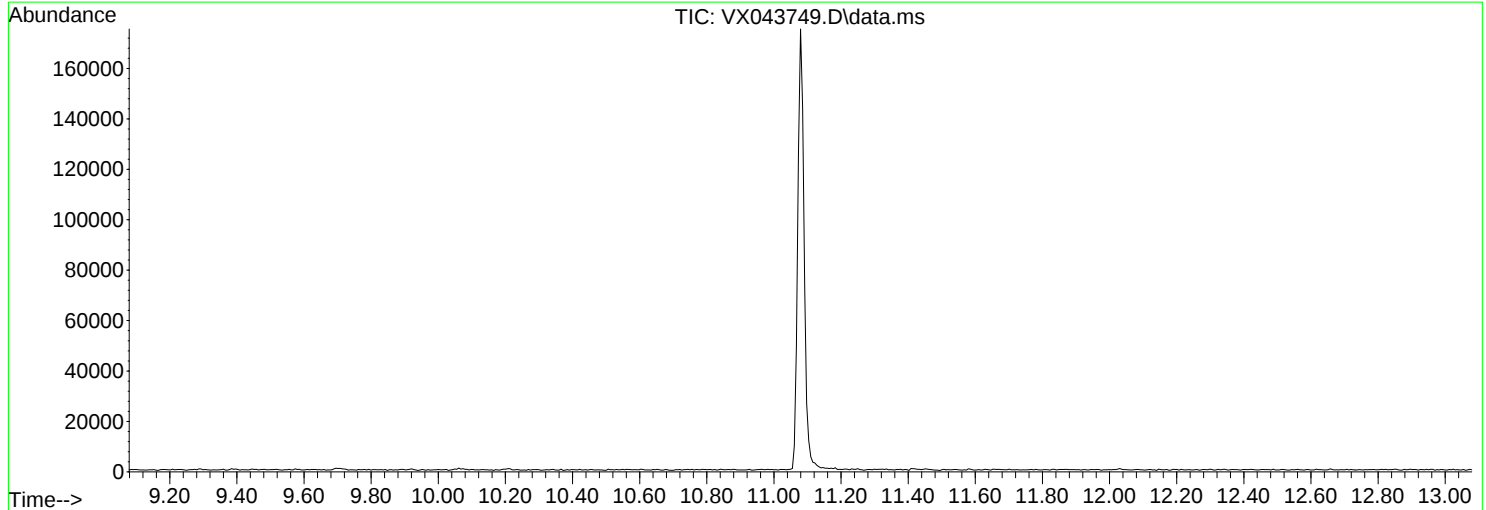

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.6	5050	PASS
75	95	30	80	45.3	14636	PASS
95	95	100	100	100.0	32309	PASS
96	95	5	9	6.6	2142	PASS
173	174	0.00	2	1.1	277	PASS
174	95	50	120	78.3	25288	PASS
175	174	5	9	7.3	1837	PASS
176	174	95	101	97.1	24557	PASS
177	176	5	9	6.9	1695	PASS

m/z	Abundance
38.90	82.0
40.00	549.0
44.10	302.0

Instrument :
MSVOA_X
ClientSampleId :
BFB695

m/z	Abundance
36.10	199.0
37.10	1532.0
38.10	1086.0
39.00	348.0
40.00	555.0
44.00	488.0
45.10	360.0
47.10	213.0
47.70	96.0
49.10	1207.0
50.00	5011.0
51.00	1537.0
55.00	73.0
56.10	571.0
57.00	742.0
60.10	289.0
61.00	1253.0
61.90	1192.0
63.00	1164.0
64.10	171.0
68.00	2495.0
69.10	2775.0
70.00	211.0
71.80	169.0
73.00	1139.0
74.10	4690.0
75.10	13435.0
76.10	1090.0
77.00	171.0
78.20	83.0
79.00	833.0
79.90	224.0
80.90	1074.0
81.90	278.0
86.00	57.0
87.00	1186.0
88.00	982.0
90.90	252.0
92.00	824.0
93.00	1194.0
94.10	3134.0
95.00	28456.0
96.10	2097.0
103.80	140.0
106.10	105.0
117.00	163.0
118.00	147.0
119.10	154.0
127.80	79.0
129.90	93.0
130.80	82.0
134.80	78.0
137.20	79.0
140.90	428.0
143.00	411.0
147.70	92.0
173.00	139.0
174.00	19096.0
175.00	1142.0
176.00	18216.0
177.00	1186.0

Instrument :
MSVOA_X
ClientSampleId :
BFB695

m/z	Abundance
36.00	358.0
37.20	1517.0
38.10	1112.0
39.20	482.0
40.00	375.0
44.00	436.0
45.10	324.0
47.00	236.0
48.00	294.0
49.10	1375.0
50.10	6057.0
51.00	1823.0
55.00	113.0
56.10	574.0
57.10	843.0
60.00	505.0
61.10	1777.0
62.00	1539.0
63.10	1111.0
64.00	214.0
68.00	3513.0
69.00	3140.0
70.00	276.0
71.90	170.0
73.00	1577.0
74.00	5774.0
75.10	17200.0
76.00	1313.0
76.90	336.0
78.90	1340.0
80.20	253.0
81.00	1342.0
81.90	372.0
87.00	1411.0
87.90	1299.0
91.00	155.0
92.10	1285.0
93.00	1551.0
94.10	4803.0
95.10	38096.0
96.10	2375.0
103.80	146.0
105.80	212.0
116.10	177.0
117.00	215.0
117.90	165.0
118.80	149.0
119.20	143.0
127.90	209.0
129.90	162.0
131.00	110.0
134.80	119.0
137.00	152.0
141.00	529.0
143.00	490.0
145.90	79.0
147.80	112.0
154.90	77.0
172.00	61.0
173.00	286.0
174.00	30248.0
175.00	2286.0
176.00	28728.0
177.00	2127.0

Instrument :
MSVOA_X
ClientSampleId :
BFB695

m/z	Abundance
36.00	193.0
37.10	1111.0
38.00	999.0
39.00	597.0
40.00	498.0
44.00	532.0
45.00	197.0
46.90	121.0
47.30	235.0
48.00	217.0
49.10	1015.0
50.10	4081.0
51.10	1479.0
56.00	308.0
56.90	610.0
60.00	251.0
61.00	1167.0
62.00	1150.0
63.00	962.0
64.10	145.0
68.00	2229.0
69.00	2578.0
70.20	216.0
72.10	163.0
73.10	1032.0
74.00	4398.0
75.10	13274.0
76.10	1113.0
77.10	157.0
78.20	66.0
78.90	1059.0
79.90	293.0
80.90	904.0
82.00	251.0
86.90	1192.0
88.00	1137.0
91.10	100.0
92.10	915.0
93.00	1176.0
94.00	3116.0
95.10	30376.0
96.00	1955.0
97.10	52.0
103.90	206.0
106.00	218.0
115.70	92.0
116.90	206.0
118.10	131.0
118.90	297.0
127.90	166.0
129.90	142.0
131.10	96.0
136.90	63.0
141.00	529.0
142.90	325.0
146.00	58.0
147.90	88.0
149.70	75.0
154.90	256.0
172.00	63.0
173.00	405.0
174.00	26520.0
175.00	2084.0
176.00	26728.0
177.00	1773.0
178.10	60.0

Instrument :
MSVOA_X
ClientSampleId :
BFB695