

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX110918\
Data File : VX005883.D
Acq On : 10 Nov 2018 01:44
Operator : JC/MD
Sample : J5889-06
Misc : 13.07g/5mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WALL-F

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X110718W.M
Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.709	66	91	92	rBV	13624	74962	13.14%	2.195%
2	2.282	177	185	189	rBV	3449	5721	1.00%	0.168%
3	5.501	701	713	727	rBV	67424	200712	35.17%	5.877%
4	5.659	728	739	757	rVB2	132116	375717	65.84%	11.001%
5	6.068	795	806	822	rBV2	76384	210769	36.94%	6.171%
6	6.860	925	936	954	rBV2	169774	432825	75.85%	12.673%
7	8.713	1233	1240	1256	rBV	345389	570648	100.00%	16.709%
8	10.116	1464	1470	1487	rBV	348597	485792	85.13%	14.224%
9	11.140	1633	1638	1653	rVB	301003	384383	67.36%	11.255%
10	12.079	1787	1792	1807	rBV	403038	505471	88.58%	14.800%
11	14.267	2141	2151	2160	rVB	3887	12056	2.11%	0.353%
12	14.371	2160	2168	2176	rBV6	3386	8115	1.42%	0.238%
13	14.786	2227	2236	2248	rVB7	8253	26035	4.56%	0.762%
14	15.060	2274	2281	2287	rBV5	7581	19351	3.39%	0.567%
15	15.139	2290	2294	2301	rVB7	4124	9576	1.68%	0.280%
16	15.255	2303	2313	2320	rBV9	2903	8878	1.56%	0.260%
17	15.359	2322	2330	2334	rBV7	3767	10958	1.92%	0.321%
18	15.493	2342	2352	2353	rBV8	2454	6798	1.19%	0.199%
19	15.548	2355	2361	2370	rVV7	9301	29206	5.12%	0.855%
20	15.694	2373	2385	2387	rVV9	5752	20176	3.54%	0.591%
21	15.724	2387	2390	2400	rVB7	6940	17107	3.00%	0.501%


Sum of corrected areas: 3415256

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX110918\
Data File : VX005883.D
Acq On : 10 Nov 2018 01:44
Operator : JC/MD
Sample : J5889-06
Misc : 13.07g/5mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WALL-F

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X110718W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

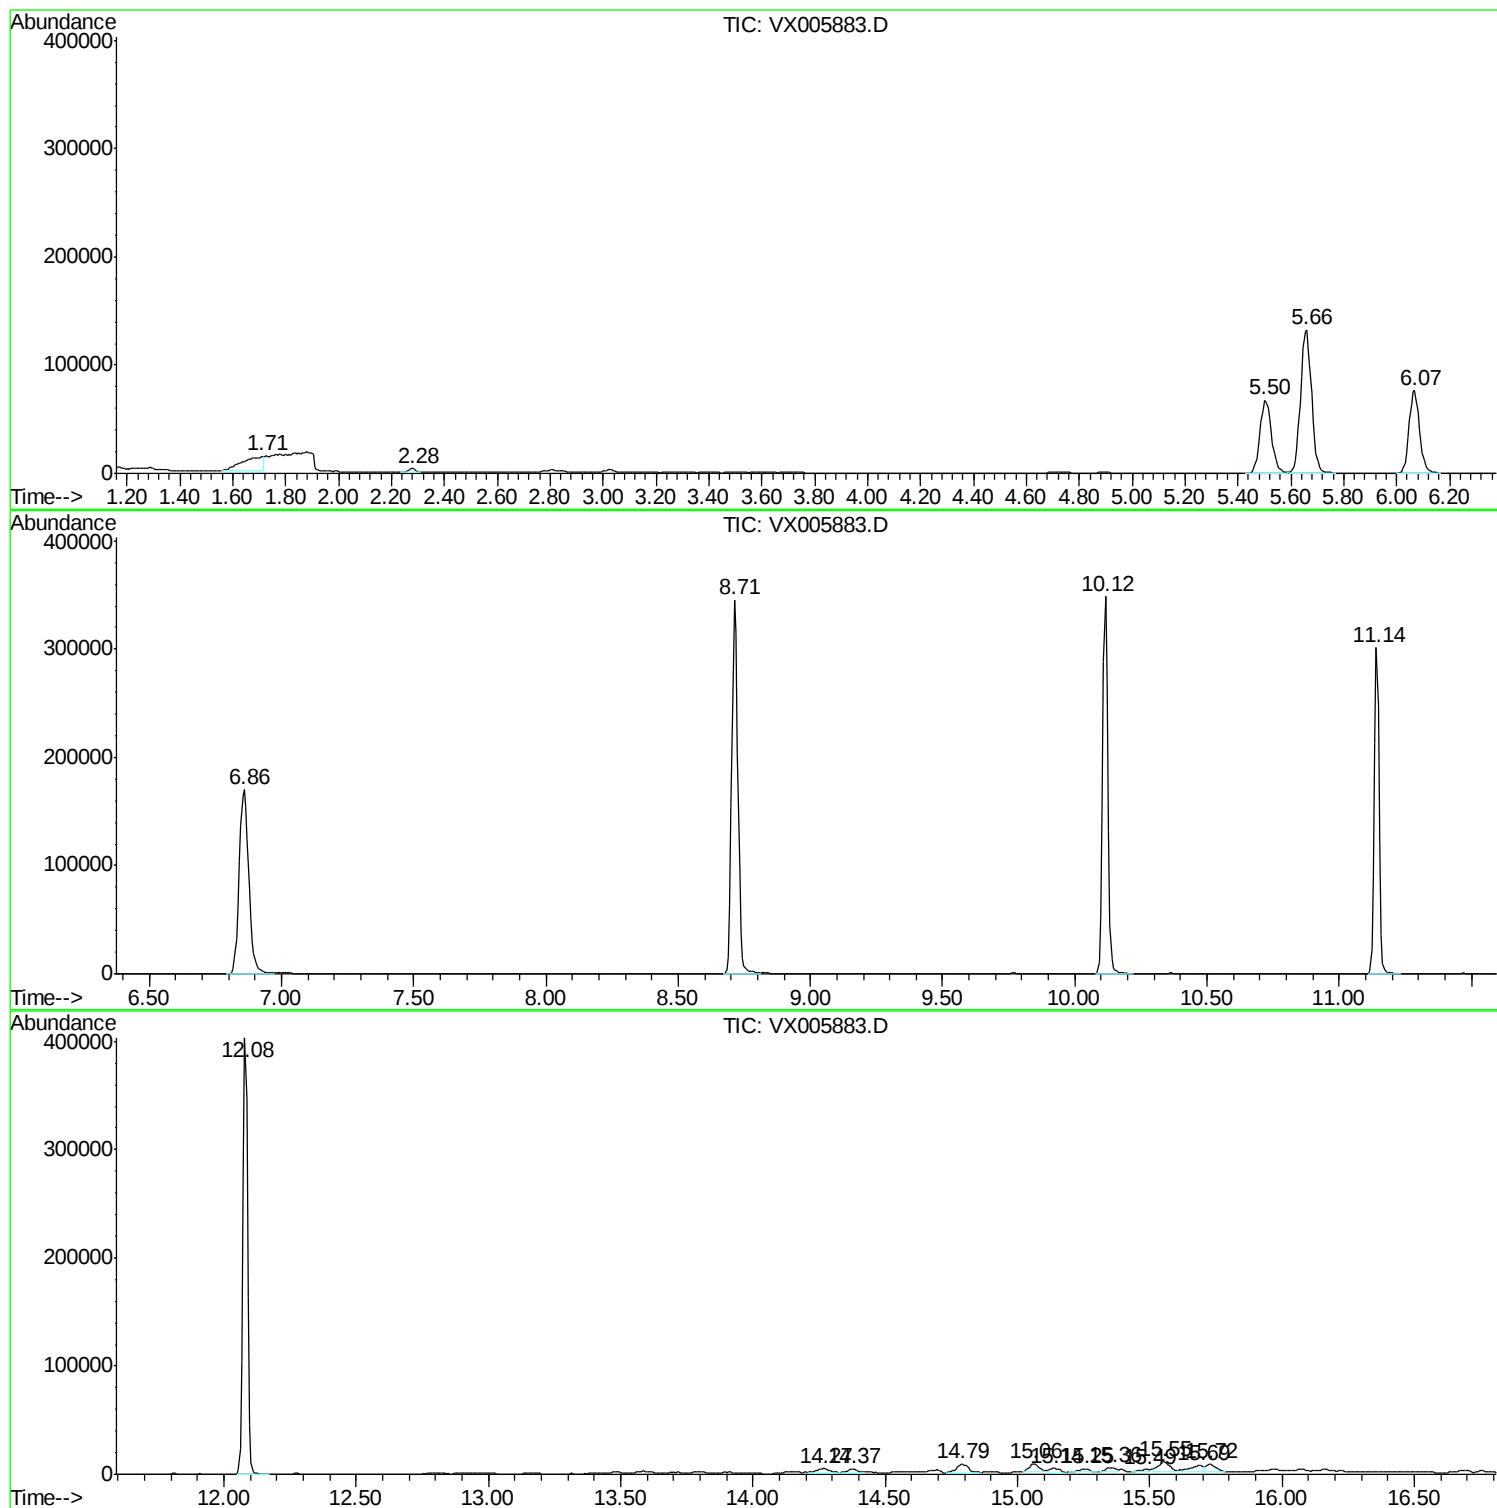

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX110918\
Data File : VX005883.D
Acq On : 10 Nov 2018 01:44
Operator : JC/MD
Sample : J5889-06
Misc : 13.07µL/5mL/100µL/5.0mL/MSVOA_X/MEOH
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WALL-F










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X110718W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown1.71 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.71	9.98 ug/l	74962	Pentafluorobenzene	5.66

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Bis(2-chloroethyl) sulfone	190	C4H8Cl2O2S	000471-03-4	12
2			Methane, chloromethoxy-	80	C2H5ClO	000107-30-2	9
3			2-[2-(2-Chloro-ethoxy)-ethoxy]-p...	216	C10H13ClO3	1000317-46-1	9
4			Ethane, 1-chloro-2-iodo-	190	C2H4ClI	000624-70-4	9
5			1-Bromo-1-chloroethane	142	C2H4BrCl	000593-96-4	9

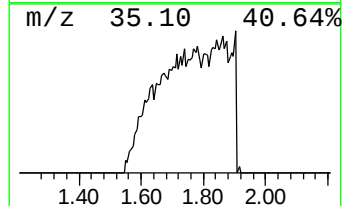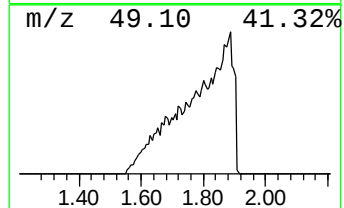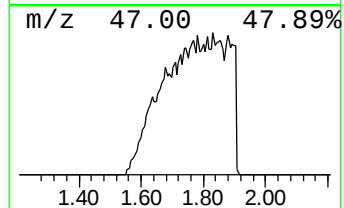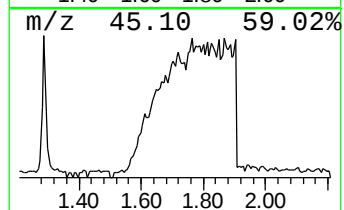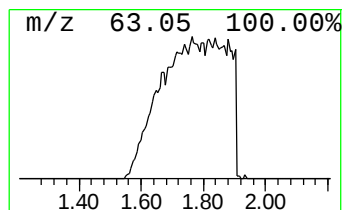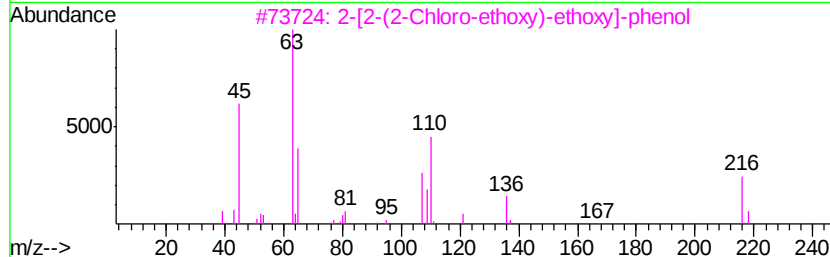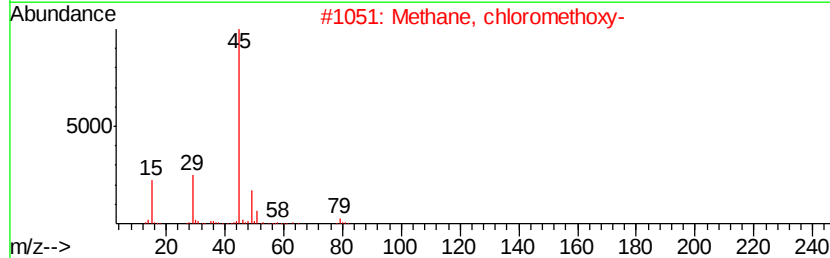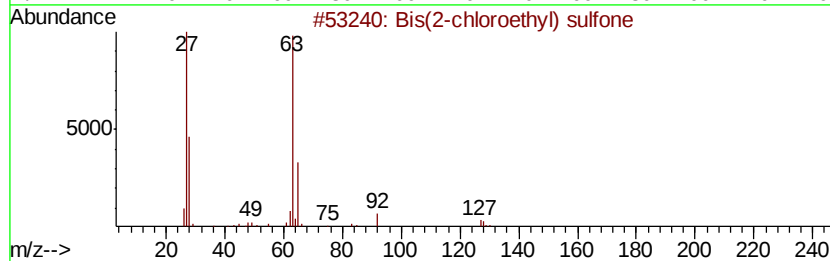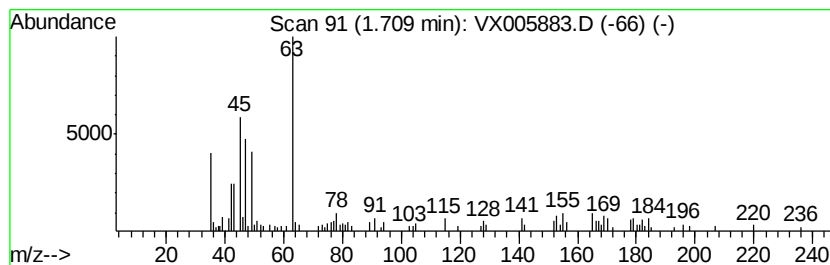

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX110918\
Data File : VX005883.D
Acq On : 10 Nov 2018 01:44
Operator : JC/MD
Sample : J5889-06
Misc : 13.07g/5mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WALL-F

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X110718W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown1.71	1.71	10.0	ug/l	74962	1	5.66	375717	50.0