

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110921\
 Data File : VX025110.D
 Acq On : 09 Nov 2021 10:30
 Operator : JC/MD
 Sample : VX1109MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK633

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110821WMA.M
 Title : VOC Analysis

Signal : TIC: VX025110.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rBV	96455	98121	14.54%	1.945%
2	1.672	92	96	103	rVB	75502	96700	14.33%	1.917%
3	2.306	192	200	216	rBV	148063	246603	36.55%	4.888%
4	2.477	226	228	230	rBV	472	511	0.08%	0.010%
5	2.575	242	244	246	rBV2	664	496	0.07%	0.010%
6	2.776	274	277	279	rBV3	715	969	0.14%	0.019%
7	2.861	290	291	294	rBV	394	350	0.05%	0.007%
8	2.934	301	303	306	rBV2	526	371	0.05%	0.007%
9	3.062	322	324	325	rBV2	485	351	0.05%	0.007%
10	3.178	339	343	344	rBV	450	425	0.06%	0.008%
11	3.416	377	382	385	rBB	571	897	0.13%	0.018%
12	3.550	402	404	406	rBV2	598	487	0.07%	0.010%
13	3.611	411	414	416	rBV2	220	285	0.04%	0.006%
14	3.636	416	418	421	rVV	392	294	0.04%	0.006%
15	3.690	424	427	428	rVV	323	363	0.05%	0.007%
16	3.715	428	431	432	rVV2	348	353	0.05%	0.007%
17	4.154	501	503	506	rVB2	328	285	0.04%	0.006%
18	4.184	506	508	511	rBV2	535	538	0.08%	0.011%
19	4.263	518	521	522	rBV2	363	334	0.05%	0.007%
20	4.459	545	553	570	rBV	53249	155891	23.11%	3.090%
21	4.678	588	589	592	rBV2	301	321	0.05%	0.006%
22	4.806	607	610	613	rBV2	485	603	0.09%	0.012%
23	4.922	626	629	633	rBV2	360	603	0.09%	0.012%
24	5.062	640	652	667	rVB2	92893	291369	43.19%	5.776%
25	5.208	674	676	678	rBV2	426	420	0.06%	0.008%
26	5.300	689	691	693	rBV2	294	299	0.04%	0.006%
27	5.678	751	753	755	rBV	329	369	0.05%	0.007%
28	5.970	789	801	813	rBV4	223995	674621	100.00%	13.373%
29	6.190	835	837	842	rVB	682	622	0.09%	0.012%
30	6.233	842	844	846	rBV	403	418	0.06%	0.008%
31	6.300	854	855	857	rBV	403	259	0.04%	0.005%
32	6.598	901	904	905	rBV2	354	321	0.05%	0.006%
33	6.763	922	931	943	rVV	164609	394539	58.48%	7.821%
34	6.940	958	960	962	rVB	793	537	0.08%	0.011%
35	6.982	965	967	969	rBV	375	306	0.05%	0.006%
36	7.031	973	975	979	rBV	357	419	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110921\
 Data File : VX025110.D
 Acq On : 09 Nov 2021 10:30
 Operator : JC/MD
 Sample : VX1109MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK633

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110821WMA.M
 Title : VOC Analysis

37	7.245	1006	1010	1011	rBV	332	320	0.05%	0.006%
38	7.312	1012	1021	1033	rVB	142446	312053	46.26%	6.186%
39	7.434	1040	1041	1045	rBV	422	260	0.04%	0.005%
40	7.476	1045	1048	1054	rVB2	755	1438	0.21%	0.029%
41	7.604	1067	1069	1070	rBV	511	360	0.05%	0.007%
42	7.854	1108	1110	1112	rVB	293	263	0.04%	0.005%
43	7.885	1112	1115	1117	rVB	358	388	0.06%	0.008%
44	7.909	1117	1119	1121	rBV	768	797	0.12%	0.016%
45	8.055	1139	1143	1145	rBV3	563	721	0.11%	0.014%
46	8.147	1152	1158	1161	rBV2	434	739	0.11%	0.015%
47	8.330	1179	1188	1198	rBV	99249	167520	24.83%	3.321%
48	8.653	1234	1241	1248	rBV	322762	513115	76.06%	10.172%
49	8.811	1266	1267	1269	rVB	565	256	0.04%	0.005%
50	8.952	1285	1290	1298	rBV	78376	114358	16.95%	2.267%
51	9.049	1305	1306	1310	rVB	653	506	0.08%	0.010%
52	9.311	1347	1349	1351	rVB	461	329	0.05%	0.007%
53	9.384	1356	1361	1375	rVV	243432	346958	51.43%	6.878%
54	9.598	1393	1396	1400	rBV2	547	565	0.08%	0.011%
55	9.744	1419	1420	1425	rVB2	512	568	0.08%	0.011%
56	9.787	1425	1427	1429	rBV	387	430	0.06%	0.009%
57	9.854	1435	1438	1439	rBV2	426	419	0.06%	0.008%
58	9.945	1452	1453	1457	rVB2	407	310	0.05%	0.006%
59	9.982	1457	1459	1460	rBV	301	284	0.04%	0.006%
60	10.055	1465	1471	1479	rBV	352903	467544	69.30%	9.268%
61	10.195	1491	1494	1496	rBV2	627	668	0.10%	0.013%
62	10.549	1547	1552	1553	rBV	491	502	0.07%	0.010%
63	10.604	1559	1561	1565	rBV3	366	414	0.06%	0.008%
64	10.951	1614	1618	1619	rBV2	564	742	0.11%	0.015%
65	11.122	1639	1646	1650	rBV3	2648	4685	0.69%	0.093%
66	11.195	1652	1658	1667	rVB	242512	305422	45.27%	6.054%
67	11.366	1684	1686	1687	rBV	308	270	0.04%	0.005%
68	11.512	1708	1710	1713	rBV	608	606	0.09%	0.012%
69	11.652	1732	1733	1736	rBV	411	397	0.06%	0.008%
70	11.750	1745	1749	1754	rBV2	2798	3413	0.51%	0.068%
71	11.823	1759	1761	1762	rBV	419	257	0.04%	0.005%
72	11.933	1776	1779	1783	rBV3	1061	1110	0.16%	0.022%
73	12.024	1789	1794	1802	rBV	323914	396637	58.79%	7.863%
74	12.323	1834	1843	1849	rBV	313213	413874	61.35%	8.204%
75	12.549	1878	1880	1882	rBV	354	373	0.06%	0.007%
76	12.731	1908	1910	1913	rVB	388	277	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110921\
 Data File : VX025110.D
 Acq On : 09 Nov 2021 10:30
 Operator : JC/MD
 Sample : VX1109MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK633

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110821WMA.M
 Title : VOC Analysis

77	12.914	1936	1940	1945	rVB2	593	654	0.10%	0.013%
78	12.957	1945	1947	1948	rBV2	359	262	0.04%	0.005%
79	13.018	1955	1957	1960	rBV	318	319	0.05%	0.006%
80	13.055	1960	1963	1965	rBV	615	559	0.08%	0.011%
81	13.116	1971	1973	1977	rBV2	1296	1150	0.17%	0.023%
82	13.280	1997	2000	2002	rVB	543	624	0.09%	0.012%
83	13.402	2018	2020	2022	rBV	303	332	0.05%	0.007%
84	13.475	2029	2032	2034	rBV	307	287	0.04%	0.006%
85	13.554	2043	2045	2048	rBV	396	657	0.10%	0.013%
86	13.756	2076	2078	2080	rBV	385	410	0.06%	0.008%
87	13.963	2108	2112	2119	rVB4	1512	2252	0.33%	0.045%
88	14.140	2139	2141	2143	rBV2	503	415	0.06%	0.008%
89	14.237	2155	2157	2158	rBV2	360	303	0.04%	0.006%
90	14.487	2197	2198	2200	rBV	452	320	0.05%	0.006%
91	14.518	2202	2203	2207	rBV	619	727	0.11%	0.014%
92	14.603	2215	2217	2218	rBV	498	315	0.05%	0.006%
93	14.963	2274	2276	2277	rBV	616	462	0.07%	0.009%
94	15.219	2316	2318	2320	rBV	362	271	0.04%	0.005%
95	15.286	2327	2329	2334	rBV2	513	876	0.13%	0.017%
96	15.743	2400	2404	2405	rBV	732	900	0.13%	0.018%
97	16.005	2444	2447	2449	rBV	489	599	0.09%	0.012%
98	16.280	2490	2492	2493	rBV	373	245	0.04%	0.005%
99	16.505	2527	2529	2532	rBV	385	369	0.05%	0.007%
100	16.566	2536	2539	2541	rBV	419	520	0.08%	0.010%


Sum of corrected areas: 5044626

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110921\
Data File : VX025110.D
Acq On : 09 Nov 2021 10:30
Operator : JC/MD
Sample : VX1109MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK633

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

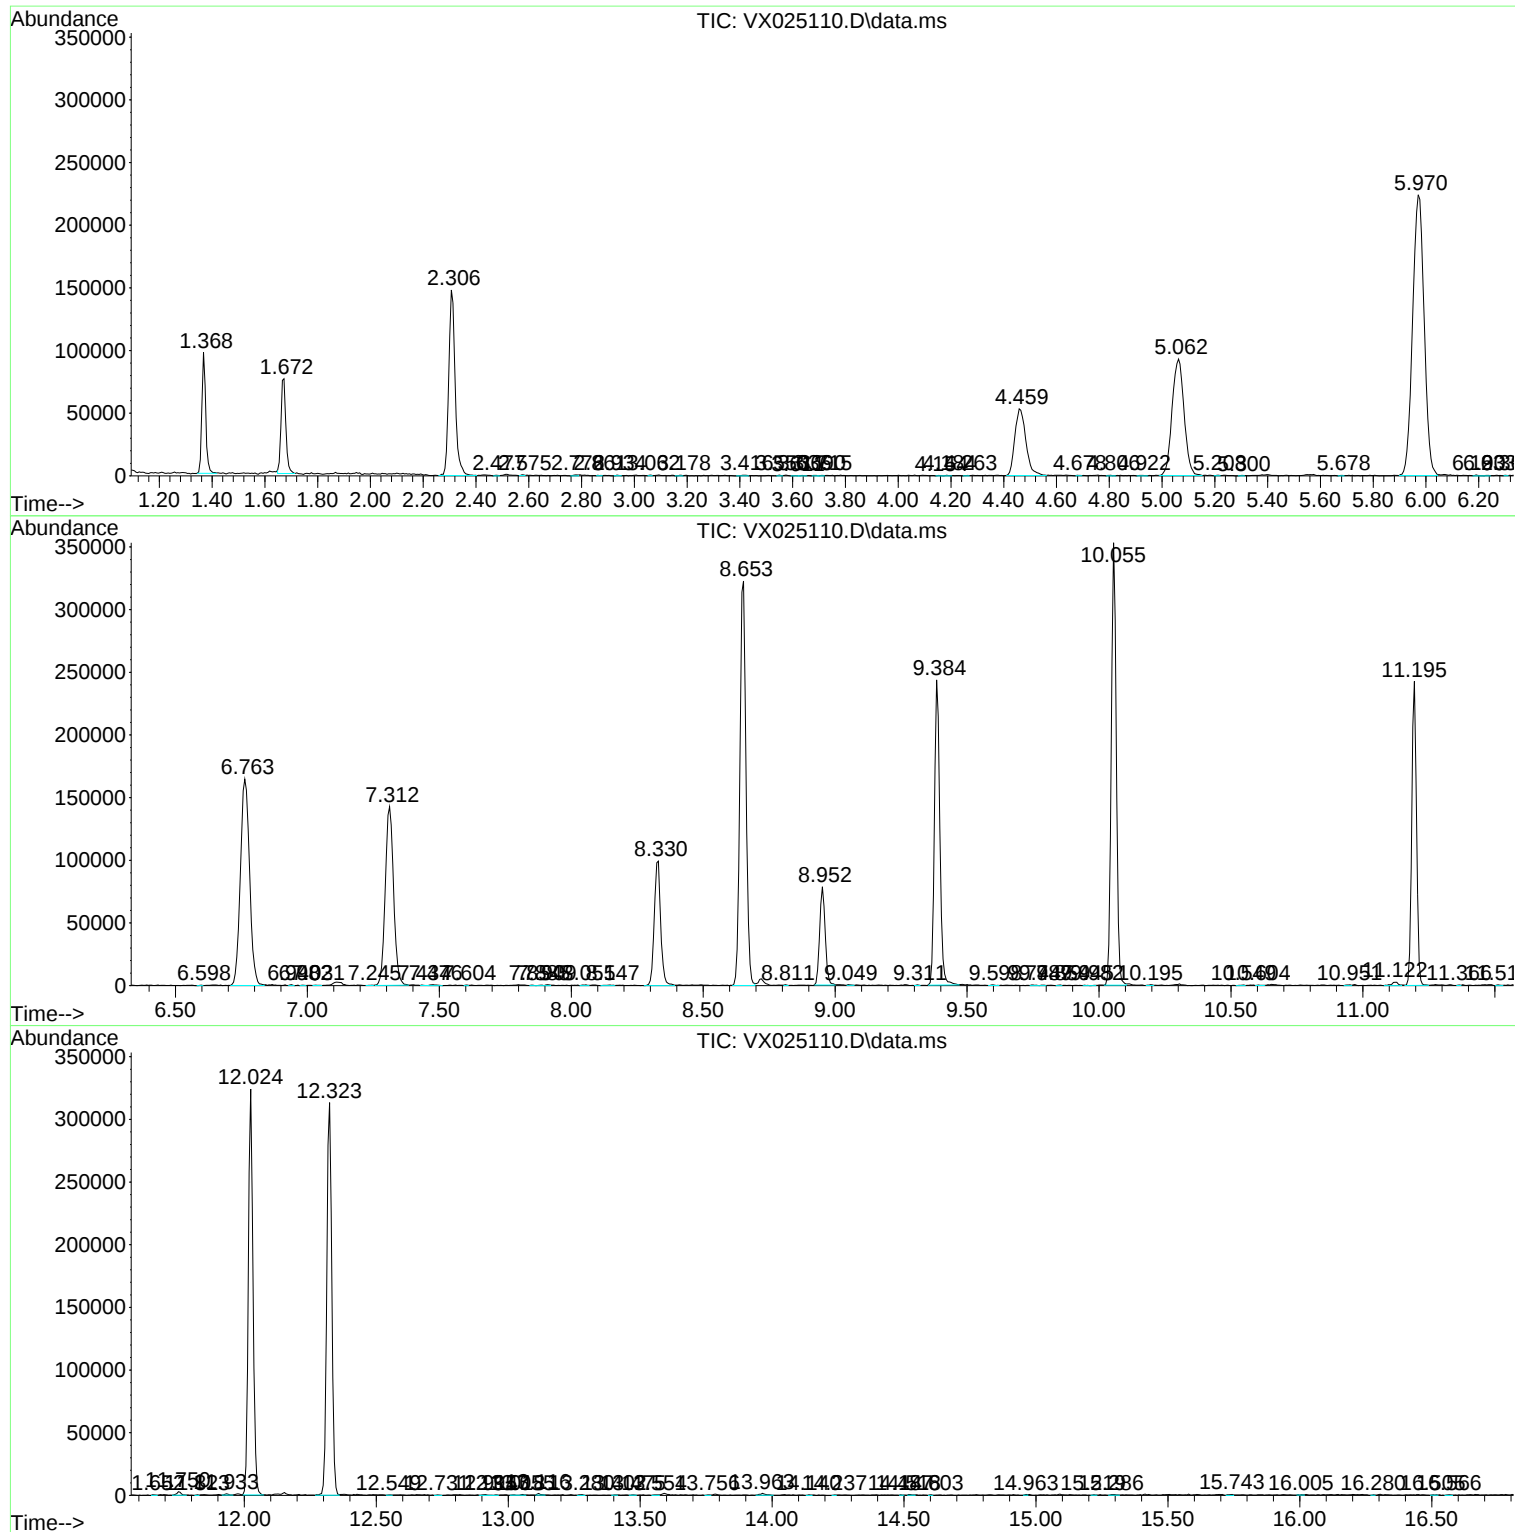

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110921\
Data File : VX025110.D
Acq On : 09 Nov 2021 10:30
Operator : JC/MD
Sample : VX1109MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK633

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110921\
Data File : VX025110.D
Acq On : 09 Nov 2021 10:30
Operator : JC/MD
Sample : VX1109MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK633

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc