

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110921\
 Data File : VX025115.D
 Acq On : 09 Nov 2021 12:31
 Operator : JC/MD
 Sample : M4464-07DL 1000X
 Misc : 7.45g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GB7K5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110821WMA.M
 Title : VOC Analysis

Signal : TIC: VX025115.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	54	rVB	88817	92027	10.85%	1.512%
2	1.666	91	95	103	rVB	77585	93631	11.04%	1.539%
3	2.307	195	200	213	rVB	142299	235645	27.77%	3.873%
4	2.666	257	259	264	rBV	289	354	0.04%	0.006%
5	2.910	297	299	300	rBV	378	266	0.03%	0.004%
6	3.093	326	329	331	rBV	422	537	0.06%	0.009%
7	3.215	347	349	351	rBV2	417	282	0.03%	0.005%
8	3.367	371	374	375	rBV	481	438	0.05%	0.007%
9	3.501	394	396	398	rBV	546	458	0.05%	0.008%
10	3.629	413	417	423	rBV3	668	1254	0.15%	0.021%
11	3.879	457	458	461	rBV3	167	185	0.02%	0.003%
12	3.904	461	462	463	rBV3	410	240	0.03%	0.004%
13	3.989	473	476	479	rBV	598	597	0.07%	0.010%
14	4.020	479	481	484	rVV	370	373	0.04%	0.006%
15	4.221	511	514	517	rVB	288	347	0.04%	0.006%
16	4.264	517	521	522	rBV2	379	408	0.05%	0.007%
17	4.379	538	540	543	rBV	436	411	0.05%	0.007%
18	4.465	545	554	567	rBV	55510	160911	18.97%	2.644%
19	4.788	605	607	613	rVB	400	586	0.07%	0.010%
20	4.843	613	616	618	rBV	387	399	0.05%	0.007%
21	4.861	618	619	621	rBV2	373	251	0.03%	0.004%
22	5.178	669	671	674	rBV2	543	397	0.05%	0.007%
23	5.318	691	694	695	rBV	548	532	0.06%	0.009%
24	5.556	727	733	739	rBV3	1177	3220	0.38%	0.053%
25	5.629	744	745	746	rBV	393	175	0.02%	0.003%
26	5.690	753	755	758	rVB2	306	338	0.04%	0.006%
27	5.763	765	767	772	rVB	327	396	0.05%	0.007%
28	5.977	786	802	816	rBV3	223961	665782	78.47%	10.942%
29	6.233	843	844	845	rBV	439	298	0.04%	0.005%
30	6.324	856	859	861	rVB	378	389	0.05%	0.006%
31	6.361	861	865	870	rVB	528	788	0.09%	0.013%
32	6.416	870	874	876	rBV2	481	541	0.06%	0.009%
33	6.470	881	883	887	rBV	332	406	0.05%	0.007%
34	6.611	901	906	908	rBV2	460	682	0.08%	0.011%
35	6.684	915	918	919	rBV2	332	384	0.05%	0.006%
36	6.769	922	932	945	rVV	165564	392466	46.26%	6.450%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110921\
 Data File : VX025115.D
 Acq On : 09 Nov 2021 12:31
 Operator : JC/MD
 Sample : M4464-07DL 1000X
 Misc : 7.45g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GB7K5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110821WMA.M
 Title : VOC Analysis

37	7.129	982	991	1005	rBV2	217579	480999	56.69%	7.905%
38	7.257	1010	1012	1013	rBV2	370	232	0.03%	0.004%
39	7.312	1013	1021	1031	rBV	139272	309331	36.46%	5.084%
40	7.568	1062	1063	1066	rVB	392	282	0.03%	0.005%
41	7.598	1066	1068	1070	rBV	302	286	0.03%	0.005%
42	7.732	1087	1090	1092	rBV2	411	606	0.07%	0.010%
43	8.086	1146	1148	1153	rBV2	466	611	0.07%	0.010%
44	8.190	1162	1165	1167	rVB	758	539	0.06%	0.009%
45	8.220	1168	1170	1171	rBV	667	486	0.06%	0.008%
46	8.330	1181	1188	1199	rVB	97948	161200	19.00%	2.649%
47	8.525	1217	1220	1221	rBV	466	455	0.05%	0.007%
48	8.586	1228	1230	1232	rBV	536	525	0.06%	0.009%
49	8.653	1235	1241	1247	rVV	332783	509990	60.11%	8.381%
50	8.720	1247	1252	1266	rVB	547431	848427	100.00%	13.943%
51	8.848	1272	1273	1275	rBV2	365	303	0.04%	0.005%
52	8.952	1285	1290	1298	rVB	75364	110778	13.06%	1.821%
53	9.116	1314	1317	1320	rVB	423	505	0.06%	0.008%
54	9.153	1320	1323	1325	rBV	455	501	0.06%	0.008%
55	9.275	1339	1343	1348	rBV2	5596	8084	0.95%	0.133%
56	9.385	1356	1361	1369	rBV	244708	351108	41.38%	5.770%
57	9.592	1393	1395	1398	rBV2	458	546	0.06%	0.009%
58	9.787	1426	1427	1429	rBV2	357	299	0.04%	0.005%
59	9.878	1439	1442	1444	rBV	611	679	0.08%	0.011%
60	9.964	1455	1456	1457	rBV	474	265	0.03%	0.004%
61	10.055	1466	1471	1482	rVB	336935	469389	55.32%	7.714%
62	10.159	1487	1488	1491	rBV2	293	338	0.04%	0.006%
63	10.195	1491	1494	1499	rVB7	1936	3070	0.36%	0.050%
64	10.305	1508	1512	1518	rVB3	4911	6778	0.80%	0.111%
65	10.366	1518	1522	1525	rBV3	1964	2220	0.26%	0.036%
66	10.427	1528	1532	1534	rBV2	366	541	0.06%	0.009%
67	10.512	1545	1546	1550	rBV2	395	366	0.04%	0.006%
68	10.848	1599	1601	1606	rBV4	960	1570	0.19%	0.026%
69	11.037	1628	1632	1634	rBV3	843	874	0.10%	0.014%
70	11.195	1652	1658	1668	rBV	254984	308814	36.40%	5.075%
71	11.756	1746	1750	1758	rVB3	6404	9227	1.09%	0.152%
72	11.811	1758	1759	1761	rBV3	451	376	0.04%	0.006%
73	11.872	1767	1769	1770	rVB	562	288	0.03%	0.005%
74	11.890	1770	1772	1774	rBV2	955	857	0.10%	0.014%
75	11.933	1777	1779	1783	rBV4	1796	2700	0.32%	0.044%
76	12.024	1788	1794	1801	rBV	313730	404727	47.70%	6.651%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110921\
 Data File : VX025115.D
 Acq On : 09 Nov 2021 12:31
 Operator : JC/MD
 Sample : M4464-07DL 1000X
 Misc : 7.45g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GB7K5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110821WMA.M
 Title : VOC Analysis

77	12.219	1824	1826	1827	rBV	602	355	0.04%	0.006%
78	12.323	1837	1843	1851	rVB	321481	415494	48.97%	6.828%
79	12.427	1857	1860	1863	rVB	2945	2909	0.34%	0.048%
80	13.000	1952	1954	1955	rVB	731	379	0.04%	0.006%
81	13.067	1959	1965	1966	rBV3	525	801	0.09%	0.013%
82	13.146	1976	1978	1980	rBV	338	323	0.04%	0.005%
83	13.518	2037	2039	2042	rVB	306	282	0.03%	0.005%
84	13.542	2042	2043	2044	rBV	320	227	0.03%	0.004%
85	13.957	2109	2111	2114	rBV2	478	500	0.06%	0.008%
86	14.048	2124	2126	2130	rBV2	613	613	0.07%	0.010%
87	14.146	2141	2142	2145	rBV	734	605	0.07%	0.010%
88	14.225	2154	2155	2158	rBV	506	467	0.06%	0.008%
89	14.286	2163	2165	2166	rVB	274	182	0.02%	0.003%
90	14.329	2169	2172	2174	rBV2	657	705	0.08%	0.012%
91	14.432	2187	2189	2193	rBV2	442	671	0.08%	0.011%
92	14.548	2207	2208	2212	rVB	498	371	0.04%	0.006%
93	14.621	2215	2220	2223	rBV	520	898	0.11%	0.015%
94	14.774	2243	2245	2249	rBV	529	580	0.07%	0.010%
95	14.804	2249	2250	2253	rBV	420	352	0.04%	0.006%
96	14.847	2255	2257	2260	rBV	586	501	0.06%	0.008%
97	15.030	2284	2287	2290	rVB2	523	502	0.06%	0.008%
98	15.170	2308	2310	2314	rBV2	745	720	0.08%	0.012%
99	16.414	2512	2514	2515	rBV	449	279	0.03%	0.005%
100	16.694	2558	2560	2563	rVB	768	567	0.07%	0.009%




Sum of corrected areas: 6084849

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110921\
Data File : VX025115.D
Acq On : 09 Nov 2021 12:31
Operator : JC/MD
Sample : M4464-07DL 1000X
Misc : 7.45g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GB7K5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

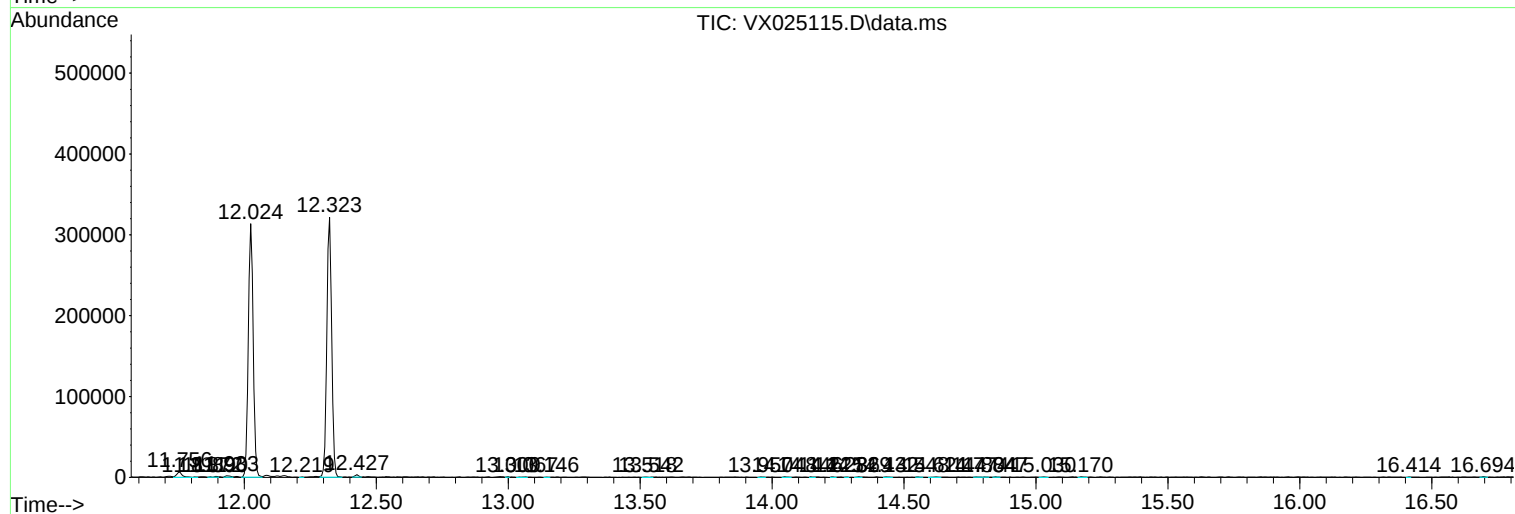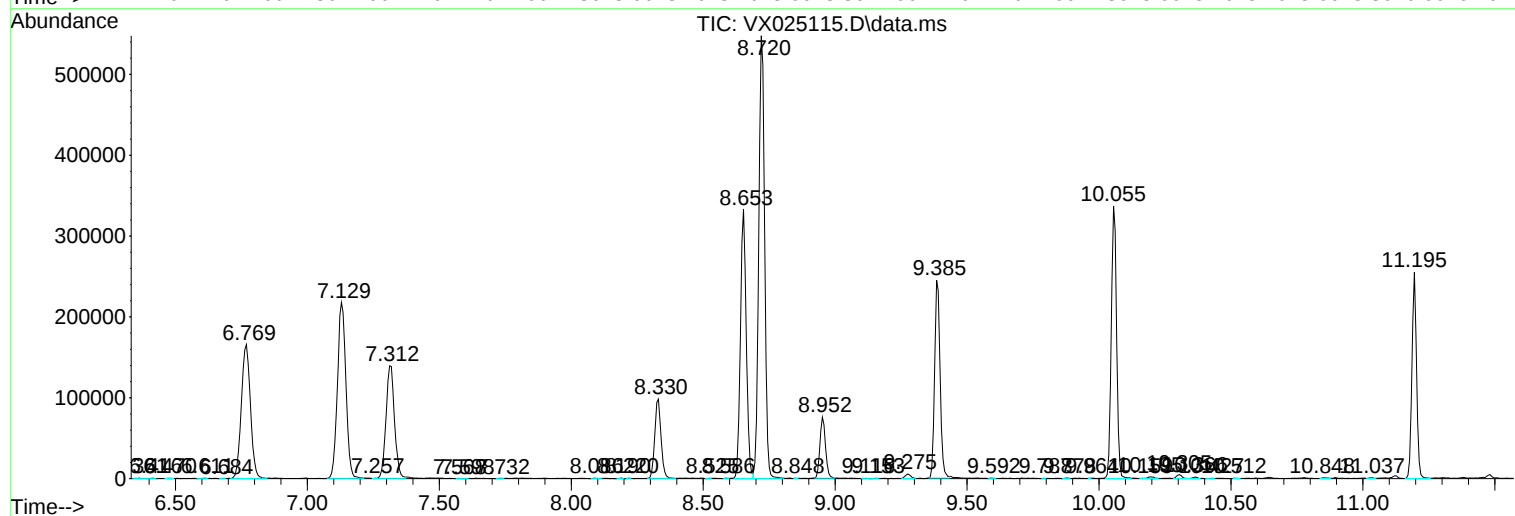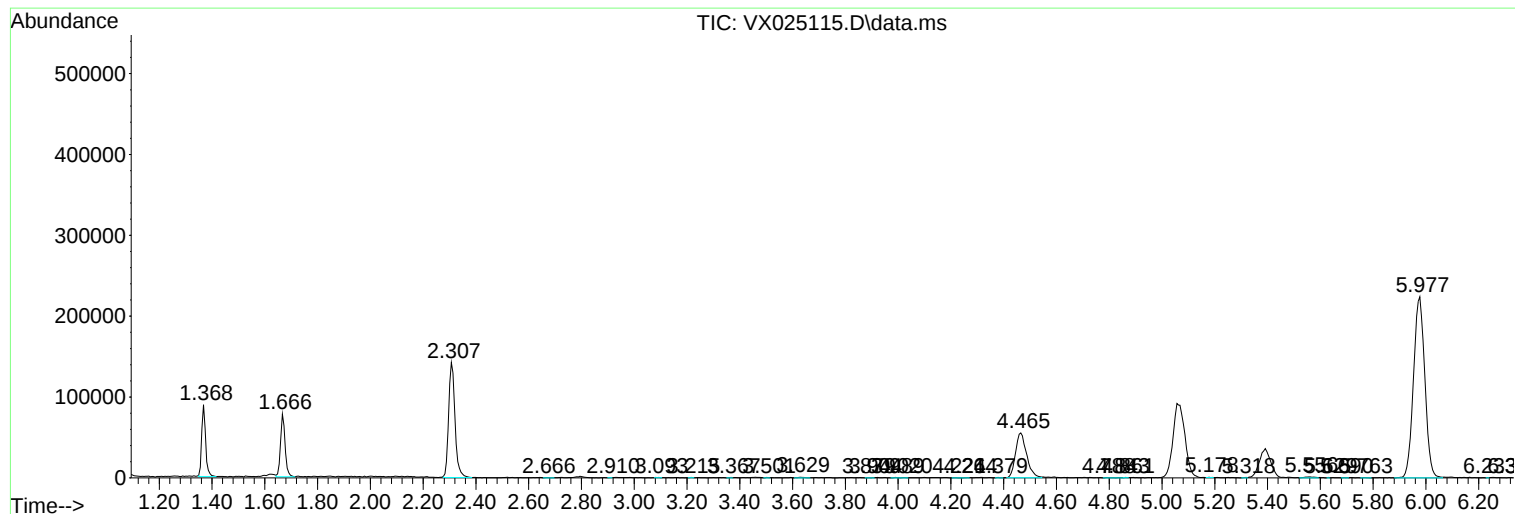

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110921\
Data File : VX025115.D
Acq On : 09 Nov 2021 12:31
Operator : JC/MD
Sample : M4464-07DL 1000X
Misc : 7.45g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GB7K5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110921\
Data File : VX025115.D
Acq On : 09 Nov 2021 12:31
Operator : JC/MD
Sample : M4464-07DL 1000X
Misc : 7.45g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GB7K5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc