

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110921\
 Data File : VX025123.D
 Acq On : 09 Nov 2021 16:35
 Operator : JC/MD
 Sample : M4543-02 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110821WMA.M

Title : VOC Analysis

Signal : TIC: VX025123.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	53	rVB	77194	77362	13.02%	1.746%
2	1.672	92	96	105	rVB	71903	91399	15.38%	2.062%
3	2.306	195	200	216	rVB	120736	196851	33.12%	4.442%
4	2.471	226	227	230	rBV	365	397	0.07%	0.009%
5	2.697	262	264	265	rBV	492	434	0.07%	0.010%
6	2.764	273	275	276	rBV	438	445	0.07%	0.010%
7	2.788	276	279	284	rVB5	2469	3544	0.60%	0.080%
8	3.014	314	316	318	rVB5	364	339	0.06%	0.008%
9	3.081	325	327	333	rVB2	792	746	0.13%	0.017%
10	3.196	344	346	348	rBV	381	395	0.07%	0.009%
11	3.294	360	362	364	rBV	395	385	0.06%	0.009%
12	3.544	400	403	404	rBV	342	349	0.06%	0.008%
13	3.617	414	415	419	rVB2	402	444	0.07%	0.010%
14	3.654	419	421	425	rBV2	234	346	0.06%	0.008%
15	3.721	430	432	437	rBB2	336	422	0.07%	0.010%
16	3.757	437	438	440	rBV2	570	461	0.08%	0.010%
17	3.904	460	462	466	rBV2	575	696	0.12%	0.016%
18	3.946	466	469	471	rBV2	293	337	0.06%	0.008%
19	4.239	515	517	519	rVV	345	317	0.05%	0.007%
20	4.391	539	542	544	rBV	444	436	0.07%	0.010%
21	4.464	546	554	569	rVV	52335	151055	25.41%	3.409%
22	4.641	582	583	586	rBV2	478	524	0.09%	0.012%
23	4.812	609	611	615	rBV	406	485	0.08%	0.011%
24	4.855	615	618	620	rBV2	604	578	0.10%	0.013%
25	4.928	627	630	631	rBV2	385	337	0.06%	0.008%
26	4.946	631	633	635	rVB	536	364	0.06%	0.008%
27	4.983	635	639	641	rBV2	289	491	0.08%	0.011%
28	5.068	641	653	668	rVB2	79556	246654	41.50%	5.566%
29	5.275	686	687	689	rBV	428	332	0.06%	0.007%
30	5.544	729	731	734	rVB2	683	521	0.09%	0.012%
31	5.720	757	760	761	rBV	326	323	0.05%	0.007%
32	5.763	765	767	771	rVB	481	493	0.08%	0.011%
33	5.861	780	783	785	rBV	295	350	0.06%	0.008%
34	5.976	787	802	819	rVV2	198097	594378	100.00%	13.412%
35	6.141	825	829	832	rBV2	694	648	0.11%	0.015%
36	6.385	866	869	871	rBV	390	480	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110921\
 Data File : VX025123.D
 Acq On : 09 Nov 2021 16:35
 Operator : JC/MD
 Sample : M4543-02 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110821WMA.M
 Title : VOC Analysis

37	6.519	888	891	894	rVB	383	498	0.08%	0.011%
38	6.574	899	900	904	rBV	346	352	0.06%	0.008%
39	6.653	911	913	916	rVB2	462	328	0.06%	0.007%
40	6.763	921	931	943	rBV	142212	336089	56.54%	7.584%
41	7.116	982	989	994	rBV5	2998	6123	1.03%	0.138%
42	7.312	1013	1021	1033	rBV2	121734	275376	46.33%	6.214%
43	7.482	1045	1049	1053	rBV2	841	1273	0.21%	0.029%
44	7.641	1073	1075	1077	rVB	523	321	0.05%	0.007%
45	7.763	1092	1095	1097	rBV	474	590	0.10%	0.013%
46	7.805	1100	1102	1104	rVV2	533	324	0.05%	0.007%
47	7.891	1114	1116	1119	rVB2	473	356	0.06%	0.008%
48	8.232	1169	1172	1174	rBV2	329	402	0.07%	0.009%
49	8.324	1181	1187	1197	rVB	84087	140058	23.56%	3.160%
50	8.500	1214	1216	1219	rBV	504	566	0.10%	0.013%
51	8.653	1231	1241	1248	rBV	278597	432565	72.78%	9.761%
52	8.951	1285	1290	1301	rBV	67011	100510	16.91%	2.268%
53	9.208	1330	1332	1334	rVB	630	429	0.07%	0.010%
54	9.262	1339	1341	1344	rBV	386	406	0.07%	0.009%
55	9.336	1350	1353	1355	rBV	249	403	0.07%	0.009%
56	9.384	1355	1361	1374	rBV	225310	334137	56.22%	7.540%
57	9.677	1406	1409	1411	rVB2	576	567	0.10%	0.013%
58	9.787	1424	1427	1431	rBV	355	540	0.09%	0.012%
59	10.055	1466	1471	1480	rVV	307431	414931	69.81%	9.363%
60	10.201	1492	1495	1497	rBV2	634	774	0.13%	0.017%
61	10.402	1525	1528	1533	rVB	492	559	0.09%	0.013%
62	10.555	1551	1553	1555	rBV2	598	420	0.07%	0.009%
63	10.628	1564	1565	1569	rBV	477	484	0.08%	0.011%
64	10.713	1578	1579	1581	rBV	457	355	0.06%	0.008%
65	10.902	1608	1610	1613	rBV2	443	509	0.09%	0.011%
66	10.982	1620	1623	1624	rBV	412	345	0.06%	0.008%
67	11.122	1643	1646	1649	rBV2	2055	2686	0.45%	0.061%
68	11.195	1653	1658	1665	rBV	224302	282252	47.49%	6.369%
69	11.475	1700	1704	1707	rBV3	524	882	0.15%	0.020%
70	11.695	1737	1740	1741	rBV3	450	469	0.08%	0.011%
71	11.756	1745	1750	1752	rBV3	1878	2367	0.40%	0.053%
72	11.847	1762	1765	1767	rVB	594	551	0.09%	0.012%
73	11.902	1771	1774	1777	rBV	408	553	0.09%	0.012%
74	11.933	1777	1779	1783	rVB2	1368	1434	0.24%	0.032%
75	11.988	1786	1788	1789	rBV2	424	317	0.05%	0.007%
76	12.024	1789	1794	1800	rBV	285227	349971	58.88%	7.897%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110921\
 Data File : VX025123.D
 Acq On : 09 Nov 2021 16:35
 Operator : JC/MD
 Sample : M4543-02 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110821WMA.M
 Title : VOC Analysis

77	12.323	1837	1843	1849	rBV	277532	353288	59.44%	7.972%
78	12.542	1875	1879	1881	rBV2	504	636	0.11%	0.014%
79	12.804	1921	1922	1927	rVV2	392	470	0.08%	0.011%
80	13.158	1975	1980	1984	rBV3	419	845	0.14%	0.019%
81	13.231	1991	1992	1994	rBV	475	406	0.07%	0.009%
82	13.317	2005	2006	2008	rBV	421	324	0.05%	0.007%
83	13.408	2019	2021	2024	rVB	572	611	0.10%	0.014%
84	13.591	2049	2051	2053	rBV	382	401	0.07%	0.009%
85	13.670	2062	2064	2066	rBV	467	371	0.06%	0.008%
86	13.957	2109	2111	2114	rBV	496	490	0.08%	0.011%
87	14.115	2134	2137	2141	rBV	509	904	0.15%	0.020%
88	14.286	2163	2165	2169	rBV	260	412	0.07%	0.009%
89	14.481	2194	2197	2198	rBV	436	523	0.09%	0.012%
90	14.530	2203	2205	2207	rVB	481	330	0.06%	0.007%
91	14.560	2207	2210	2211	rBV	441	323	0.05%	0.007%
92	14.603	2215	2217	2219	rBV	328	376	0.06%	0.008%
93	14.700	2230	2233	2235	rBV	353	444	0.07%	0.010%
94	15.377	2342	2344	2347	rVB	528	442	0.07%	0.010%
95	15.408	2347	2349	2353	rBV2	394	538	0.09%	0.012%
96	15.737	2402	2403	2406	rBV	483	455	0.08%	0.010%
97	16.328	2499	2500	2502	rBV	522	421	0.07%	0.010%
98	16.548	2534	2536	2538	rBV	845	617	0.10%	0.014%
99	16.651	2550	2553	2557	rVB	468	710	0.12%	0.016%
100	16.694	2557	2560	2564	rBV	645	1031	0.17%	0.023%


Sum of corrected areas: 4431558

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110921\
Data File : VX025123.D
Acq On : 09 Nov 2021 16:35
Operator : JC/MD
Sample : M4543-02 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

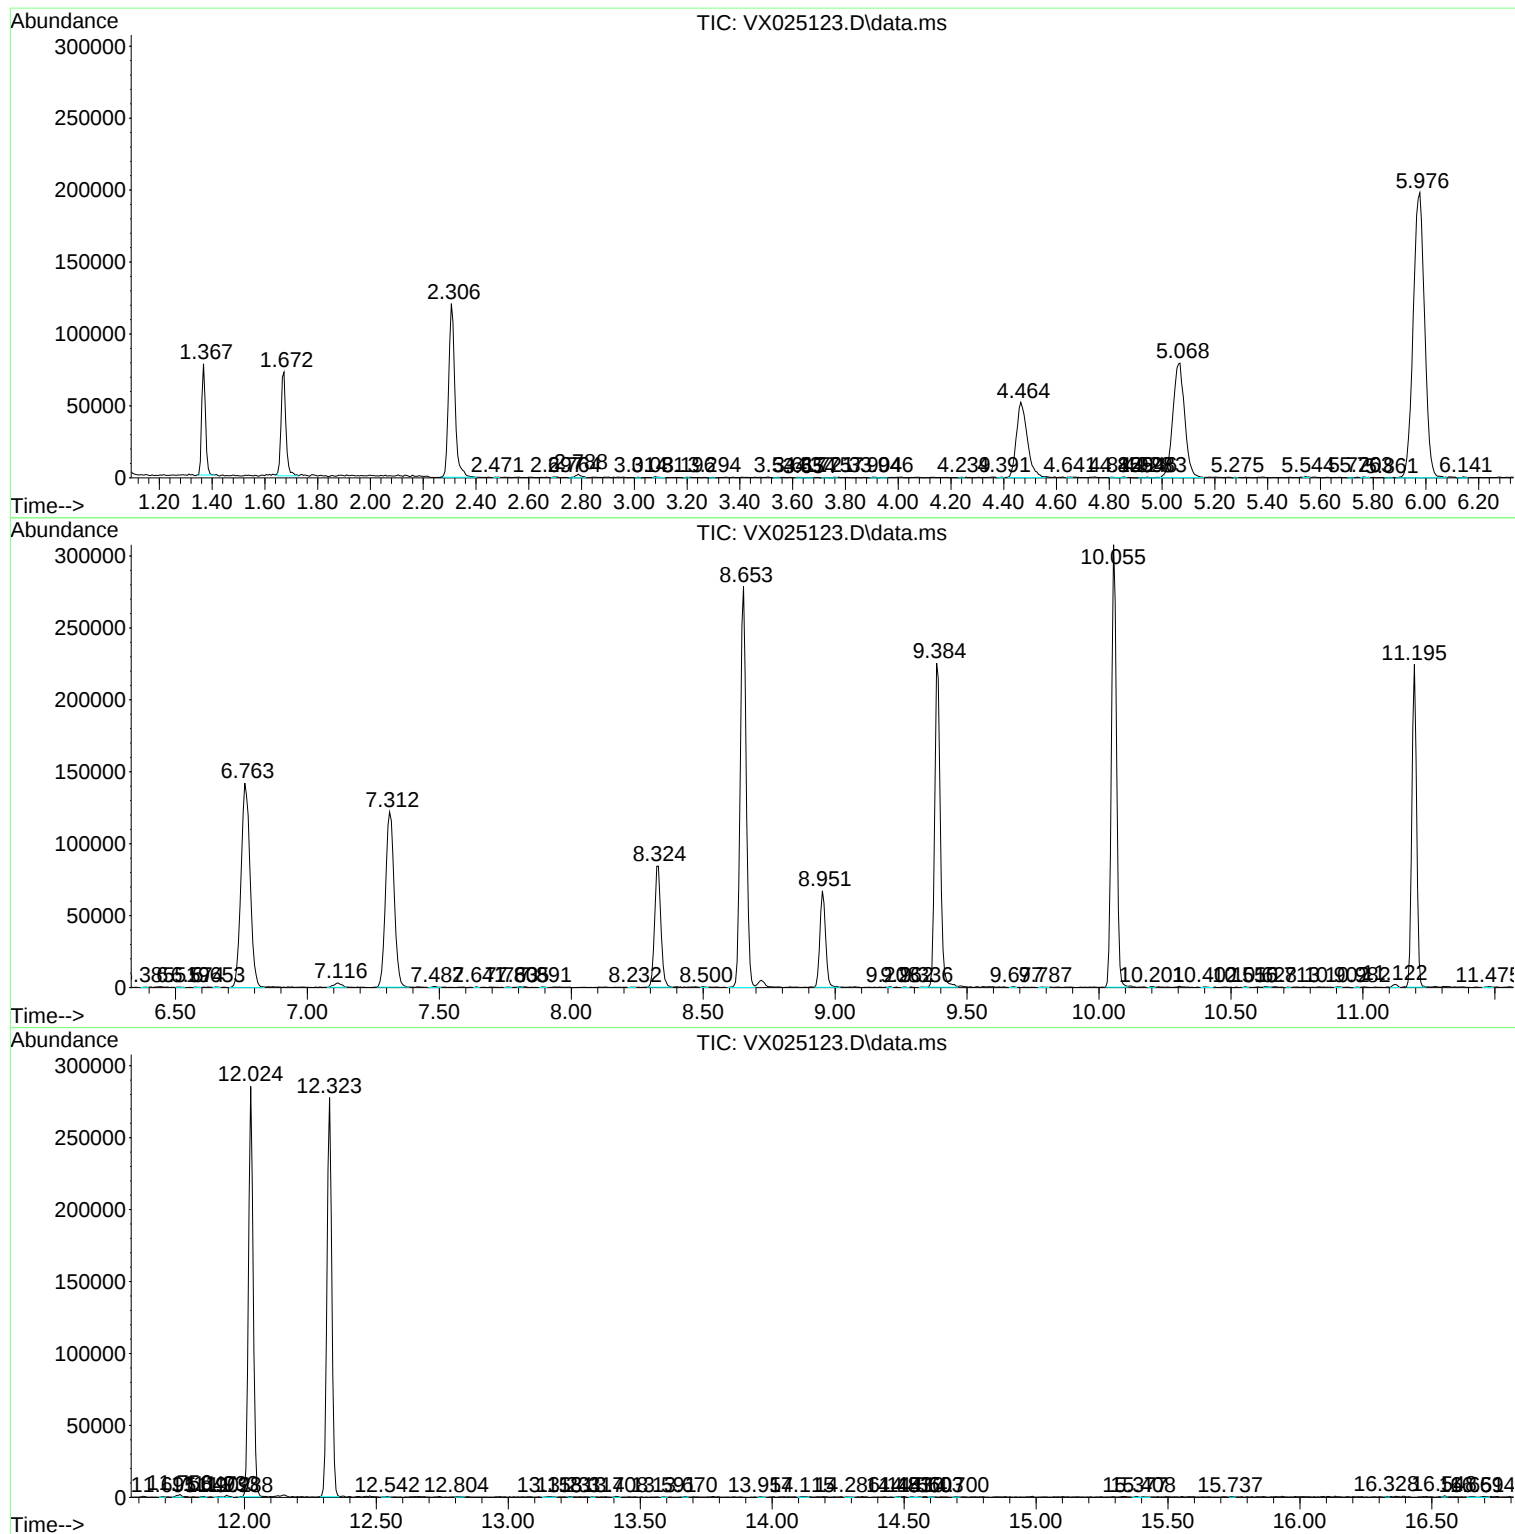

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110921\
Data File : VX025123.D
Acq On : 09 Nov 2021 16:35
Operator : JC/MD
Sample : M4543-02 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110921\
Data File : VX025123.D
Acq On : 09 Nov 2021 16:35
Operator : JC/MD
Sample : M4543-02 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc