
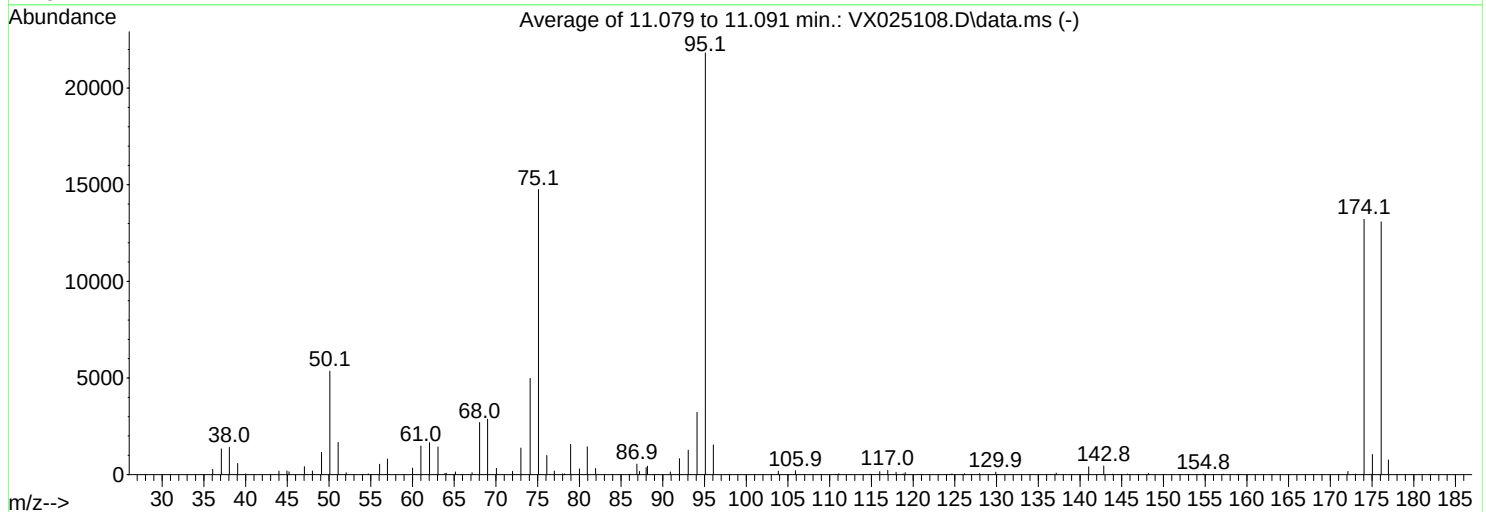


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110921\
 Data File : VX025108.D
 Acq On : 09 Nov 2021 08:57
 Operator : JC/MD
 Sample : BFB612
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB612

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110821WMA.M
 Title : VOC Analysis
 Last Update : Wed Nov 10 02:50:07 2021

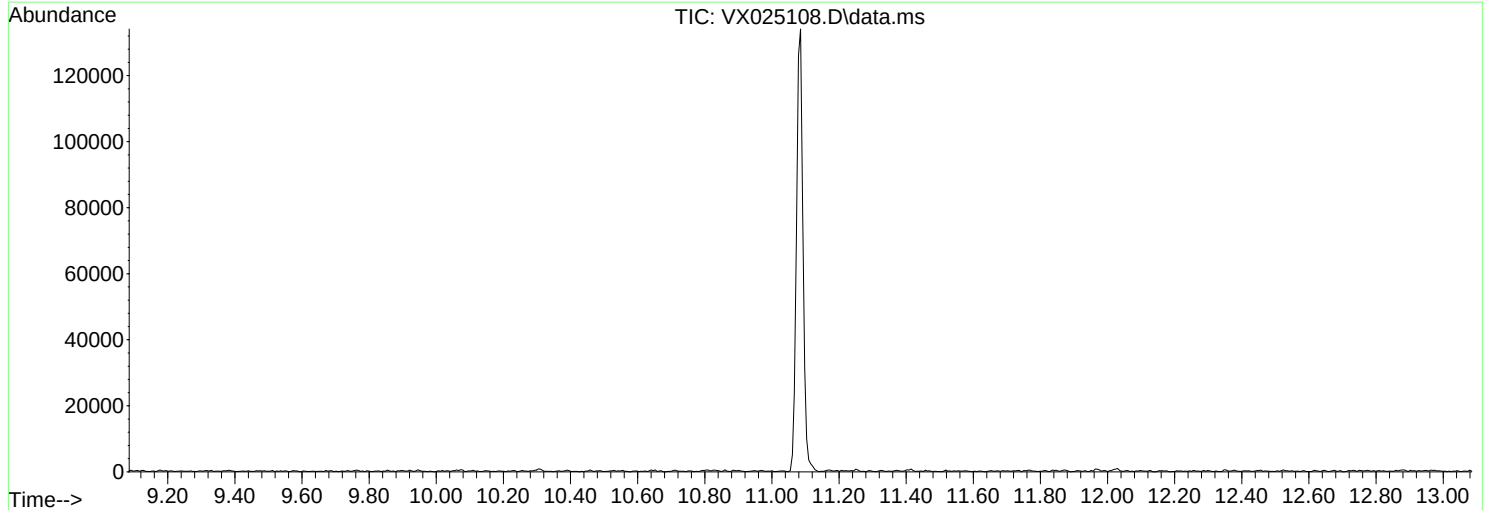

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.6	5359	PASS
75	95	30	80	67.6	14757	PASS
95	95	100	100	100.0	21825	PASS
96	95	5	9	7.1	1542	PASS
173	174	0.00	2	0.3	36	PASS
174	95	50	120	60.5	13212	PASS
175	174	5	9	7.9	1041	PASS
176	174	95	101	99.0	13078	PASS
177	176	5	9	5.8	759	PASS

m/z	Abundance
40.10	51.0
44.00	101.0

Instrument :
MSVOA_X
ClientSampleId :
BFB612

m/z	Abundance
36.10	392.0
37.10	1655.0
38.00	1886.0
39.00	605.0
43.90	407.0
44.90	262.0
45.20	255.0
47.10	607.0
48.00	286.0
49.10	1293.0
50.10	5966.0
51.10	1868.0
52.10	144.0
54.70	125.0
56.10	617.0
57.00	1046.0
60.00	415.0
61.00	1323.0
62.10	2352.0
63.10	1819.0
63.90	207.0
65.10	232.0
67.20	111.0
68.10	2628.0
69.10	3153.0
70.00	421.0
72.00	376.0
73.00	1479.0
74.10	6356.0
75.10	17008.0
76.10	1172.0
77.00	344.0
78.00	133.0
78.90	1621.0
80.10	389.0
80.90	1678.0
81.90	372.0
86.10	67.0
86.90	917.0
88.00	1090.0
90.90	140.0
92.00	775.0
93.00	1311.0
94.10	3831.0
95.10	25120.0
96.10	2003.0
103.90	162.0
105.90	145.0
116.00	162.0
116.90	222.0
118.00	107.0
119.00	181.0
124.60	59.0
127.90	63.0
129.90	116.0
137.20	140.0
141.10	361.0
142.90	460.0
152.00	50.0
173.00	108.0
174.00	12608.0
175.10	1040.0
176.10	12886.0
176.90	817.0

Instrument :
MSVOA_X
ClientSampleId :
BFB612

m/z	Abundance
36.00	183.0
37.10	1517.0
38.10	1358.0
39.10	858.0
40.00	125.0
44.00	284.0
45.00	310.0
46.90	340.0
48.00	190.0
49.10	1426.0
50.10	6642.0
51.10	2134.0
52.00	143.0
56.00	662.0
57.00	782.0
60.00	360.0
61.00	2215.0
62.10	1639.0
63.00	1416.0
64.10	145.0
65.20	178.0
67.10	181.0
68.00	3688.0
69.00	3453.0
70.10	203.0
72.10	74.0
73.10	1899.0
74.10	5242.0
75.10	17176.0
76.10	1392.0
77.00	153.0
79.00	2150.0
79.90	337.0
81.00	1661.0
82.00	309.0
86.90	719.0
88.20	770.0
90.90	215.0
92.00	1153.0
93.10	1706.0
94.10	3822.0
95.10	25632.0
96.00	1884.0
103.80	220.0
105.90	294.0
111.10	65.0
114.90	83.0
116.00	236.0
117.00	278.0
117.90	168.0
119.10	137.0
124.70	62.0
126.20	59.0
128.00	86.0
129.90	133.0
137.10	121.0
140.90	517.0
142.90	526.0
148.20	81.0
154.80	90.0
157.20	87.0
172.10	238.0
174.10	16166.0
175.10	1126.0
176.10	15586.0
177.00	1016.0

Instrument :
MSVOA_X
ClientSampleId :
BFB612

m/z	Abundance
36.00	248.0
37.10	831.0
38.10	1004.0
39.10	264.0
40.00	159.0
44.10	153.0
45.20	204.0
47.00	290.0
48.00	91.0
49.00	735.0
50.00	3468.0
51.00	1004.0
56.00	345.0
57.00	611.0
60.10	252.0
61.10	903.0
61.90	979.0
63.10	1065.0
64.00	72.0
68.00	1778.0
68.90	2023.0
70.00	347.0
72.00	81.0
72.90	744.0
74.10	3345.0
75.10	10087.0
76.00	421.0
77.00	86.0
78.20	125.0
79.00	938.0
80.10	158.0
80.90	973.0
81.90	266.0
87.20	497.0
88.10	534.0
90.80	81.0
92.00	559.0
93.00	796.0
94.10	2039.0
95.10	14722.0
96.10	738.0
103.80	156.0
105.90	190.0
110.70	61.0
111.10	94.0
116.00	83.0
117.00	180.0
118.00	109.0
118.80	122.0
126.10	87.0
129.90	146.0
141.10	341.0
142.80	345.0
143.90	83.0
145.70	98.0
148.20	108.0
172.10	264.0
174.10	10861.0
175.00	956.0
176.10	10763.0
177.00	444.0

Instrument :
MSVOA_X
ClientSampleId :
BFB612