

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110922\
 Data File : VX032684.D
 Acq On : 09 Nov 2022 17:01
 Operator : JC/MD
 Sample : N5512-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 AUD-1911-TOTE

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
 Title : SW846 8260

Signal : TIC: VX032684.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.270	24	30	39	rBV	17006	52174	9.25%	1.610%
2	1.349	41	43	50	rVB3	3393	6403	1.13%	0.198%
3	1.453	57	60	73	rVB	7921	11313	2.00%	0.349%
4	2.386	208	213	223	rVB	3610	7028	1.25%	0.217%
5	2.947	297	305	315	rBV	5848	14077	2.49%	0.434%
6	5.385	694	705	721	rBV2	67410	198262	35.13%	6.119%
7	5.556	721	733	747	rVV	113457	321225	56.92%	9.914%
8	5.958	789	799	812	rBV	75354	199034	35.27%	6.143%
9	6.763	921	931	945	rBV	178286	417655	74.01%	12.890%
10	8.647	1234	1240	1251	rBV	350966	564337	100.00%	17.417%
11	10.055	1465	1471	1484	rBV	362532	479949	85.05%	14.813%
12	10.305	1507	1512	1517	rBV3	5198	7861	1.39%	0.243%
13	11.079	1634	1639	1647	rBV	335638	426007	75.49%	13.148%
14	11.756	1745	1750	1755	rVB	7622	9880	1.75%	0.305%
15	12.024	1788	1794	1801	rBV	371370	458434	81.23%	14.149%
16	12.853	1924	1930	1936	rBV3	8840	13648	2.42%	0.421%
17	13.292	1998	2002	2008	rVB4	4800	6850	1.21%	0.211%
18	13.774	2074	2081	2086	rBV	4111	6299	1.12%	0.194%
19	14.195	2146	2150	2159	rBV7	5390	11806	2.09%	0.364%
20	14.640	2218	2223	2229	rVB	8098	11723	2.08%	0.362%
21	14.780	2241	2246	2251	rBV	6566	8970	1.59%	0.277%
22	15.615	2378	2383	2386	rBV2	4843	7194	1.27%	0.222%




Sum of corrected areas: 3240129

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110922\
Data File : VX032684.D
Acq On : 09 Nov 2022 17:01
Operator : JC/MD
Sample : N5512-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-1911-TOTE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

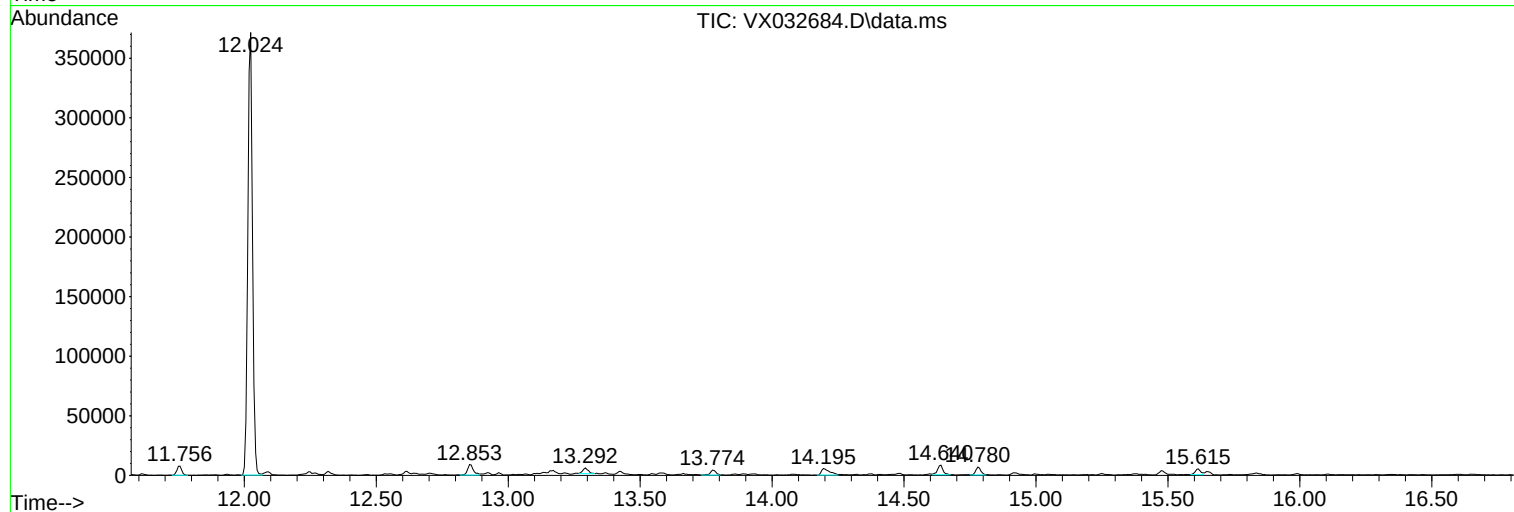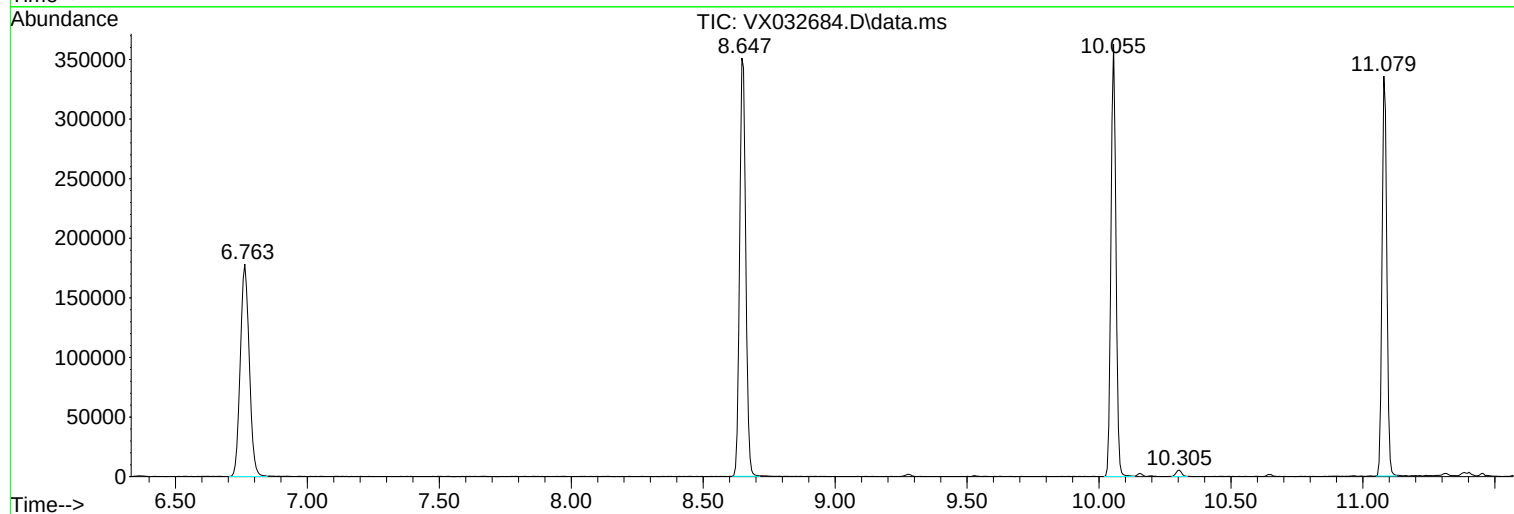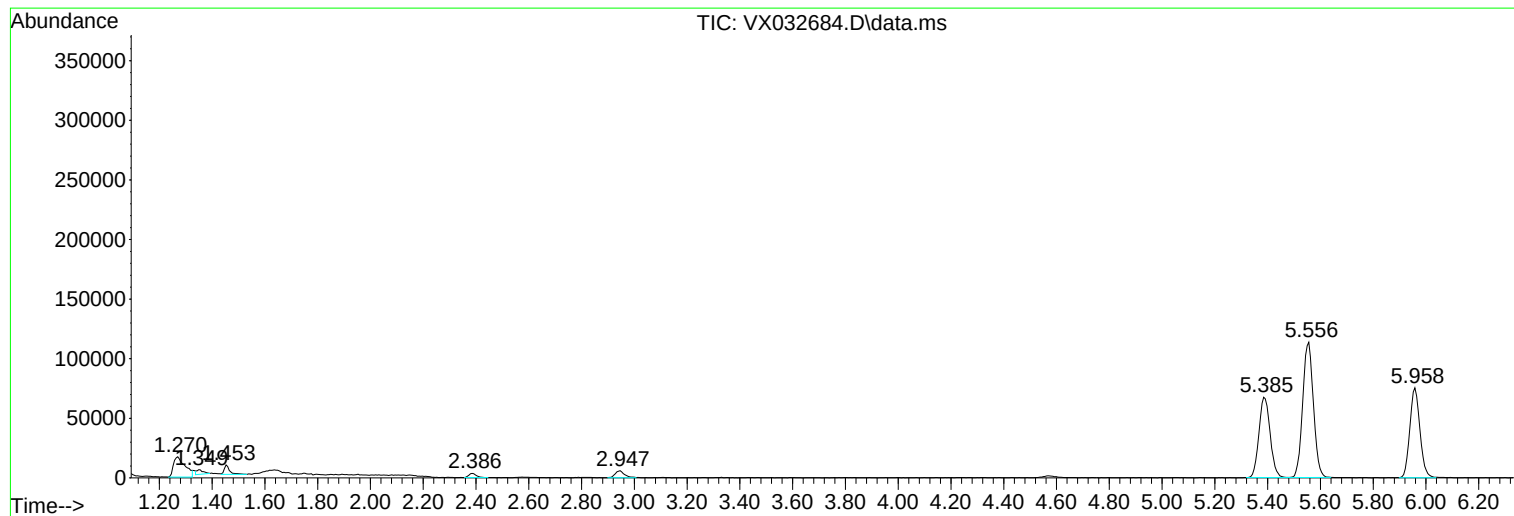

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110922\
Data File : VX032684.D
Acq On : 09 Nov 2022 17:01
Operator : JC/MD
Sample : N5512-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-1911-TOTE










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.270	8.12 ug/l	52174	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	90
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	5
5			Ethyl Chloride	64	C2H5Cl	000075-00-3	4

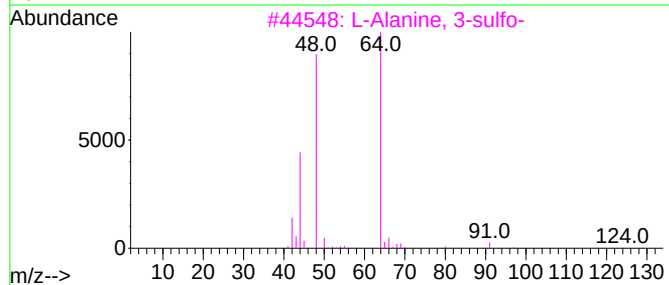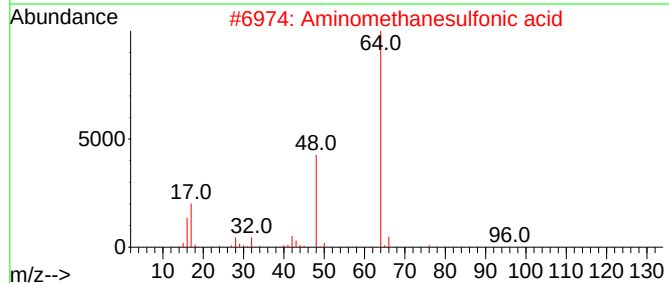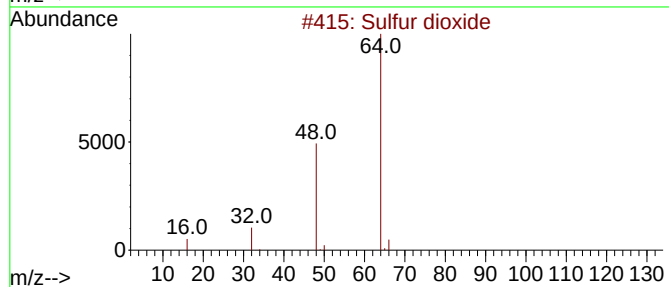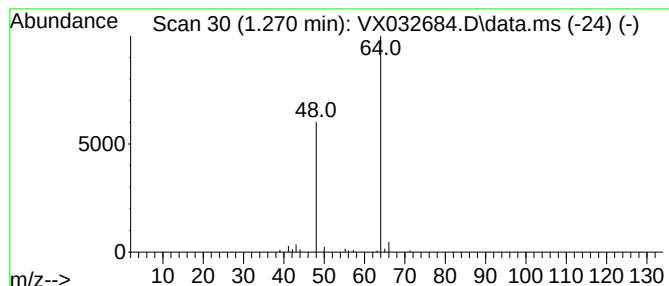

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX110922\
Data File : VX032684.D
Acq On : 09 Nov 2022 17:01
Operator : JC/MD
Sample : N5512-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-1911-TOTE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.270	8.1	ug/l	52174	1	5.556	321225	50.0